

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051220\
 Data File : PS010245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2020 19:03
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 00:02:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.921	315.3E6	272.5E6	448.506	508.181
Target Compounds							
2) T	3,5-DICHL...	6.486	6.100	51531707	286043	53.415	<MDL #
5) T	DICAMBA	0.000	7.089	0	1080793	N.D.	<MDL
6) T	MCP	0.000	7.154	0	30727051	N.D.	16.739
8) T	DICHLORPROP	0.000	7.743	0	4513707	N.D.	7.995
9) T	2,4-D	8.418	7.943	56329431	1377151	79.735	1.986 #
10) T	Pentachlo...	0.000	8.441	0	344682	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.799	0	399218	N.D.	<MDL
12) T	2,4,5-T	0.000	9.183	0	298400	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	455204	N.D.	1.142
14) T	DINOSEB	0.000	10.023	0	156745	N.D.	<MDL
15) T	Picloram	10.993	11.006	20401438	1360439	4.450	<MDL #
16) T	DCPA	0.000	10.954	0	384234	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051220\
Data File : PS010245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2020 19:03
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 00:02:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

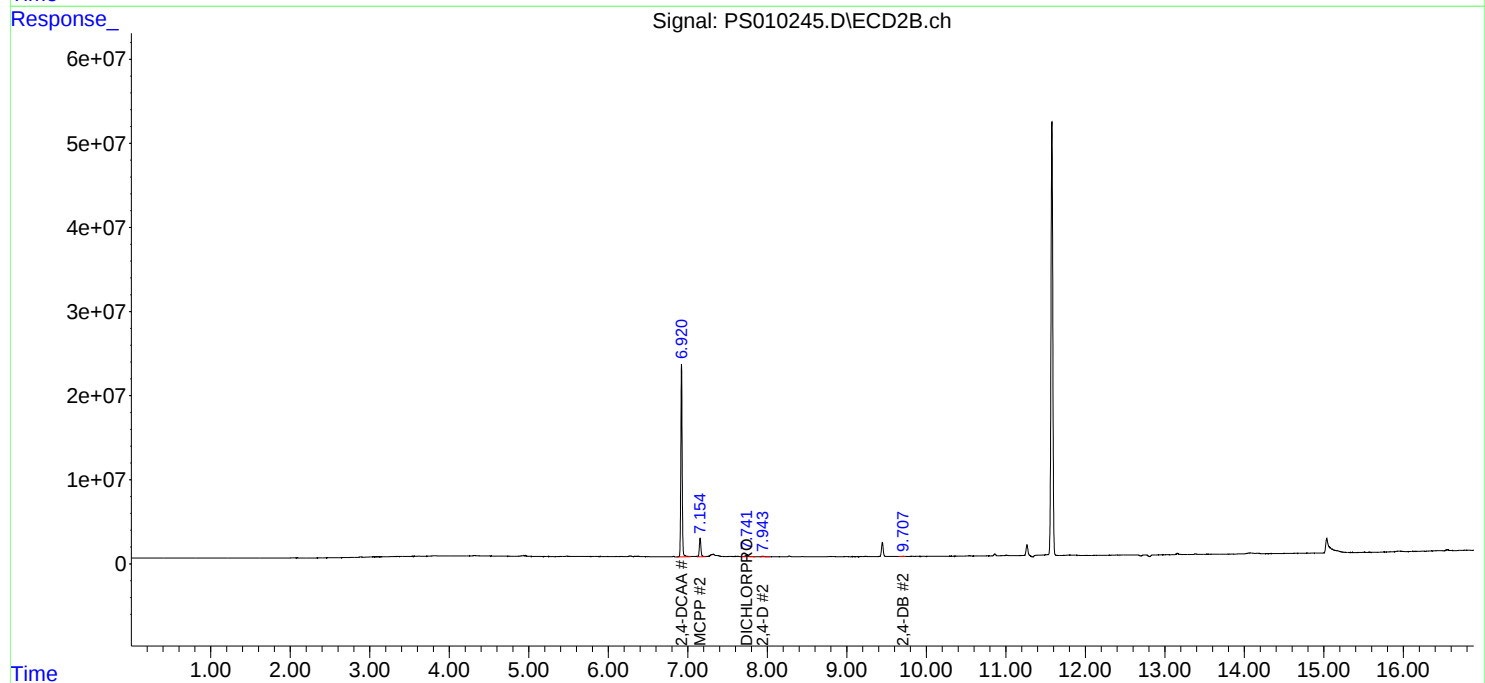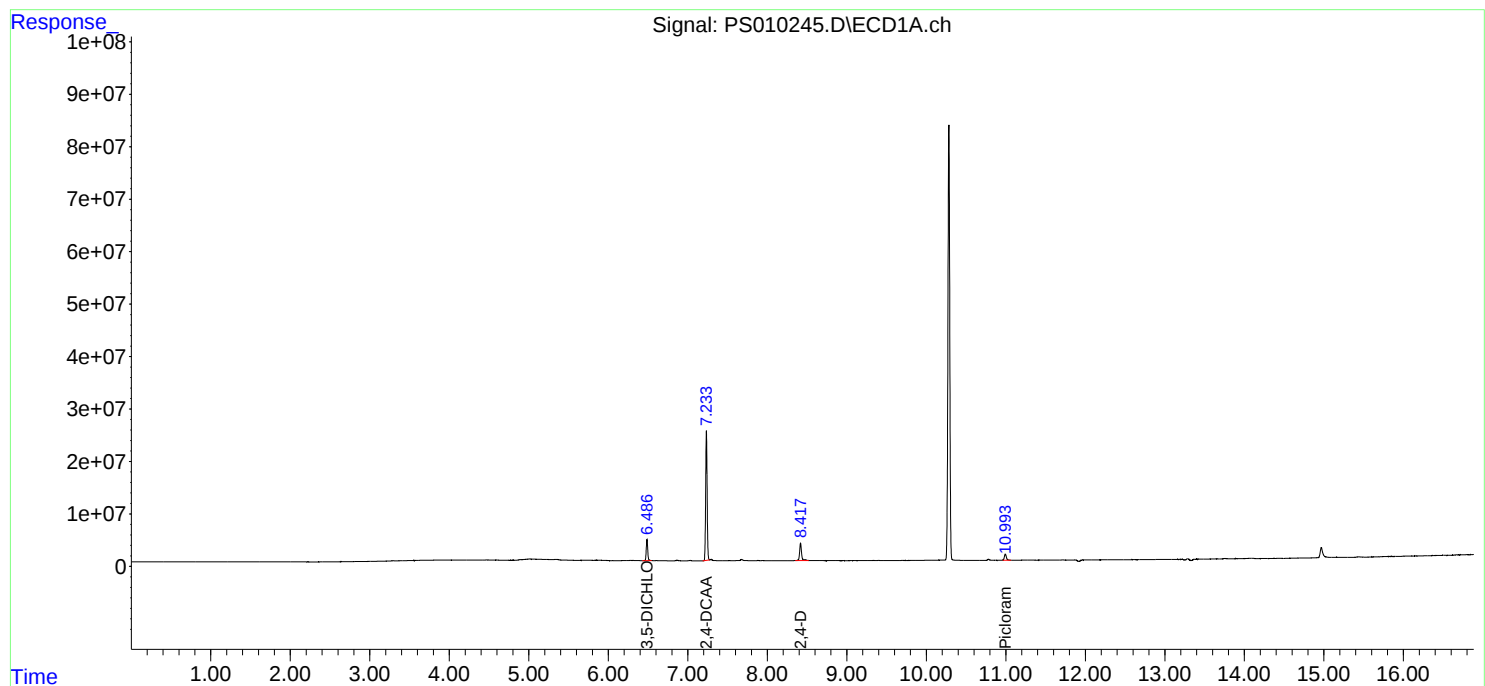


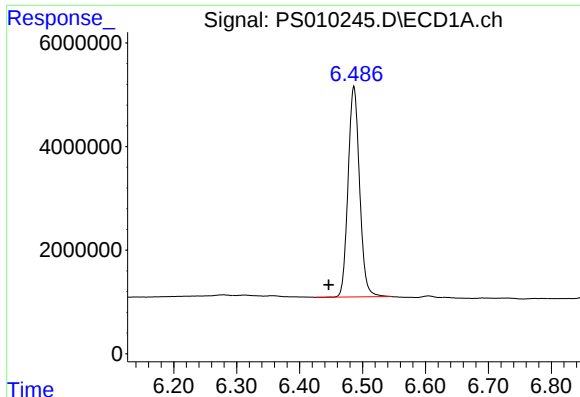

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.486 min
Delta R.T.: 0.040 min
Response: 51531707
Conc: 53.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

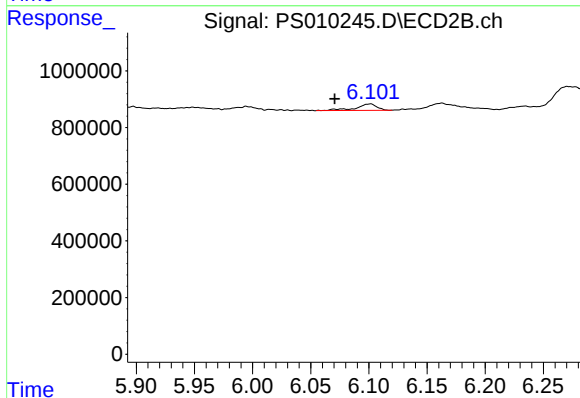


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 286043
Conc: N.D.

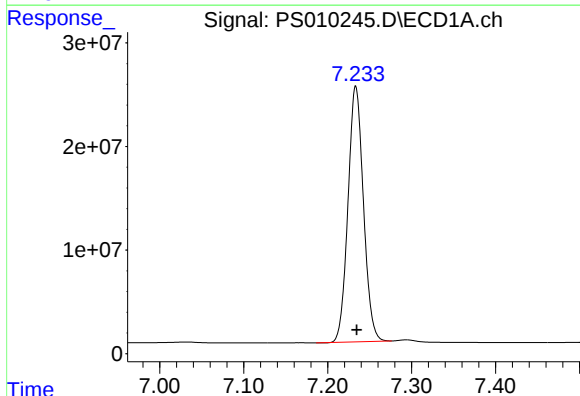


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.001 min
Response: 315341832
Conc: 448.51 ng/ml

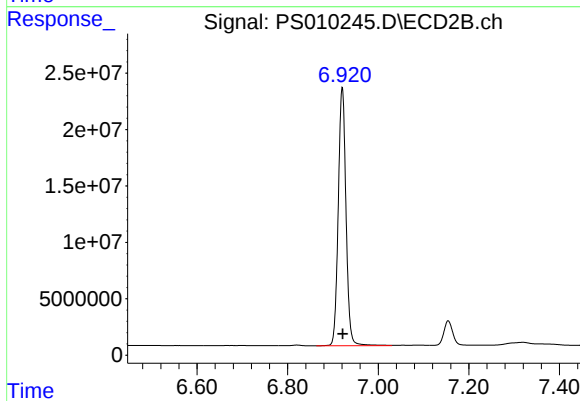

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 272532788
Conc: 508.18 ng/ml

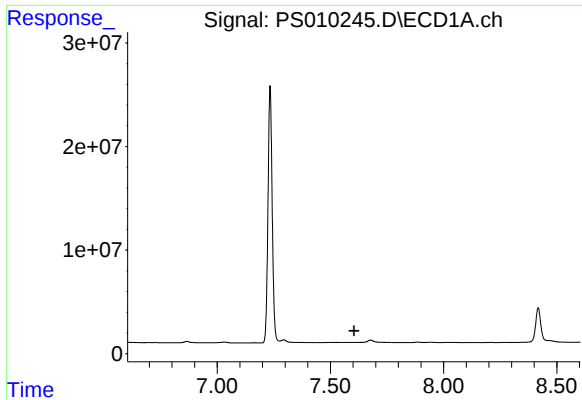

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

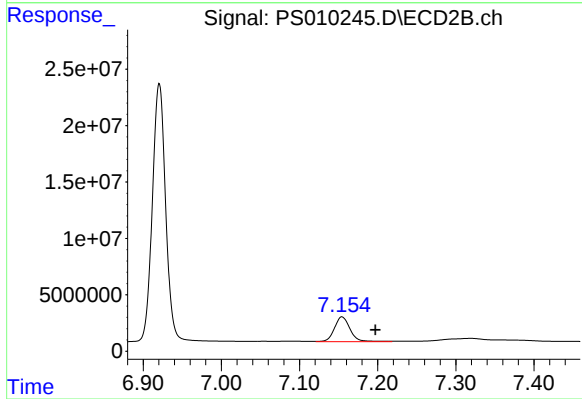


#6 MCP

R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 30727051
Conc: 16.74 ug/ml

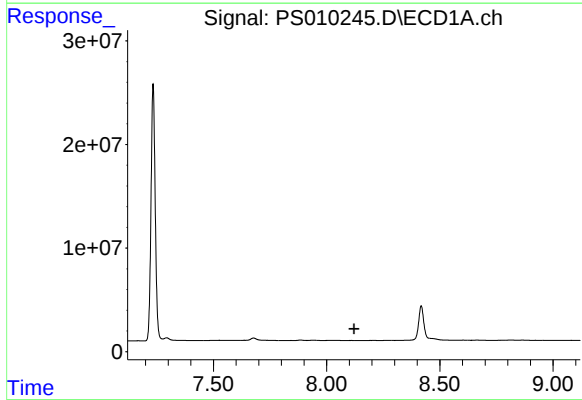


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

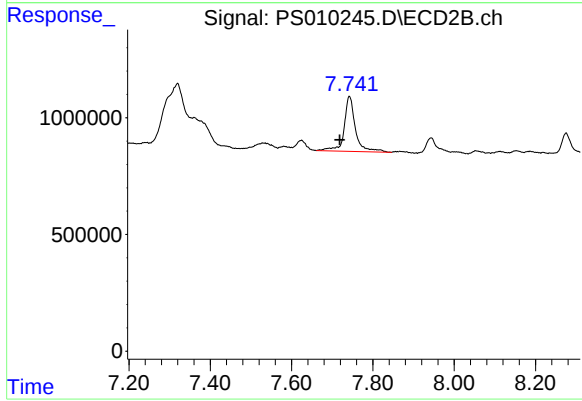

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.024 min
Response: 4513707
Conc: 7.99 ng/ml

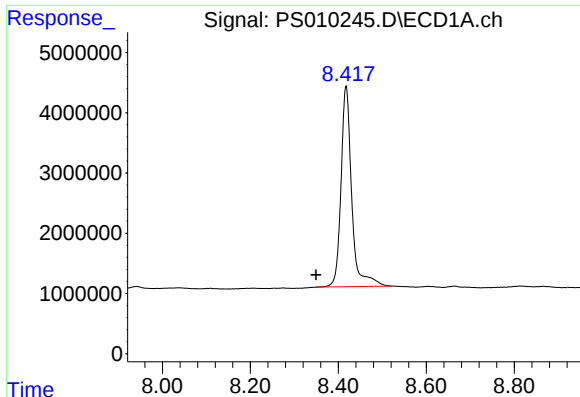

#9 2,4-D


R.T.: 8.418 min
Delta R.T.: 0.069 min
Response: 56329431
Conc: 79.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

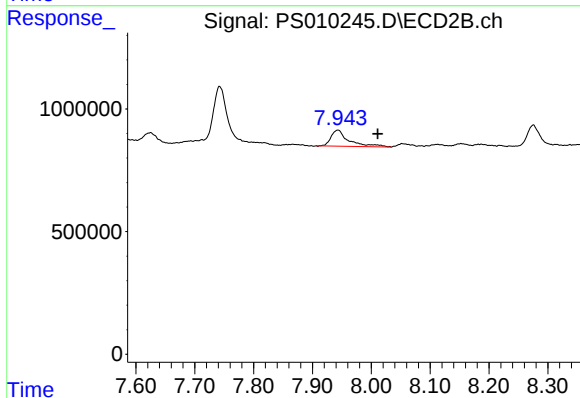


#9 2,4-D

R.T.: 7.943 min
Delta R.T.: -0.068 min
Response: 1377151
Conc: 1.99 ng/ml

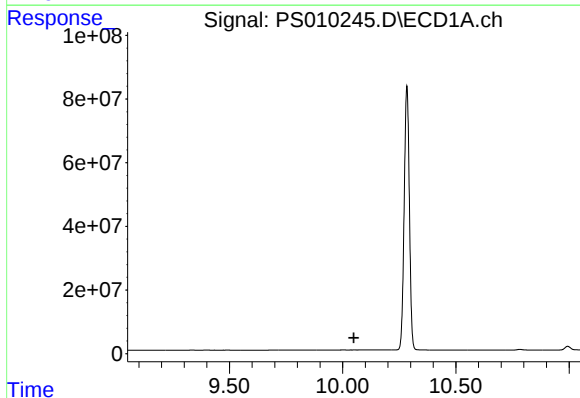


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

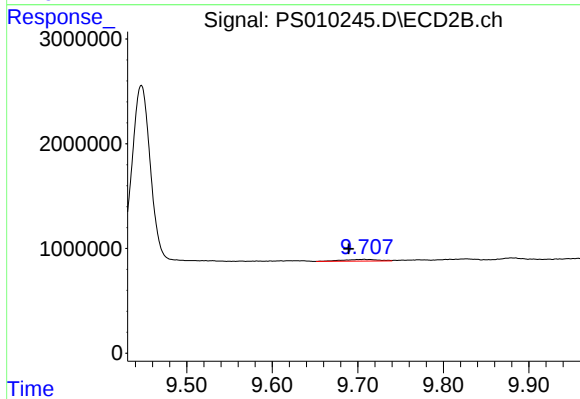

#13 2,4-DB


R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 455204
Conc: 1.14 ng/ml

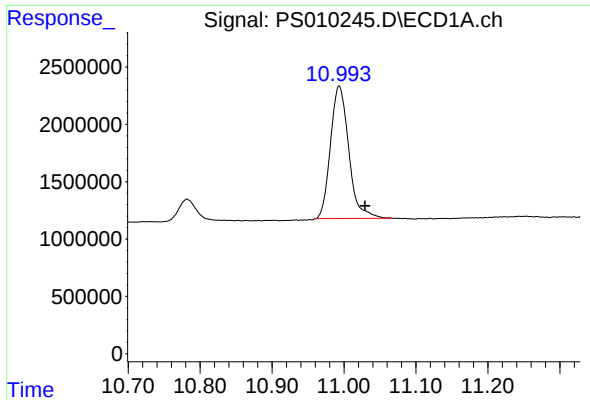

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.036 min
Response: 20401438
Conc: 4.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

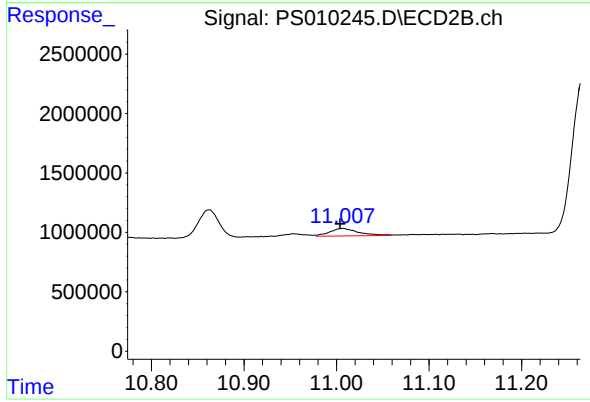

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.003 min
Response: 1360439
Conc: N.D.