

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051221\
 Data File : PS014998.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2021 08:35
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 11:25:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.161	6.889	704.1E6	269.1E6	420.808	556.104 #
Target Compounds							
9) T	2,4-D	8.327f	0.000	4209680	0	2.366	N.D. #
12) T	2,4,5-T	9.390	0.000	13153431	0	1.438	N.D. #
15) T	Picloram	10.984f	11.009f	114.2E6	43504165	9.403	10.918
16) T	DCPA	11.361	0.000	4657033	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051221\
Data File : PS014998.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2021 08:35
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 11:25:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

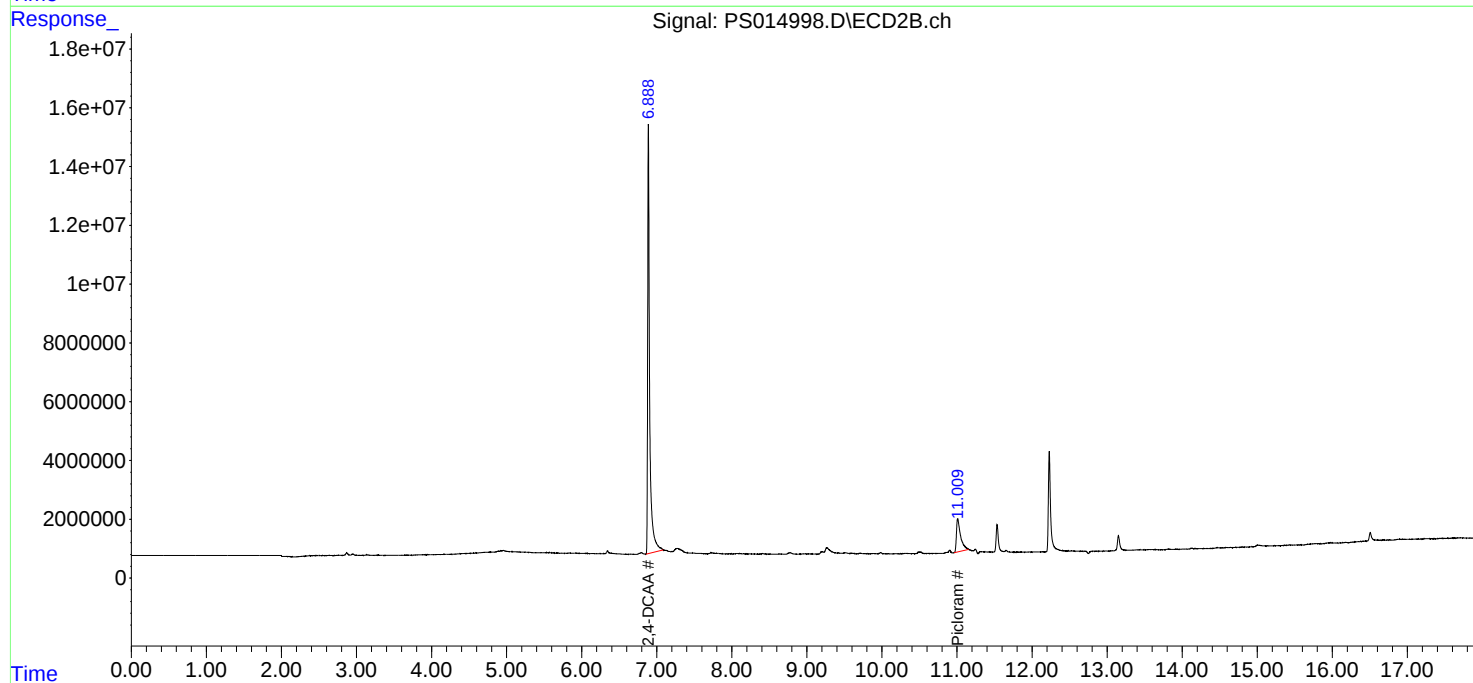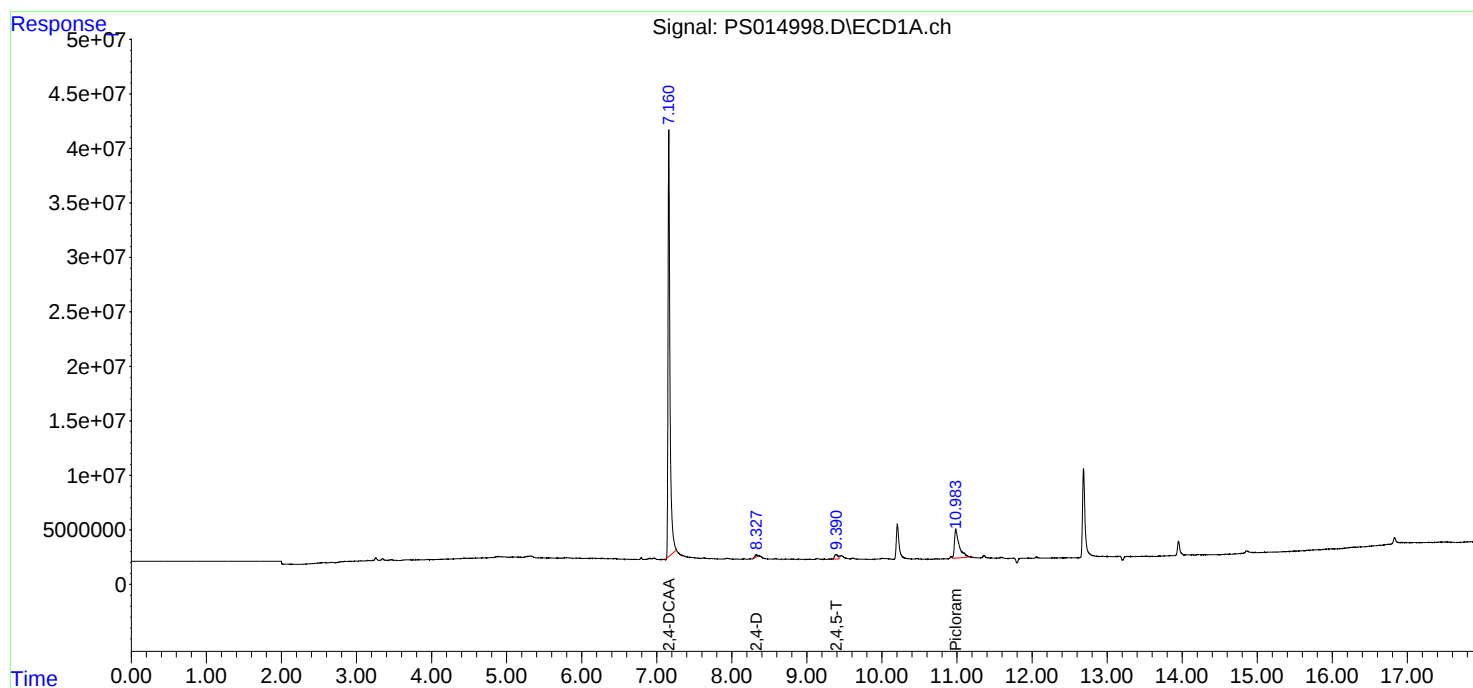


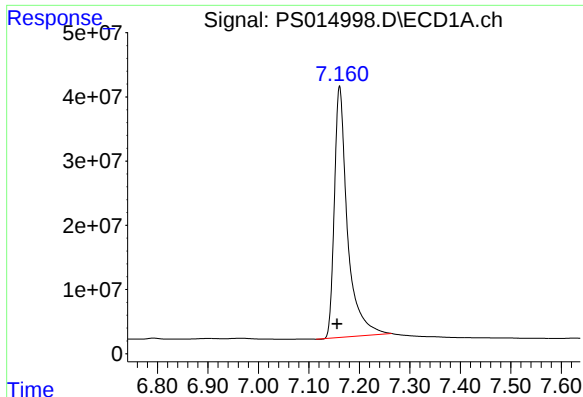

#4 2,4-DCAA


R.T.: 7.161 min
Delta R.T.: 0.005 min
Response: 704116929
Conc: 420.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

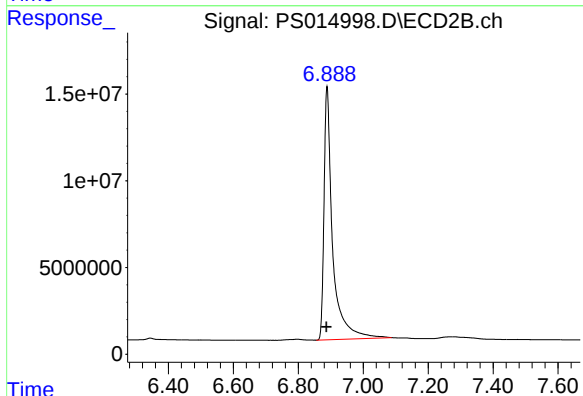


#4 2,4-DCAA

R.T.: 6.889 min
Delta R.T.: 0.002 min
Response: 269106022
Conc: 556.10 ng/ml

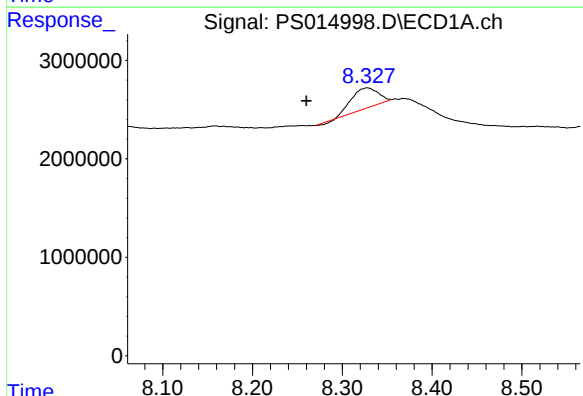


#9 2,4-D

R.T.: 8.327 min
Delta R.T.: 0.067 min
Response: 4209680
Conc: 2.37 ng/ml

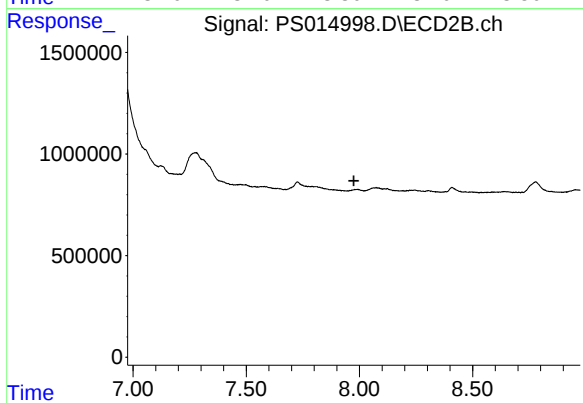

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

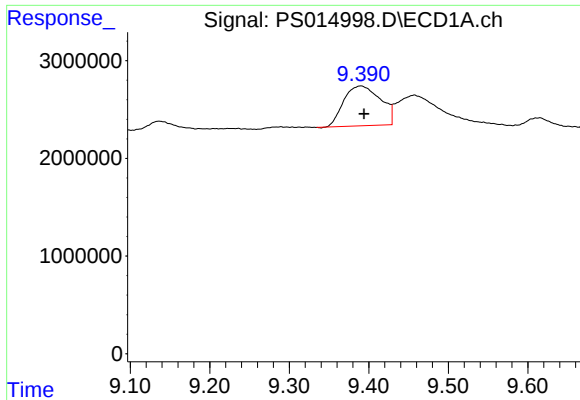

#12 2,4,5-T


R.T.: 9.390 min
Delta R.T.: -0.003 min
Response: 13153431
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

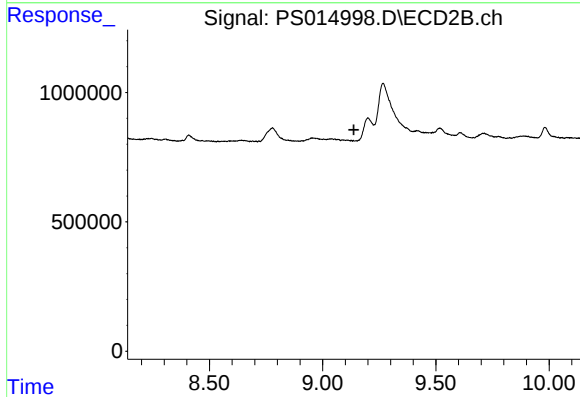


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.138 min
Response: 0
Conc: N.D.

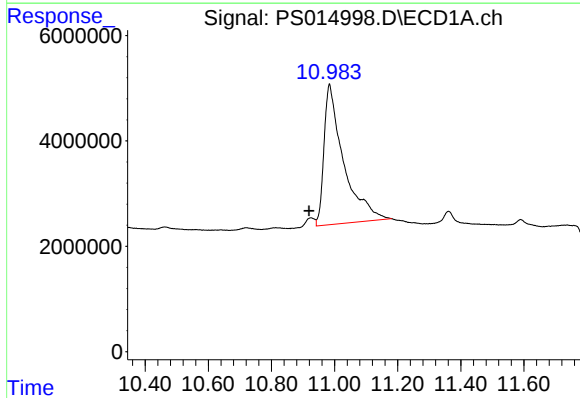

#15 Picloram

R.T.: 10.984 min
Delta R.T.: 0.065 min
Response: 114222108
Conc: 9.40 ng/ml

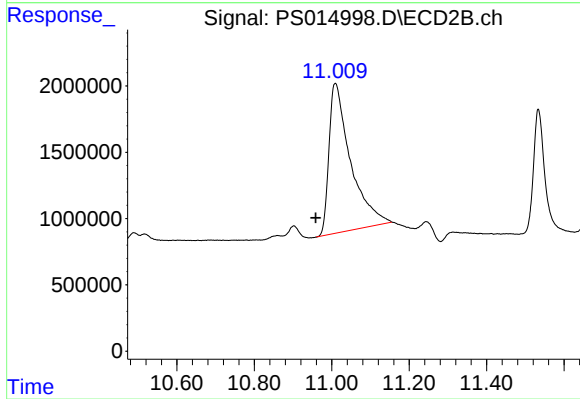

#15 Picloram

R.T.: 11.009 min
Delta R.T.: 0.051 min
Response: 43504165
Conc: 10.92 ng/ml