

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051222\
 Data File : PS019382.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2022 09:48
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 01:21:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	0.000	2015710	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.439	5.905f	-295063	140546	N.D.	<MDL
5) T	DICAMBA	7.412	7.023f	1152026	3178860	<MDL	<MDL #
6) T	MCP	7.603	7.108	-890739	347992	N.D.	<MDL
8) T	DICHLORPROP	8.115	7.618	353788	11747763	<MDL	13.708 #
9) T	2,4-D	8.336	7.934f	1233106	262514	<MDL	<MDL #
10) T	Pentachlo...	8.660	8.306	9522547	1305127	<MDL	<MDL #
11) T	2,4,5-TP ...	9.208	8.672	151121	758986	<MDL	<MDL #
12) T	2,4,5-T	9.470	9.061	2720490	657222	<MDL	<MDL #
13) T	2,4-DB	10.081f	9.570	2387150	703606	<MDL	1.238 #
14) T	DINOSEB	0.000	9.877	0	386570	N.D.	<MDL
15) T	Picloram	10.989	10.890	611.2E6	28957989	20.909	4.842 #
16) T	DCPA	11.466	10.814	1740188	12691665	<MDL	2.162 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051222\
Data File : PS019382.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2022 09:48
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 01:21:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

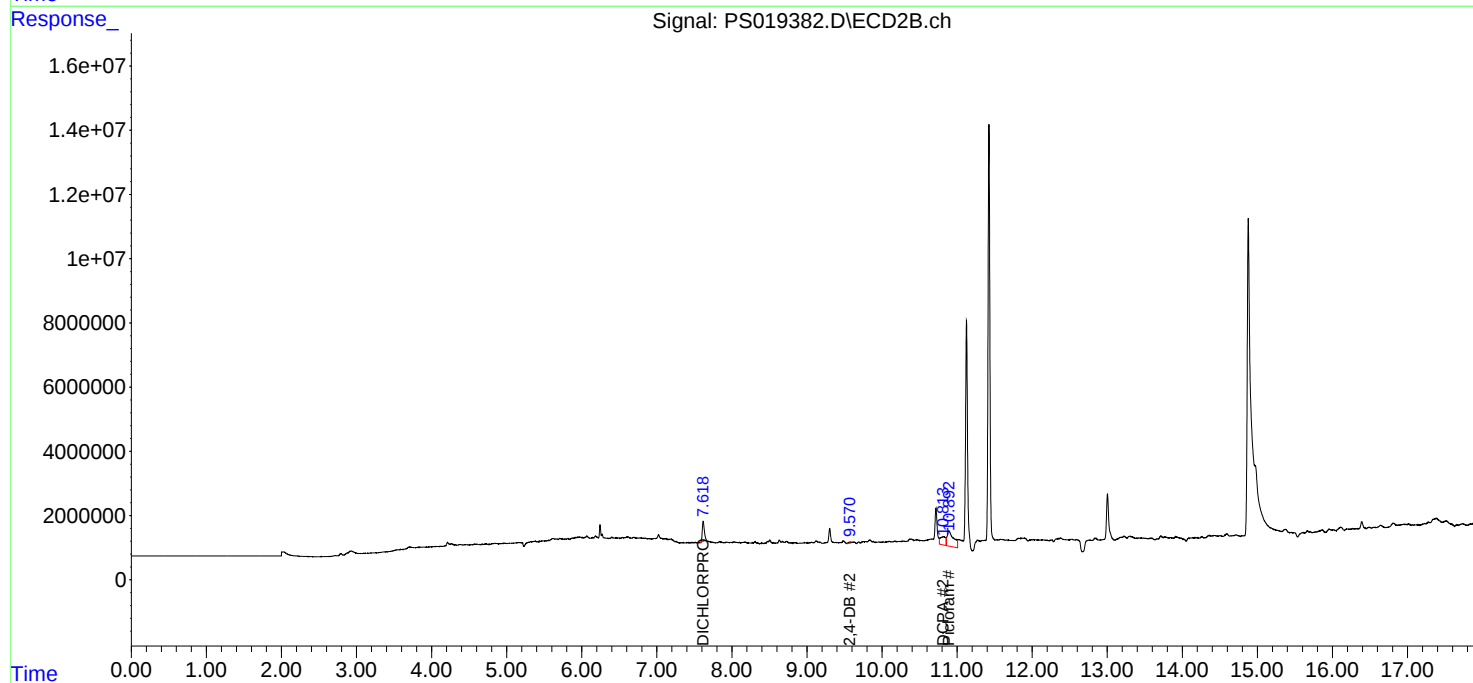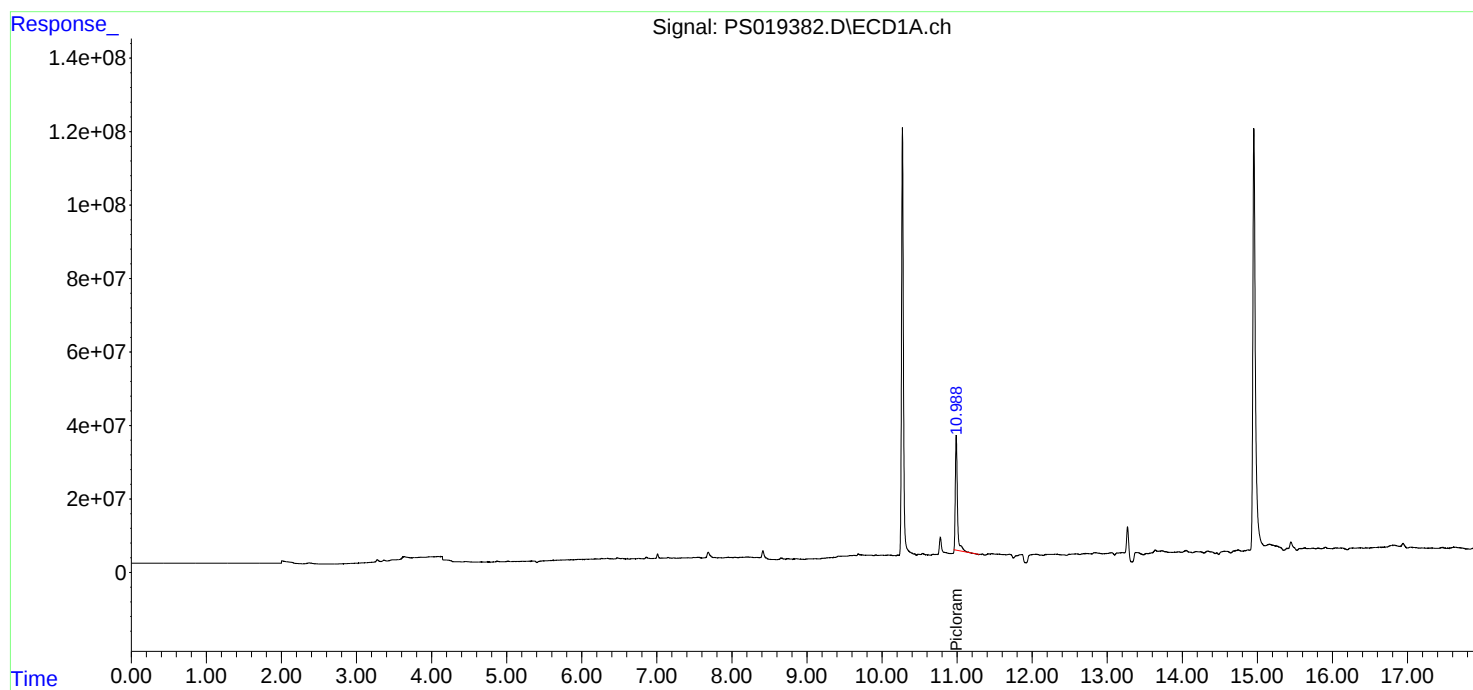


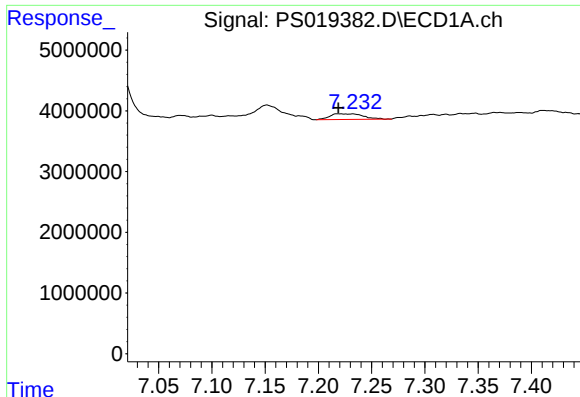

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: 0.002 min
Response: 2015710
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

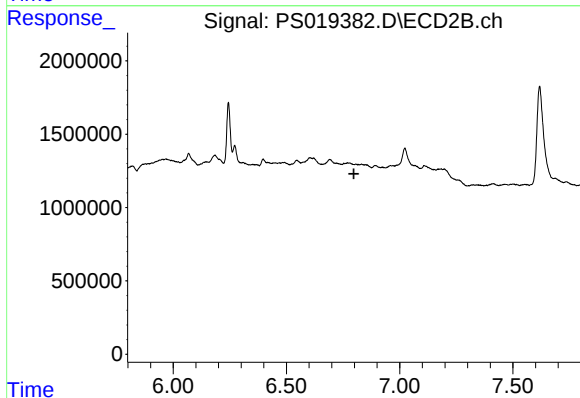


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.798 min
Response: 0
Conc: N.D.

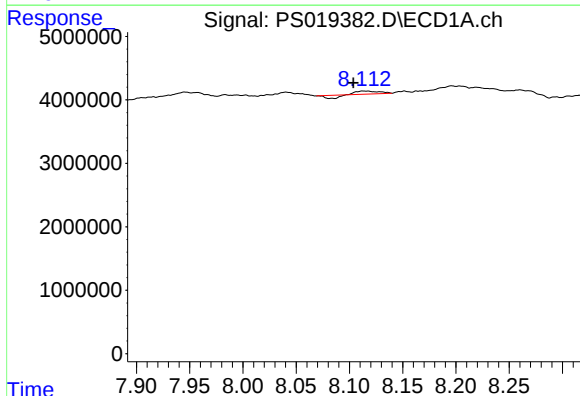


#8 DICHLORPROP

R.T.: 8.115 min
Delta R.T.: 0.011 min
Response: 353788
Conc: N.D.

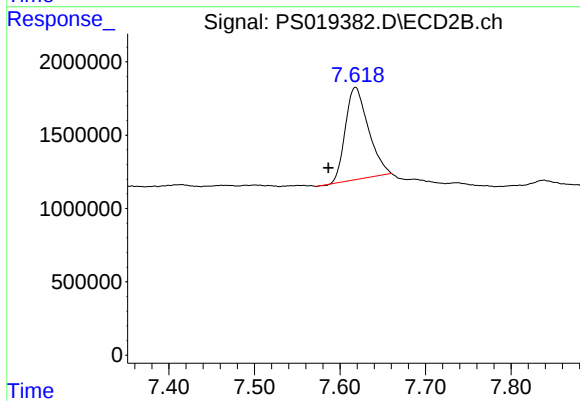

#8 DICHLORPROP


R.T.: 7.618 min
Delta R.T.: 0.032 min
Response: 11747763
Conc: 13.71 ng/ml

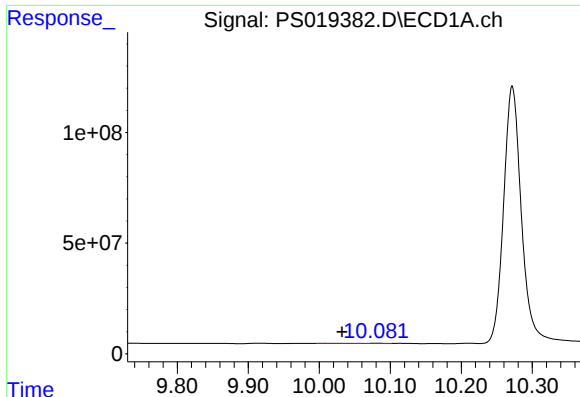

#13 2,4-DB


R.T.: 10.081 min
Delta R.T.: 0.049 min
Response: 2387150
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

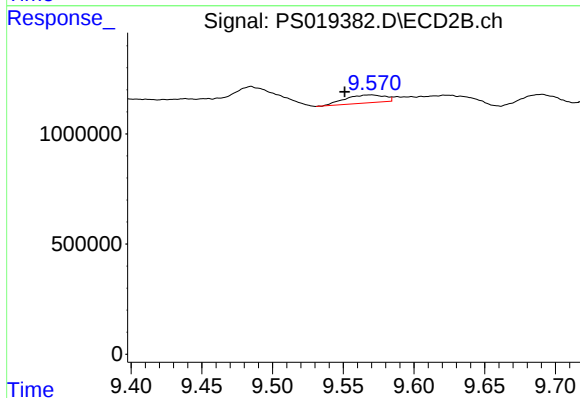


#13 2,4-DB

R.T.: 9.570 min
Delta R.T.: 0.019 min
Response: 703606
Conc: 1.24 ng/ml

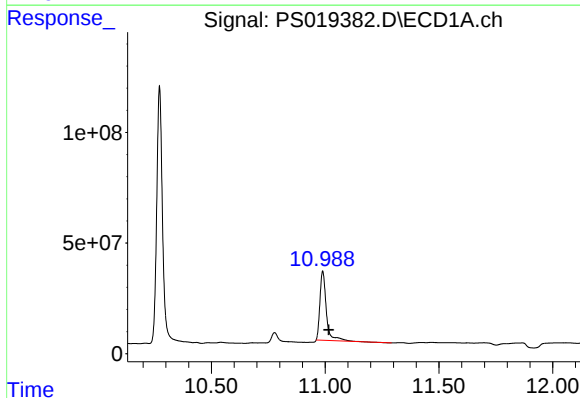


#15 Picloram

R.T.: 10.989 min
Delta R.T.: -0.027 min
Response: 611157949
Conc: 20.91 ng/ml

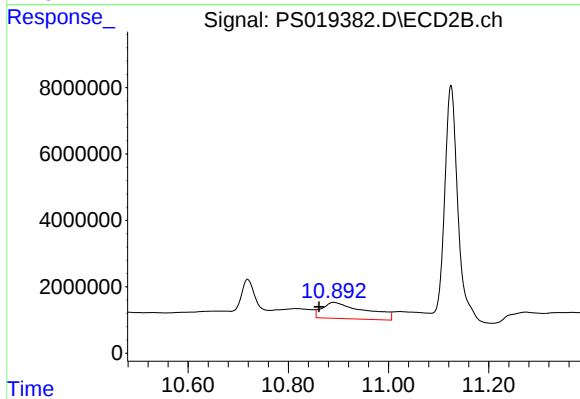

#15 Picloram


R.T.: 10.890 min
Delta R.T.: 0.028 min
Response: 28957989
Conc: 4.84 ng/ml

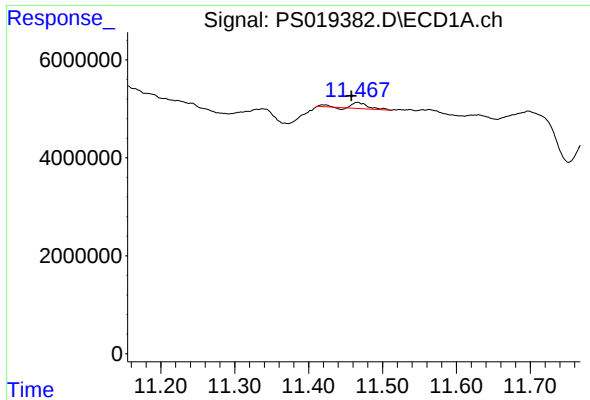

#16 DCPA

R.T.: 11.466 min
Delta R.T.: 0.008 min
Response: 1740188
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

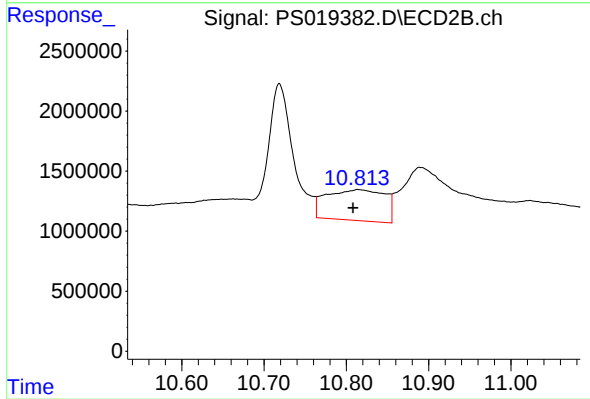

#16 DCPA

R.T.: 10.814 min
Delta R.T.: 0.006 min
Response: 12691665
Conc: 2.16 ng/ml