

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051223\
 Data File : PS023014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2023 18:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:13:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
 Quant Title : 8080.M
 QLast Update : Wed May 10 16:09:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.483	6.858	831.1E6	307.6E6	546.438	548.187
Target Compounds							
1) T	Dalapon	2.585	0.000	4056747	0	2.509	N.D. #
3) T	4-Nitroph...	6.316	0.000	6208539	0	5.897	N.D. #
5) T	DICAMBA	6.629	0.000	5677	0	<MDL	N.D. #
6) T	MCP	6.818	0.000	1221545	0	<MDL	N.D. #
7) T	MCPA	6.937	7.312	206617	7528033	<MDL	2.843 #
8) T	DICHLORPROP	7.239	7.665	831742	2560308	<MDL	4.137 #
9) T	2,4-D	7.406	7.881f	8510274	855994	3.677	1.196 #
10) T	Pentachlo...	7.677	0.000	1100337	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.214	0.000	15403792	0	1.319	N.D. #
12) T	2,4,5-T	8.481	9.100	5723241	877889	<MDL	<MDL #
13) T	2,4-DB	8.938f	0.000	38750855	0	16.518	N.D. #
14) T	DINOSEB	10.065	0.000	1660015	0	<MDL	N.D. #
15) T	Picloram	9.895	10.905	28349906	2580624	1.653	<MDL #
16) T	DCPA	10.333	10.905	2419436	2580624	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051223\
Data File : PS023014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2023 18:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:13:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051023.M
Quant Title : 8080.M
QLast Update : Wed May 10 16:09:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

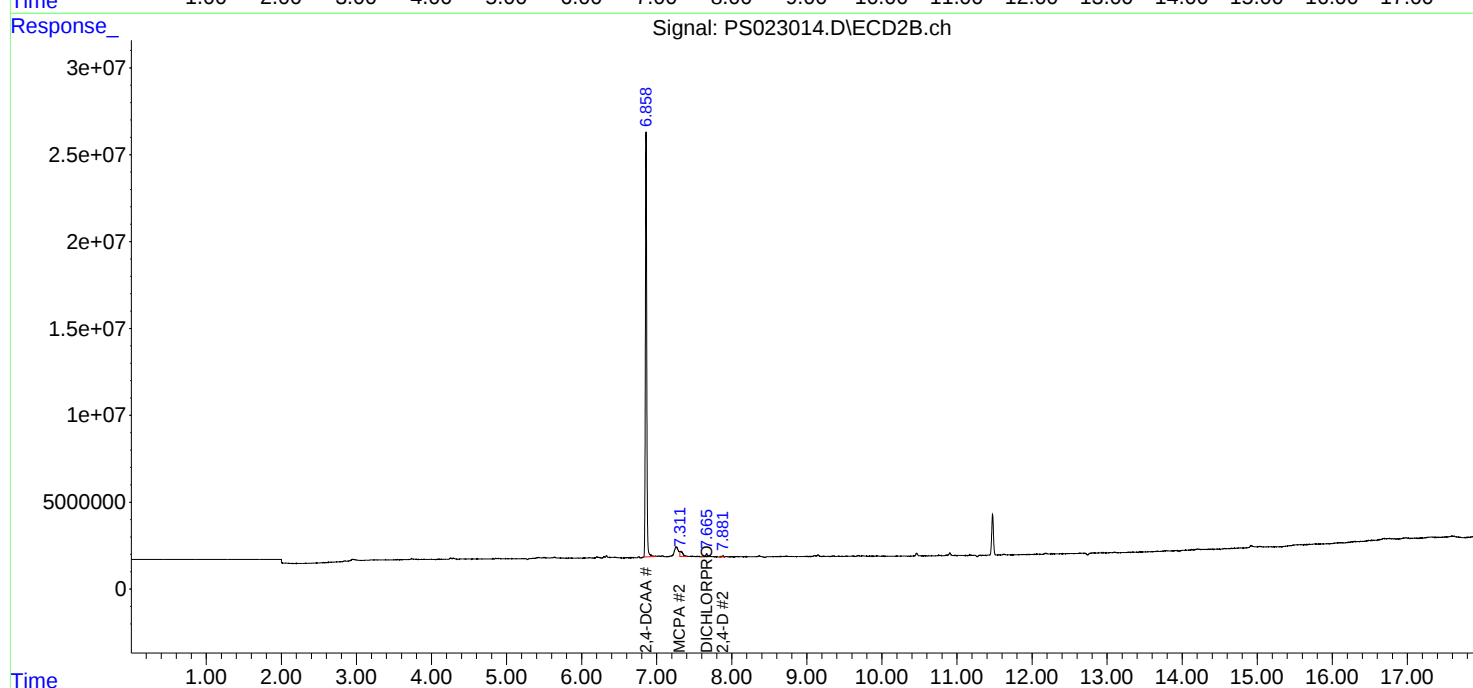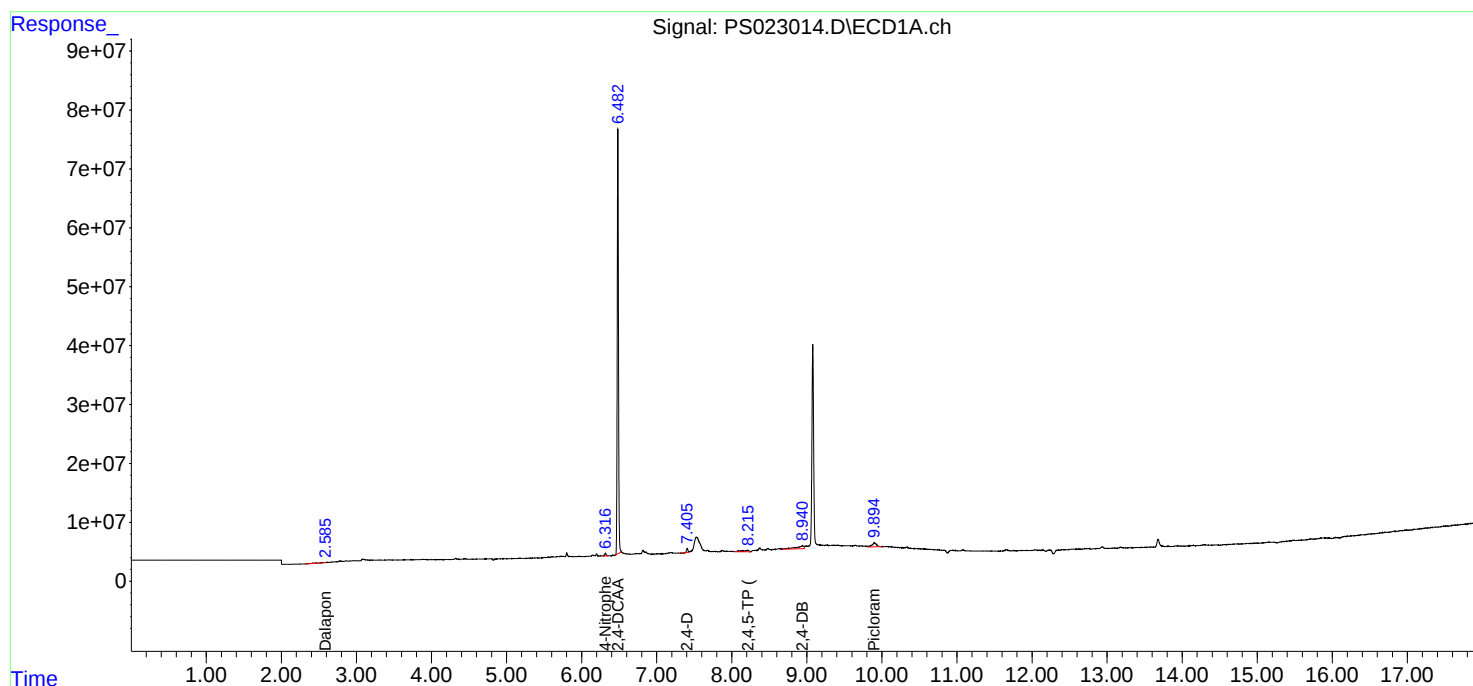


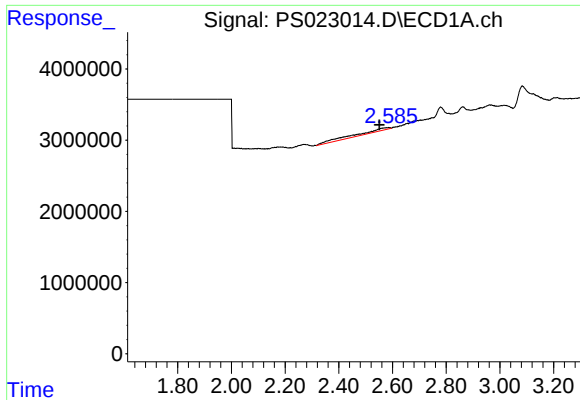

#1 Dalapon


R.T.: 2.585 min
Delta R.T.: 0.034 min
Response: 4056747
Conc: 2.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

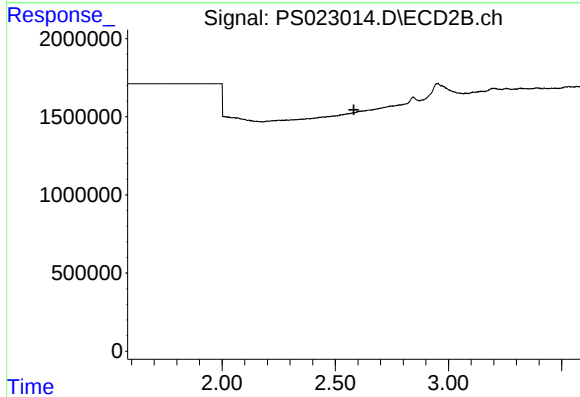


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.582 min
Response: 0
Conc: N.D.

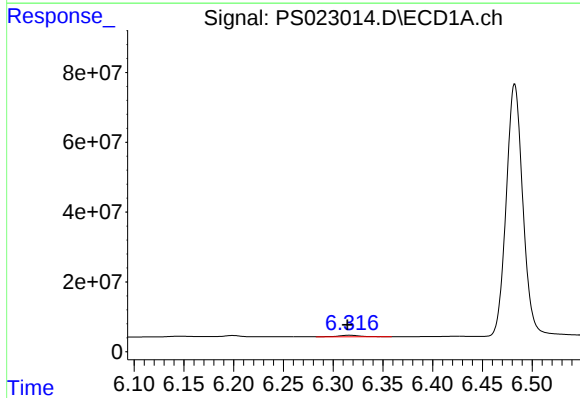


#3 4-Nitrophenol

R.T.: 6.316 min
Delta R.T.: 0.002 min
Response: 6208539
Conc: 5.90 ng/ml

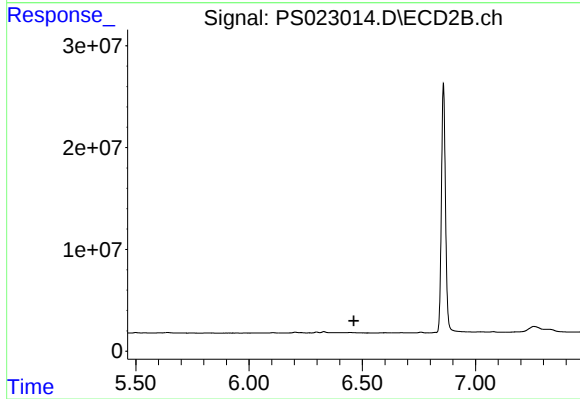

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.463 min
Response: 0
Conc: N.D.

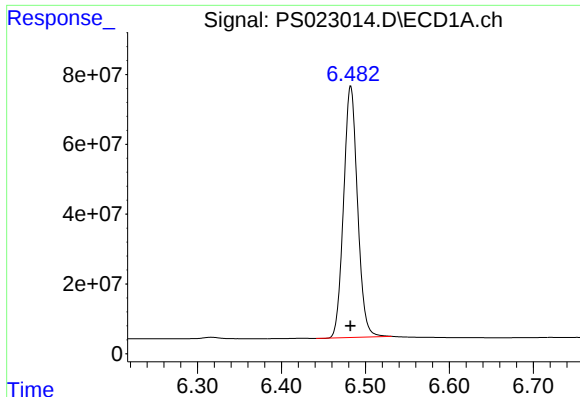

#4 2,4-DCAA


R.T.: 6.483 min
Delta R.T.: 0.000 min
Response: 831129761
Conc: 546.44 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

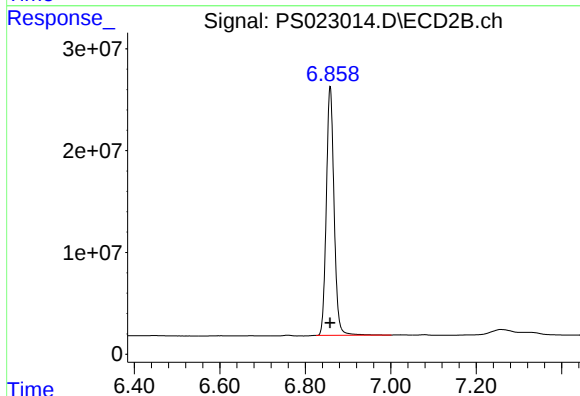


#4 2,4-DCAA

R.T.: 6.858 min
Delta R.T.: 0.000 min
Response: 307596222
Conc: 548.19 ng/ml

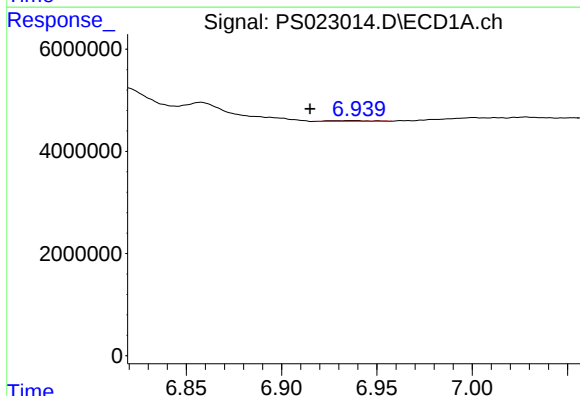


#7 MCPA

R.T.: 6.937 min
Delta R.T.: 0.022 min
Response: 206617
Conc: N.D.

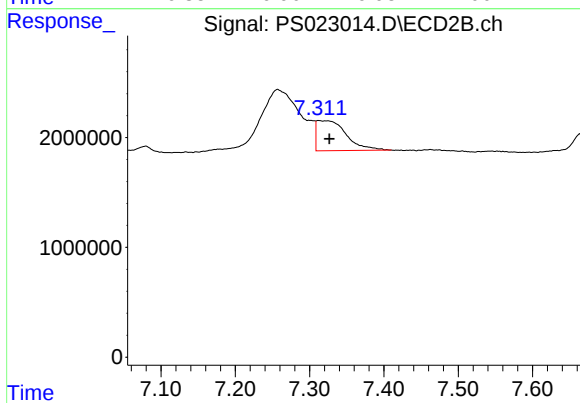

#7 MCPA


R.T.: 7.312 min
Delta R.T.: -0.015 min
Response: 7528033
Conc: 2.84 ug/ml

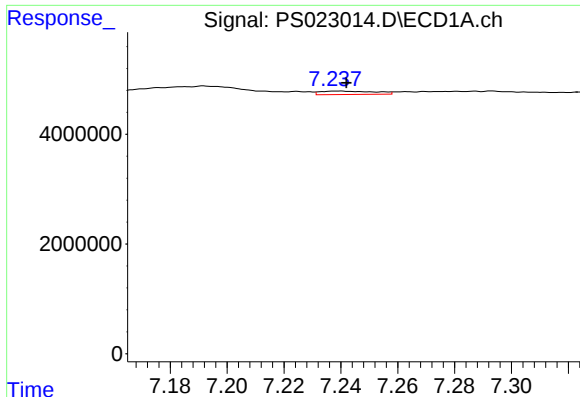

#8 DICHLORPROP


R.T.: 7.239 min
Delta R.T.: -0.003 min
Response: 831742
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

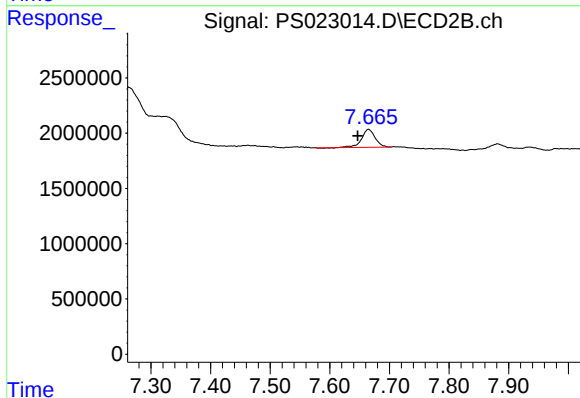


#8 DICHLORPROP

R.T.: 7.665 min
Delta R.T.: 0.018 min
Response: 2560308
Conc: 4.14 ng/ml

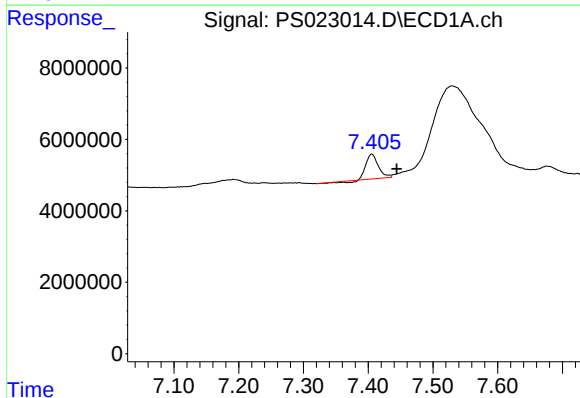


#9 2,4-D

R.T.: 7.406 min
Delta R.T.: -0.039 min
Response: 8510274
Conc: 3.68 ng/ml

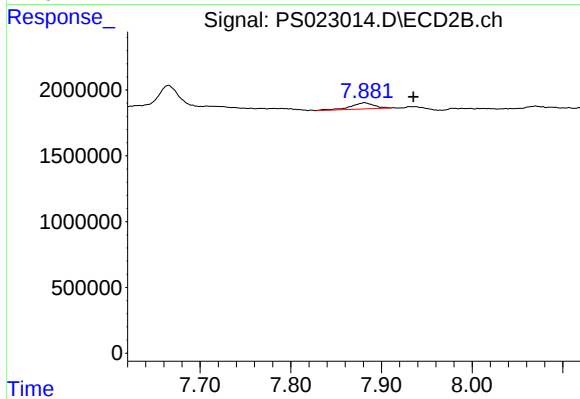

#9 2,4-D


R.T.: 7.881 min
Delta R.T.: -0.054 min
Response: 855994
Conc: 1.20 ng/ml

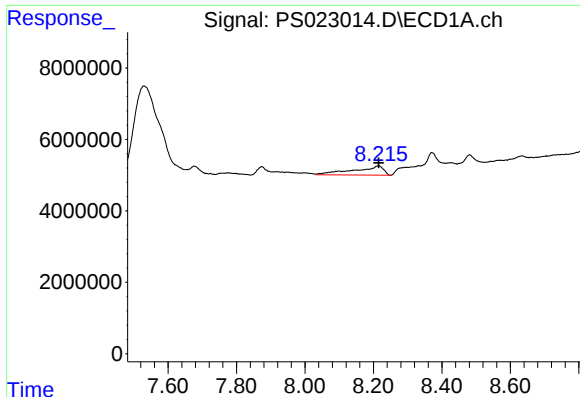

#11 2,4,5-TP (SILVEX)


R.T.: 8.214 min
Delta R.T.: -0.002 min
Response: 15403792
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

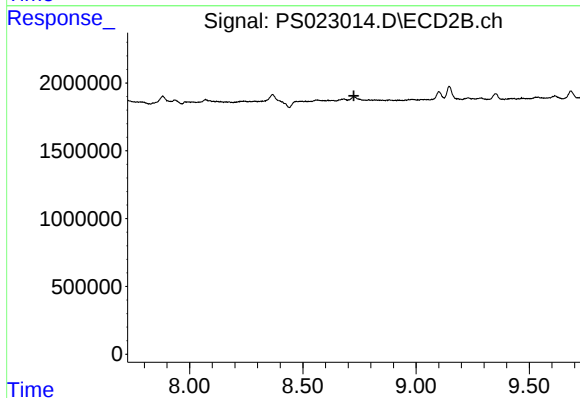


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.725 min
Response: 0
Conc: N.D.

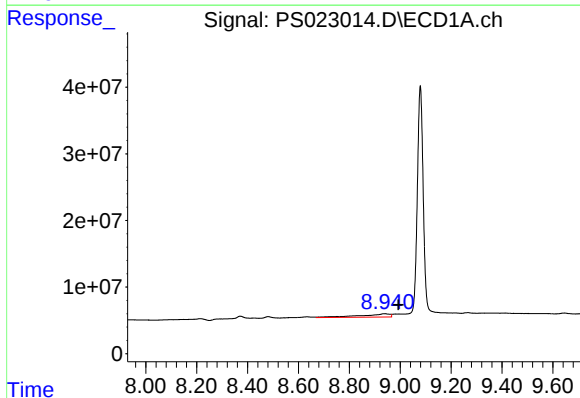


#13 2,4-DB

R.T.: 8.938 min
Delta R.T.: -0.054 min
Response: 38750855
Conc: 16.52 ng/ml

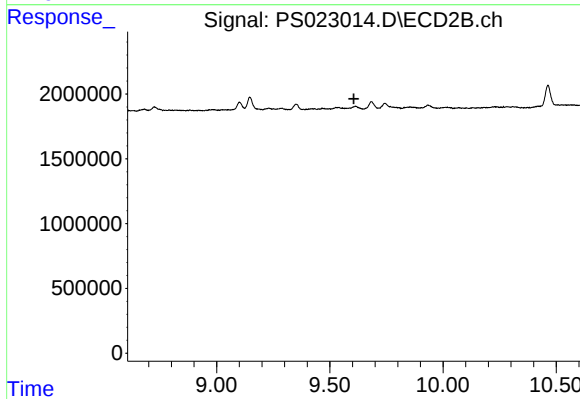

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.606 min
Response: 0
Conc: N.D.

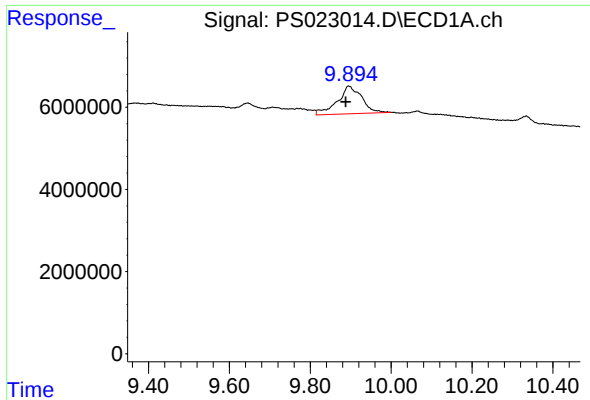

#15 Picloram

R.T.: 9.895 min
Delta R.T.: 0.007 min
Response: 28349906
Conc: 1.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

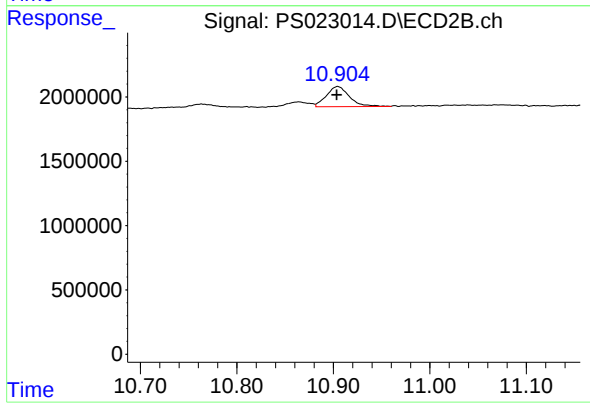

#15 Picloram

R.T.: 10.905 min
Delta R.T.: 0.001 min
Response: 2580624
Conc: N.D.