

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051319\
 Data File : PS004569.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2019 11:41
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 04:19:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) T	MCPA	0.000	6.045	0	44010912	N.D.	21.535
9) T	2,4-D	7.102	0.000	44888595	0	61.610	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051319\
Data File : PS004569.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2019 11:41
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 04:19:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

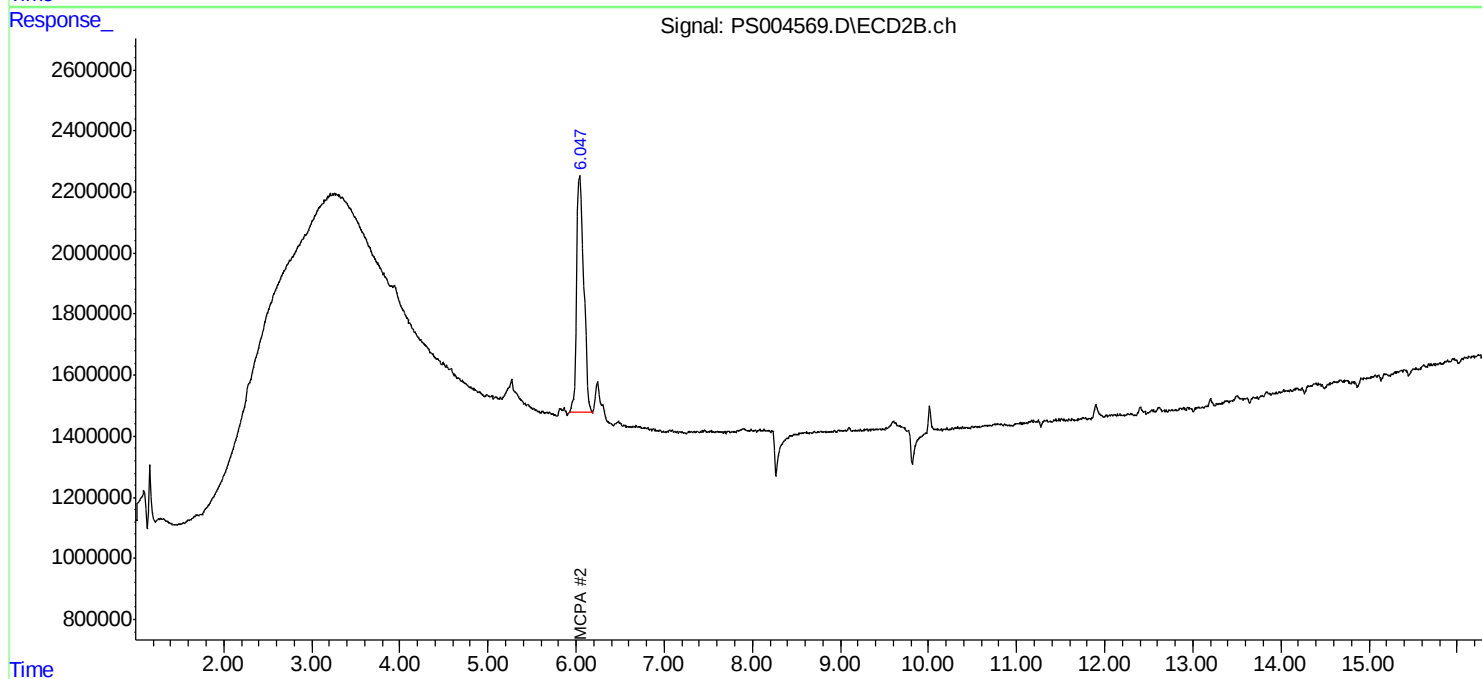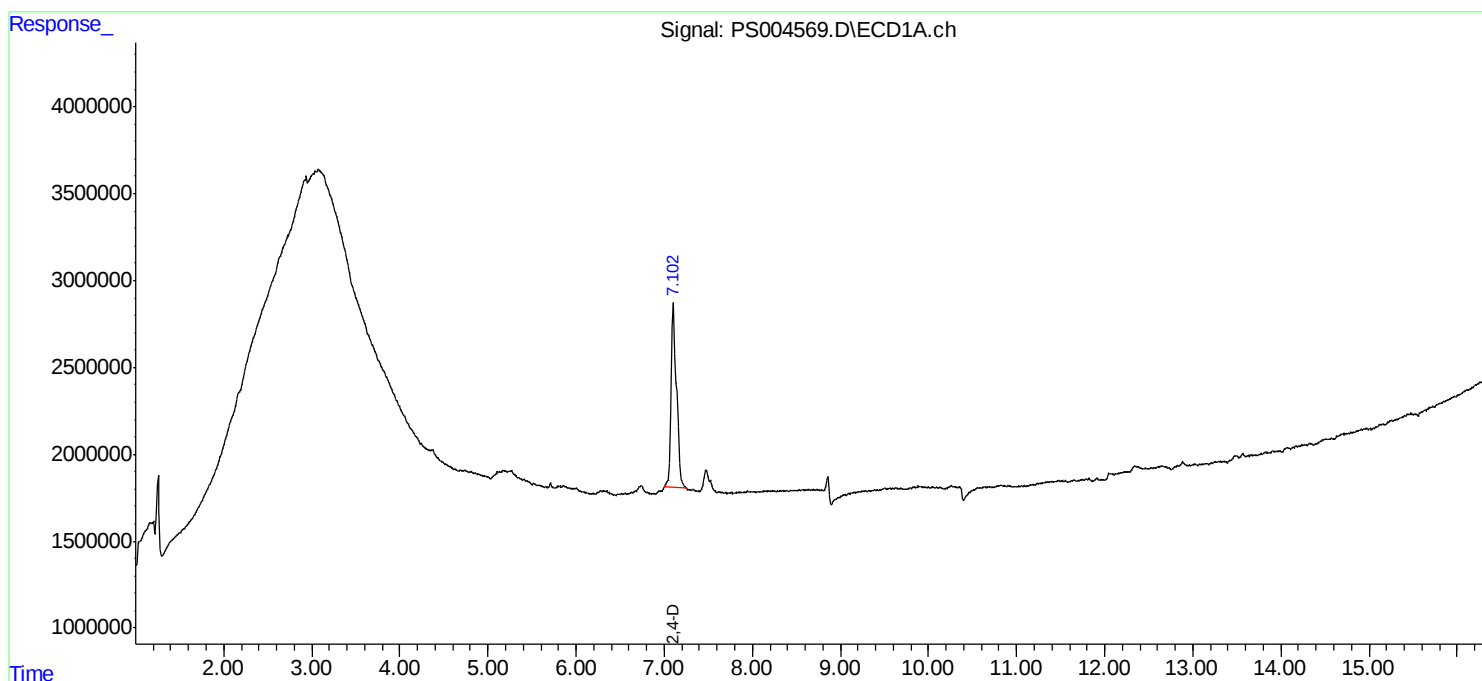


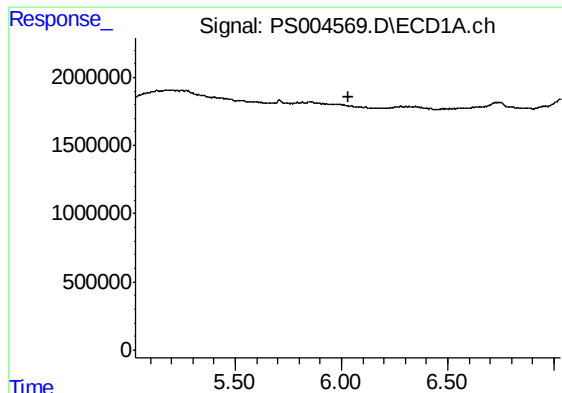

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.031 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

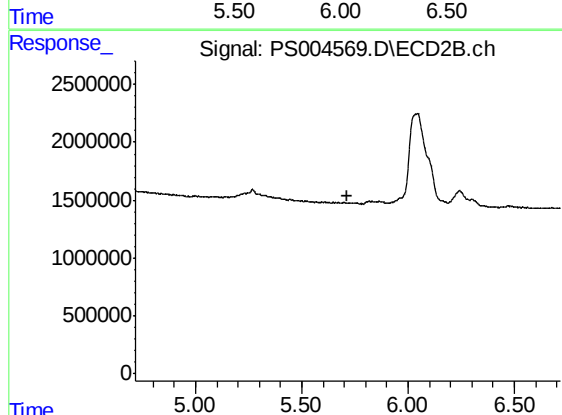


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.717 min
Response: 0
Conc: N.D.

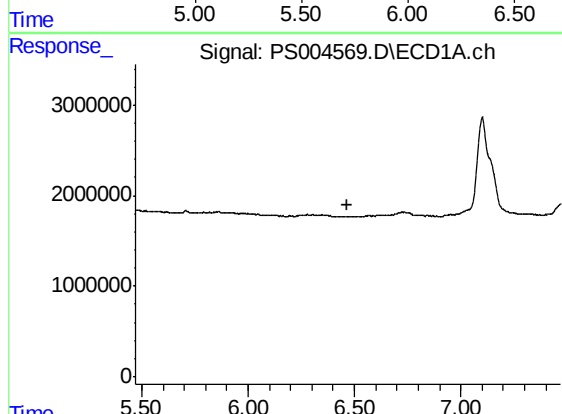


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

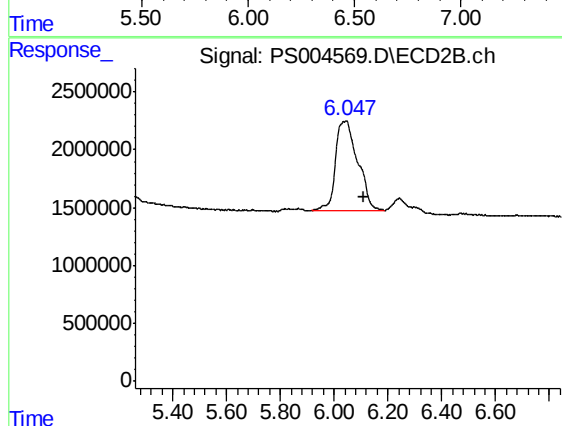

#7 MCPA


R.T.: 6.045 min
Delta R.T.: -0.067 min
Response: 44010912
Conc: 21.53 ug/ml

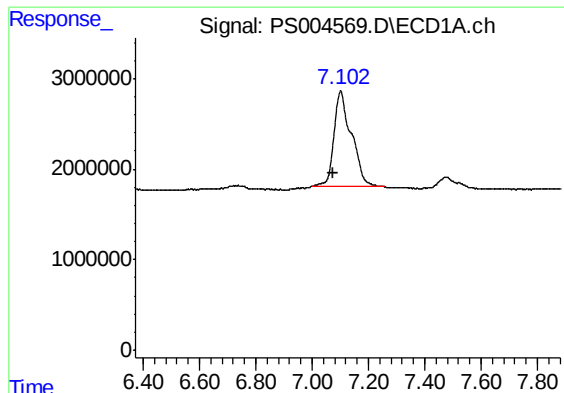

#9 2,4-D

R.T.: 7.102 min
Delta R.T.: 0.027 min
Response: 44888595
Conc: 61.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

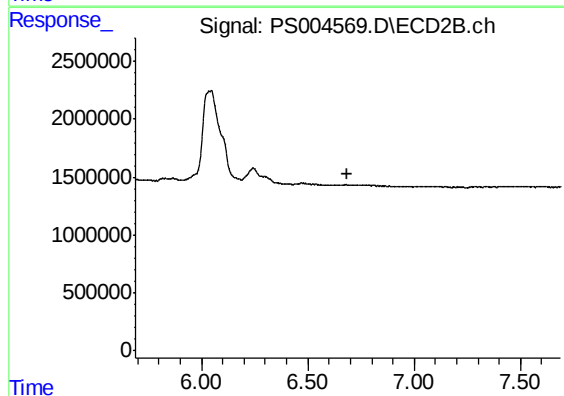

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.