

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051319\
 Data File : PS004573.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2019 13:42
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 15:14:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:13:17 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.021	5.713	509.1E6	363.0E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.409	2.066	622.3E6	472.6E6	682.500	682.500
2) T	3,5-DICHL...	5.361	5.000	577.7E6	443.3E6	697.500	697.500
3) T	4-Nitroph...	5.876	5.387	176.6E6	146.1E6	682.500	682.500
5) T	DICAMBA	6.179	5.846	1849.6E6	1356.0E6	705.000	705.000
6) T	MCPD	6.335	5.932	137.3E6	98069776	70.500	70.500
7) T	MCPA	6.472	6.117	194.1E6	138.8E6	69.750	69.750
8) T	DICHLORPROP	6.826	6.406	427.0E6	329.8E6	705.000	705.000
9) T	2,4-D	7.049	6.681	554.2E6	368.6E6	705.000	705.000
10) T	Pentachlo...	7.311	7.055	6940.4E6	4864.1E6	712.500	712.500
11) T	2,4,5-TP ...	7.852	7.420	2697.2E6	1873.4E6	712.500	712.500
12) T	2,4,5-T	8.131	7.819	2721.8E6	1674.2E6	712.500	712.500
13) T	2,4-DB	8.666	8.272	252.6E6	218.1E6	712.500	712.500
14) T	DINOSEB	9.761	8.584	2370.5E6	1424.5E6	705.000	705.000
15) T	Picloram	9.597	9.528	3397.1E6	2599.0E6	712.500	712.500
16) T	DCPA	10.033	9.485	3497.2E6	2403.4E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051319\
Data File : PS004573.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2019 13:42
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 15:14:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:13:17 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

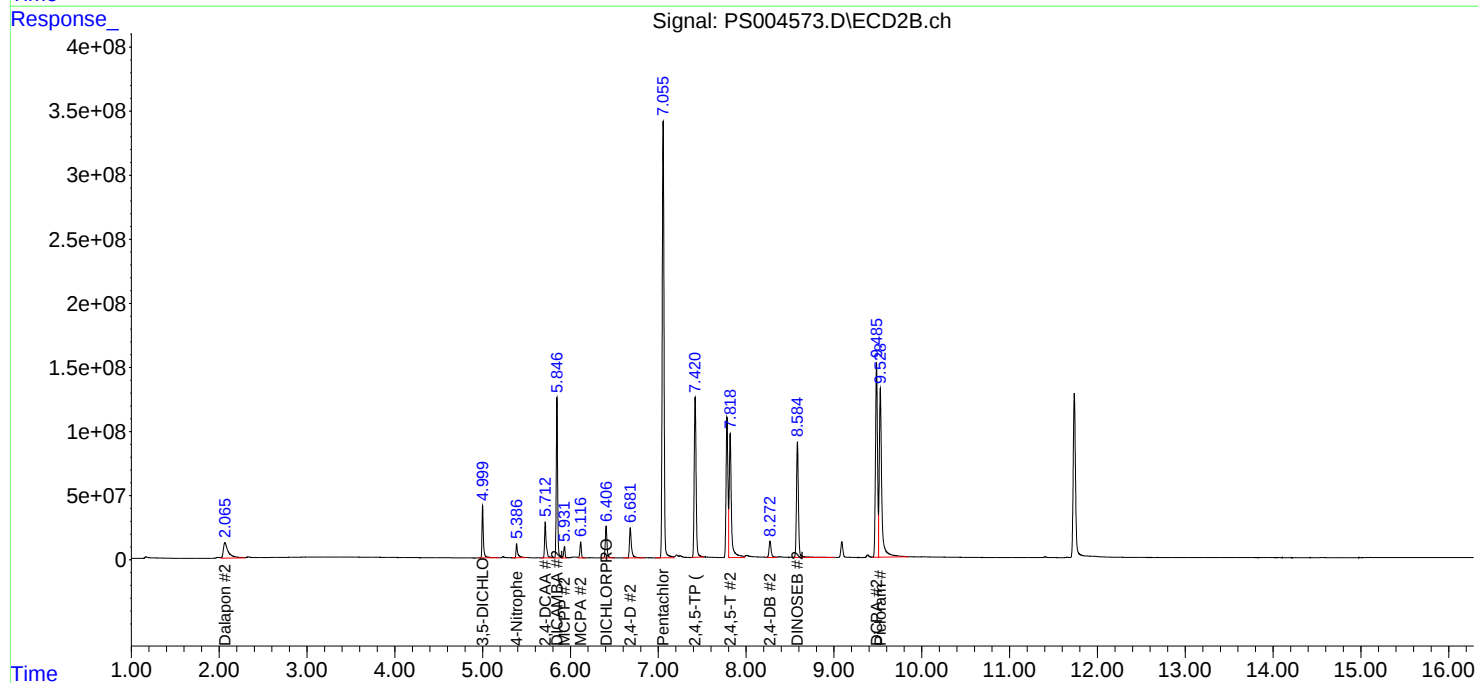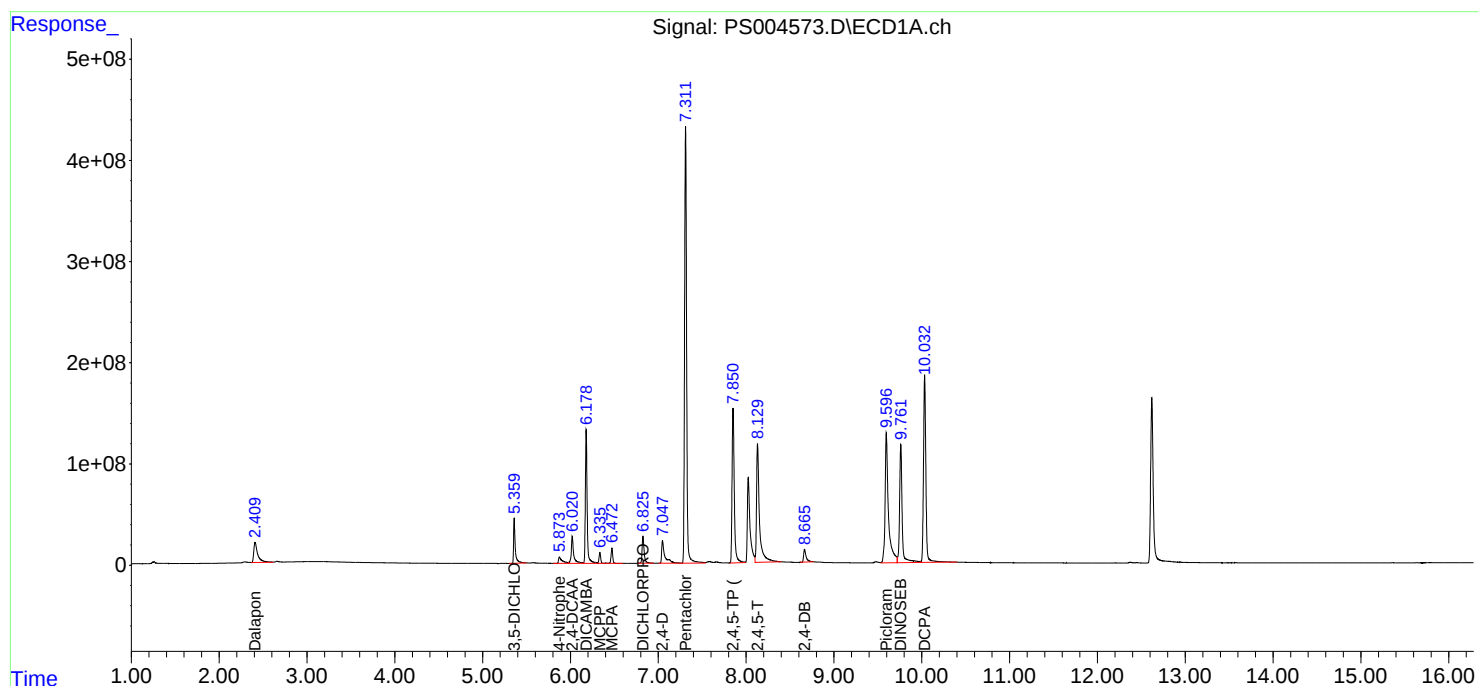


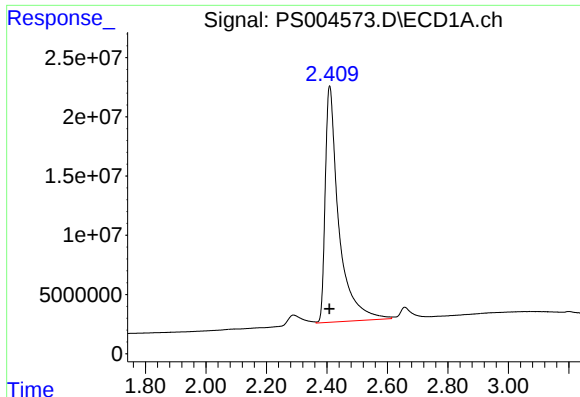

#1 Dalapon


R.T.: 2.409 min
Delta R.T.: 0.000 min
Response: 622293628
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

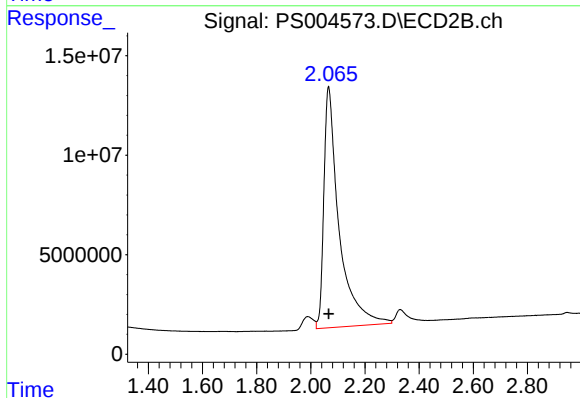


#1 Dalapon

R.T.: 2.066 min
Delta R.T.: 0.000 min
Response: 472590306
Conc: 682.50 ng/ml

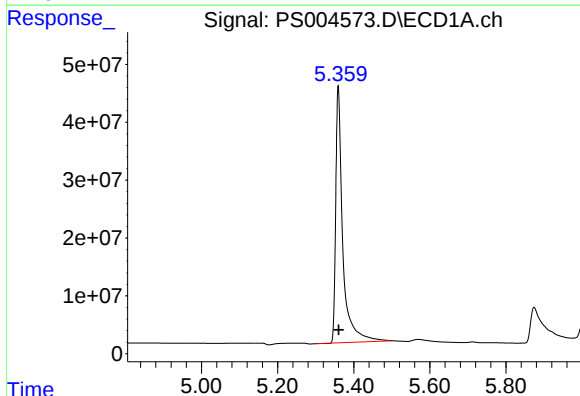


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.361 min
Delta R.T.: 0.000 min
Response: 577714960
Conc: 697.50 ng/ml

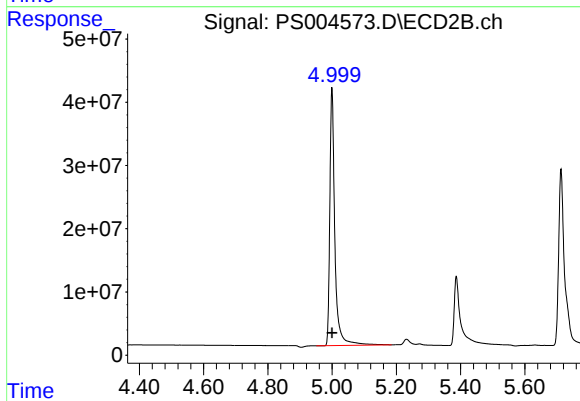

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.000 min
Delta R.T.: 0.000 min
Response: 443315077
Conc: 697.50 ng/ml

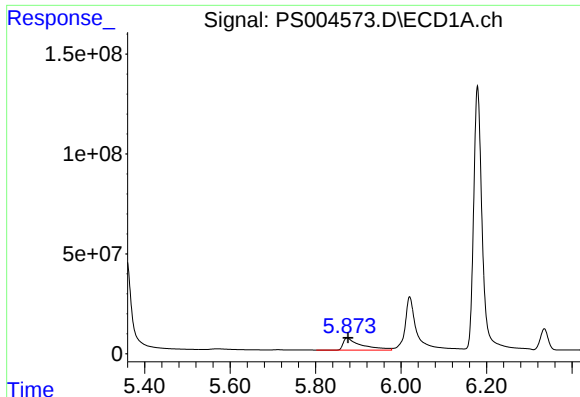

#3 4-Nitrophenol


R.T.: 5.876 min
Delta R.T.: 0.000 min
Response: 176587048
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

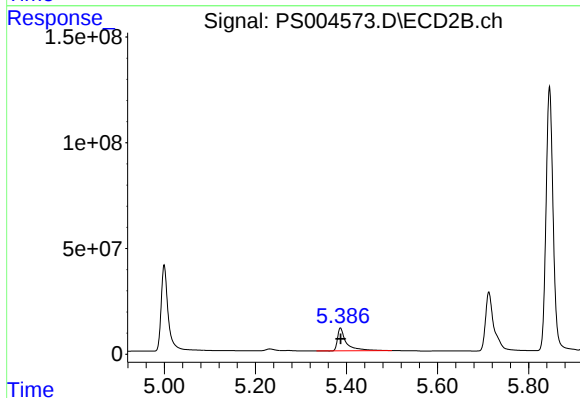


#3 4-Nitrophenol

R.T.: 5.387 min
Delta R.T.: 0.000 min
Response: 146137167
Conc: 682.50 ng/ml

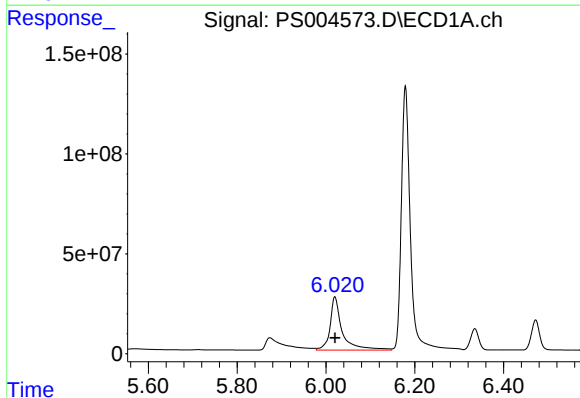


#4 2,4-DCAA

R.T.: 6.021 min
Delta R.T.: 0.000 min
Response: 509142485
Conc: 750.00 ng/ml

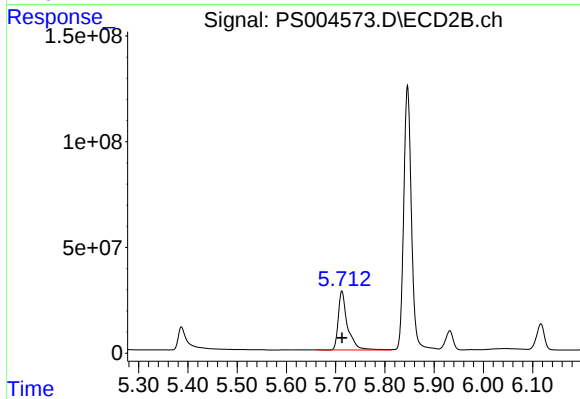

#4 2,4-DCAA


R.T.: 5.713 min
Delta R.T.: 0.000 min
Response: 362955111
Conc: 750.00 ng/ml

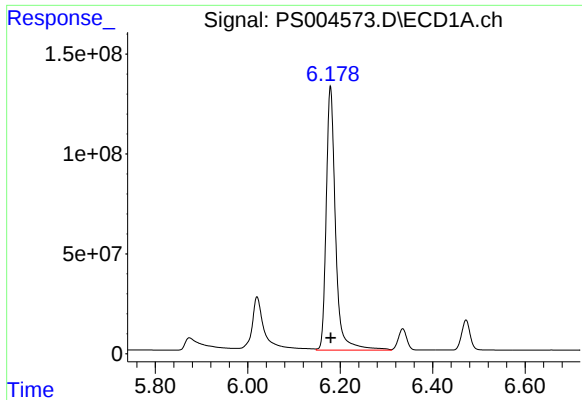

#5 DICAMBA


R.T.: 6.179 min
Delta R.T.: 0.000 min
Response: 1849564221
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

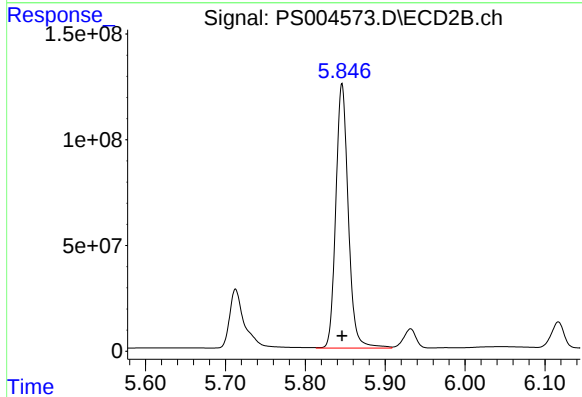


#5 DICAMBA

R.T.: 5.846 min
Delta R.T.: 0.000 min
Response: 1355971851
Conc: 705.00 ng/ml

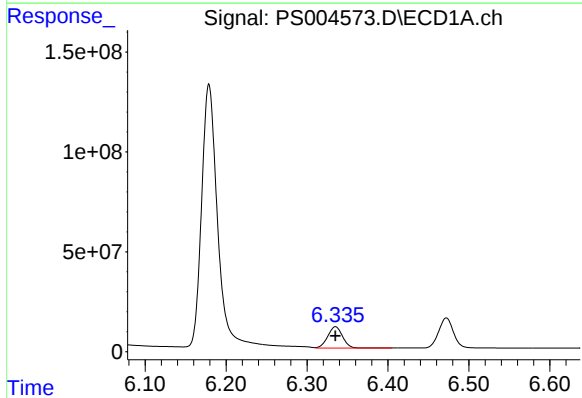


#6 MCP

R.T.: 6.335 min
Delta R.T.: 0.000 min
Response: 137345080
Conc: 70.50 ug/ml

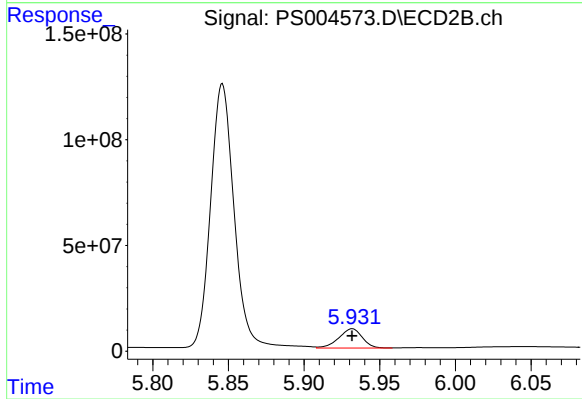

#6 MCP


R.T.: 5.932 min
Delta R.T.: 0.000 min
Response: 98069776
Conc: 70.50 ug/ml

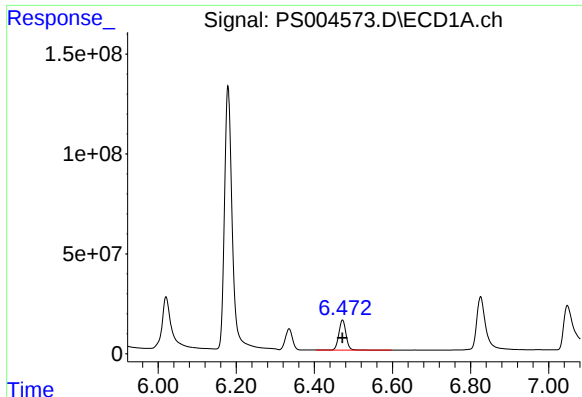

#7 MCPA


R.T.: 6.472 min
Delta R.T.: 0.000 min
Response: 194138631
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

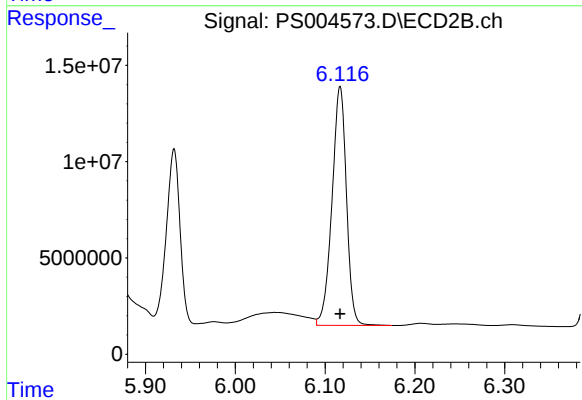


#7 MCPA

R.T.: 6.117 min
Delta R.T.: 0.000 min
Response: 138823452
Conc: 69.75 ug/ml

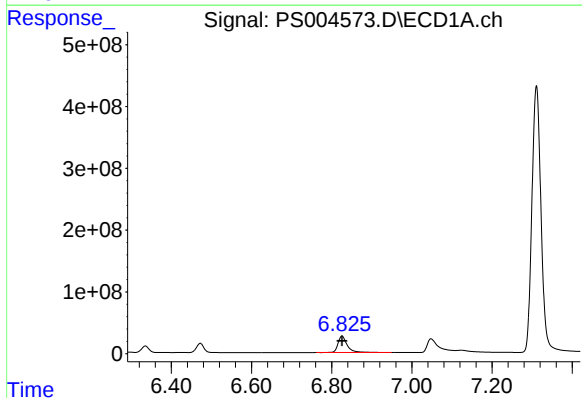


#8 DICHLORPROP

R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 426958288
Conc: 705.00 ng/ml

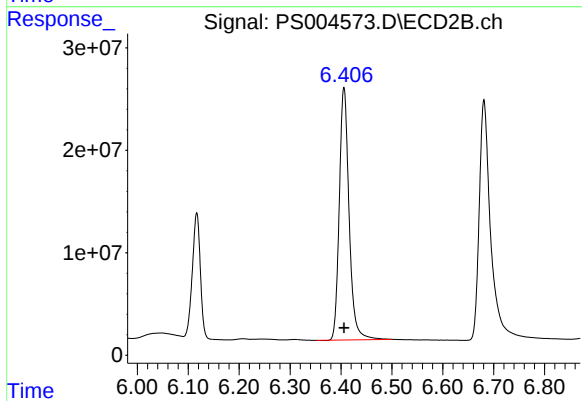

#8 DICHLORPROP


R.T.: 6.406 min
Delta R.T.: 0.000 min
Response: 329781530
Conc: 705.00 ng/ml

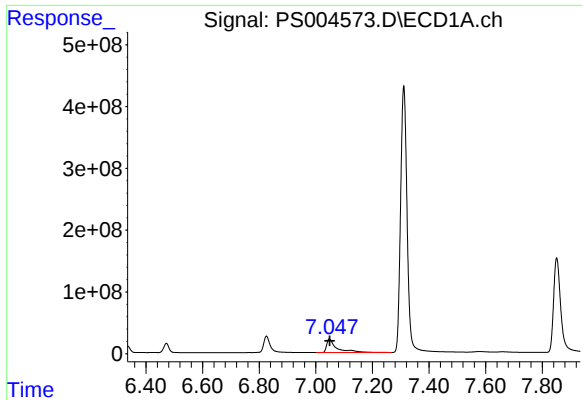

#9 2,4-D


R.T.: 7.049 min
Delta R.T.: 0.000 min
Response: 554163787
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

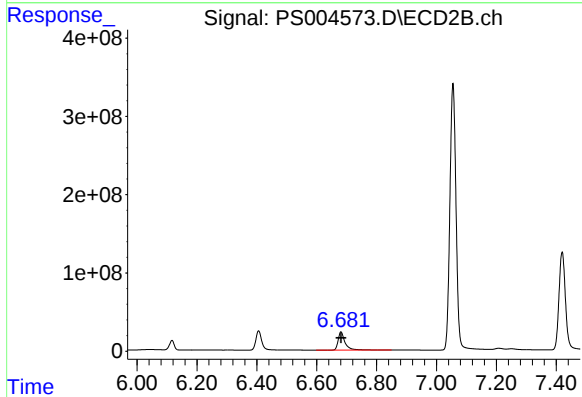


#9 2,4-D

R.T.: 6.681 min
Delta R.T.: 0.000 min
Response: 368596107
Conc: 705.00 ng/ml

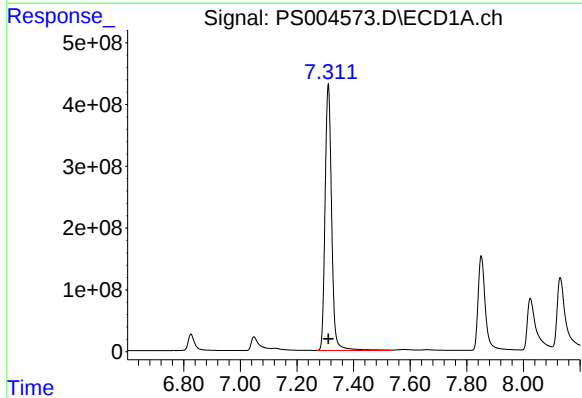


#10 Pentachlorophenol

R.T.: 7.311 min
Delta R.T.: 0.000 min
Response: 6940418833
Conc: 712.50 ng/ml

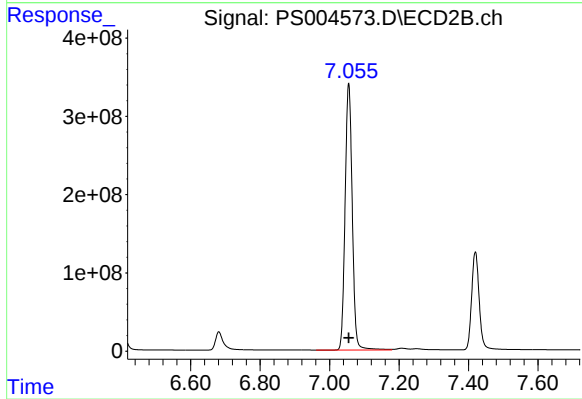

#10 Pentachlorophenol


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 4864129356
Conc: 712.50 ng/ml

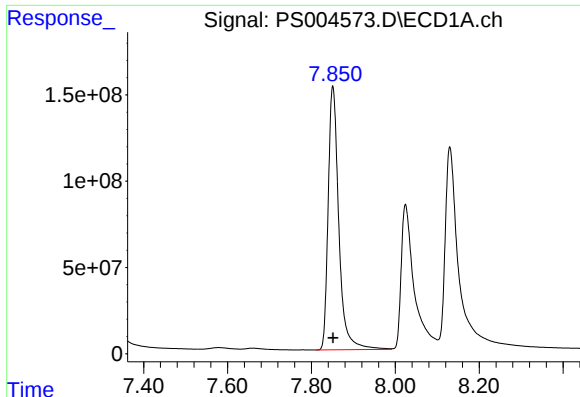

#11 2,4,5-TP (SILVEX)


R.T.: 7.852 min
Delta R.T.: 0.000 min
Response: 2697207292
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

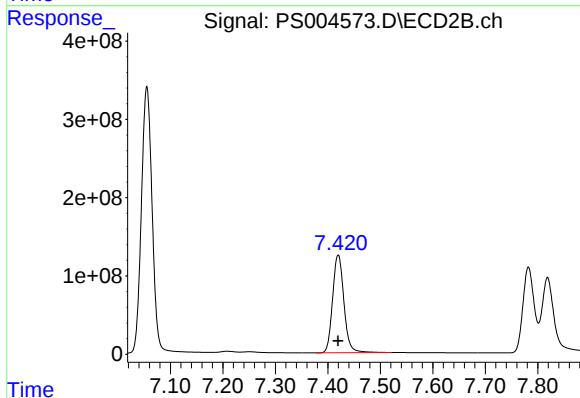


#11 2,4,5-TP (SILVEX)

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 1873420915
Conc: 712.50 ng/ml

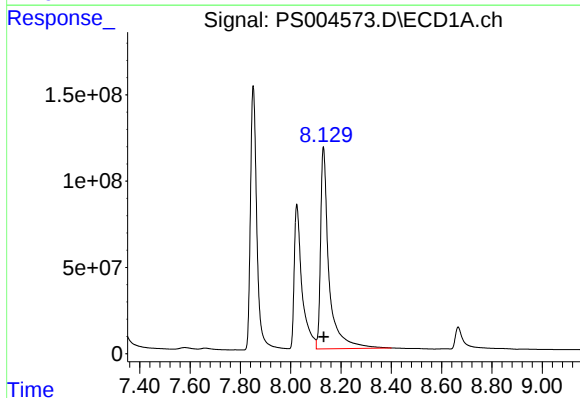


#12 2,4,5-T

R.T.: 8.131 min
Delta R.T.: 0.000 min
Response: 2721763652
Conc: 712.50 ng/ml

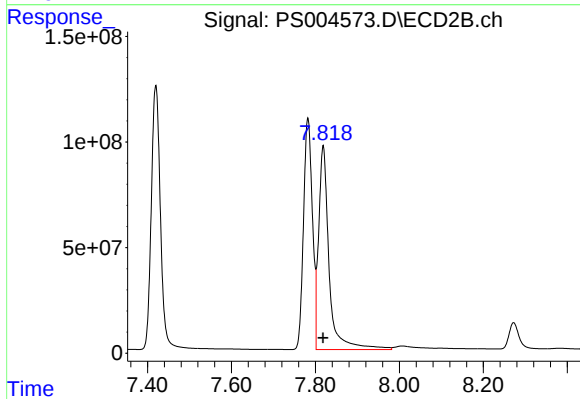

#12 2,4,5-T


R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 1674186277
Conc: 712.50 ng/ml

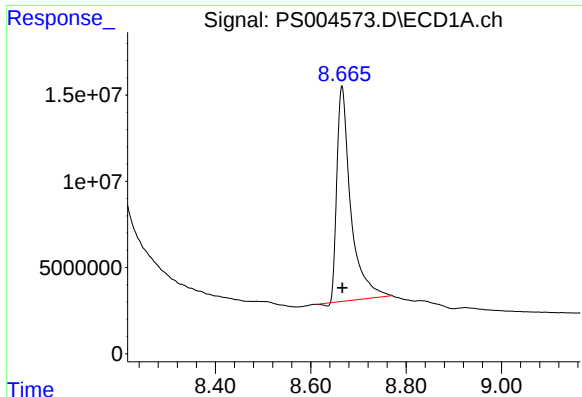

#13 2,4-DB


R.T.: 8.666 min
Delta R.T.: 0.000 min
Response: 252559918
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

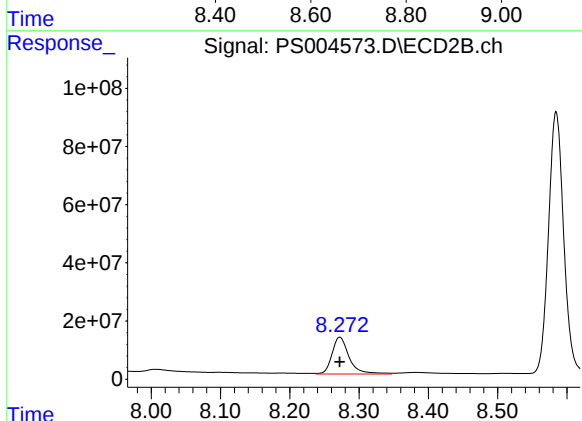


#13 2,4-DB

R.T.: 8.272 min
Delta R.T.: 0.000 min
Response: 218099727
Conc: 712.50 ng/ml

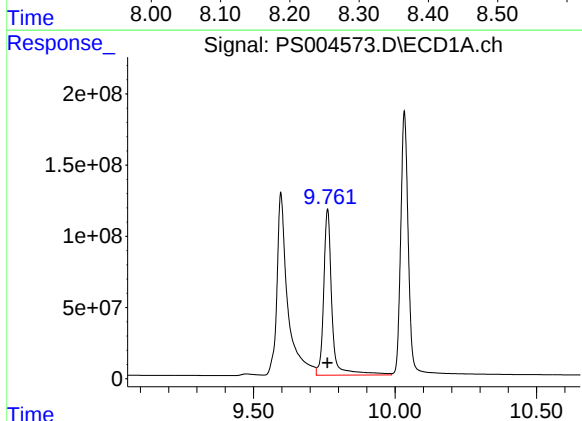


#14 DINOSEB

R.T.: 9.761 min
Delta R.T.: 0.000 min
Response: 2370534177
Conc: 705.00 ng/ml

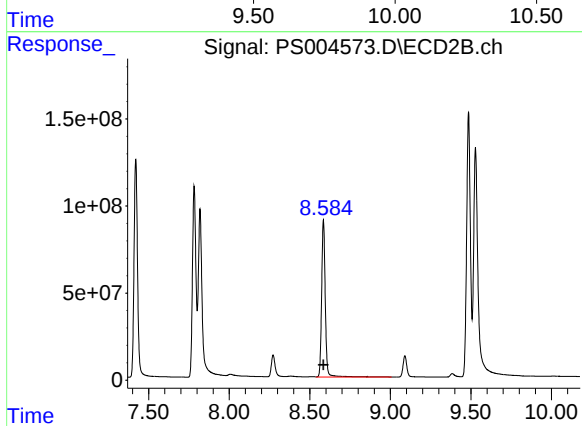

#14 DINOSEB


R.T.: 8.584 min
Delta R.T.: 0.000 min
Response: 1424470273
Conc: 705.00 ng/ml

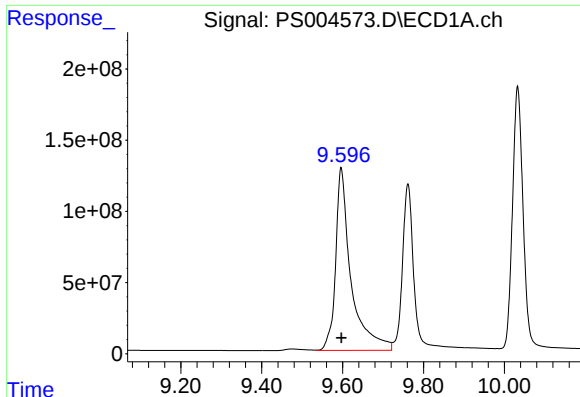

#15 Picloram


R.T.: 9.597 min
Delta R.T.: 0.000 min
Response: 3397148276
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

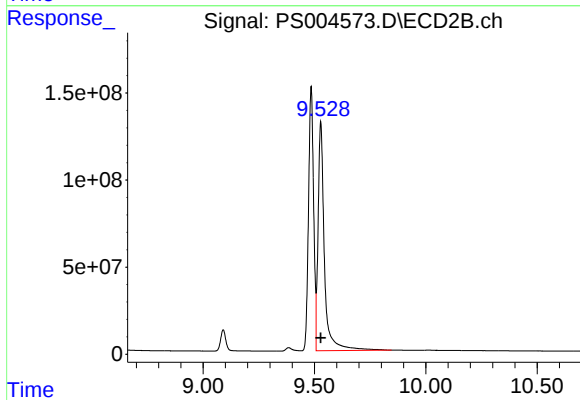


#15 Picloram

R.T.: 9.528 min
Delta R.T.: 0.000 min
Response: 2599033781
Conc: 712.50 ng/ml

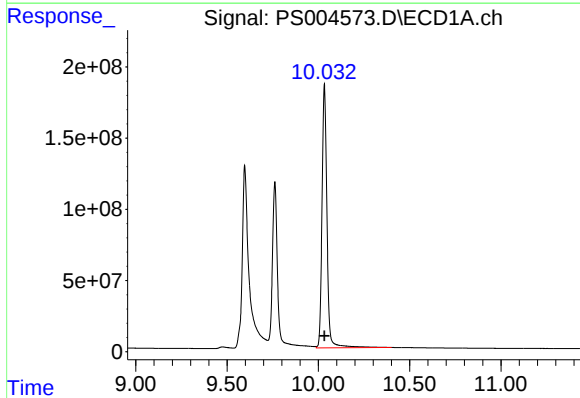

#16 DCPA

R.T.: 10.033 min
Delta R.T.: 0.000 min
Response: 3497159823
Conc: 720.00 ng/ml

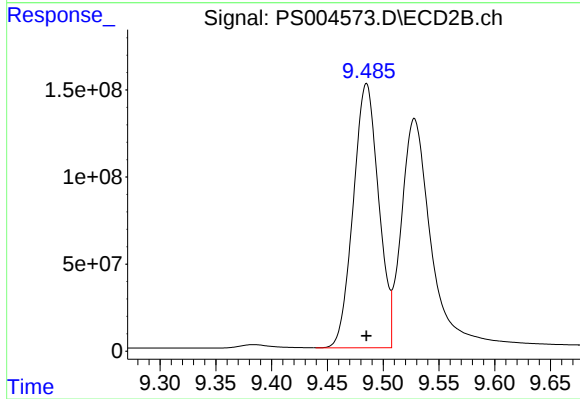

#16 DCPA

R.T.: 9.485 min
Delta R.T.: 0.000 min
Response: 2403403450
Conc: 720.00 ng/ml