

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051320\
 Data File : PS010260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 15:59
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 17:28:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.921	326.2E6	281.8E6	464.013	525.554
Target Compounds							
2) T	3,5-DICHL...	6.486	6.099	40071177	1730278	41.536	2.125 #
5) T	DICAMBA	0.000	7.089	0	1097787	N.D.	<MDL
6) T	MCP	0.000	7.155	0	27523396	N.D.	14.994
8) T	DICHLORPROP	0.000	7.742	0	3686775	N.D.	6.530
9) T	2,4-D	8.417	8.055	58455493	133103	82.745	<MDL #
10) T	Pentachlo...	0.000	8.445	0	196321	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.800	0	1338012	N.D.	<MDL
12) T	2,4,5-T	0.000	9.183	0	687142	N.D.	<MDL
13) T	2,4-DB	0.000	9.712	0	282218	N.D.	<MDL
14) T	DINOSEB	0.000	10.069	0	1680861	N.D.	<MDL
15) T	Picloram	10.993	11.004	23523394	1941299	5.131	<MDL #
16) T	DCPA	0.000	10.952	0	1117974	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051320\
Data File : PS010260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 15:59
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 17:28:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

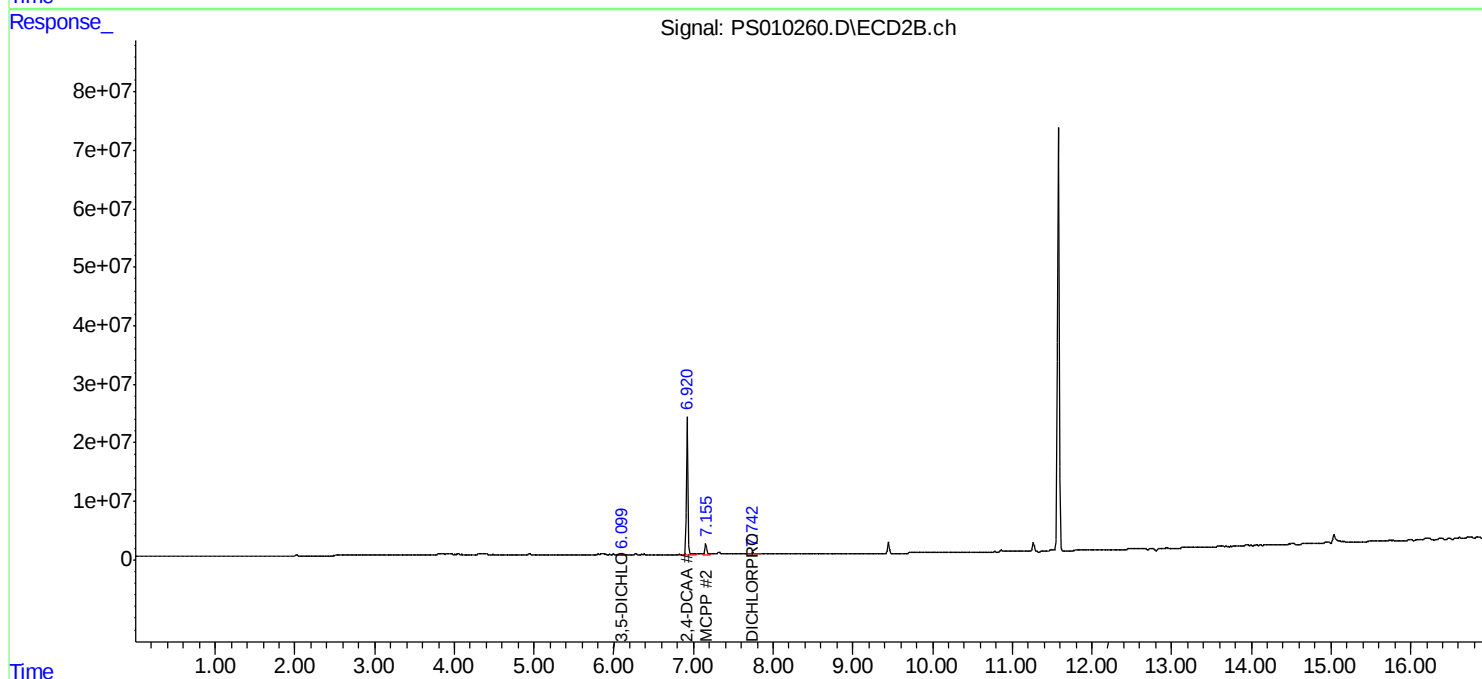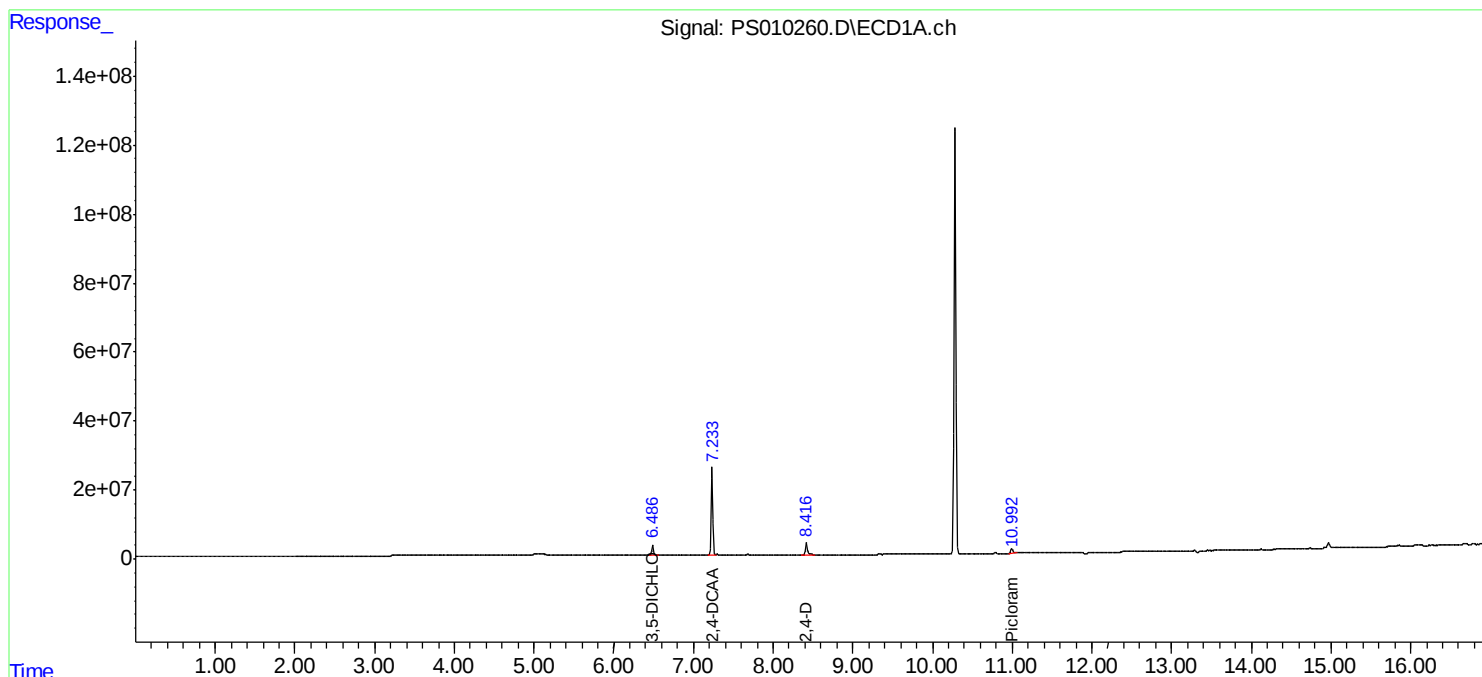


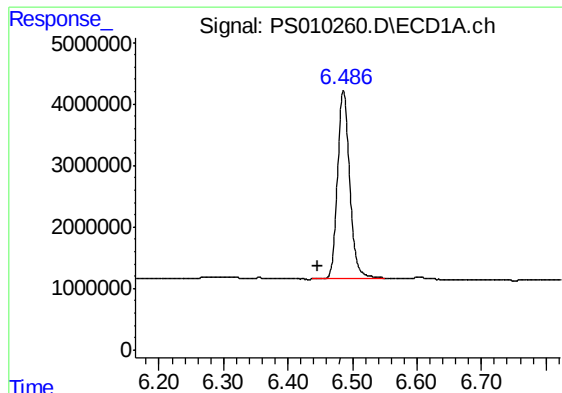

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.486 min
Delta R.T.: 0.040 min
Response: 40071177
Conc: 41.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

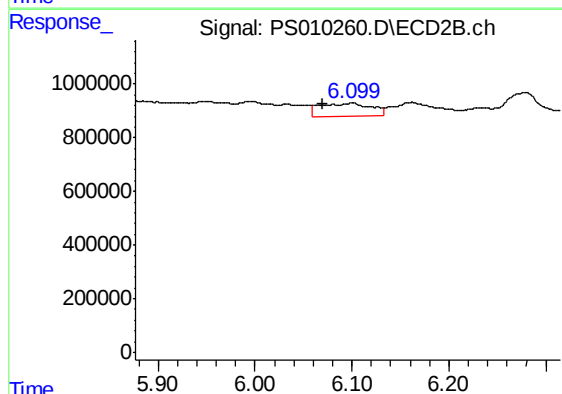


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.099 min
Delta R.T.: 0.029 min
Response: 1730278
Conc: 2.12 ng/ml

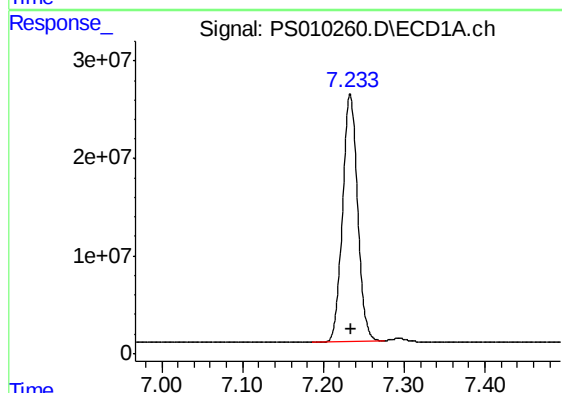


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.001 min
Response: 326244750
Conc: 464.01 ng/ml

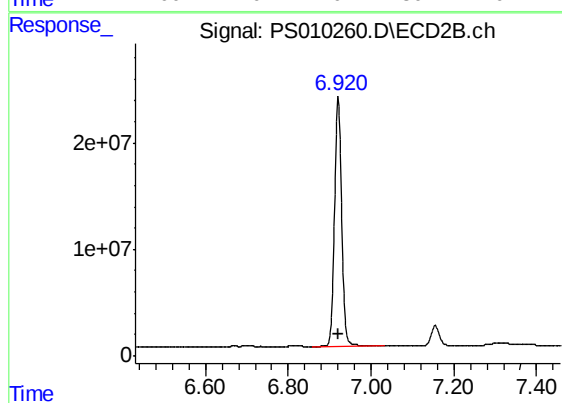

#4 2,4-DCAA


R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 281849912
Conc: 525.55 ng/ml

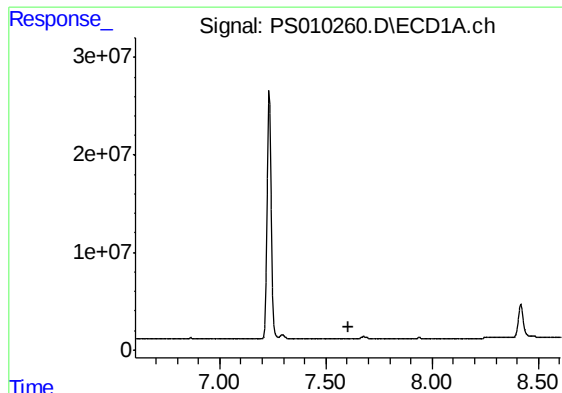

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

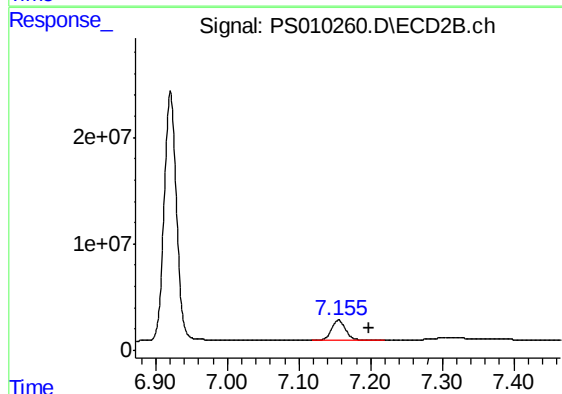


#6 MCP

R.T.: 7.155 min
Delta R.T.: -0.042 min
Response: 27523396
Conc: 14.99 ug/ml

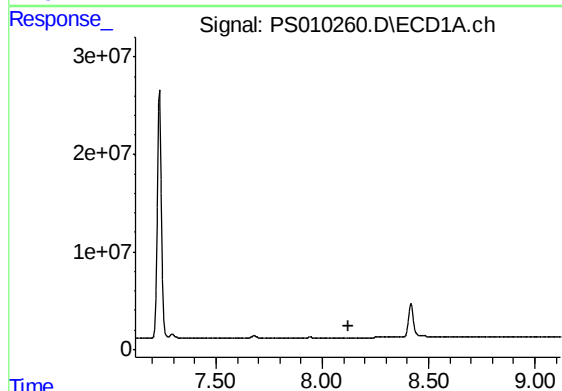


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

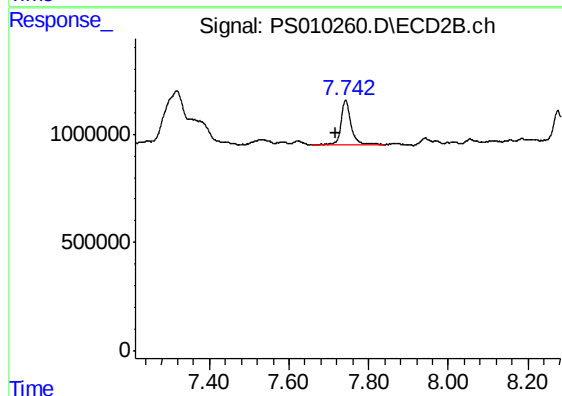

#8 DICHLORPROP


R.T.: 7.742 min
Delta R.T.: 0.024 min
Response: 3686775
Conc: 6.53 ng/ml

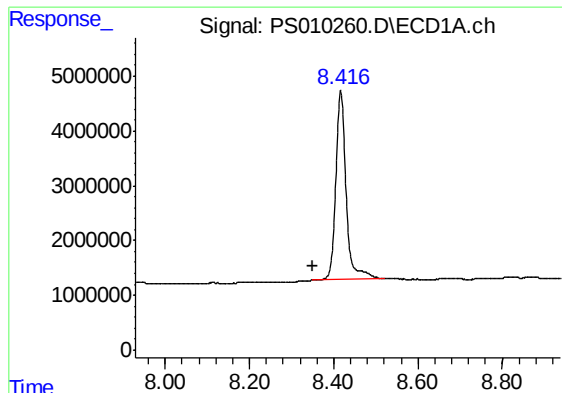

#9 2,4-D


R.T.: 8.417 min
Delta R.T.: 0.067 min
Response: 58455493
Conc: 82.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

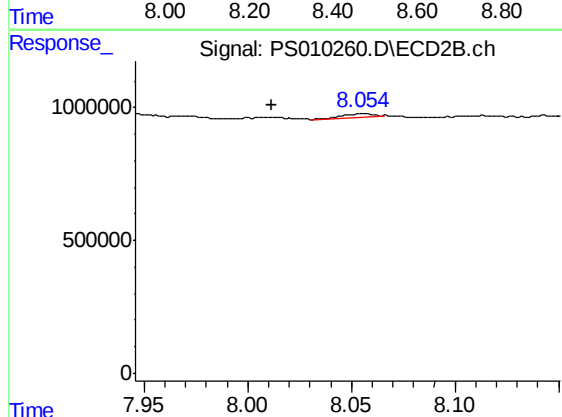


#9 2,4-D

R.T.: 8.055 min
Delta R.T.: 0.044 min
Response: 133103
Conc: N.D.

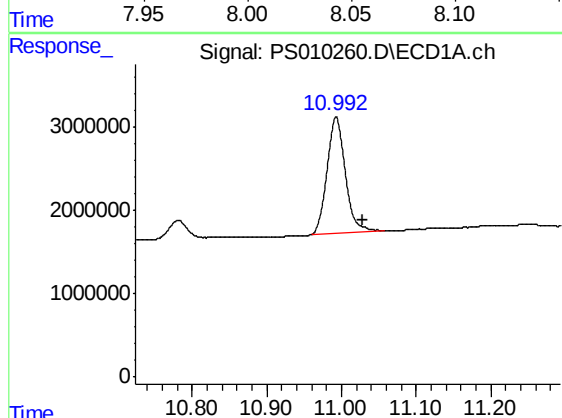

#15 Picloram

R.T.: 10.993 min
Delta R.T.: -0.036 min
Response: 23523394
Conc: 5.13 ng/ml

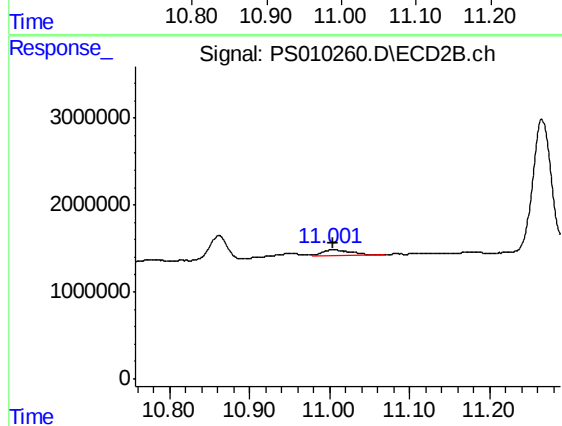

#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.000 min
Response: 1941299
Conc: N.D.