

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051320\
 Data File : PS010272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2020 20:34
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 23:13:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.920	327.3E6	284.7E6	465.558	530.819
Target Compounds							
2) T	3,5-DICHL...	6.485	6.100	32645259	419805	33.838	<MDL #
5) T	DICAMBA	0.000	7.089	0	1085286	N.D.	<MDL
6) T	MCP	0.000	7.155	0	30122878	N.D.	16.410
8) T	DICHLORPROP	0.000	7.743	0	3544689	N.D.	6.279
9) T	2,4-D	8.416	8.055	69087283	111497	97.795	<MDL #
10) T	Pentachlo...	0.000	8.442	0	361156	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.800	0	763456	N.D.	<MDL
12) T	2,4,5-T	0.000	9.183	0	456444	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	424750	N.D.	1.066
14) T	DINOSEB	0.000	10.021	0	201487	N.D.	<MDL
15) T	Picloram	10.992	11.008	26346387	1363877	5.746	<MDL #
16) T	DCPA	0.000	10.953	0	557702	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051320\
Data File : PS010272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2020 20:34
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 23:13:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

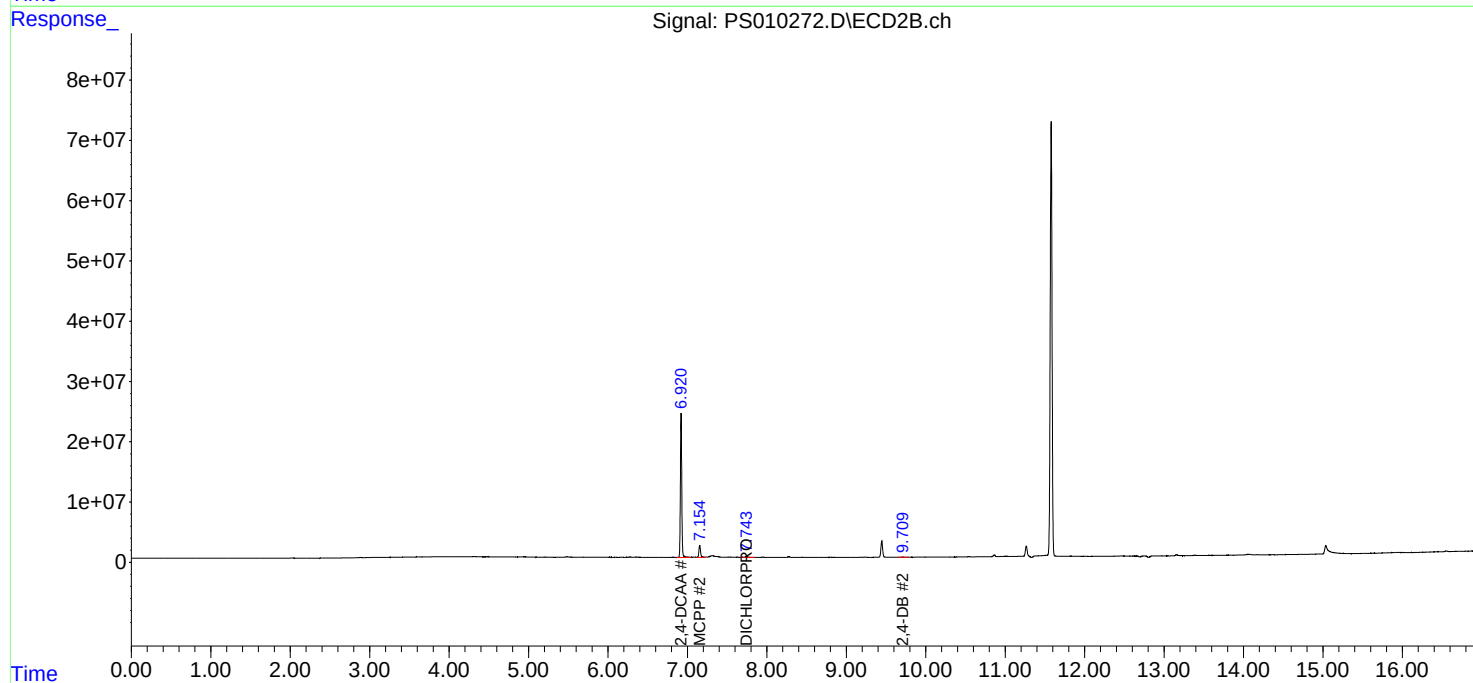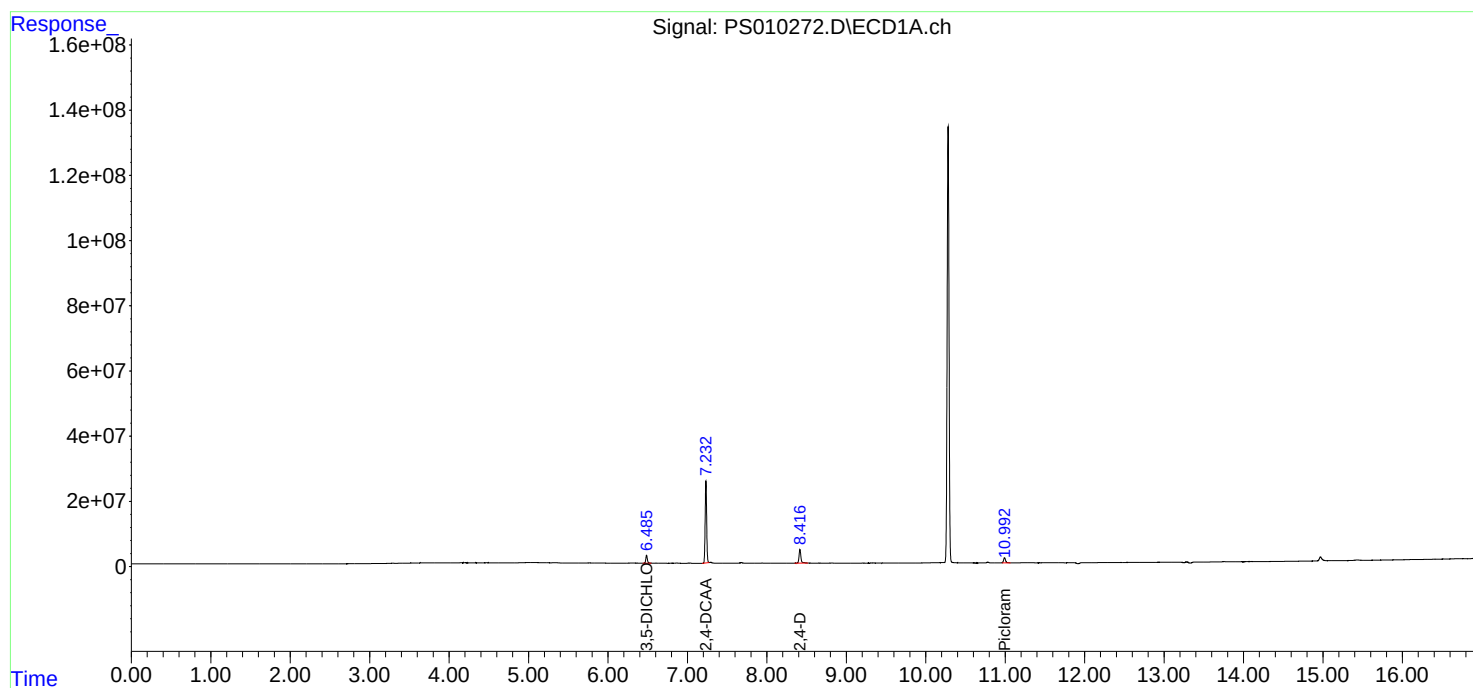


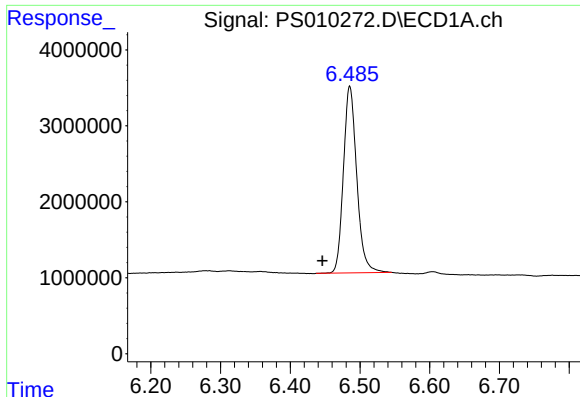

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.485 min
Delta R.T.: 0.039 min
Response: 32645259
Conc: 33.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

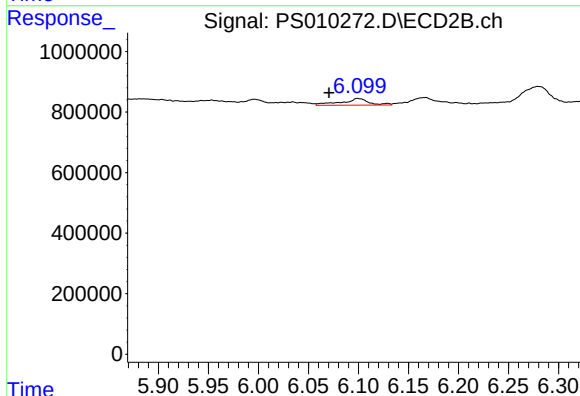


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.100 min
Delta R.T.: 0.030 min
Response: 419805
Conc: N.D.

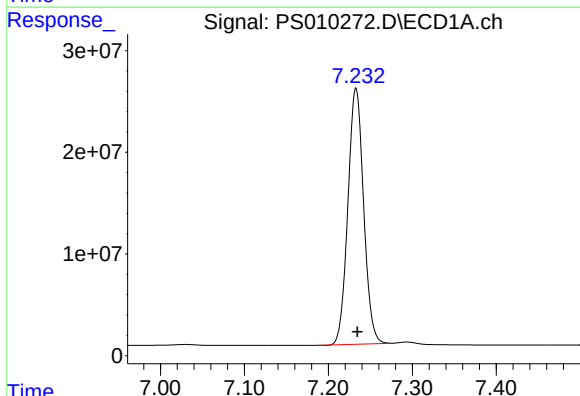


#4 2,4-DCAA

R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 327331544
Conc: 465.56 ng/ml

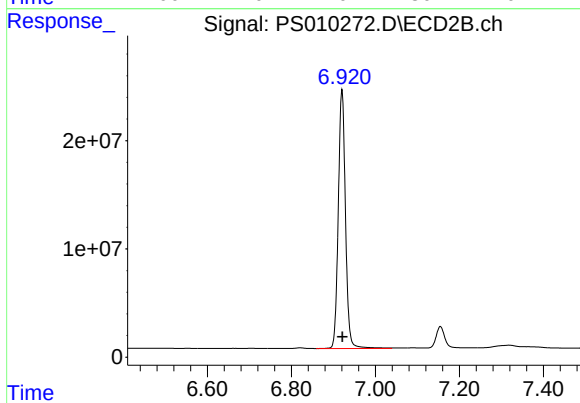

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 284673705
Conc: 530.82 ng/ml

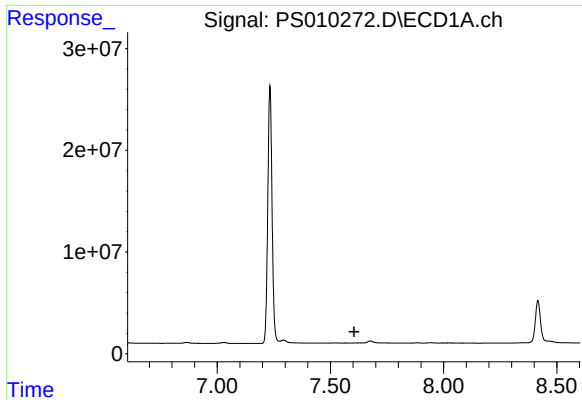

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

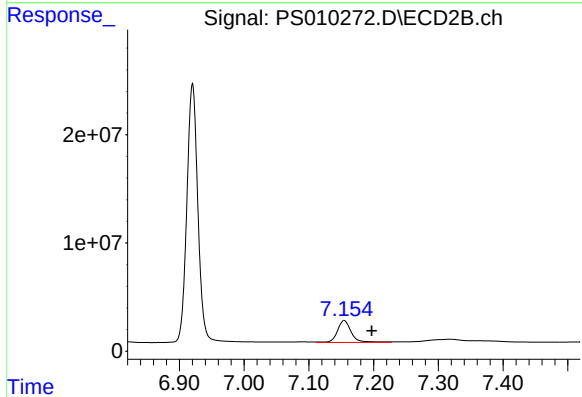


#6 MCP

R.T.: 7.155 min
Delta R.T.: -0.043 min
Response: 30122878
Conc: 16.41 ug/ml

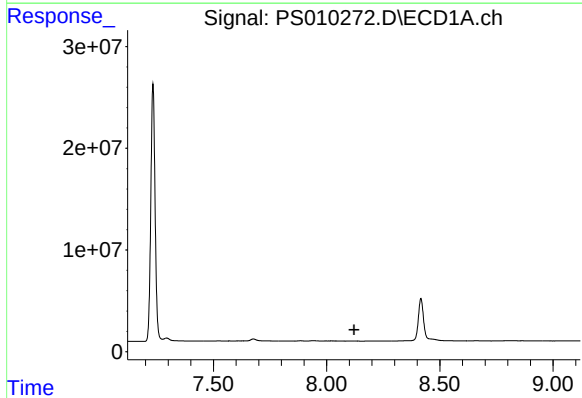


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

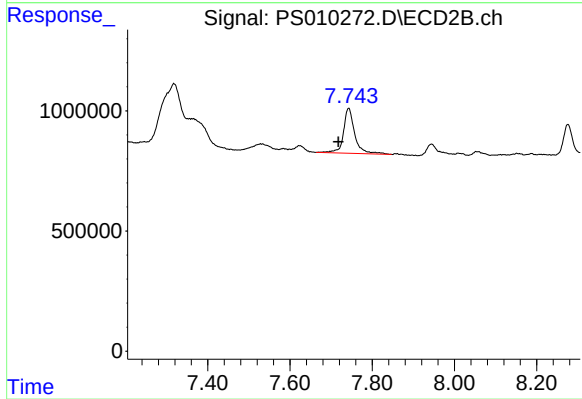

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.024 min
Response: 3544689
Conc: 6.28 ng/ml

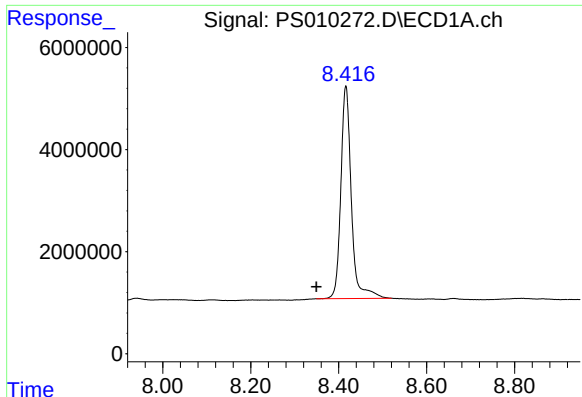

#9 2,4-D


R.T.: 8.416 min
Delta R.T.: 0.067 min
Response: 69087283
Conc: 97.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

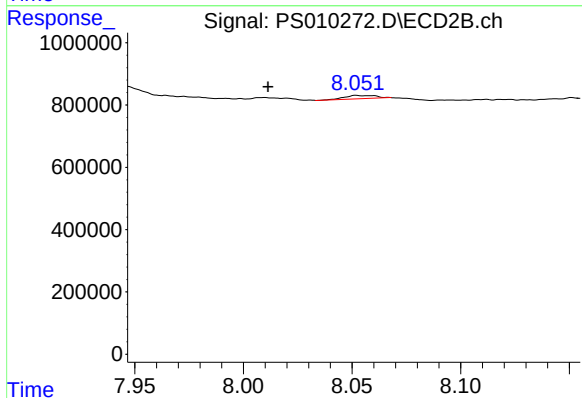


#9 2,4-D

R.T.: 8.055 min
Delta R.T.: 0.044 min
Response: 111497
Conc: N.D.

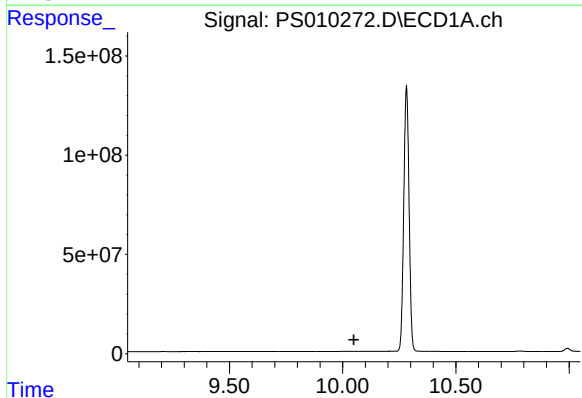


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.050 min
Response: 0
Conc: N.D.

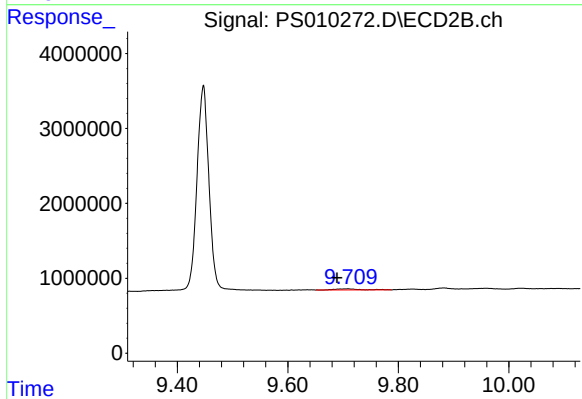

#13 2,4-DB


R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 424750
Conc: 1.07 ng/ml

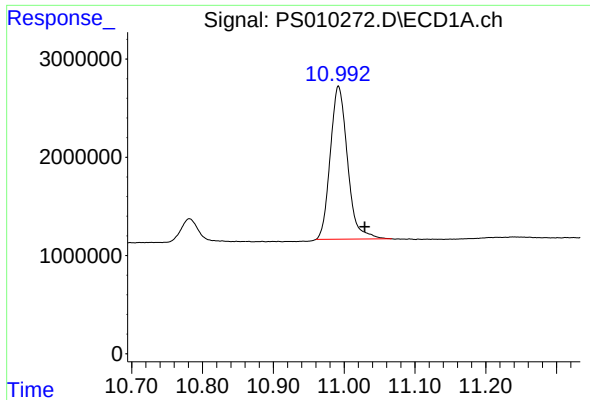

#15 Picloram

R.T.: 10.992 min
Delta R.T.: -0.037 min
Response: 26346387
Conc: 5.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

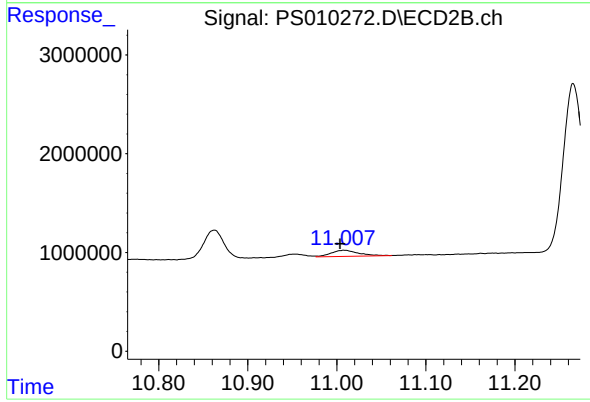

#15 Picloram

R.T.: 11.008 min
Delta R.T.: 0.005 min
Response: 1363877
Conc: N.D.