

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051322\
 Data File : PS019402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 09:05
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 15:40:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	0.000	917412	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.488f	5.969	7374168	314825	2.086	<MDL #
3) T	4-Nitroph...	0.000	6.402	0	343941	N.D.	<MDL
5) T	DICAMBA	7.419	6.973	764682	68971	<MDL	<MDL #
6) T	MCP	0.000	7.030f	0	4695616	N.D.	1.766
9) T	2,4-D	0.000	7.942f	0	417680	N.D.	<MDL
10) T	Pentachlo...	8.674	8.307	5620035	288520	<MDL	<MDL #
11) T	2,4,5-TP ...	9.210	8.649	69056	300063	<MDL	<MDL #
12) T	2,4,5-T	9.527f	9.077	3073424	352261	<MDL	<MDL #
13) T	2,4-DB	10.023	9.585	797378	406769	<MDL	<MDL #
14) T	DINOSEB	0.000	9.885	0	359979	N.D.	<MDL
15) T	Picloram	10.991	10.824	592.4E6	5642512	20.267	<MDL #
16) T	DCPA	11.466	10.824	873979	5642512	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051322\
Data File : PS019402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 09:05
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 15:40:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

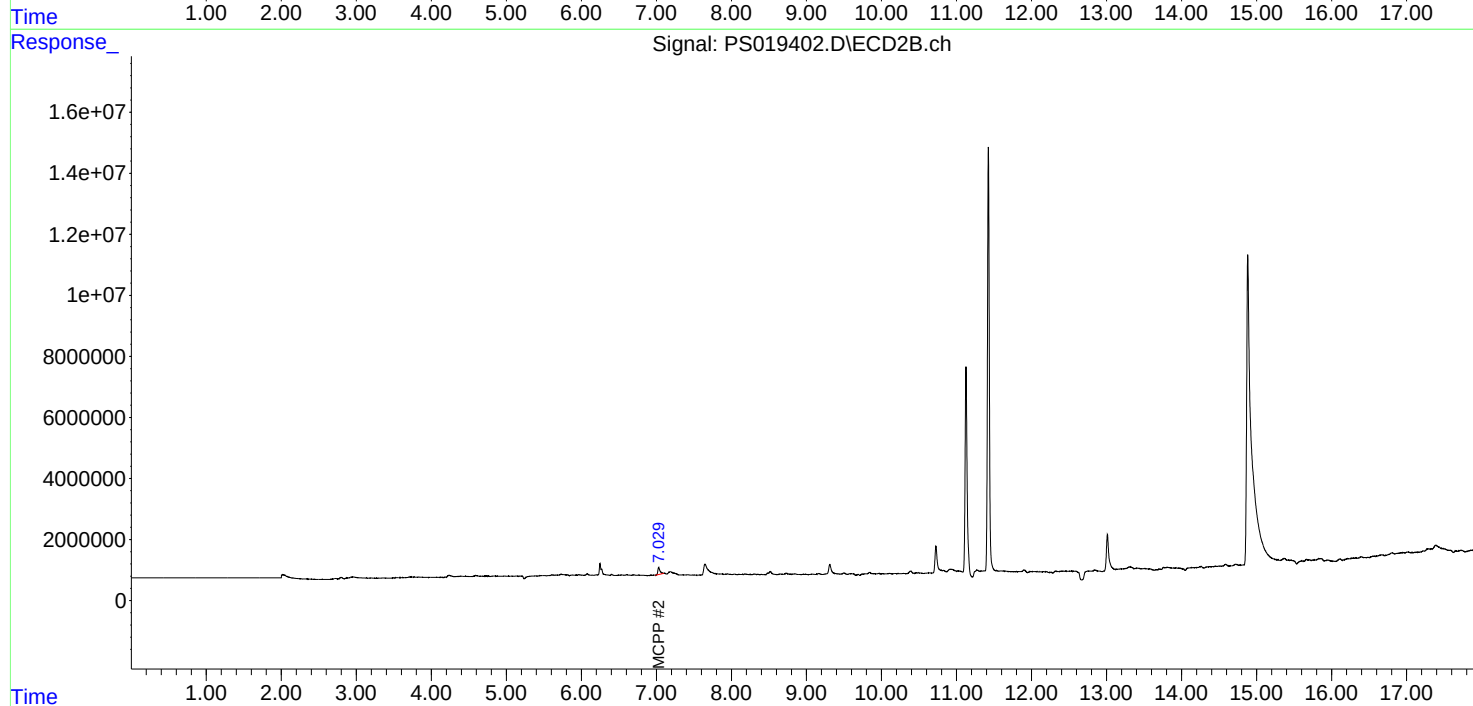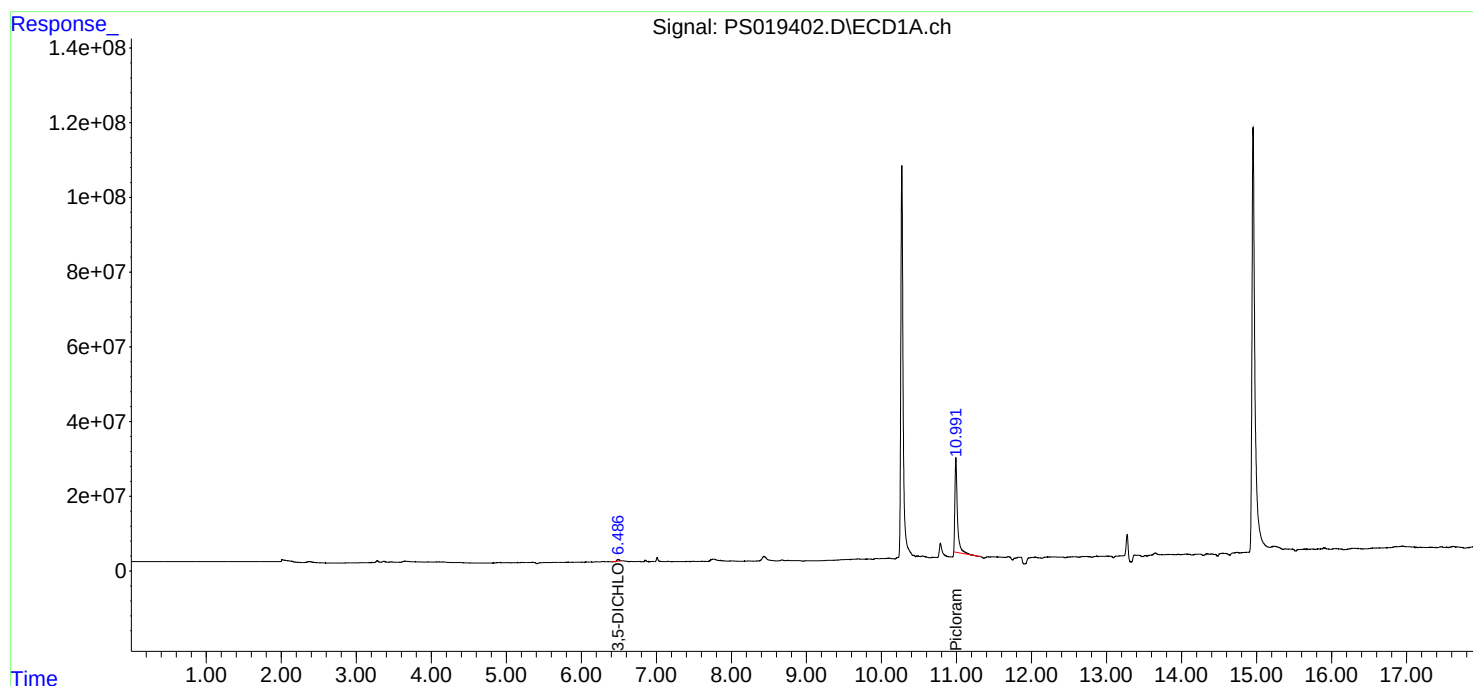


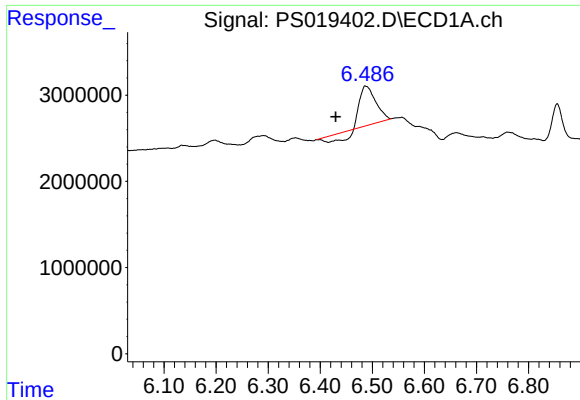

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.488 min
Delta R.T.: 0.058 min
Response: 7374168
Conc: 2.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

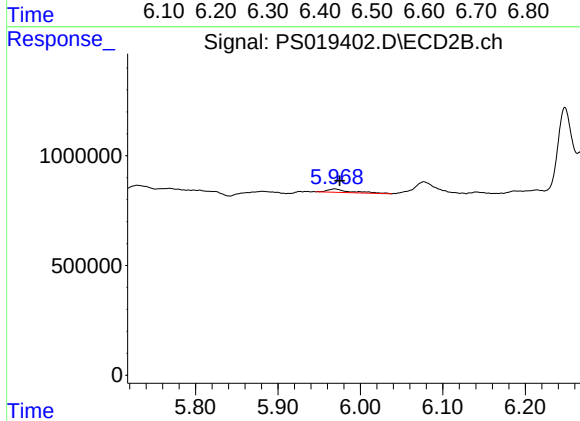


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.969 min
Delta R.T.: -0.006 min
Response: 314825
Conc: N.D.

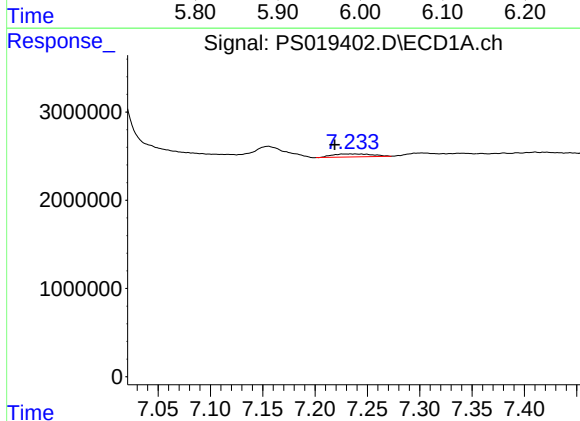


#4 2,4-DCAA

R.T.: 7.236 min
Delta R.T.: 0.017 min
Response: 917412
Conc: N.D.

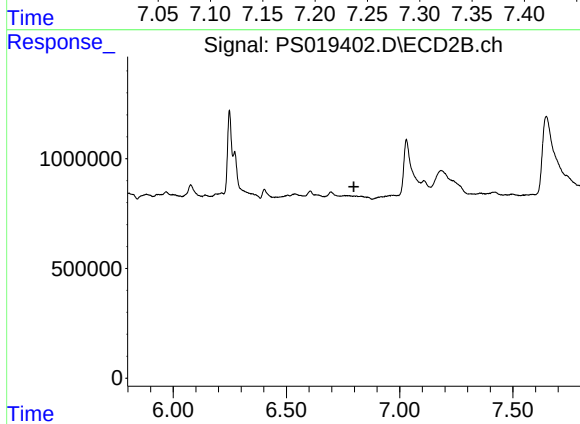

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.798 min
Response: 0
Conc: N.D.

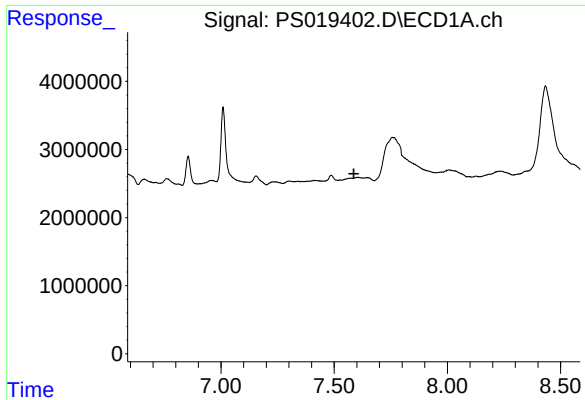

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.587 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

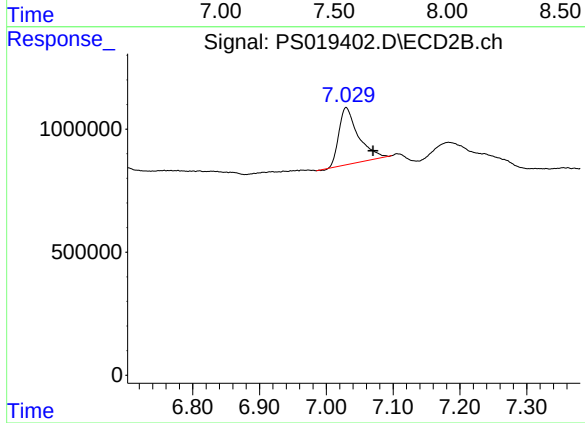


#6 MCP

R.T.: 7.030 min
Delta R.T.: -0.040 min
Response: 4695616
Conc: 1.77 ug/ml

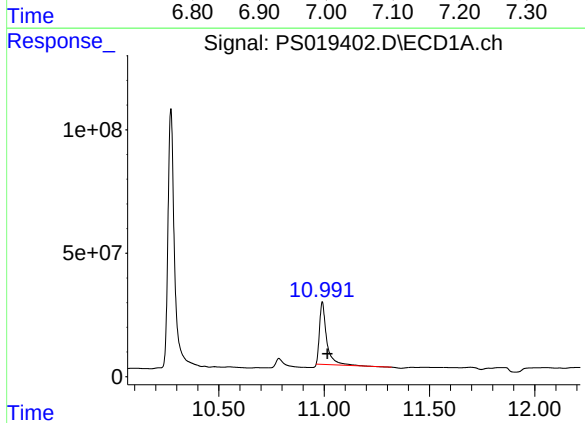

#15 Picloram

R.T.: 10.991 min
Delta R.T.: -0.024 min
Response: 592393803
Conc: 20.27 ng/ml

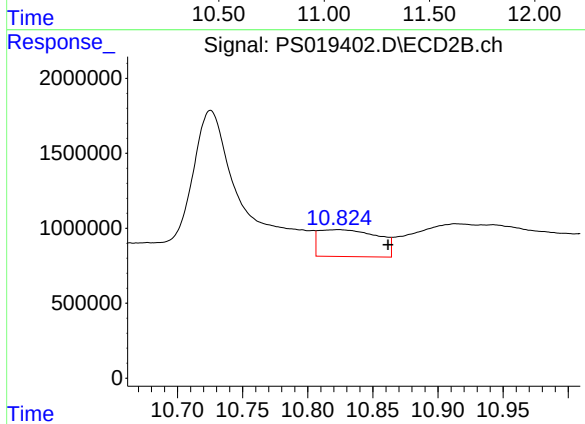

#15 Picloram

R.T.: 10.824 min
Delta R.T.: -0.038 min
Response: 5642512
Conc: N.D.