

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051322\
 Data File : PS019411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2022 16:01
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 17:11:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.224	6.797	1325.6E6	428.9E6	485.401	553.689
Target Compounds							
3) T	4-Nitroph...	7.024	0.000	3133713	0	3.234	N.D. #
8) T	DICHLORPROP	8.086	7.626	4525754	1116885	1.618	1.303
11) T	2,4,5-TP ...	0.000	8.631	0	3279276	N.D.	<MDL
12) T	2,4,5-T	9.411f	0.000	3004912	0	<MDL	N.D. #
13) T	2,4-DB	10.013	9.565	1853551	730558	<MDL	1.285 #
14) T	DINOSEB	11.156	9.886	94426167	2049194	5.719	<MDL #
15) T	Picloram	11.002	10.813f	12071309	7593918	<MDL	1.270 #
16) T	DCPA	11.471	10.813	114060	7593918	<MDL	1.294 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051322\
Data File : PS019411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2022 16:01
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 17:11:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

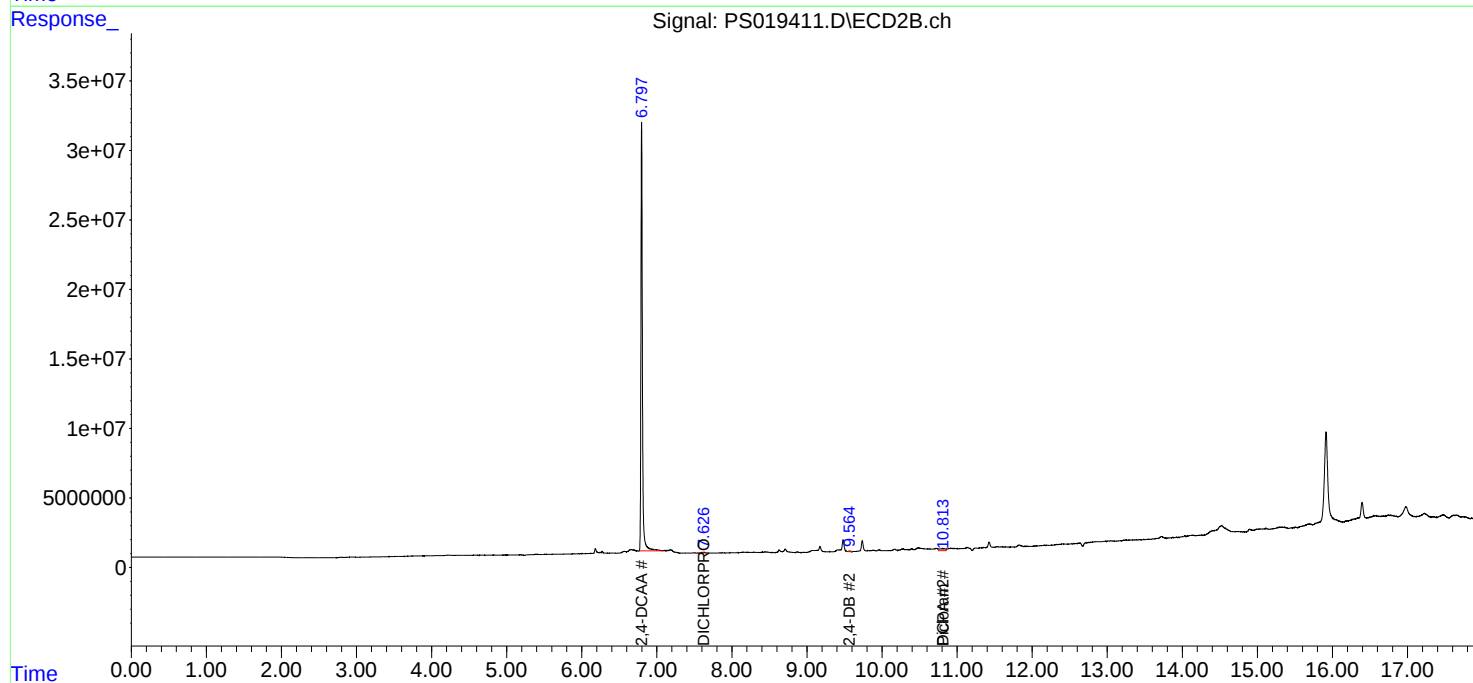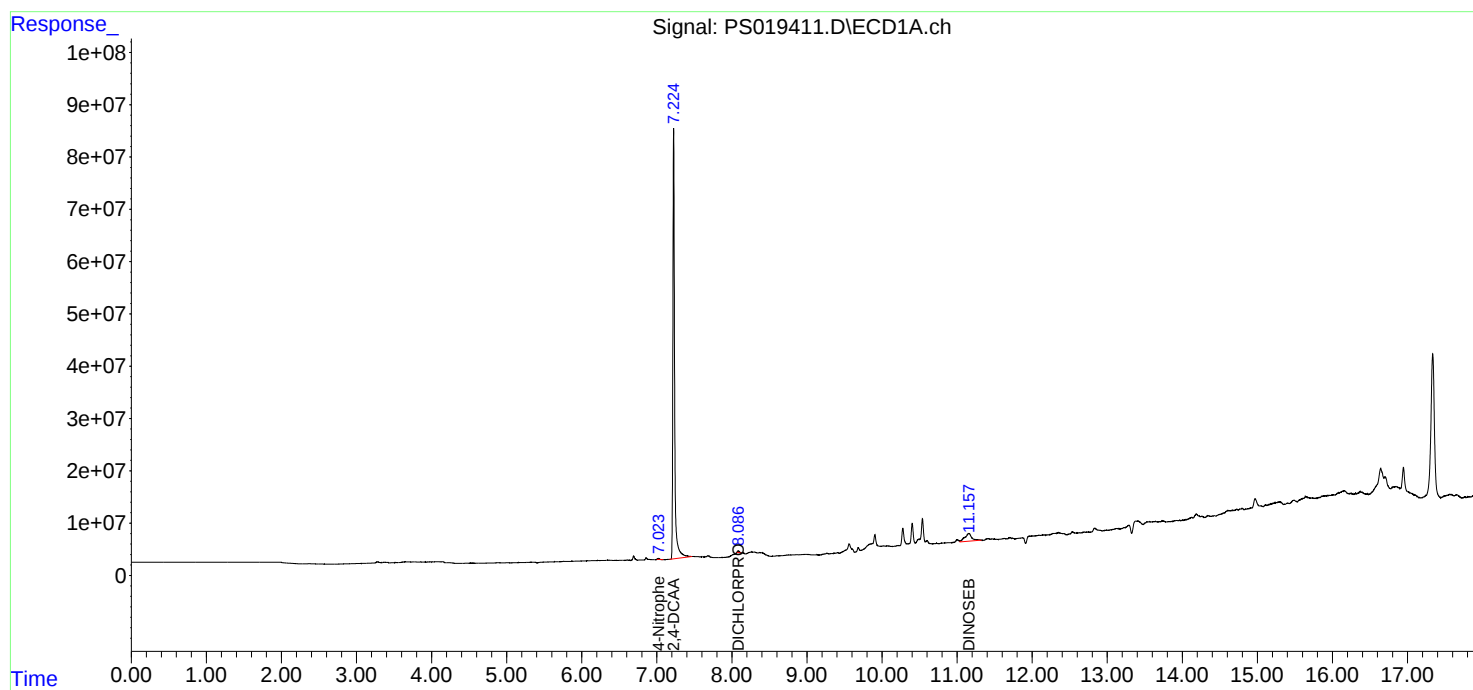


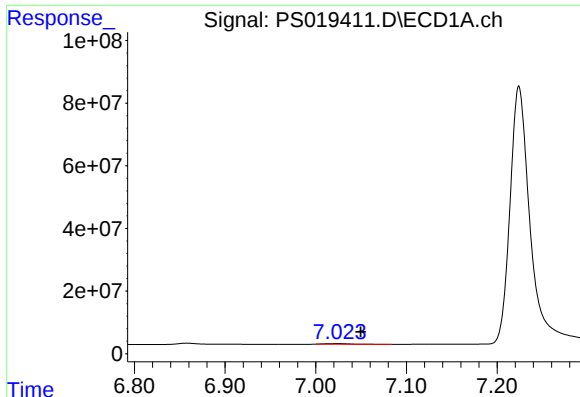

#3 4-Nitrophenol


R.T.: 7.024 min
Delta R.T.: -0.025 min
Response: 3133713
Conc: 3.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

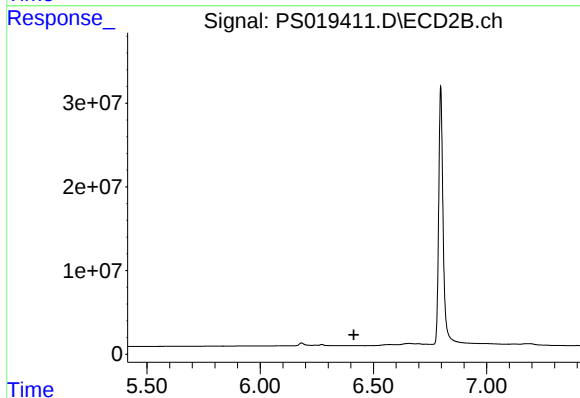


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

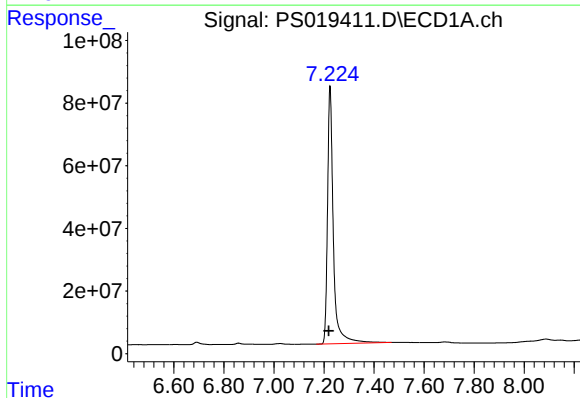


#4 2,4-DCAA

R.T.: 7.224 min
Delta R.T.: 0.005 min
Response: 1325570667
Conc: 485.40 ng/ml

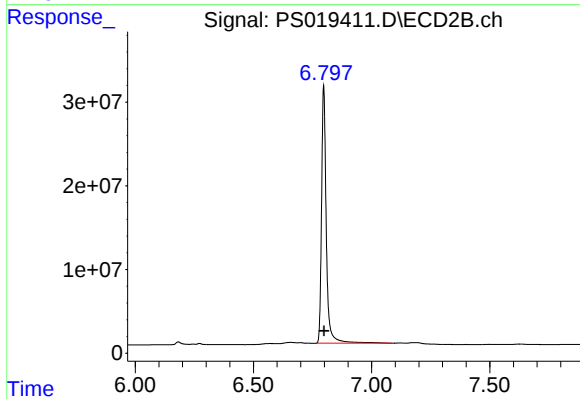

#4 2,4-DCAA


R.T.: 6.797 min
Delta R.T.: 0.000 min
Response: 428863305
Conc: 553.69 ng/ml

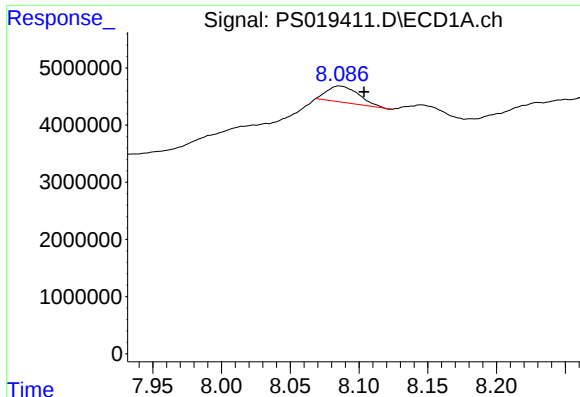

#8 DICHLORPROP


R.T.: 8.086 min
Delta R.T.: -0.018 min
Response: 4525754
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

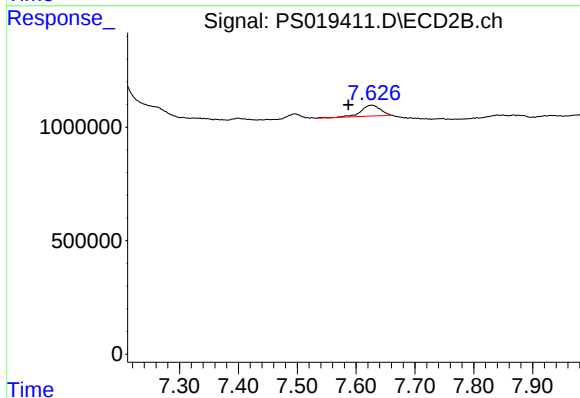


#8 DICHLORPROP

R.T.: 7.626 min
Delta R.T.: 0.040 min
Response: 1116885
Conc: 1.30 ng/ml

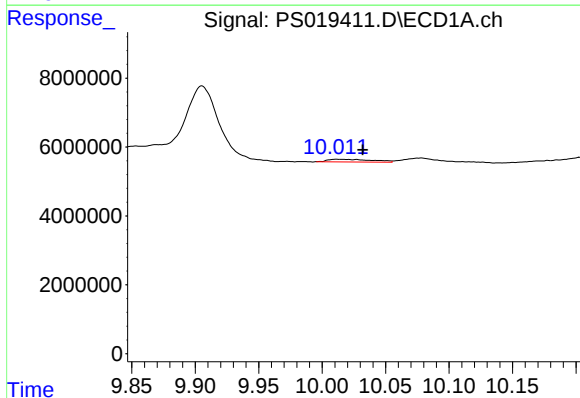


#13 2,4-DB

R.T.: 10.013 min
Delta R.T.: -0.019 min
Response: 1853551
Conc: N.D.

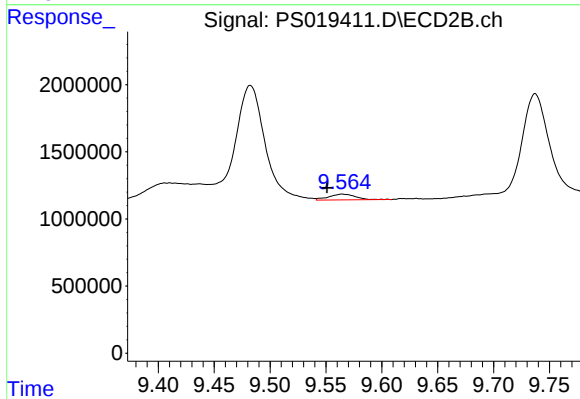

#13 2,4-DB


R.T.: 9.565 min
Delta R.T.: 0.014 min
Response: 730558
Conc: 1.28 ng/ml

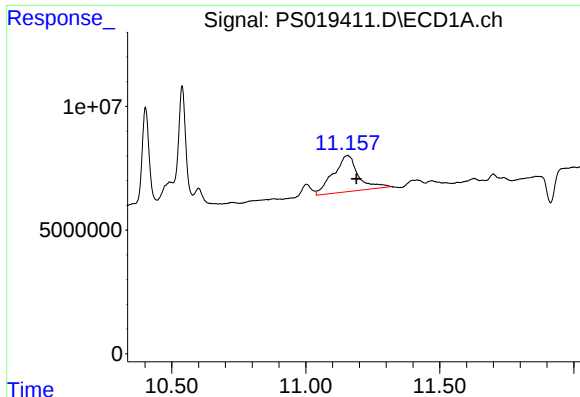

#14 DINOSEB


R.T.: 11.156 min
Delta R.T.: -0.033 min
Response: 94426167
Conc: 5.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

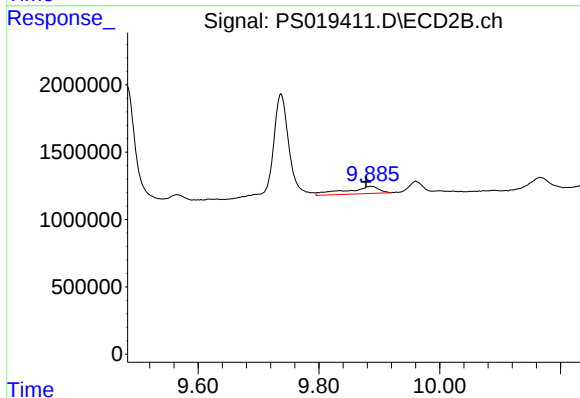


#14 DINOSEB

R.T.: 9.886 min
Delta R.T.: 0.008 min
Response: 2049194
Conc: N.D.

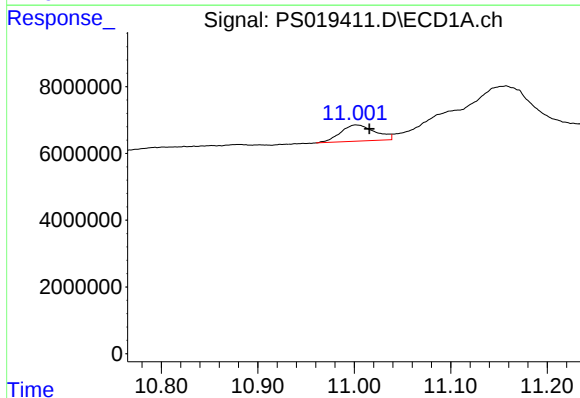


#15 Picloram

R.T.: 11.002 min
Delta R.T.: -0.013 min
Response: 12071309
Conc: N.D.

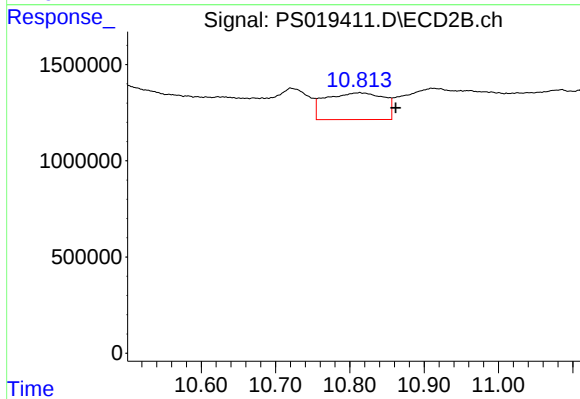

#15 Picloram


R.T.: 10.813 min
Delta R.T.: -0.049 min
Response: 7593918
Conc: 1.27 ng/ml

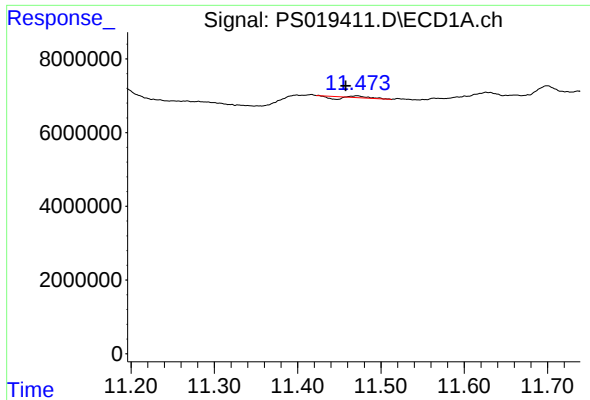

#16 DCPA

R.T.: 11.471 min
Delta R.T.: 0.013 min
Response: 114060
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

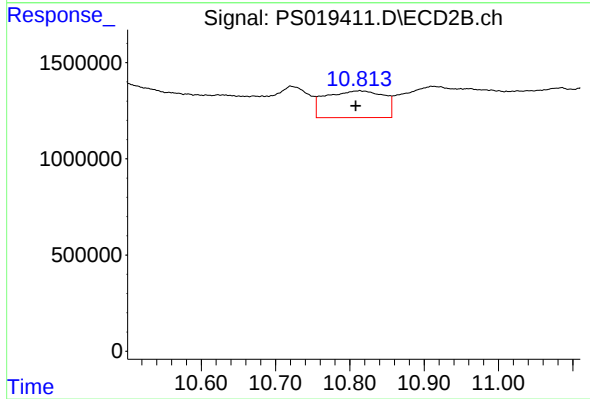

#16 DCPA

R.T.: 10.813 min
Delta R.T.: 0.005 min
Response: 7593918
Conc: 1.29 ng/ml