

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS051419\  
 Data File : PS004586.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 14 May 2019 07:27  
 Operator : EI\SJ  
 Sample : HEXANE  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 HEXANE

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 14 11:29:43 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS051319.M  
 Quant Title : 8080.M  
 QLast Update : Mon May 13 15:36:52 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

#### System Monitoring Compounds

| Target Compounds |          |       |       |          |          |                |
|------------------|----------|-------|-------|----------|----------|----------------|
| 15) T            | Picloram | 9.659 | 9.534 | 72875048 | 21229644 | 16.413 5.772 # |
| 16) T            | DCPA     | 0.000 | 9.534 | 0        | 21229644 | N.D. 6.225     |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS051419\  
Data File : PS004586.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 14 May 2019 07:27  
Operator : EI\SJ  
Sample : HEXANE  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: May 14 11:29:43 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS051319.M  
Quant Title : 8080.M  
QLast Update : Mon May 13 15:36:52 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

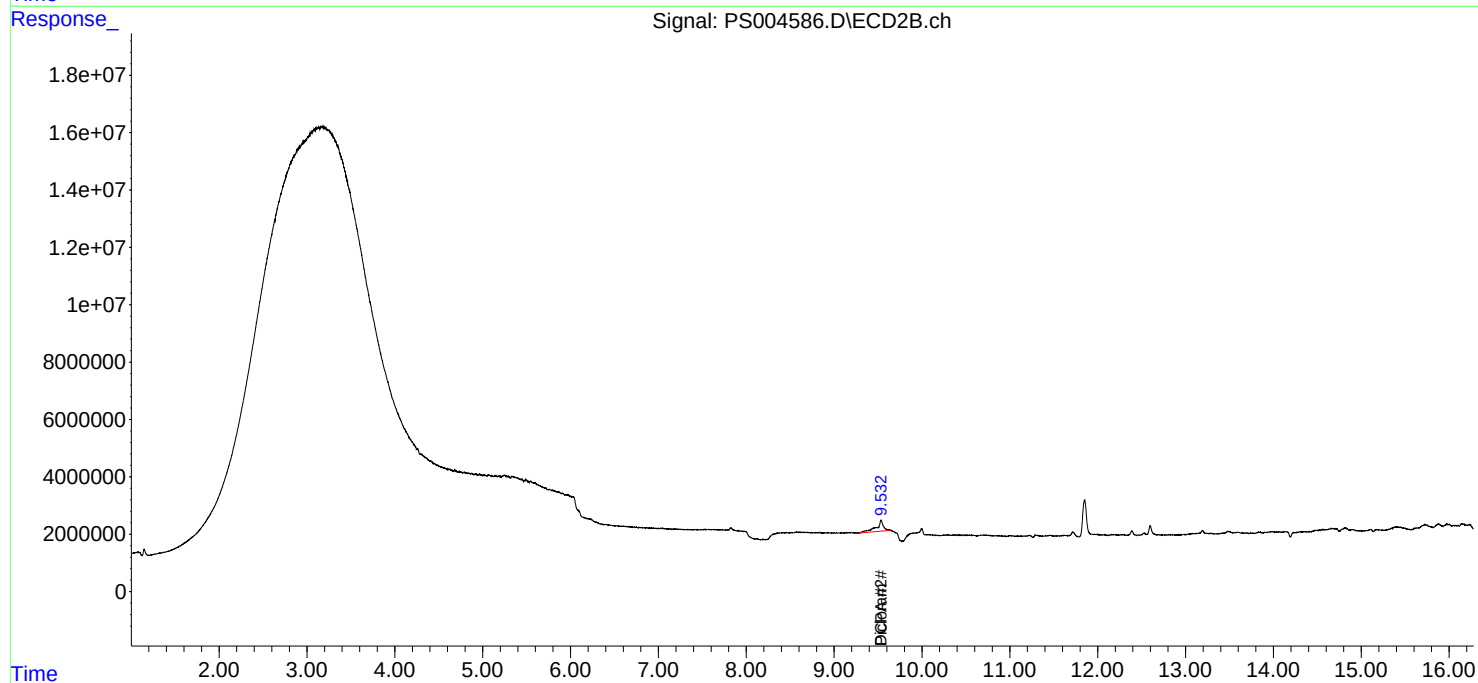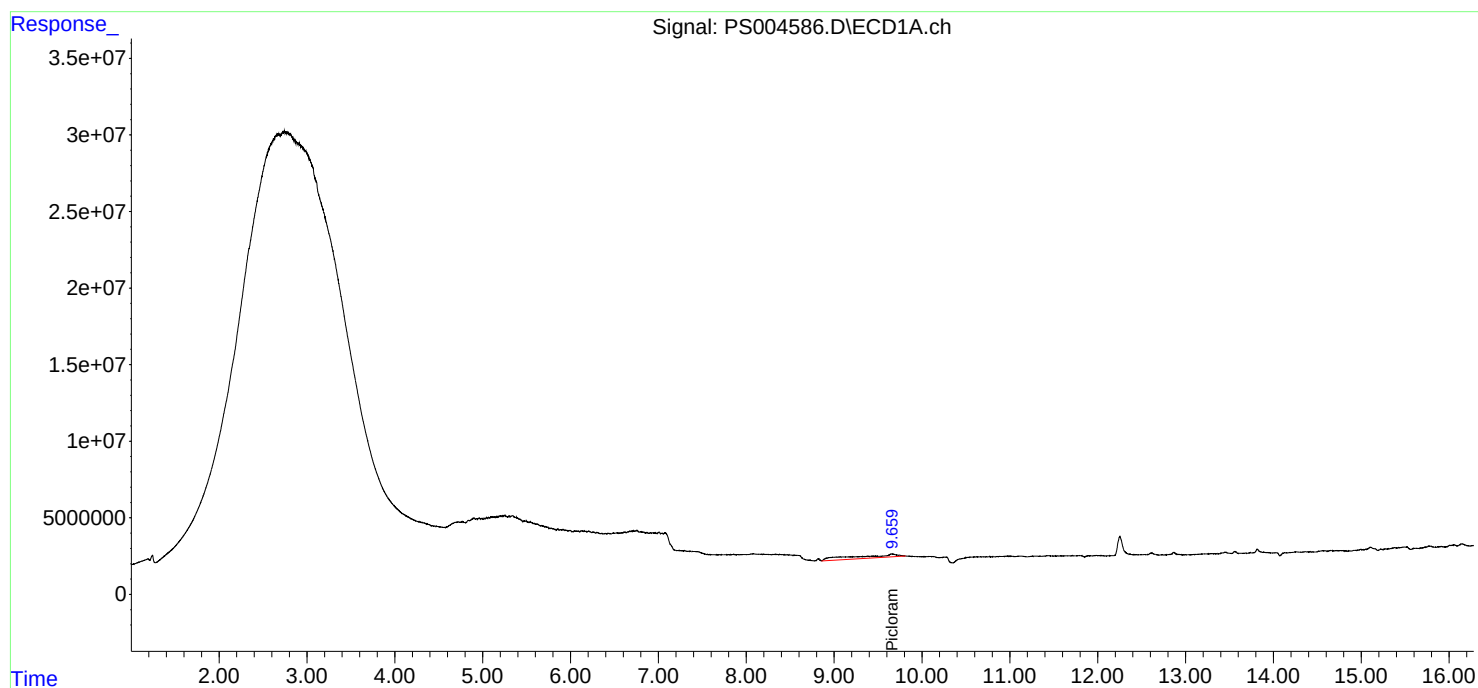


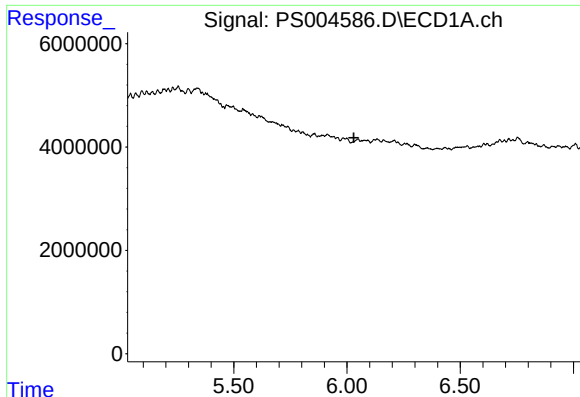

#4 2,4-DCAA


R.T.: 0.000 min  
Exp R.T.: 6.031 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

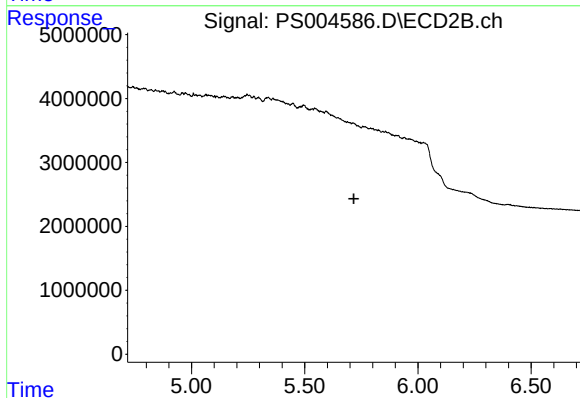


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T.: 5.717 min  
Response: 0  
Conc: N.D.

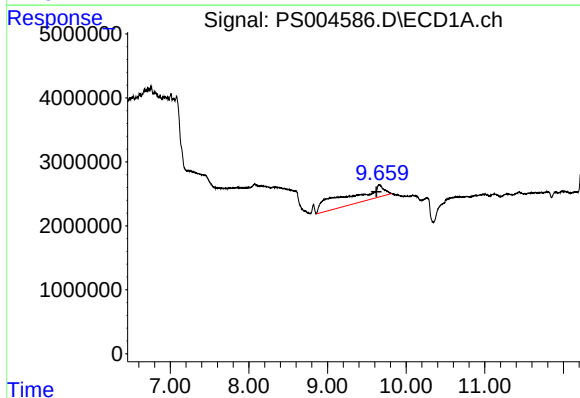


#15 Picloram

R.T.: 9.659 min  
Delta R.T.: 0.039 min  
Response: 72875048  
Conc: 16.41 ng/ml

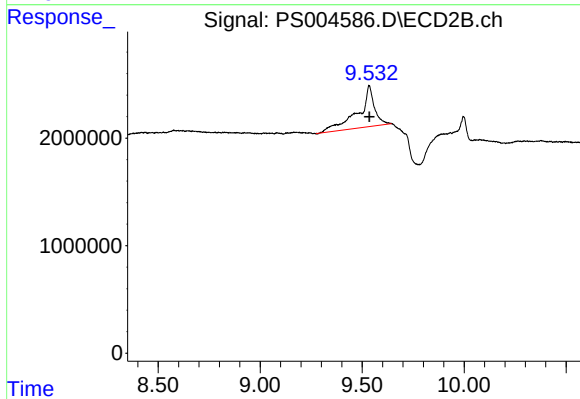

#15 Picloram


R.T.: 9.534 min  
Delta R.T.: -0.002 min  
Response: 21229644  
Conc: 5.77 ng/ml

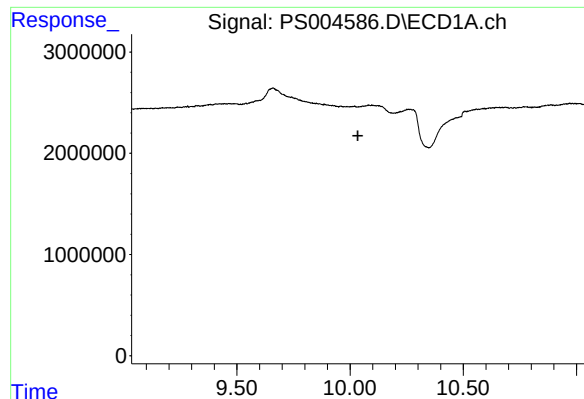

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 10.035 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
HEXANE

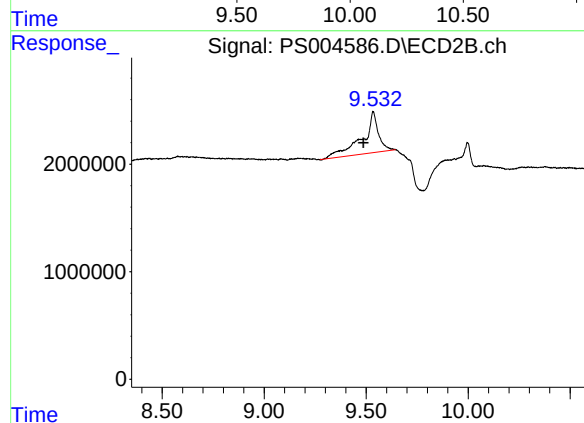

#16 DCPA

R.T.: 9.534 min  
Delta R.T.: 0.048 min  
Response: 21229644  
Conc: 6.22 ng/ml