

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
 Data File : PS004601.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 15:43
 Operator : EI\SJ
 Sample : K2807-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 K2807-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:12:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.009	5.704	143.4E6	92832093	201.739	184.672
Target Compounds							
1) T	Dalapon	2.376	2.042	190.4E6	197.7E6	201.514	281.986 #
2) T	3,5-DICHL...	5.418	5.018	6417053	155.2E6	7.577	235.935 #
3) T	4-Nitroph...	5.931	5.365	6865896	17128128	27.036	77.468 #
5) T	DICAMBA	6.144	5.882	11674681	3951440	4.368	2.016 #
6) T	MCPD	6.318	5.931	3819924	10831386	1.967	7.768 #
7) T	MCPA	6.437	6.119	5260104	7960895	1.872	3.895 #
8) T	DICHLORPROP	6.866	6.399	6546053	-651957	10.615	N.D. #
9) T	2,4-D	7.090	6.623	74270573	5029346	101.937	9.323 #
10) T	Pentachlo...	7.301	7.050	34354913	18706338	3.599	2.689 #
11) T	2,4,5-TP ...	7.912	7.364	3425122	121.2E6	<MDL	45.259 #
12) T	2,4,5-T	0.000	7.818	0	14010661	N.D.	5.822
13) T	2,4-DB	8.717	8.277	26838261	26644450	74.452	89.929
14) T	DINOSEB	0.000	8.573	0	32285663	N.D.	15.787
15) T	Picloram	9.600	9.526	81409198	70048621	18.336	19.046
16) T	DCPA	10.028	9.526	46627680	70048621	9.865	20.539 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
Data File : PS004601.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 15:43
Operator : EI\SJ
Sample : K2807-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
K2807-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:12:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

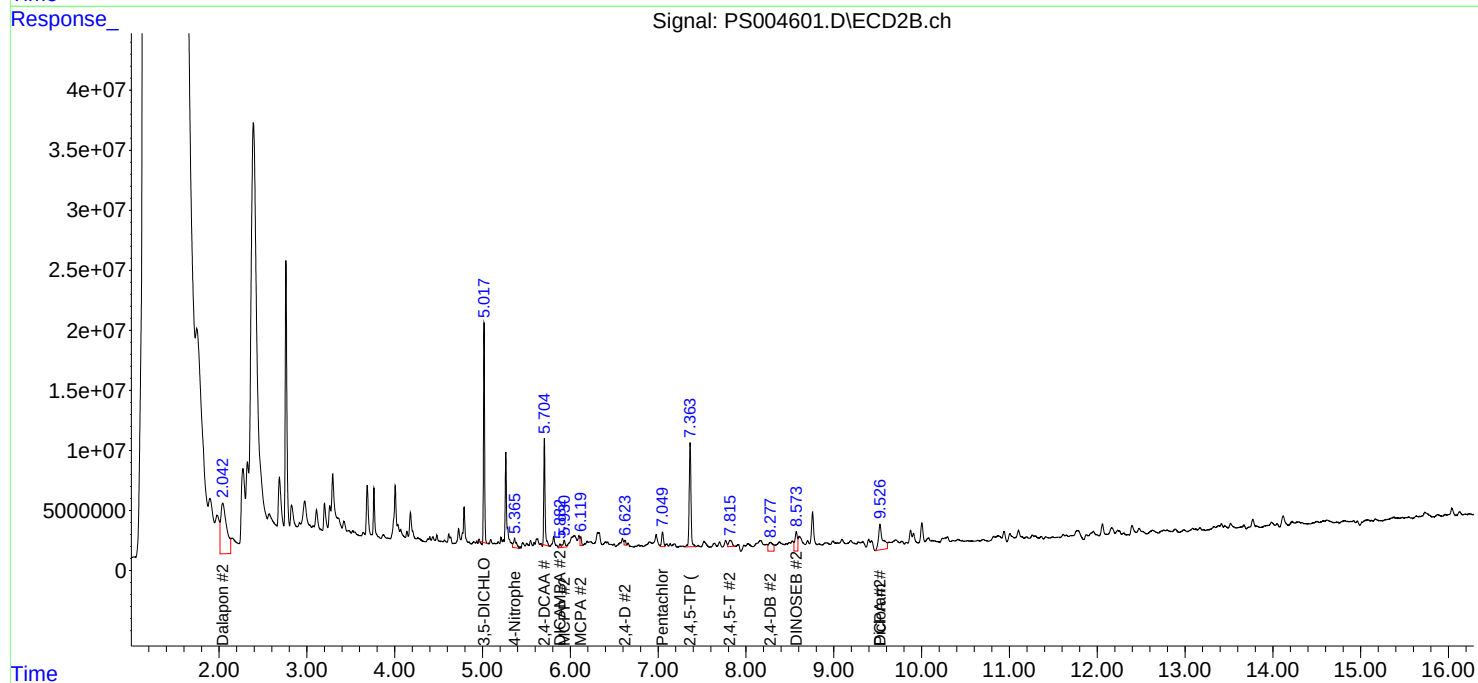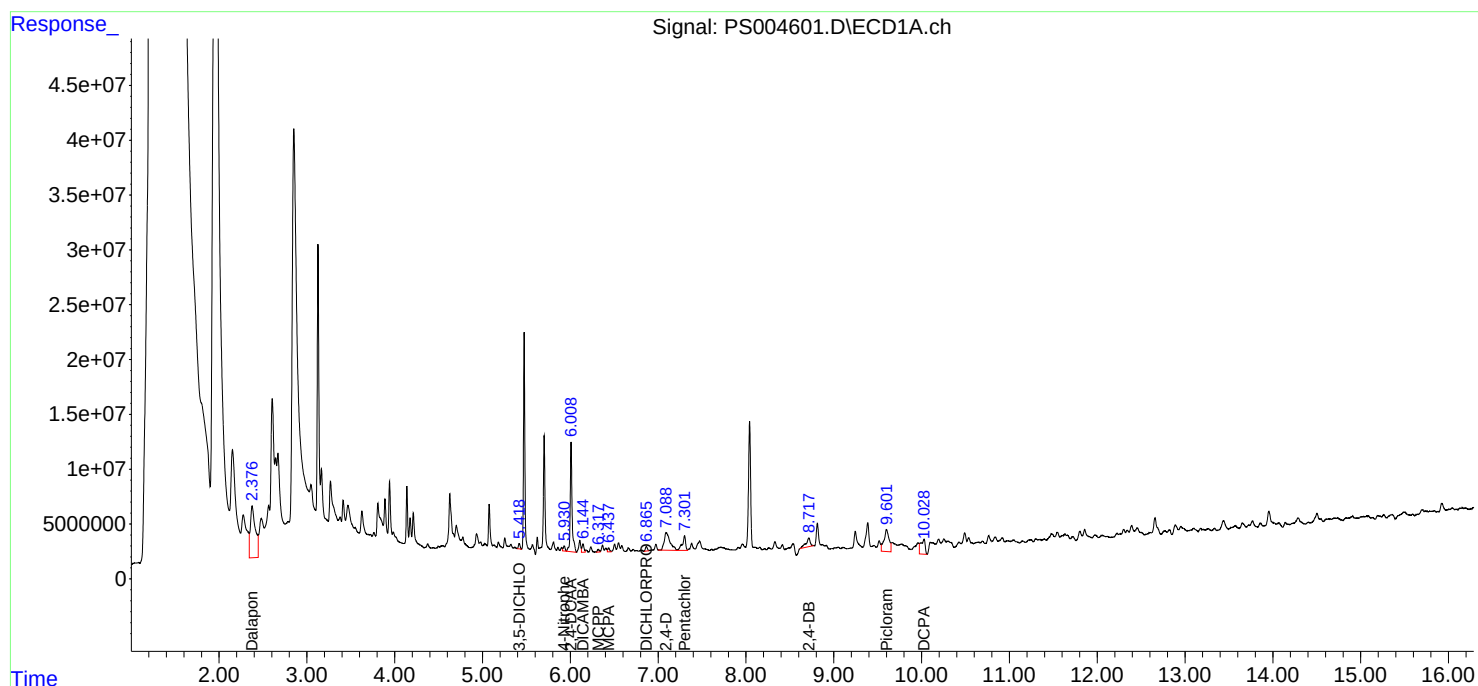


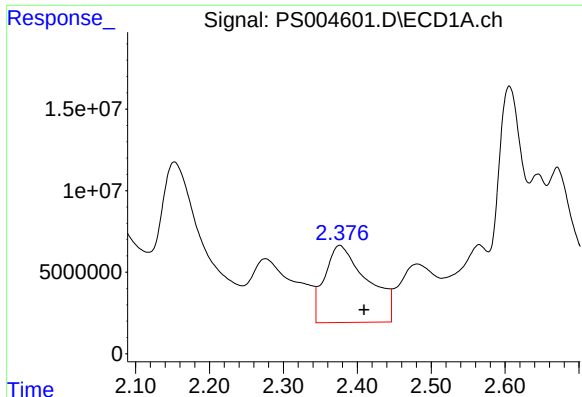

#1 Dalapon


R.T.: 2.376 min
Delta R.T.: -0.033 min
Response: 190398032
Conc: 201.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

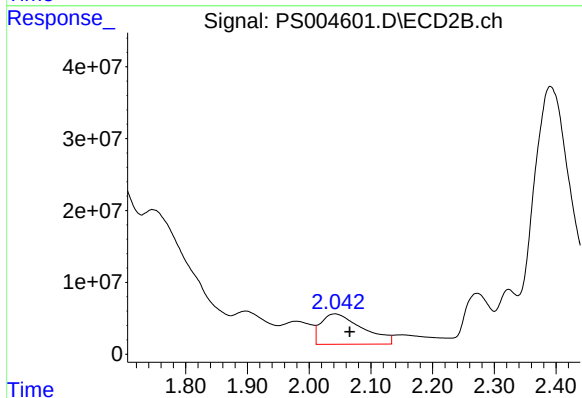


#1 Dalapon

R.T.: 2.042 min
Delta R.T.: -0.024 min
Response: 197671765
Conc: 281.99 ng/ml

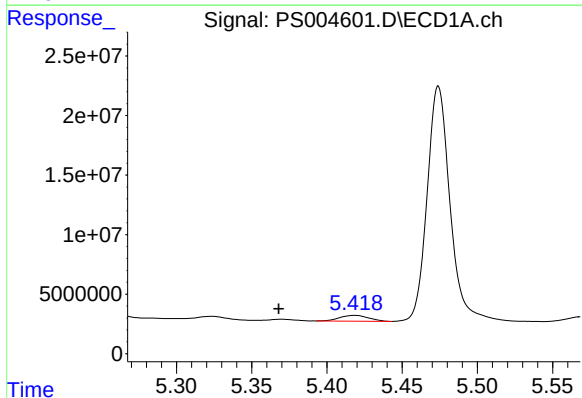


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.418 min
Delta R.T.: 0.050 min
Response: 6417053
Conc: 7.58 ng/ml

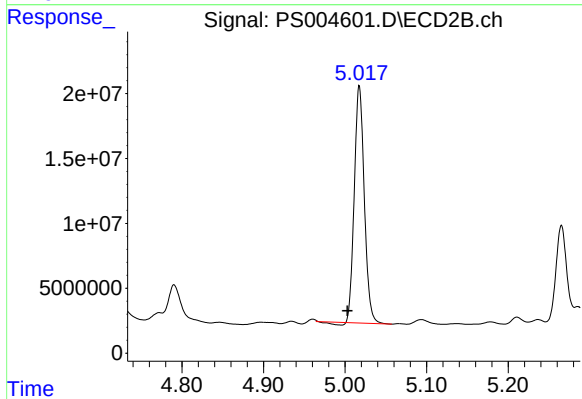

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.018 min
Delta R.T.: 0.015 min
Response: 155209178
Conc: 235.94 ng/ml

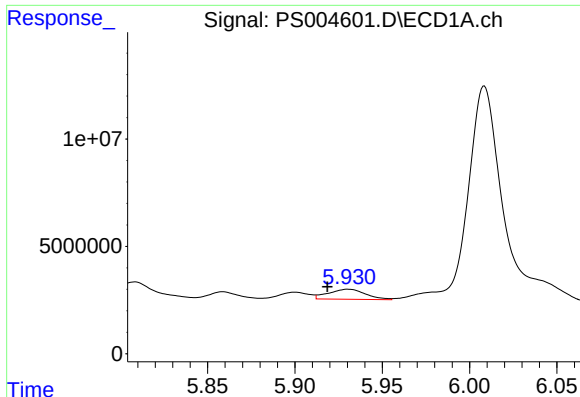

#3 4-Nitrophenol

R.T.: 5.931 min
Delta R.T.: 0.012 min
Response: 6865896
Conc: 27.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

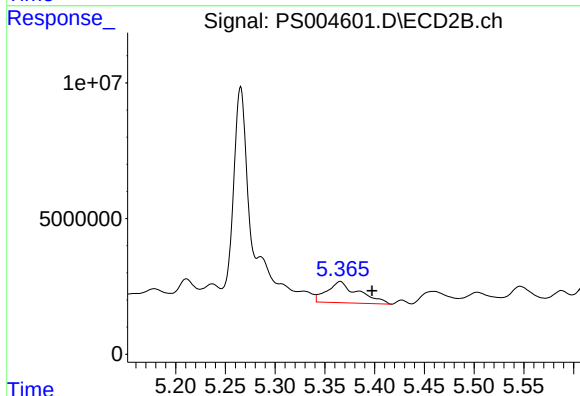

#3 4-Nitrophenol


R.T.: 5.365 min
Delta R.T.: -0.032 min
Response: 17128128
Conc: 77.47 ng/ml

#4 2,4-DCAA

R.T.: 6.009 min
Delta R.T.: -0.022 min
Response: 143381158
Conc: 201.74 ng/ml

#4 2,4-DCAA


R.T.: 5.704 min
Delta R.T.: -0.012 min
Response: 92832093
Conc: 184.67 ng/ml

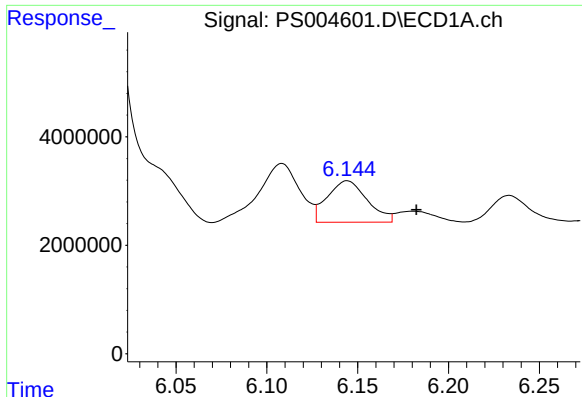

#5 DICAMBA


R.T.: 6.144 min
Delta R.T.: -0.038 min
Response: 11674681
Conc: 4.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

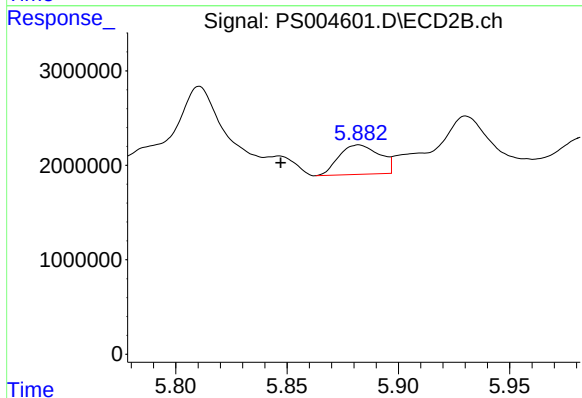


#5 DICAMBA

R.T.: 5.882 min
Delta R.T.: 0.035 min
Response: 3951440
Conc: 2.02 ng/ml

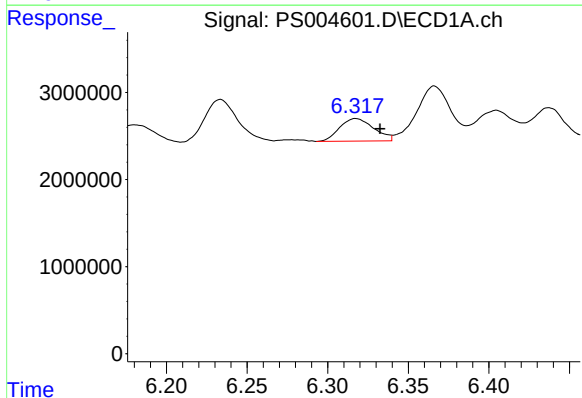


#6 MCP

R.T.: 6.318 min
Delta R.T.: -0.015 min
Response: 3819924
Conc: 1.97 ug/ml

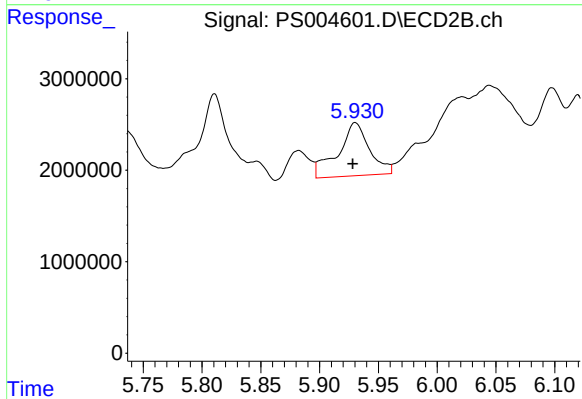

#6 MCP


R.T.: 5.931 min
Delta R.T.: 0.002 min
Response: 10831386
Conc: 7.77 ug/ml

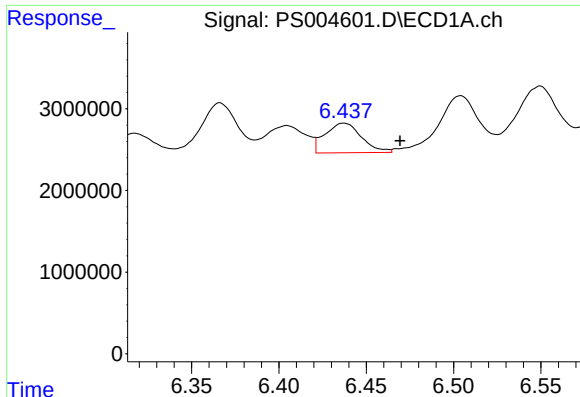

#7 MCPA


R.T.: 6.437 min
Delta R.T.: -0.032 min
Response: 5260104
Conc: 1.87 ug/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

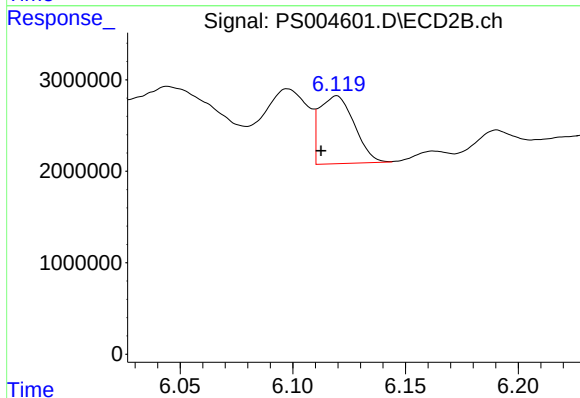


#7 MCPA

R.T.: 6.119 min
Delta R.T.: 0.006 min
Response: 7960895
Conc: 3.90 ug/ml

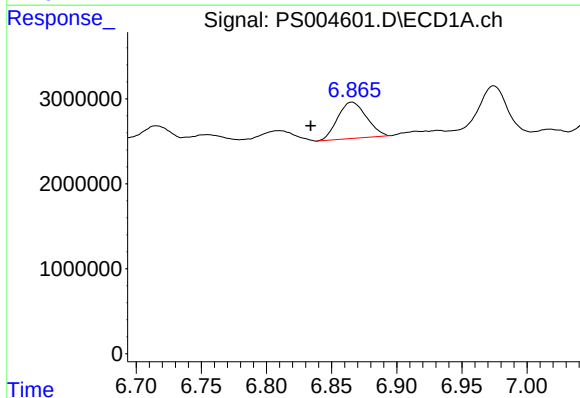


#8 DICHLORPROP

R.T.: 6.866 min
Delta R.T.: 0.032 min
Response: 6546053
Conc: 10.62 ng/ml

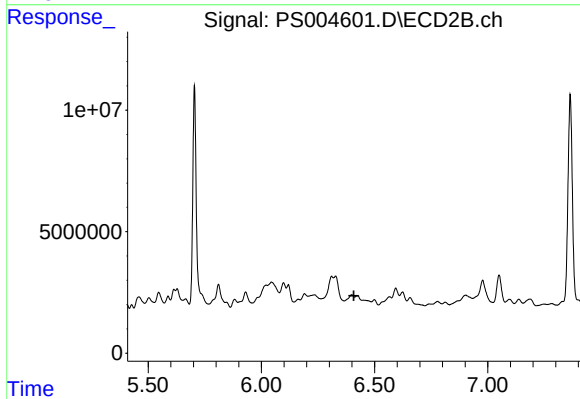

#8 DICHLORPROP


R.T.: 6.399 min
Delta R.T.: -0.010 min
Response: -651957
Conc: N.D.

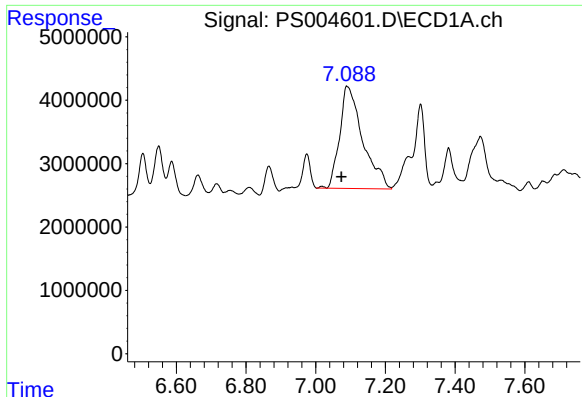

#9 2,4-D


R.T.: 7.090 min
Delta R.T.: 0.016 min
Response: 74270573
Conc: 101.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

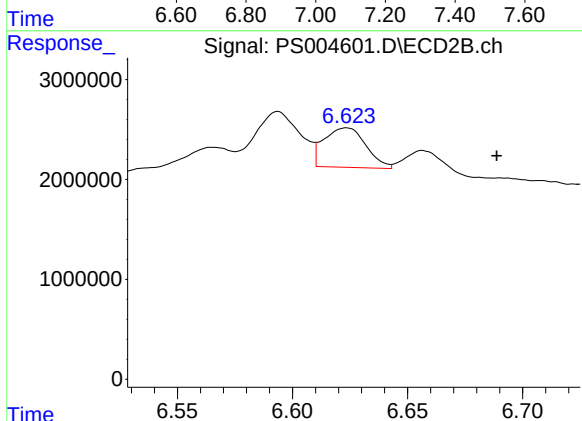


#9 2,4-D

R.T.: 6.623 min
Delta R.T.: -0.066 min
Response: 5029346
Conc: 9.32 ng/ml

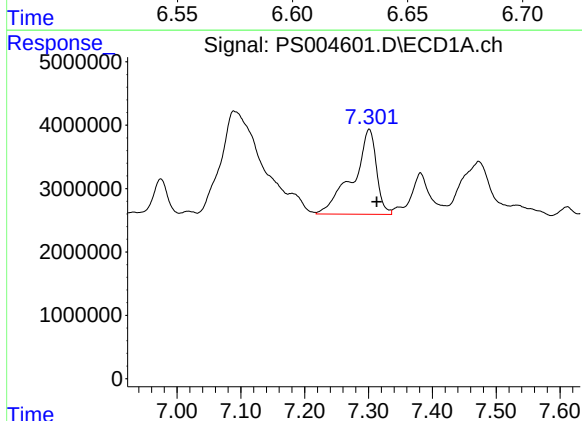


#10 Pentachlorophenol

R.T.: 7.301 min
Delta R.T.: -0.012 min
Response: 34354913
Conc: 3.60 ng/ml

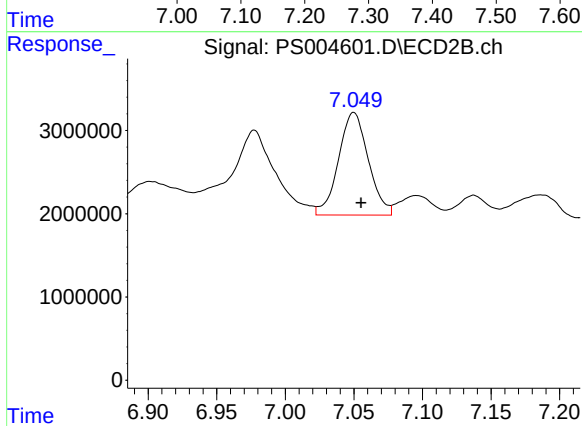

#10 Pentachlorophenol


R.T.: 7.050 min
Delta R.T.: -0.005 min
Response: 18706338
Conc: 2.69 ng/ml

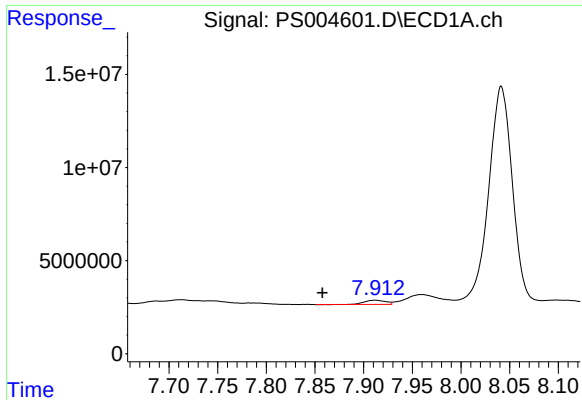

#11 2,4,5-TP (SILVEX)


R.T.: 7.912 min
Delta R.T.: 0.054 min
Response: 3425122
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
K2807-08

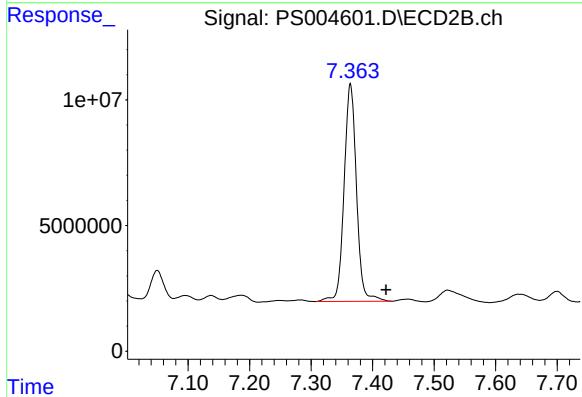


#11 2,4,5-TP (SILVEX)

R.T.: 7.364 min
Delta R.T.: -0.058 min
Response: 121243889
Conc: 45.26 ng/ml

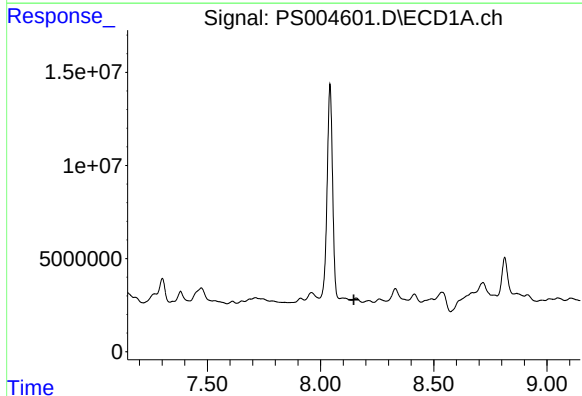


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.

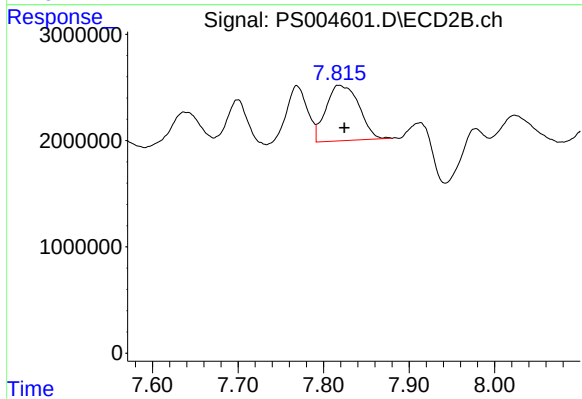

#12 2,4,5-T


R.T.: 7.818 min
Delta R.T.: -0.006 min
Response: 14010661
Conc: 5.82 ng/ml

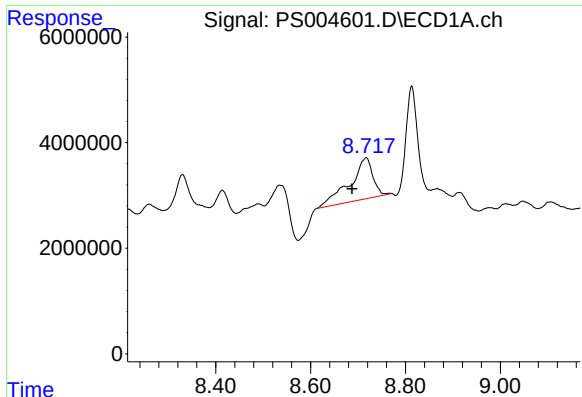

#13 2,4-DB


R.T.: 8.717 min
Delta R.T.: 0.030 min
Response: 26838261
Conc: 74.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

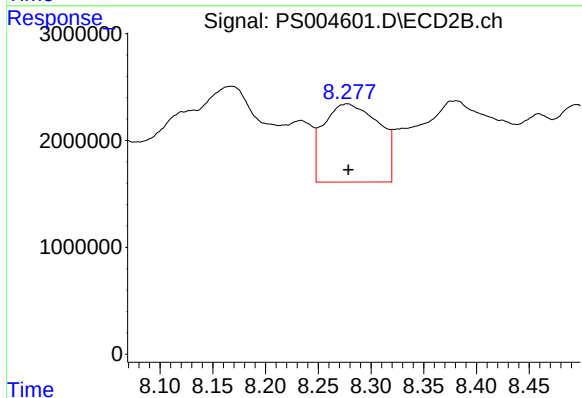


#13 2,4-DB

R.T.: 8.277 min
Delta R.T.: -0.001 min
Response: 26644450
Conc: 89.93 ng/ml

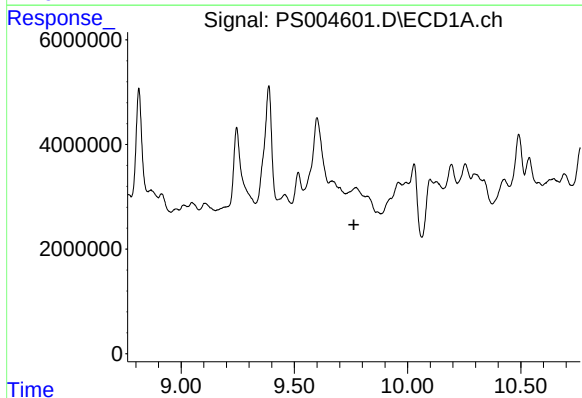


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.763 min
Response: 0
Conc: N.D.

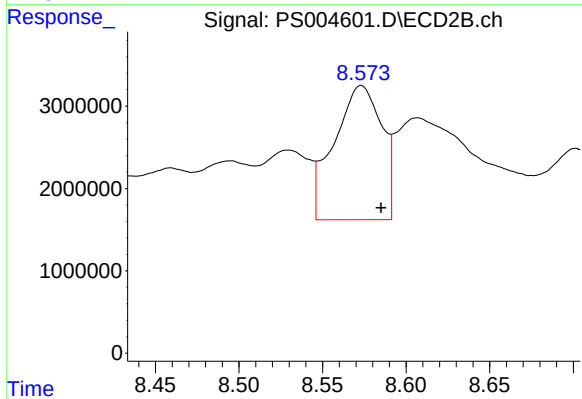

#14 DINOSEB


R.T.: 8.573 min
Delta R.T.: -0.012 min
Response: 32285663
Conc: 15.79 ng/ml

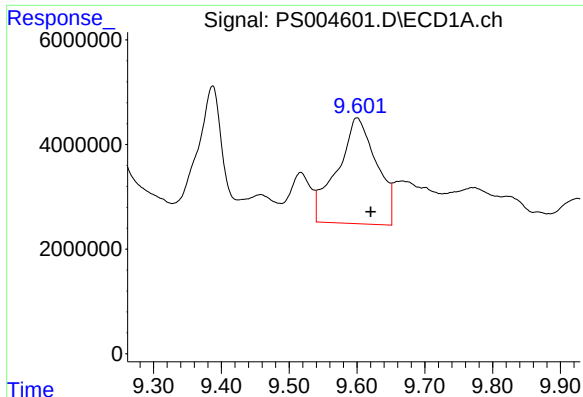

#15 Picloram


R.T.: 9.600 min
Delta R.T.: -0.020 min
Response: 81409198
Conc: 18.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
K2807-08

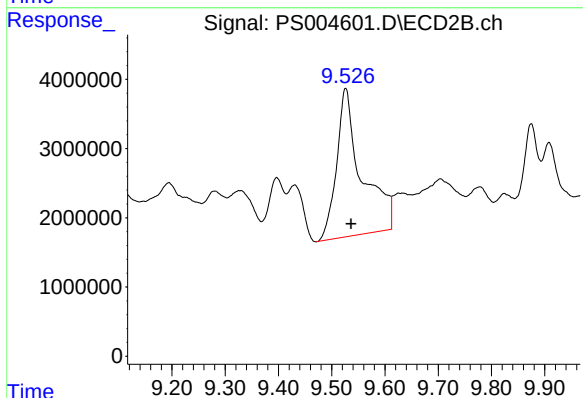


#15 Picloram

R.T.: 9.526 min
Delta R.T.: -0.010 min
Response: 70048621
Conc: 19.05 ng/ml

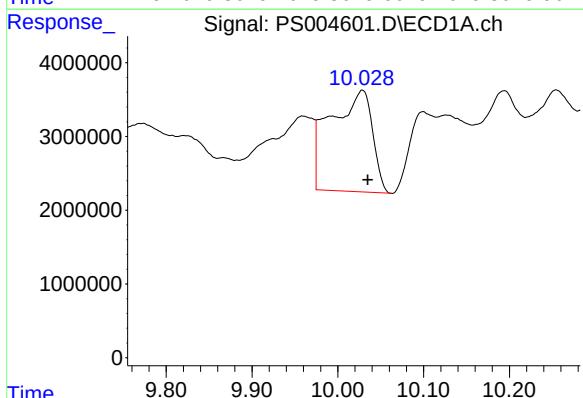

#16 DCPA

R.T.: 10.028 min
Delta R.T.: -0.006 min
Response: 46627680
Conc: 9.87 ng/ml

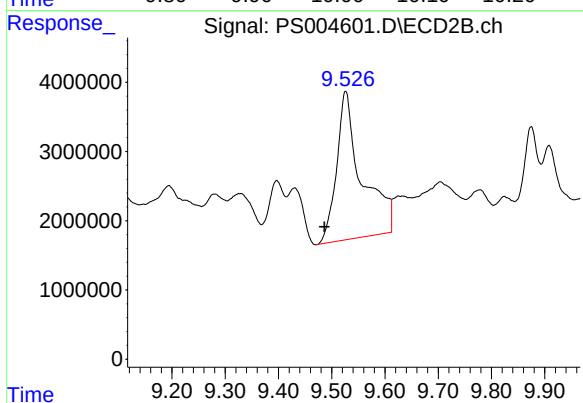

#16 DCPA

R.T.: 9.526 min
Delta R.T.: 0.040 min
Response: 70048621
Conc: 20.54 ng/ml