

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
 Data File : PS004605.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 17:49
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:13:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.031	5.727	370.7E6	261.4E6	521.592	520.043
Target Compounds							
7) T	MCPA	0.000	6.072	0	55136476	N.D.	26.978
9) T	2,4-D	7.113	0.000	74702706	0	102.530	N.D. #
12) T	2,4,5-T	0.000	7.855	0	6299479	N.D.	2.618
15) T	Picloram	9.651	9.561	29645917	26020633	6.677	7.075



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
Data File : PS004605.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 17:49
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:13:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

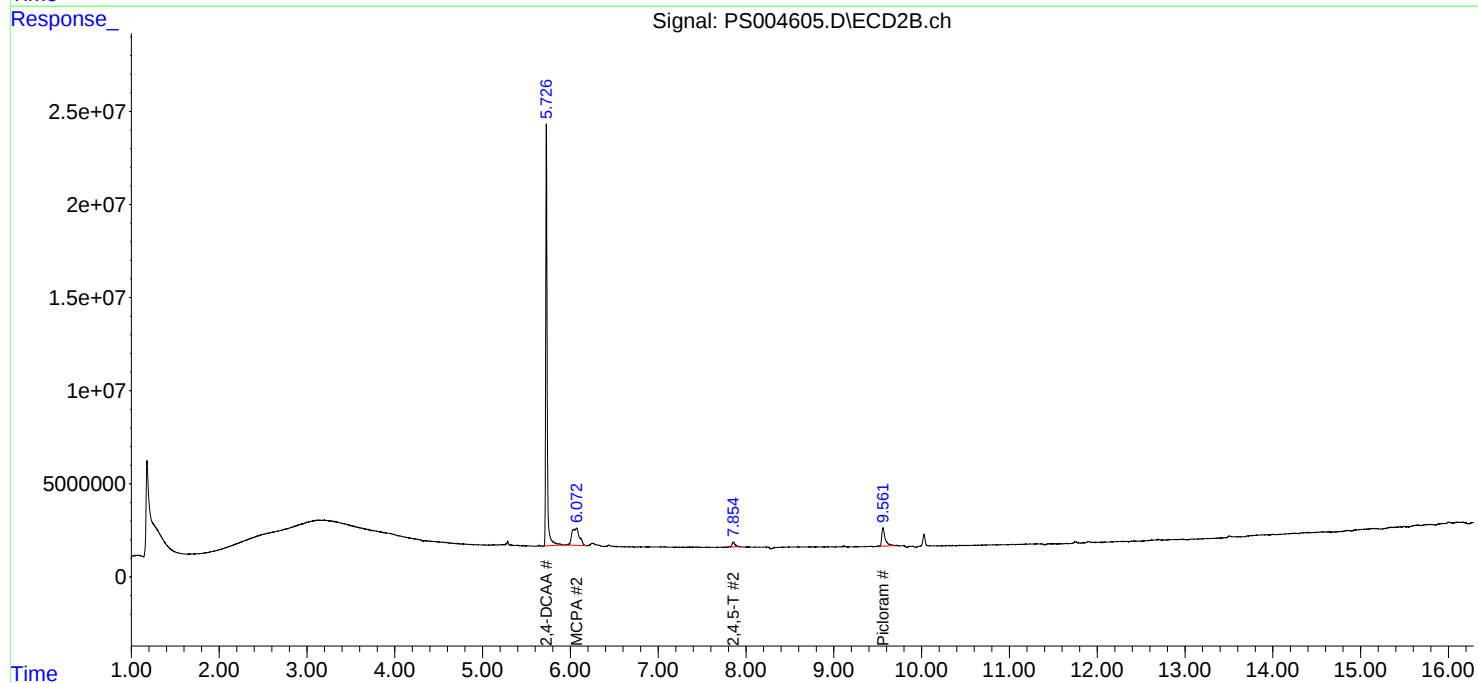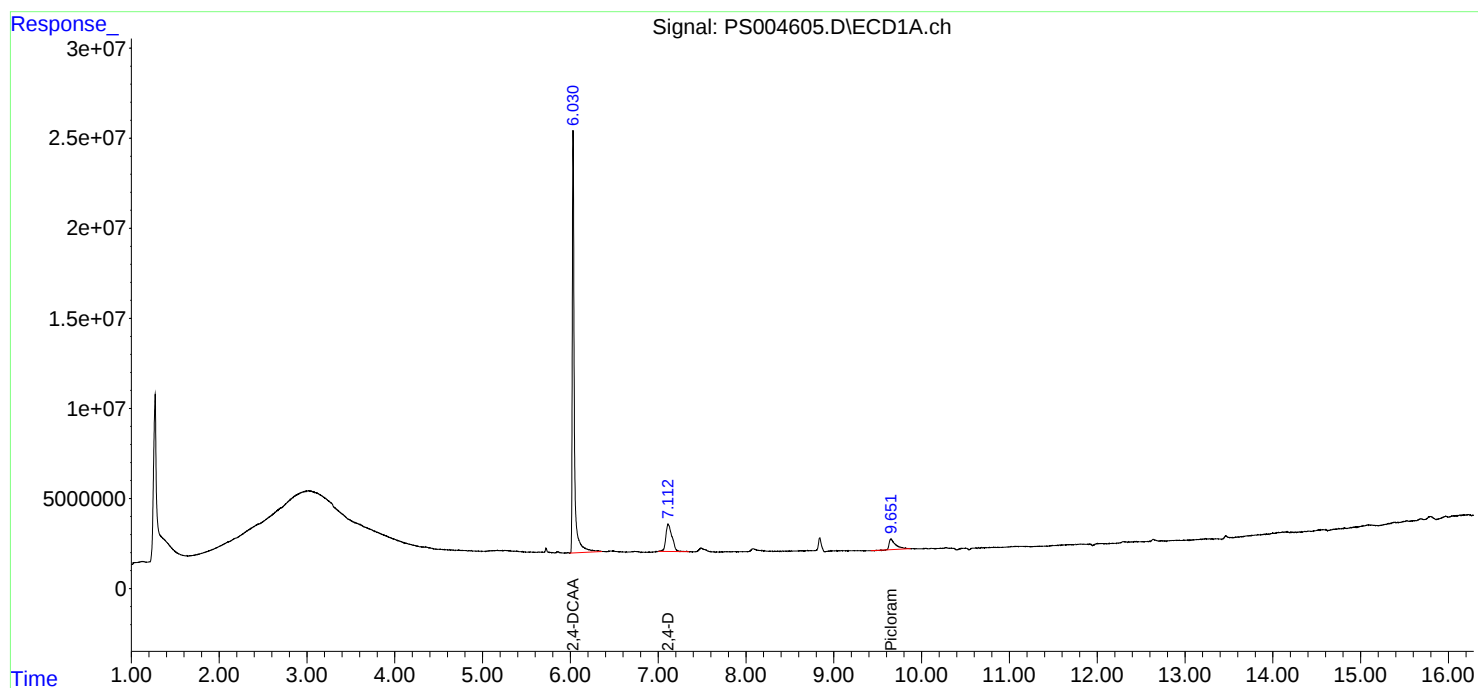


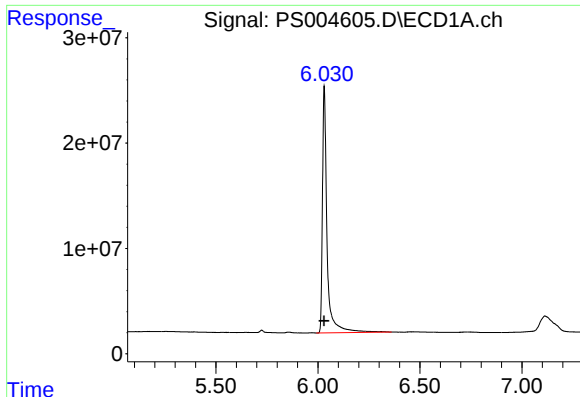

#4 2,4-DCAA


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 370709855
Conc: 521.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

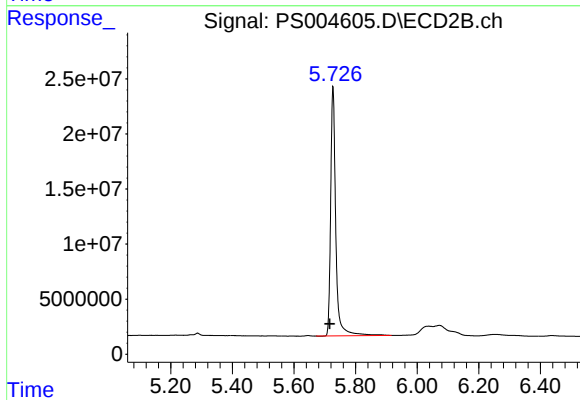


#4 2,4-DCAA

R.T.: 5.727 min
Delta R.T.: 0.010 min
Response: 261418005
Conc: 520.04 ng/ml

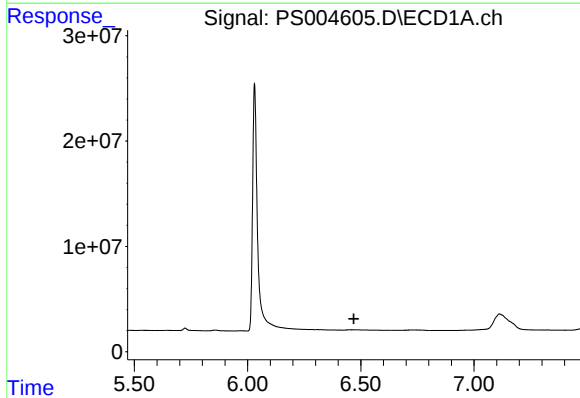


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

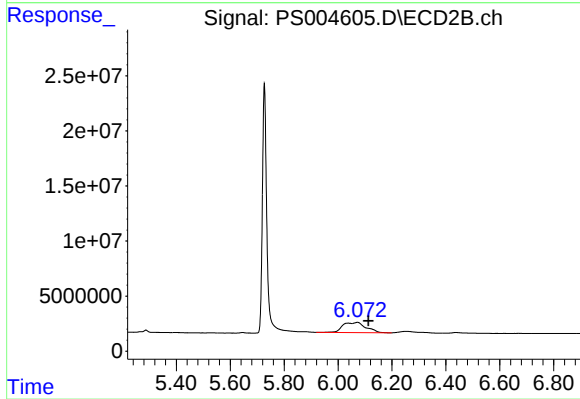

#7 MCPA


R.T.: 6.072 min
Delta R.T.: -0.041 min
Response: 55136476
Conc: 26.98 ug/ml

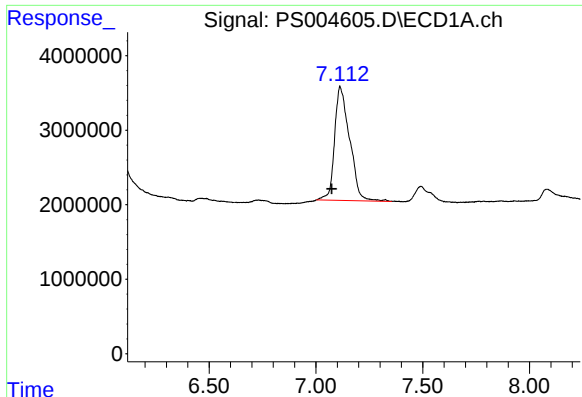

#9 2,4-D


R.T.: 7.113 min
Delta R.T.: 0.038 min
Response: 74702706
Conc: 102.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

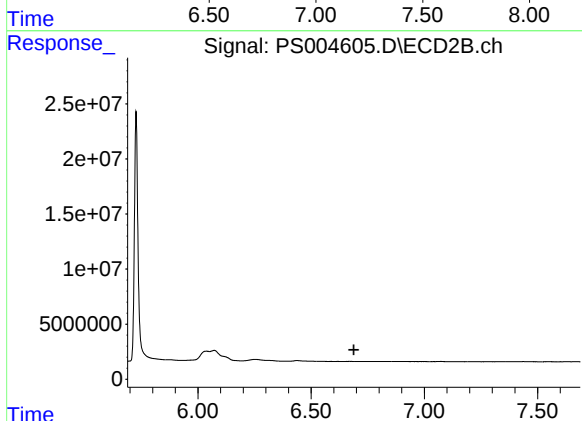


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

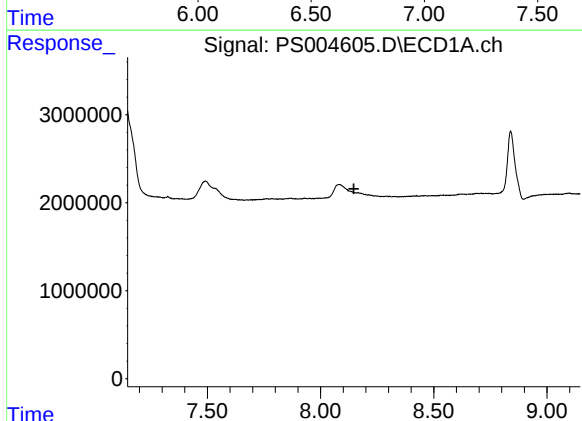


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.

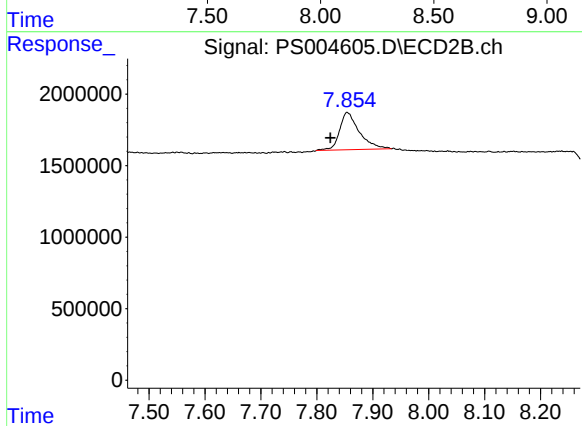

#12 2,4,5-T


R.T.: 7.855 min
Delta R.T.: 0.030 min
Response: 6299479
Conc: 2.62 ng/ml

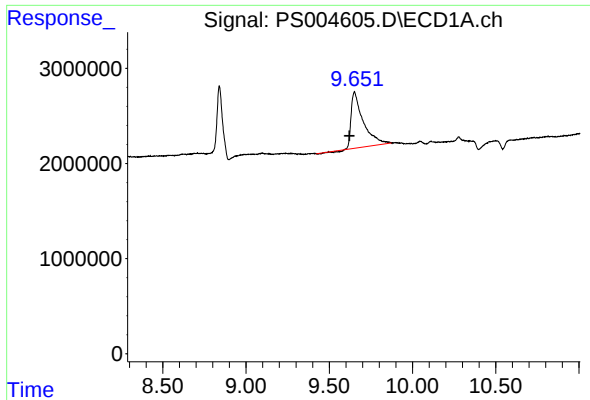

#15 Picloram

R.T.: 9.651 min
Delta R.T.: 0.031 min
Response: 29645917
Conc: 6.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

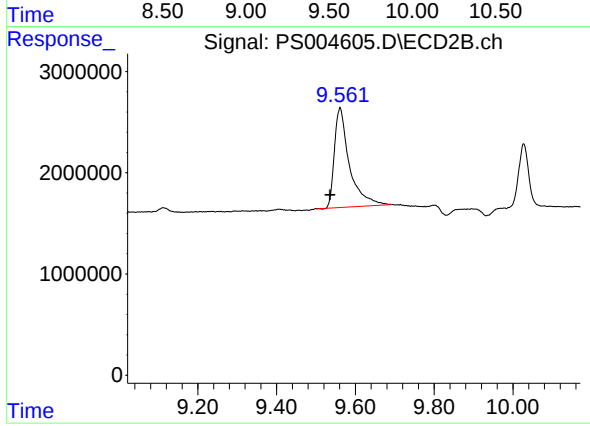

#15 Picloram

R.T.: 9.561 min
Delta R.T.: 0.025 min
Response: 26020633
Conc: 7.07 ng/ml