

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
 Data File : PS004596.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 May 2019 13:07
 Operator : EI\SJ
 Sample : K2761-03 (Sig #1); K2763-03 (Sig #2)
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 FK-SF-03-006-B

Manual Integrations
 APPROVED

Ankita
 5/15/2019 1:57:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 01:11:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.013	5.710	13452739	9533751	18.928m	18.966

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051419\
Data File : PS004596.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 May 2019 13:07
Operator : EI\SJ
Sample : K2761-03 (Sig #1); K2763-03 (Sig #2)
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
FK-SF-03-006-B


Manual Integrations
APPROVED

Ankita
5/15/2019 1:57:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 01:11:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

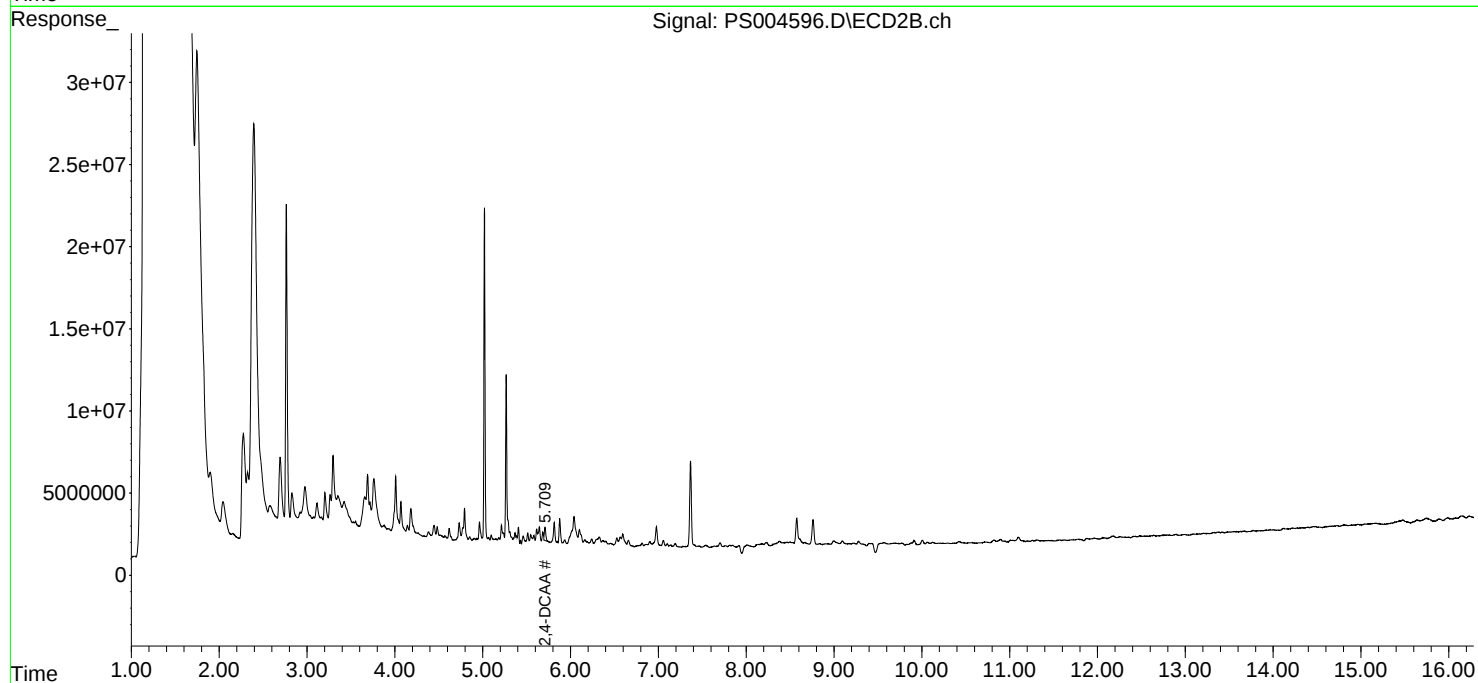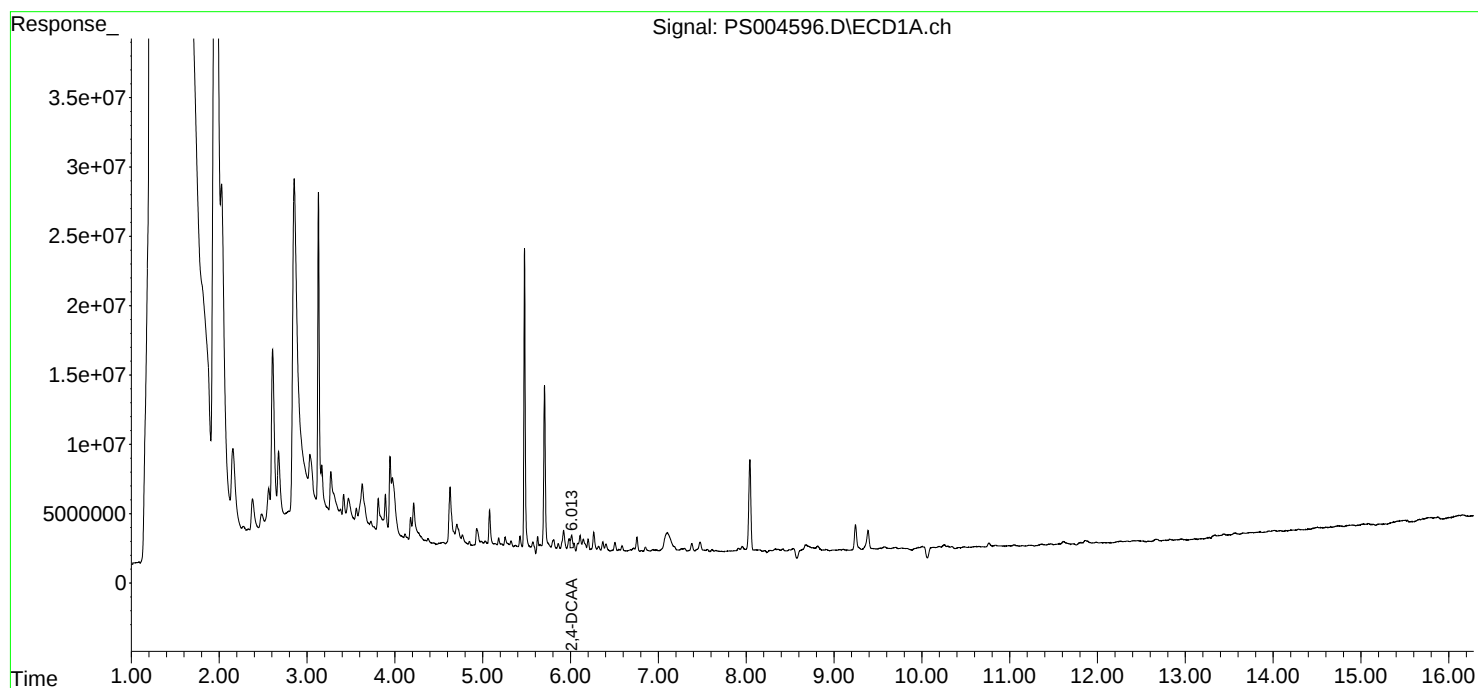

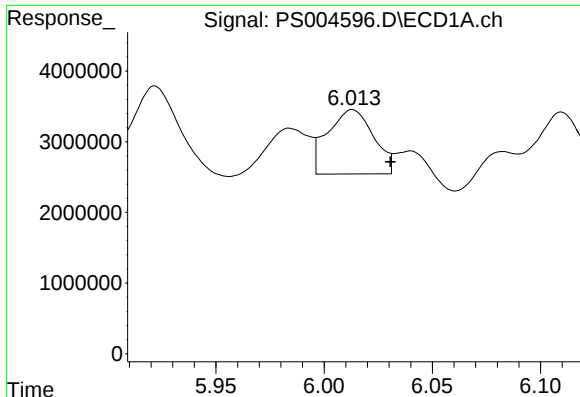


#4 2,4-DCAA

R.T.: 6.013 min
Delta R.T.: -0.018 min
Response: 13452739
Conc: 18.93 ng/ml m

Instrument :
ECD_S
ClientSampleId :
FK-SF-03-006-B

Manual Integrations
APPROVED

Ankita
5/15/2019 1:57:22 PM

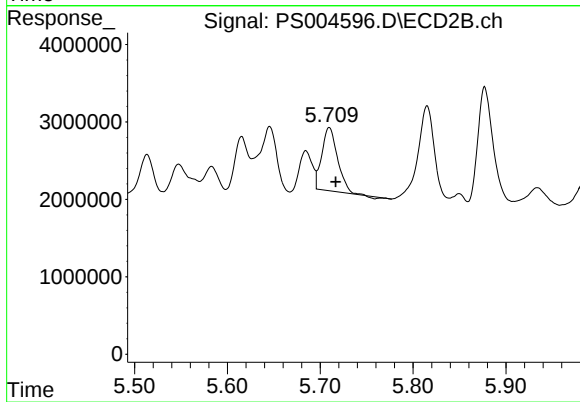

#4 2,4-DCAA

R.T.: 5.710 min
Delta R.T.: -0.007 min
Response: 9533751
Conc: 18.97 ng/ml