

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051519\
 Data File : PS004618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2019 14:46
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 00:55:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.035	5.730	323.9E6	239.0E6	455.696	475.502
Target Compounds							
7) T	MCPA	0.000	6.071	0	40218178	N.D.	19.679
9) T	2,4-D	7.119	0.000	80298430	0	110.210	N.D. #
12) T	2,4,5-T	0.000	7.856	0	6243608	N.D.	2.594
15) T	Picloram	9.651	9.563	25165430	23506399	5.668	6.391



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051519\
Data File : PS004618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2019 14:46
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 00:55:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

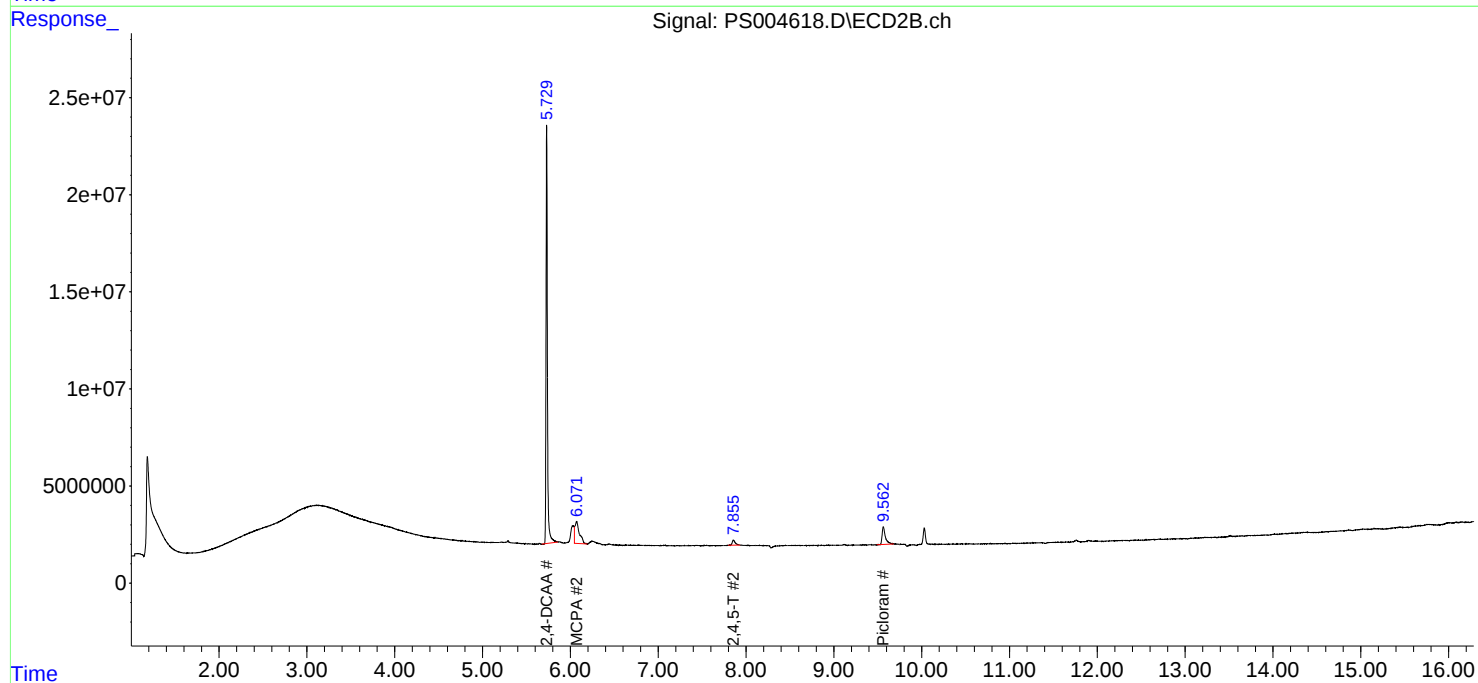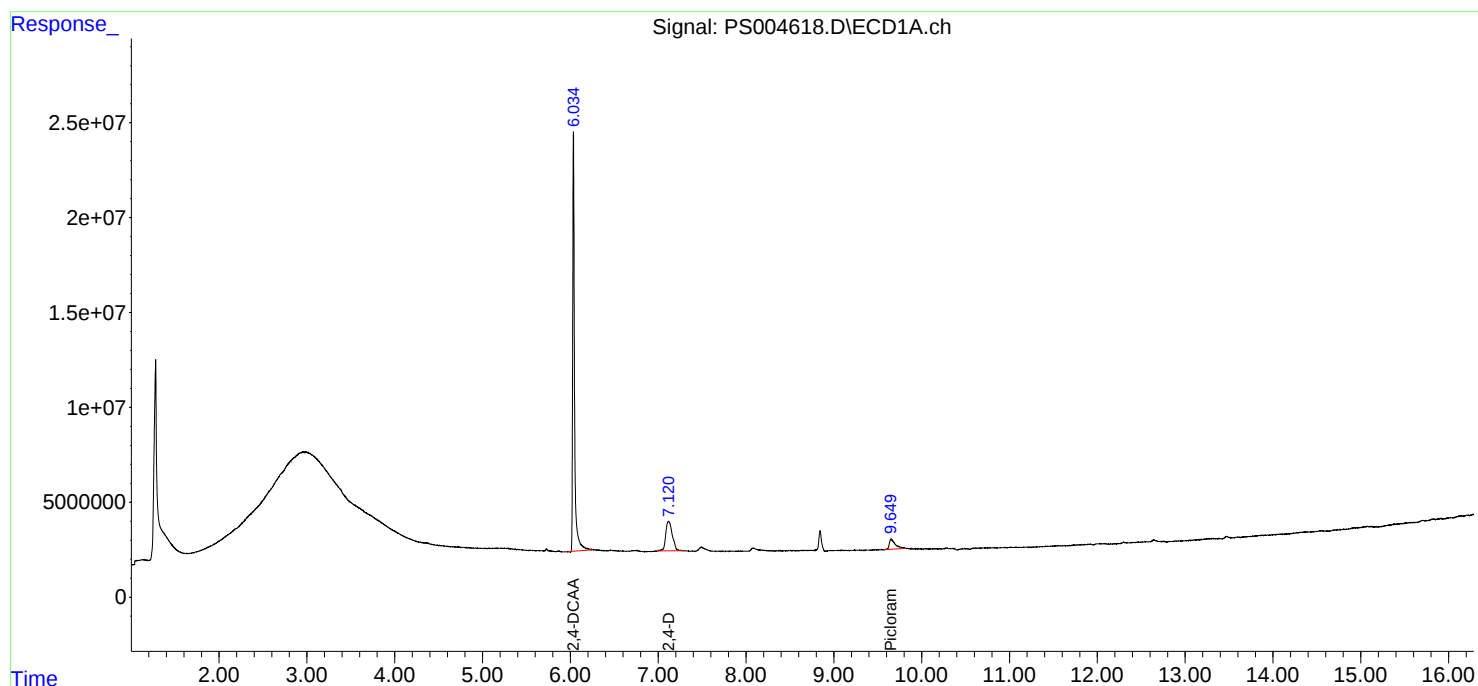


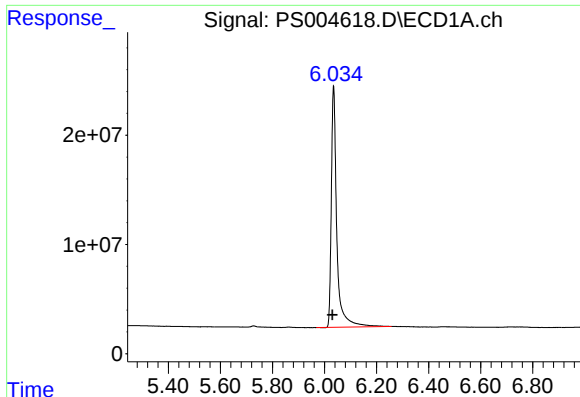

#4 2,4-DCAA


R.T.: 6.035 min
Delta R.T.: 0.004 min
Response: 323876048
Conc: 455.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

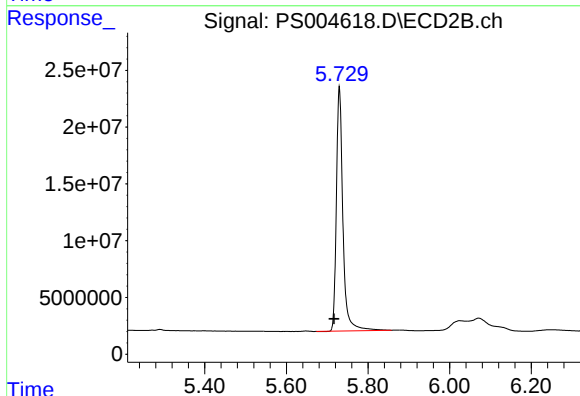


#4 2,4-DCAA

R.T.: 5.730 min
Delta R.T.: 0.013 min
Response: 239028280
Conc: 475.50 ng/ml

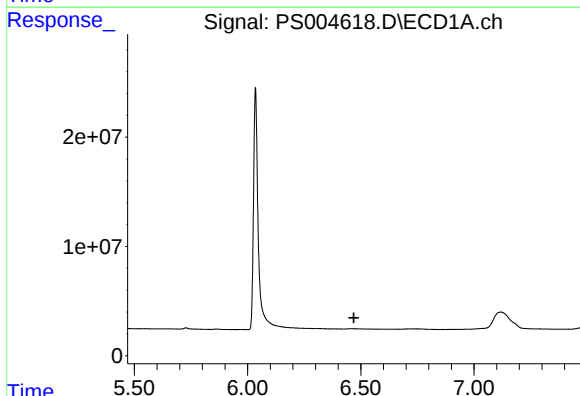


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

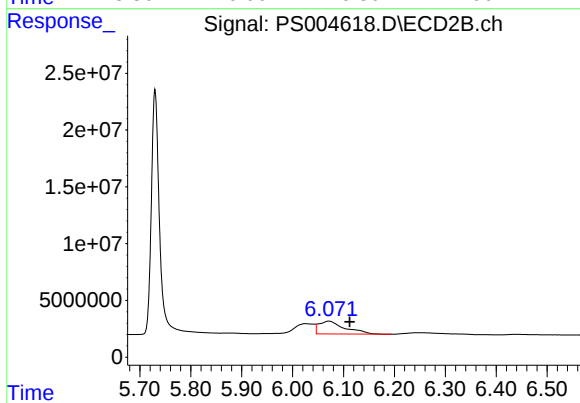

#7 MCPA


R.T.: 6.071 min
Delta R.T.: -0.041 min
Response: 40218178
Conc: 19.68 ug/ml

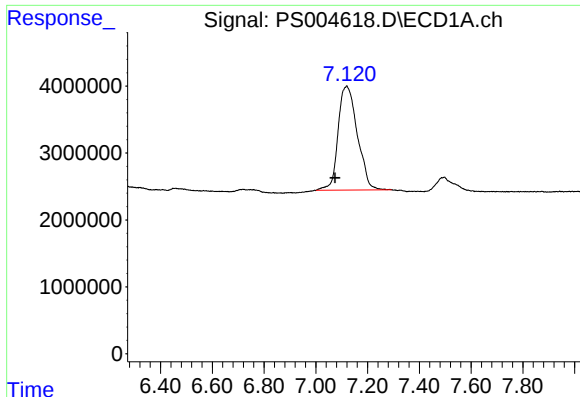

#9 2,4-D


R.T.: 7.119 min
Delta R.T.: 0.045 min
Response: 80298430
Conc: 110.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

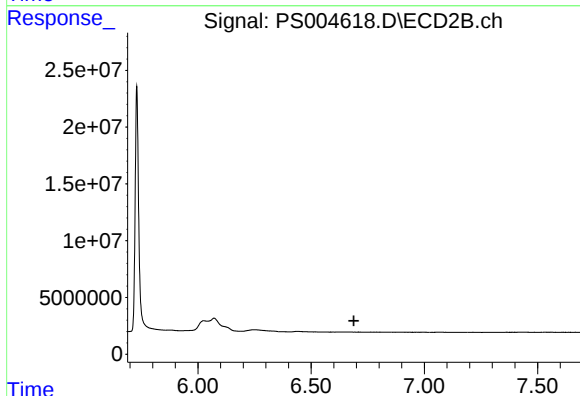


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

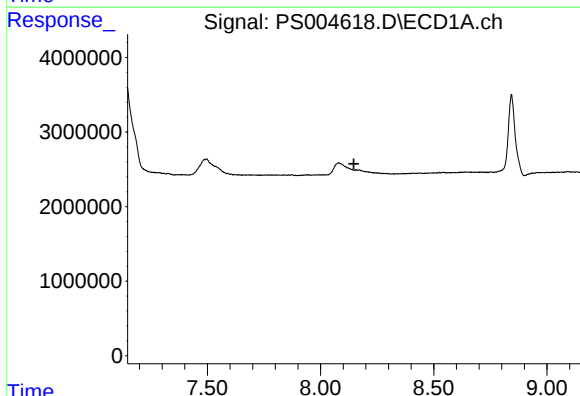


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.147 min
Response: 0
Conc: N.D.

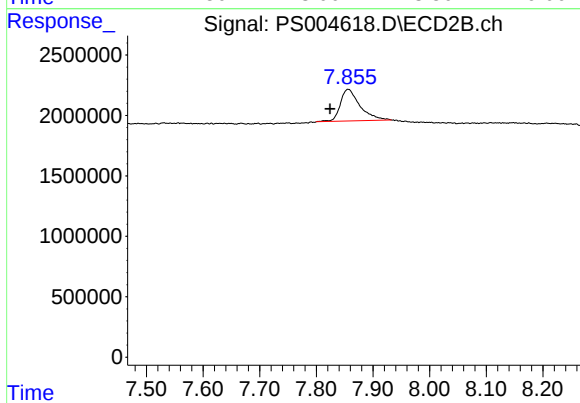

#12 2,4,5-T


R.T.: 7.856 min
Delta R.T.: 0.032 min
Response: 6243608
Conc: 2.59 ng/ml

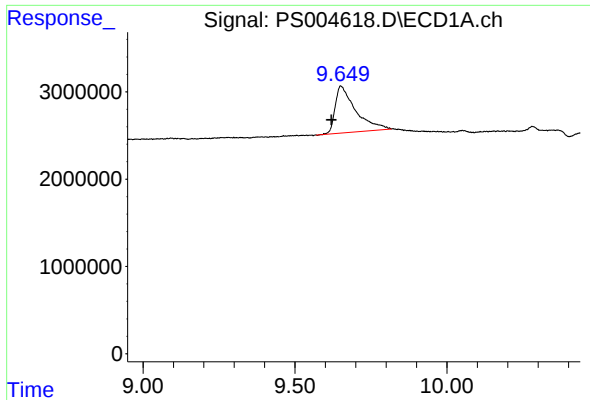

#15 Picloram

R.T.: 9.651 min
Delta R.T.: 0.031 min
Response: 25165430
Conc: 5.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

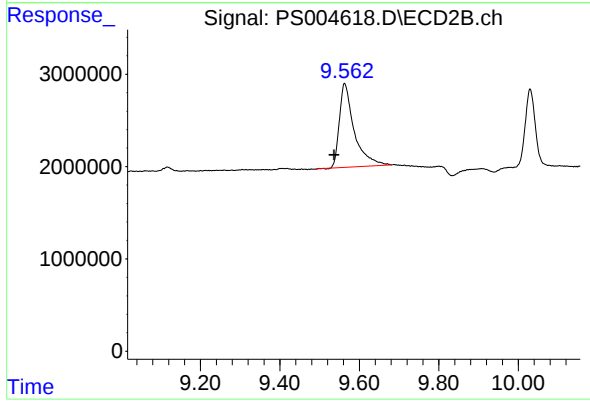

#15 Picloram

R.T.: 9.563 min
Delta R.T.: 0.027 min
Response: 23506399
Conc: 6.39 ng/ml