

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
 Data File : PS010304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2020 12:50
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 14:31:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.920	324.8E6	279.1E6	462.027	520.415
Target Compounds							
1) T	Dalapon	0.000	2.685	0	318549	N.D.	<MDL
3) T	4-Nitroph...	0.000	6.532	0	423606	N.D.	1.275
5) T	DICAMBA	0.000	7.091	0	2804724	N.D.	1.281
6) T	MCP	0.000	7.154	0	2844654	N.D.	1.550
8) T	DICHLORPROP	0.000	7.718	0	738022	N.D.	1.307
9) T	2,4-D	0.000	8.013	0	1826036	N.D.	2.633
10) T	Pentachlo...	0.000	8.441	0	483729	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	2960468	N.D.	1.022
12) T	2,4,5-T	0.000	9.183	0	5839039	N.D.	2.008
13) T	2,4-DB	0.000	9.692	0	1238699	N.D.	3.108
14) T	DINOSEB	0.000	10.023	0	1546314	N.D.	<MDL
15) T	Picloram	11.032	11.005	63849839	73588003	13.926	17.430 #
16) T	DCPA	0.000	10.951	0	4676575	N.D.	1.308



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
Data File : PS010304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2020 12:50
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 14:31:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

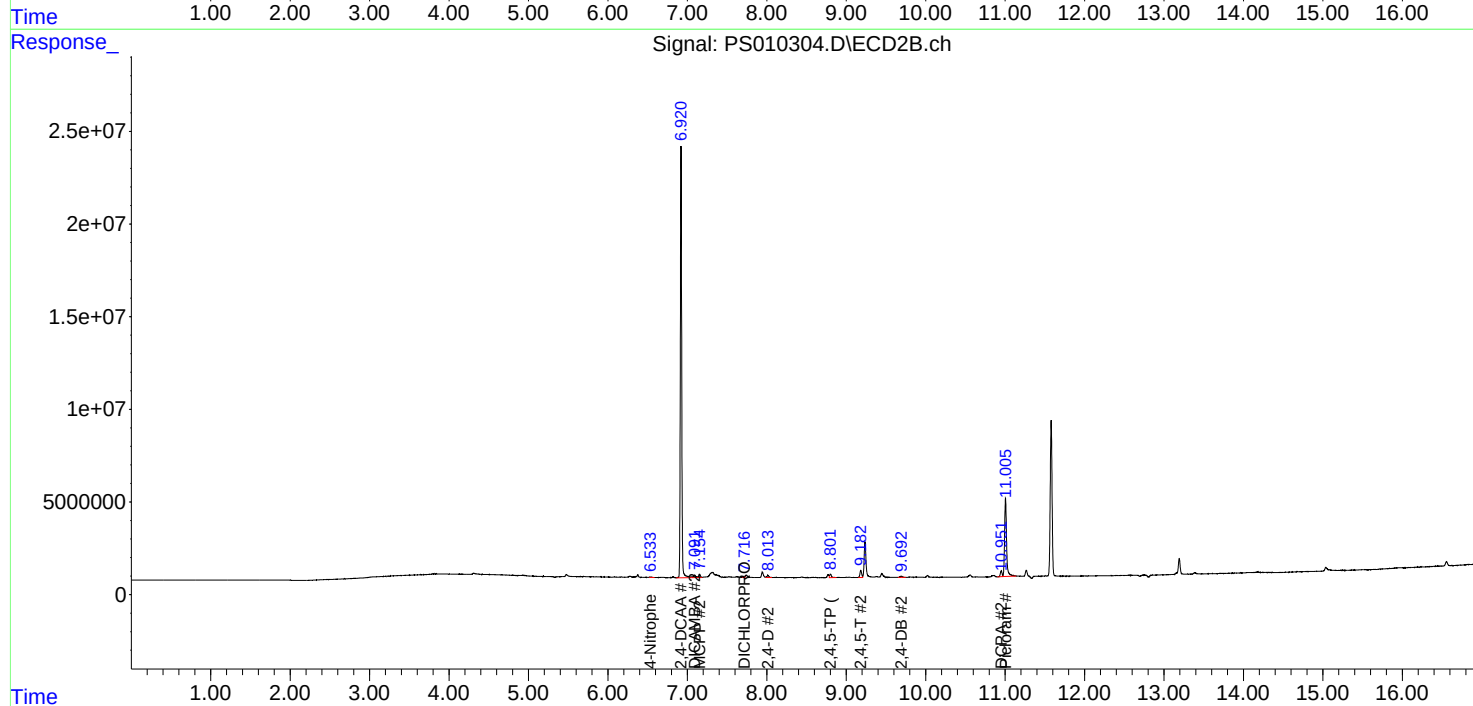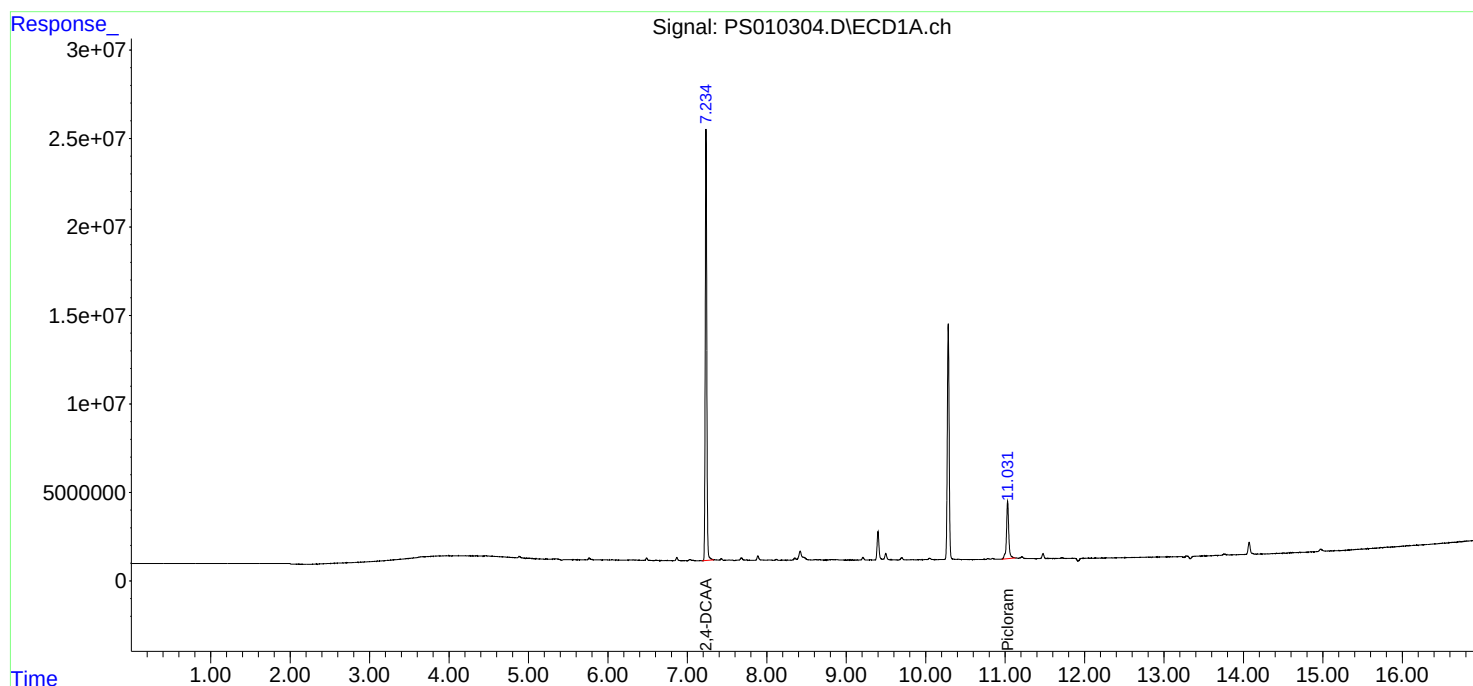


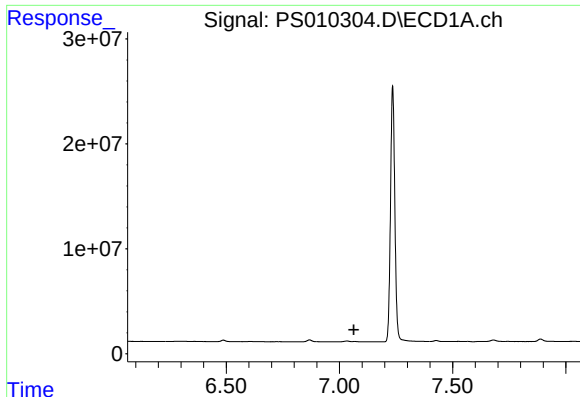

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.064 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

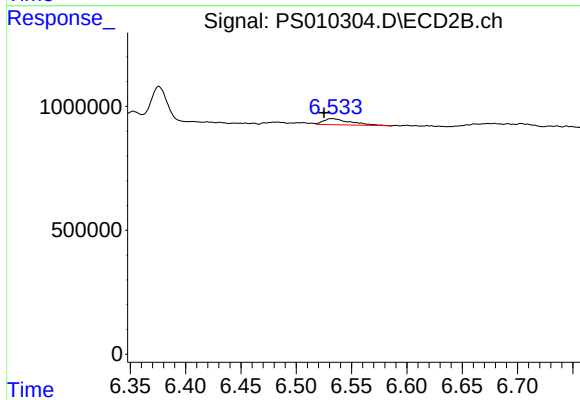


#3 4-Nitrophenol

R.T.: 6.532 min
Delta R.T.: 0.007 min
Response: 423606
Conc: 1.27 ng/ml

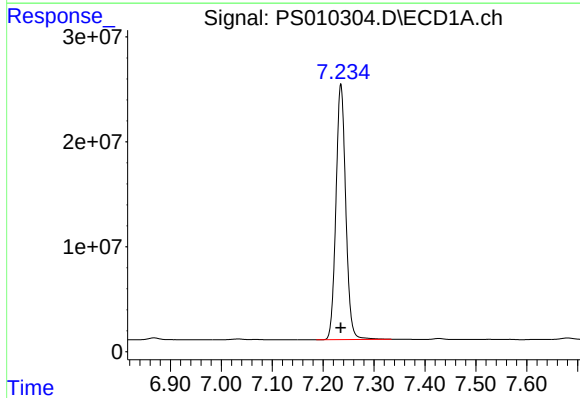


#4 2,4-DCAA

R.T.: 7.235 min
Delta R.T.: 0.000 min
Response: 324848880
Conc: 462.03 ng/ml

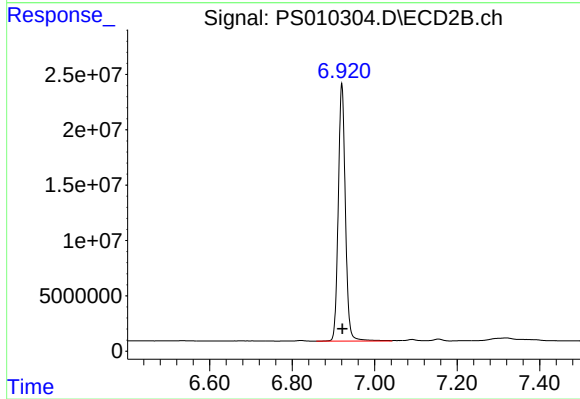

#4 2,4-DCAA


R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 279094102
Conc: 520.42 ng/ml

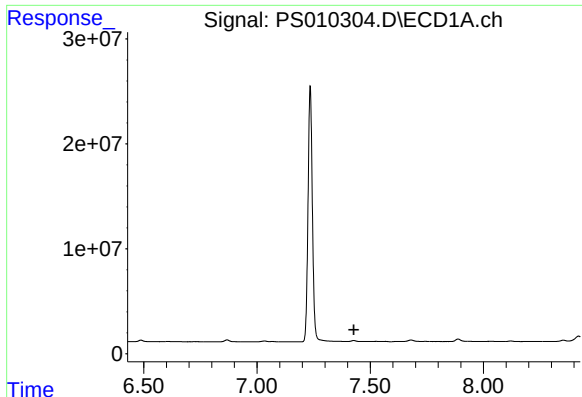

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.428 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

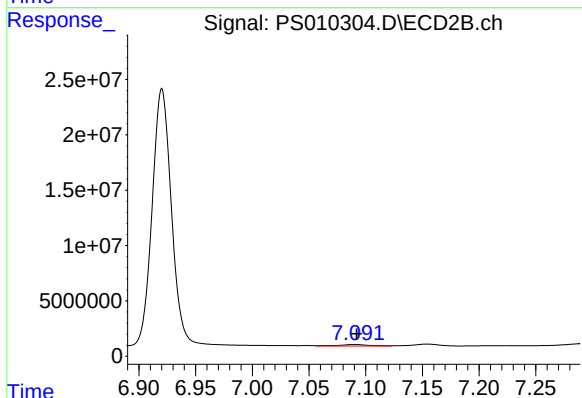


#5 DICAMBA

R.T.: 7.091 min
Delta R.T.: -0.001 min
Response: 2804724
Conc: 1.28 ng/ml

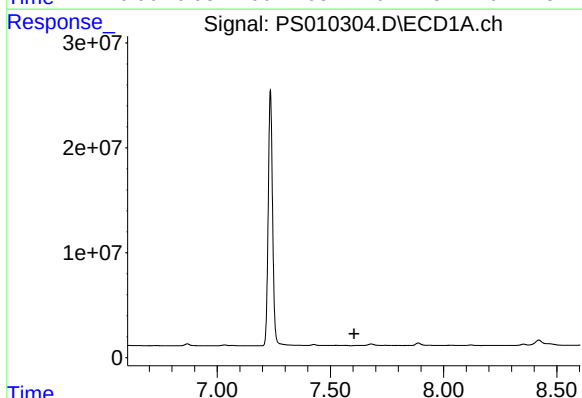


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

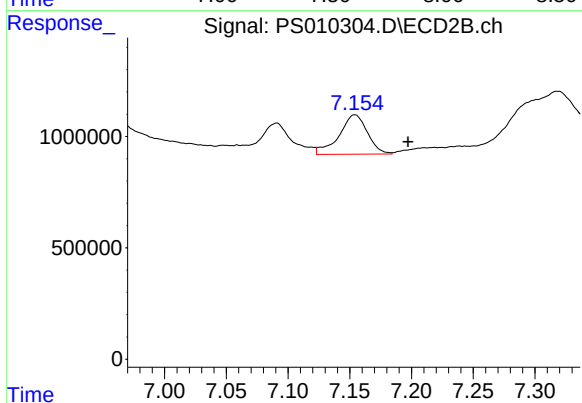

#6 MCPP


R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 2844654
Conc: 1.55 ug/ml

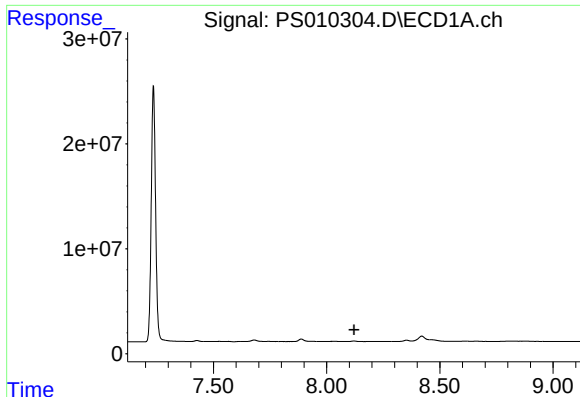

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

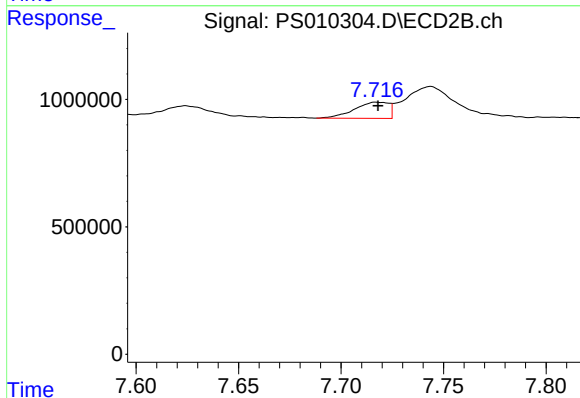


#8 DICHLORPROP

R.T.: 7.718 min
Delta R.T.: 0.000 min
Response: 738022
Conc: 1.31 ng/ml

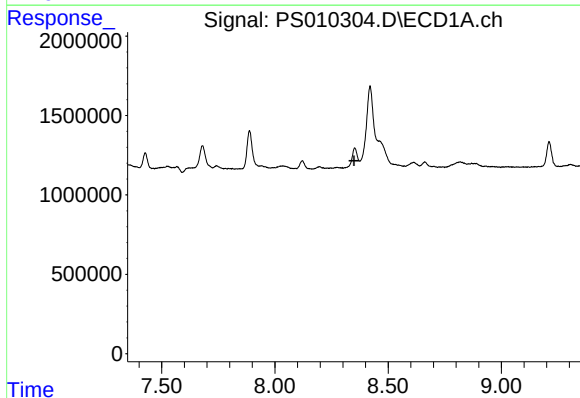


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

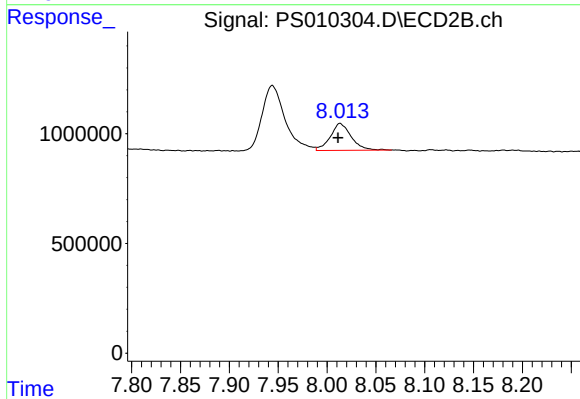

#9 2,4-D


R.T.: 8.013 min
Delta R.T.: 0.002 min
Response: 1826036
Conc: 2.63 ng/ml

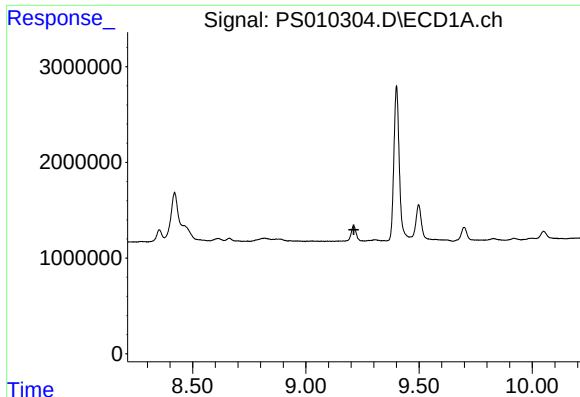

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

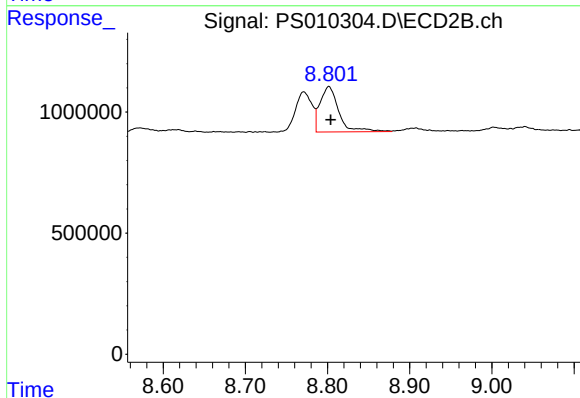


#11 2,4,5-TP (SILVEX)

R.T.: 8.802 min
Delta R.T.: -0.002 min
Response: 2960468
Conc: 1.02 ng/ml

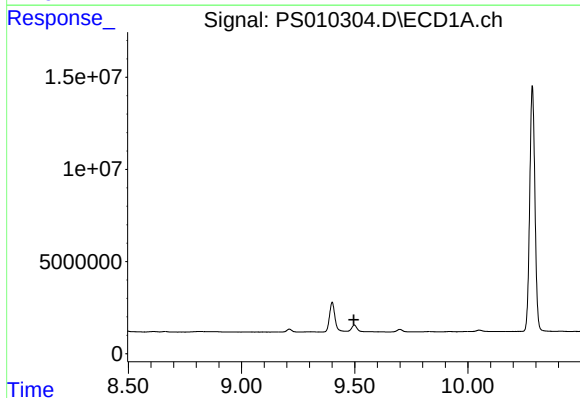


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.497 min
Response: 0
Conc: N.D.

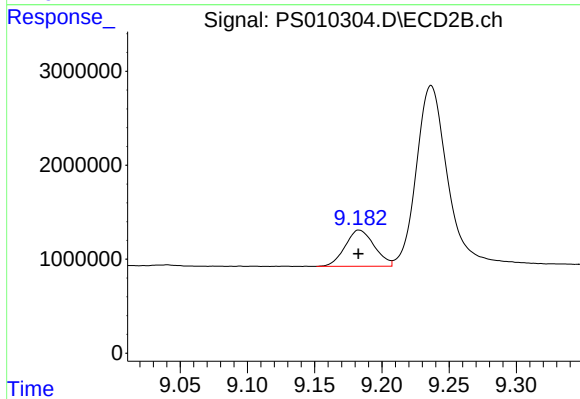

#12 2,4,5-T


R.T.: 9.183 min
Delta R.T.: 0.000 min
Response: 5839039
Conc: 2.01 ng/ml

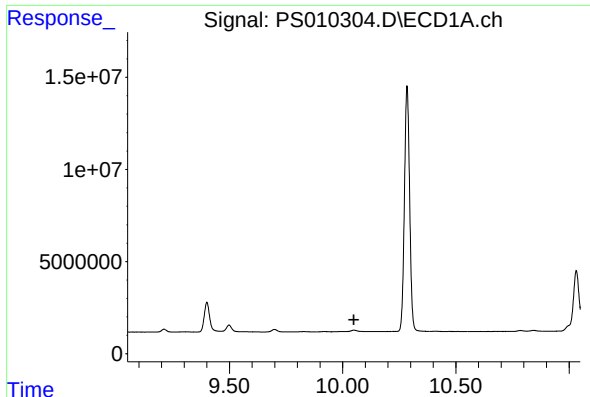

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

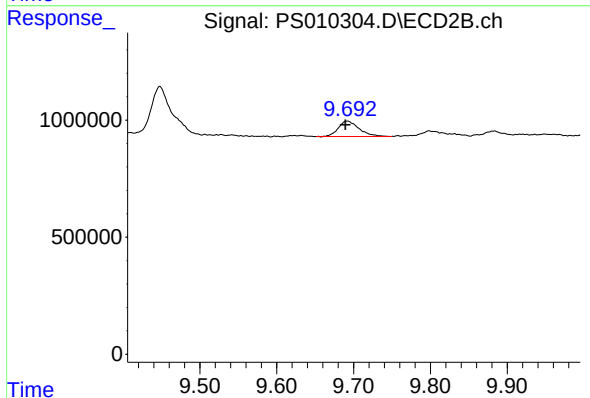


#13 2,4-DB

R.T.: 9.692 min
Delta R.T.: 0.003 min
Response: 1238699
Conc: 3.11 ng/ml

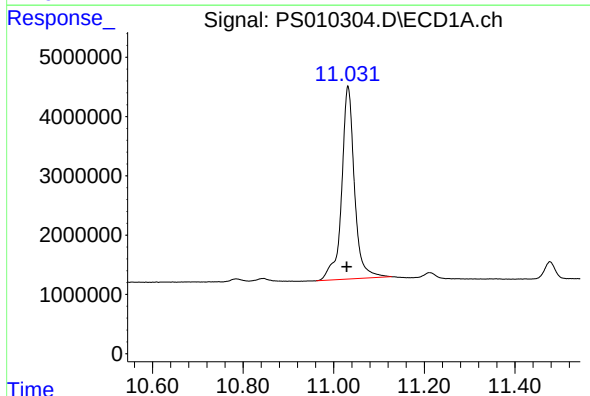


#15 Picloram

R.T.: 11.032 min
Delta R.T.: 0.002 min
Response: 63849839
Conc: 13.93 ng/ml

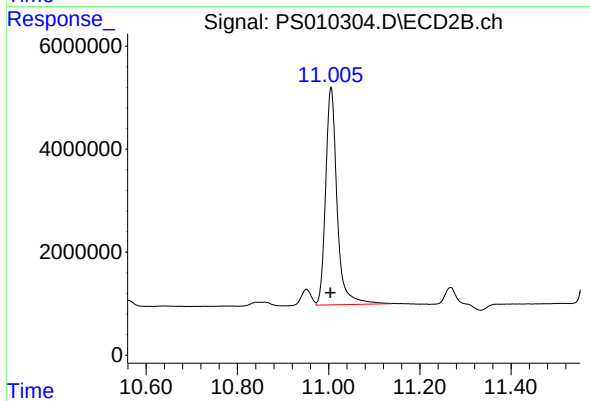

#15 Picloram


R.T.: 11.005 min
Delta R.T.: 0.002 min
Response: 73588003
Conc: 17.43 ng/ml

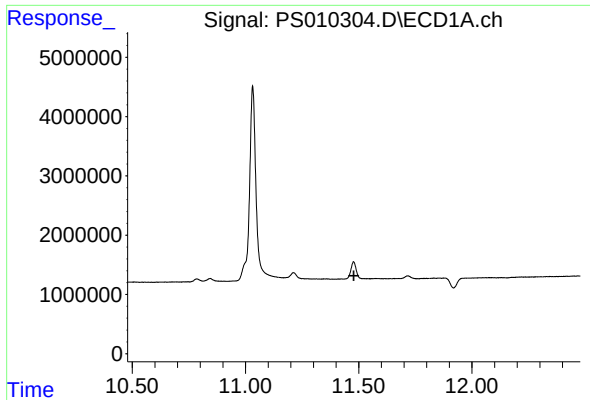

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

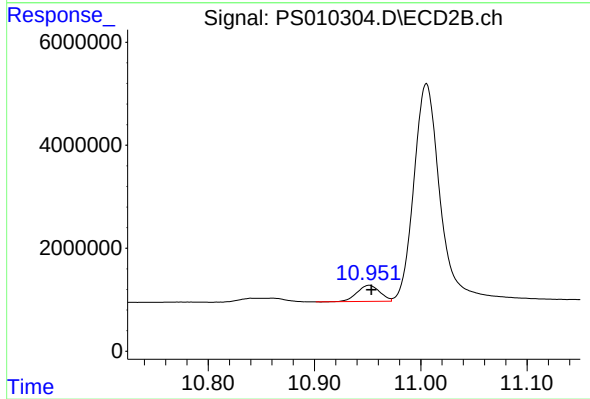

#16 DCPA

R.T.: 10.951 min
Delta R.T.: -0.002 min
Response: 4676575
Conc: 1.31 ng/ml