

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
 Data File : PS010308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2020 15:29
 Operator : DD\AJ
 Sample : PB128857TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 23:06:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.237	6.919	310.9E6	282.2E6	442.184	526.254
Target Compounds							
5) T	DICAMBA	0.000	7.084	0	6309603	N.D.	2.882
6) T	MCPD	0.000	7.200	0	5142872	N.D.	2.802
8) T	DICHLORPROP	0.000	7.740	0	744124	N.D.	1.318
11) T	2,4,5-TP ...	0.000	8.802	0	375584	N.D.	<MDL
12) T	2,4,5-T	0.000	9.179	0	1407578	N.D.	<MDL
13) T	2,4-DB	0.000	9.706	0	342128	N.D.	<MDL
14) T	DINOSEB	0.000	10.030	0	801413	N.D.	<MDL
15) T	Picloram	0.000	11.007	0	2299234	N.D.	<MDL
16) T	DCPA	0.000	10.953	0	1093652	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
Data File : PS010308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2020 15:29
Operator : DD\AJ
Sample : PB128857TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 23:06:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

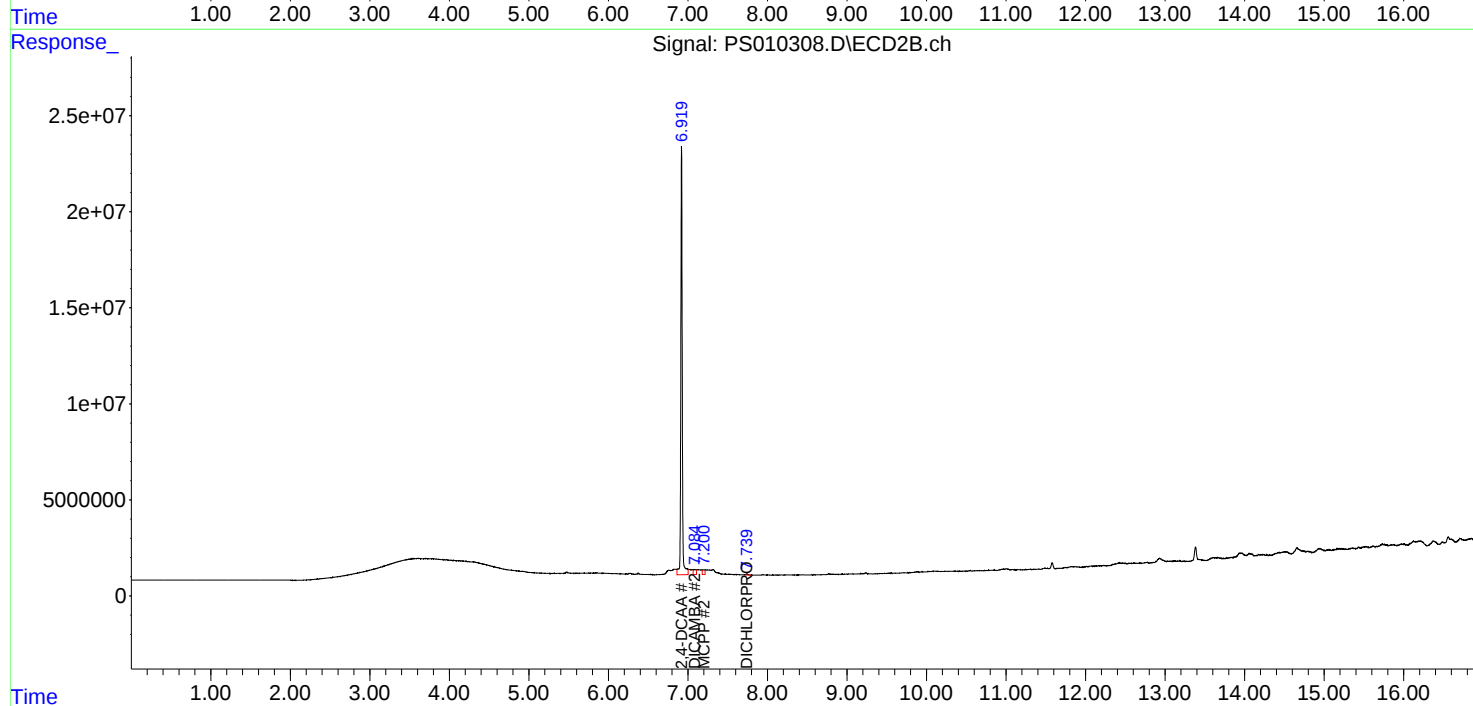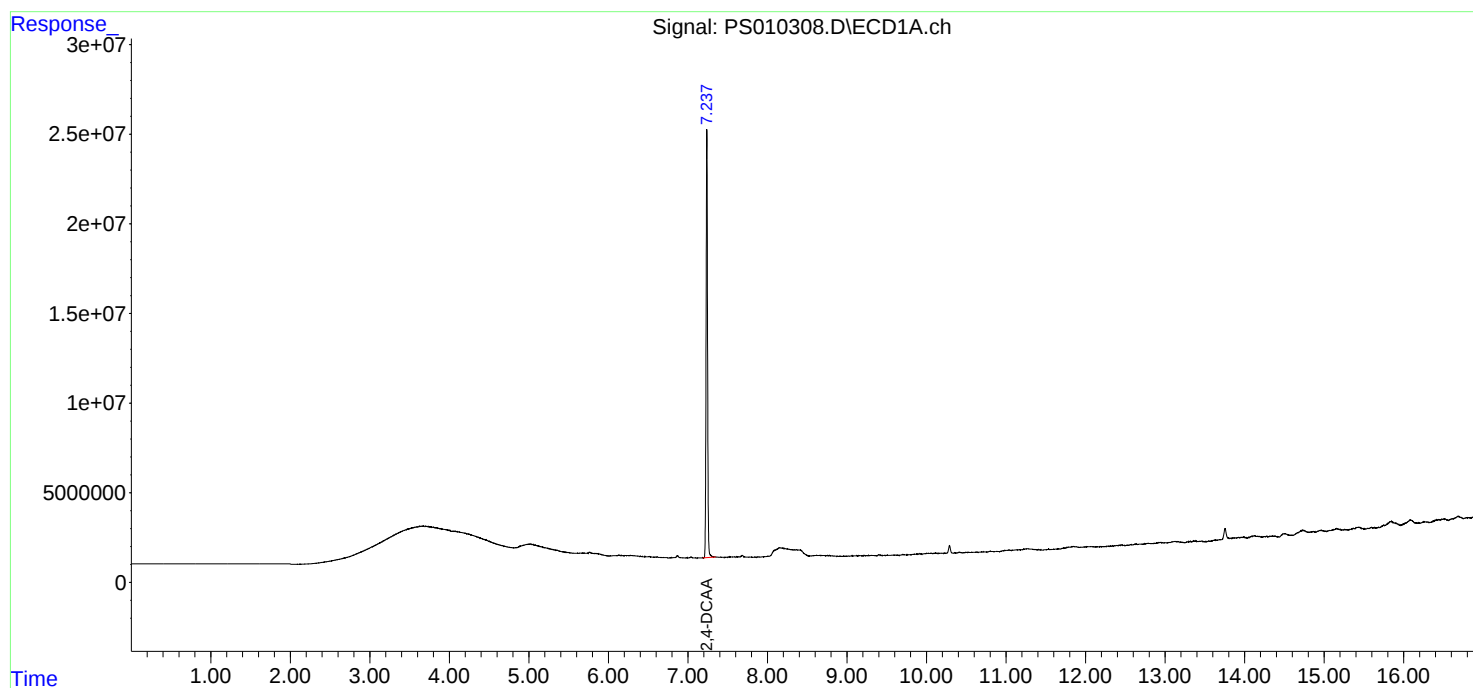


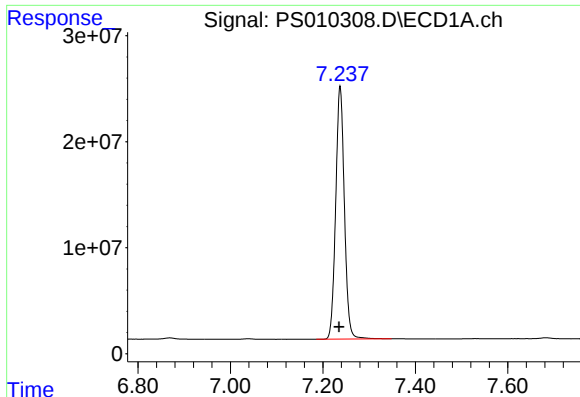

#4 2,4-DCAA


R.T.: 7.237 min
Delta R.T.: 0.003 min
Response: 310897267
Conc: 442.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

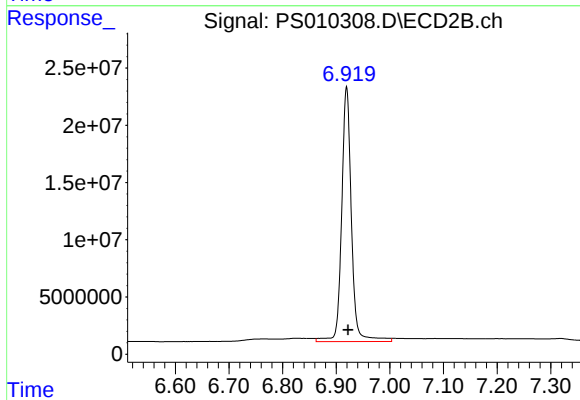


#4 2,4-DCAA

R.T.: 6.919 min
Delta R.T.: -0.002 min
Response: 282225262
Conc: 526.25 ng/ml

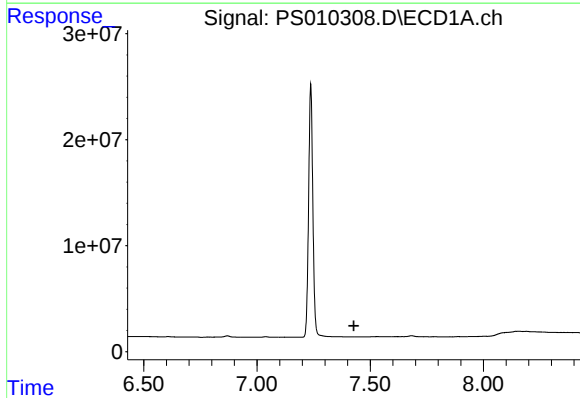


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

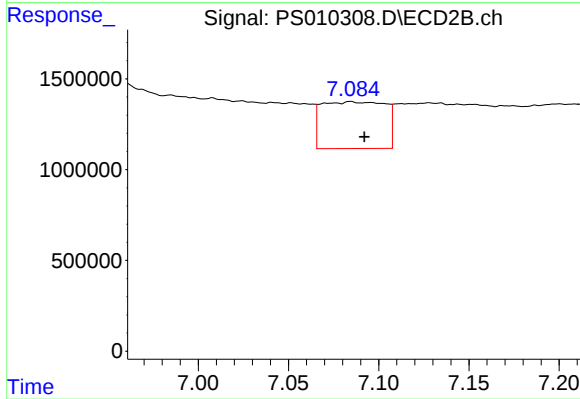

#5 DICAMBA


R.T.: 7.084 min
Delta R.T.: -0.008 min
Response: 6309603
Conc: 2.88 ng/ml

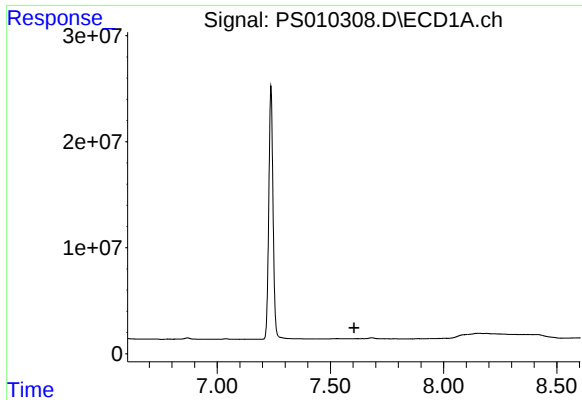

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

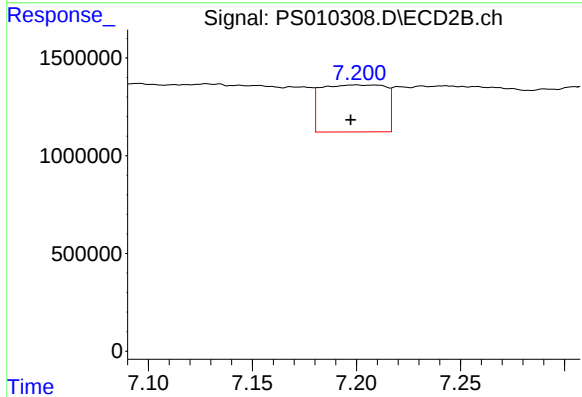


#6 MCP

R.T.: 7.200 min
Delta R.T.: 0.002 min
Response: 5142872
Conc: 2.80 ug/ml

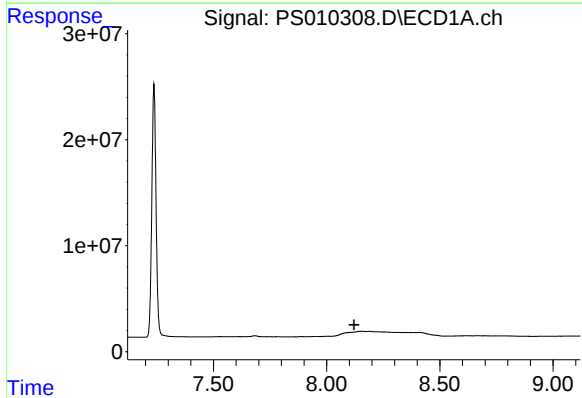

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

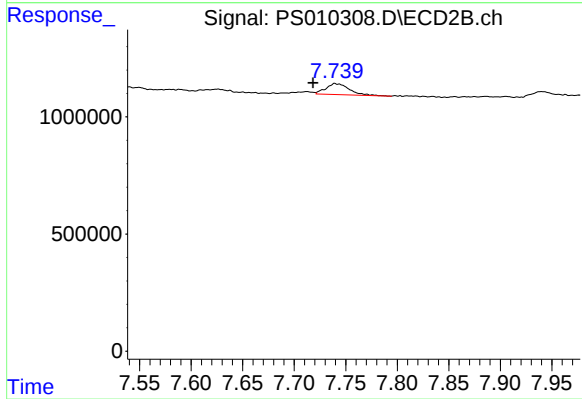

#8 DICHLORPROP

R.T.: 7.740 min
Delta R.T.: 0.022 min
Response: 744124
Conc: 1.32 ng/ml