

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
 Data File : PS010316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2020 18:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 23:08:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.921	336.5E6	289.5E6	478.650	539.781
Target Compounds							
2) T	3,5-DICHL...	0.000	6.101	0	331509	N.D.	<MDL
5) T	DICAMBA	0.000	7.092	0	2245462	N.D.	1.026
6) T	MCP	0.000	7.155	0	2898192	N.D.	1.579
8) T	DICHLORPROP	0.000	7.744	0	3356415	N.D.	5.945
9) T	2,4-D	8.418	7.944	17993359	476562	25.470	<MDL #
10) T	Pentachlo...	0.000	8.441	0	495538	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.801	0	1162263	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	676717	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	345759	N.D.	<MDL
14) T	DINOSEB	0.000	10.022	0	260983	N.D.	<MDL
15) T	Picloram	0.000	11.009	0	2060931	N.D.	<MDL
16) T	DCPA	0.000	10.952	0	791205	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051520\
Data File : PS010316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2020 18:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 23:08:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

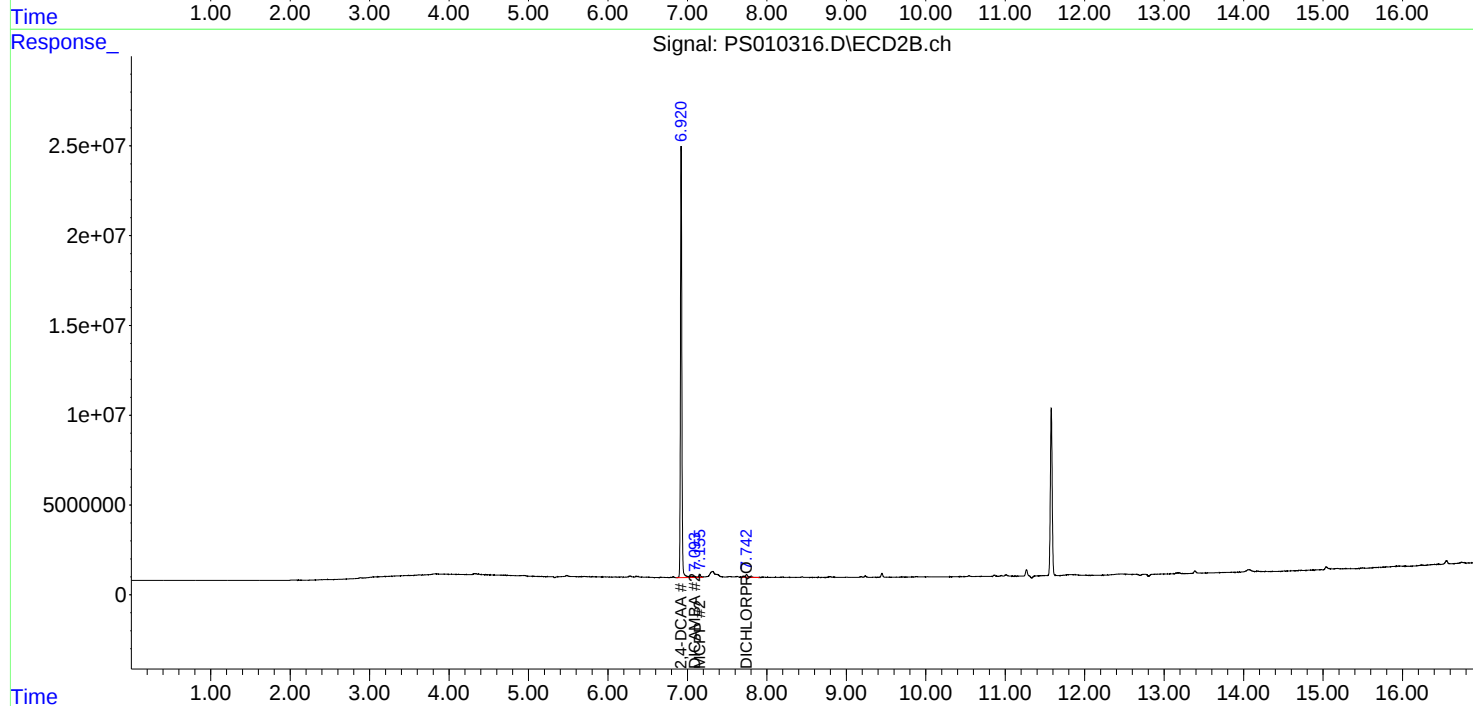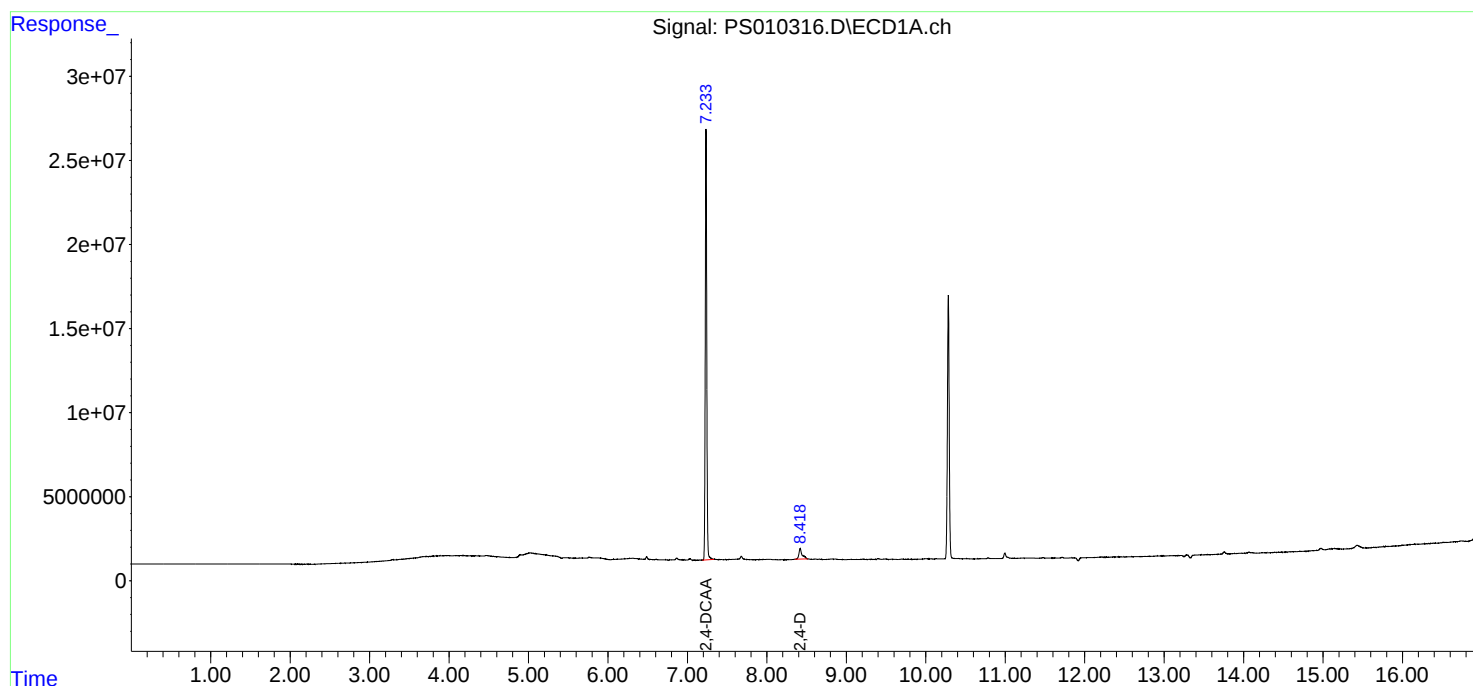


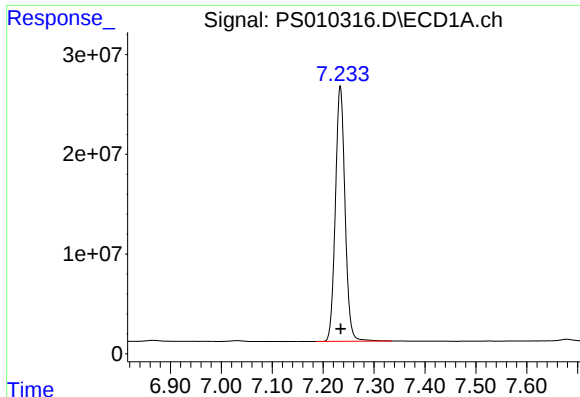

#4 2,4-DCAA


R.T.: 7.234 min
Delta R.T.: -0.001 min
Response: 336536548
Conc: 478.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

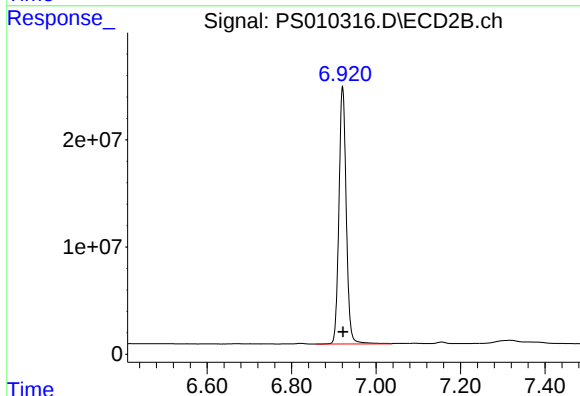


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 289479563
Conc: 539.78 ng/ml

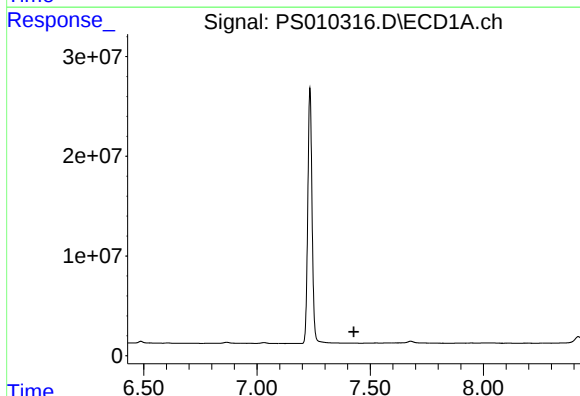


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

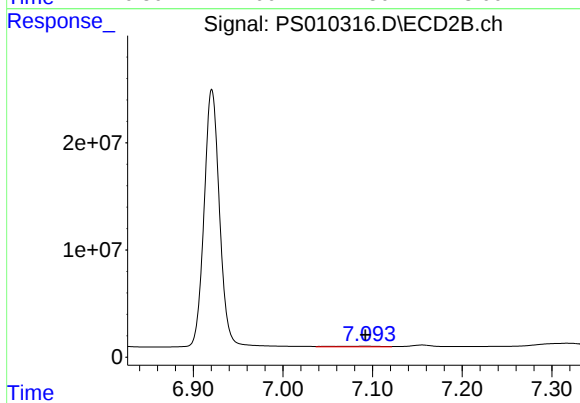

#5 DICAMBA


R.T.: 7.092 min
Delta R.T.: 0.000 min
Response: 2245462
Conc: 1.03 ng/ml

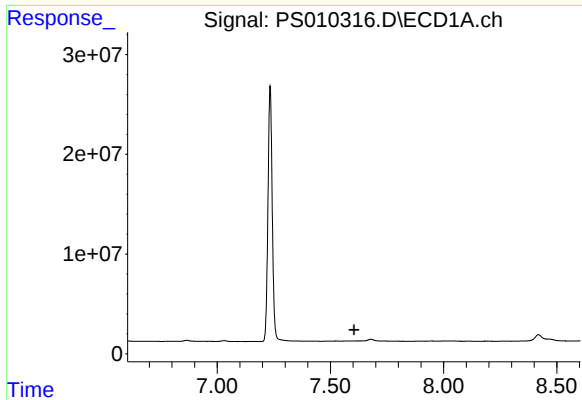

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

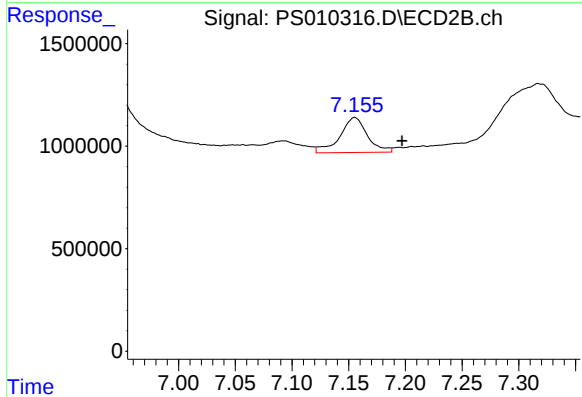


#6 MCP

R.T.: 7.155 min
Delta R.T.: -0.042 min
Response: 2898192
Conc: 1.58 ug/ml

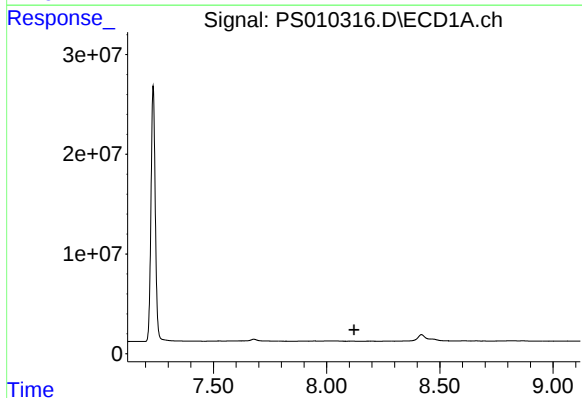


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

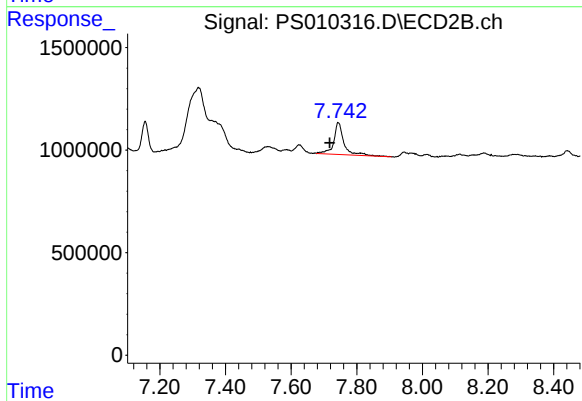

#8 DICHLORPROP


R.T.: 7.744 min
Delta R.T.: 0.026 min
Response: 3356415
Conc: 5.95 ng/ml

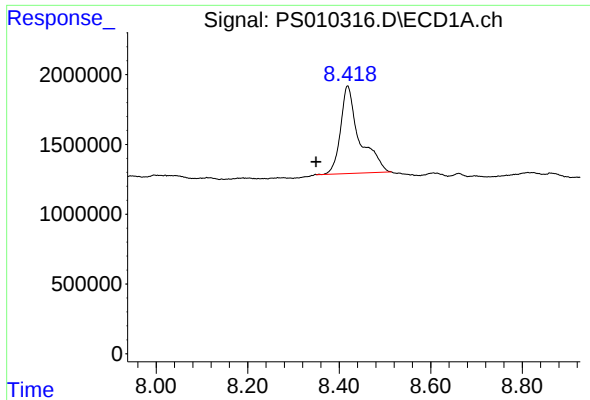

#9 2,4-D

R.T.: 8.418 min
Delta R.T.: 0.069 min
Response: 17993359
Conc: 25.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

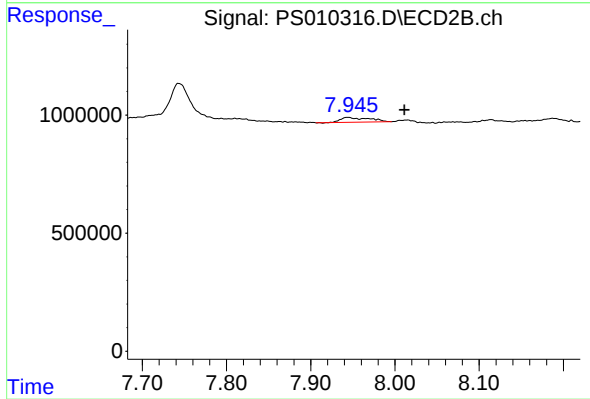

#9 2,4-D

R.T.: 7.944 min
Delta R.T.: -0.067 min
Response: 476562
Conc: N.D.