

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
 Data File : PS004621.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 08:40
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:02:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.031	5.711	333.9E6	254.4E6	469.843	506.096
Target Compounds							
7) T	MCPA	0.000	6.045	0	39105337	N.D.	19.134
9) T	2,4-D	7.117	0.000	44820598	0	61.516	N.D. #
15) T	Picloram	0.000	9.552	0	10284167	N.D.	2.796
16) T	DCPA	0.000	9.552	0	10284167	N.D.	3.015



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
Data File : PS004621.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 08:40
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:02:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

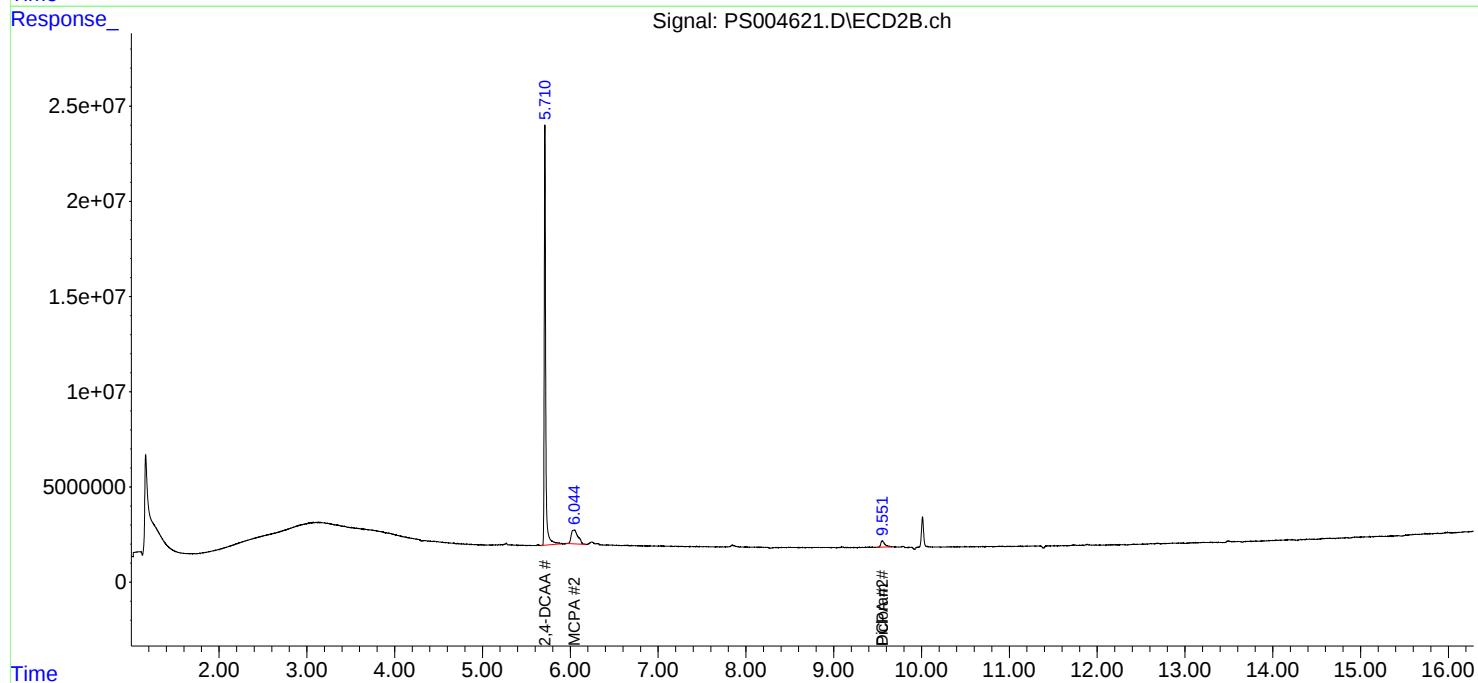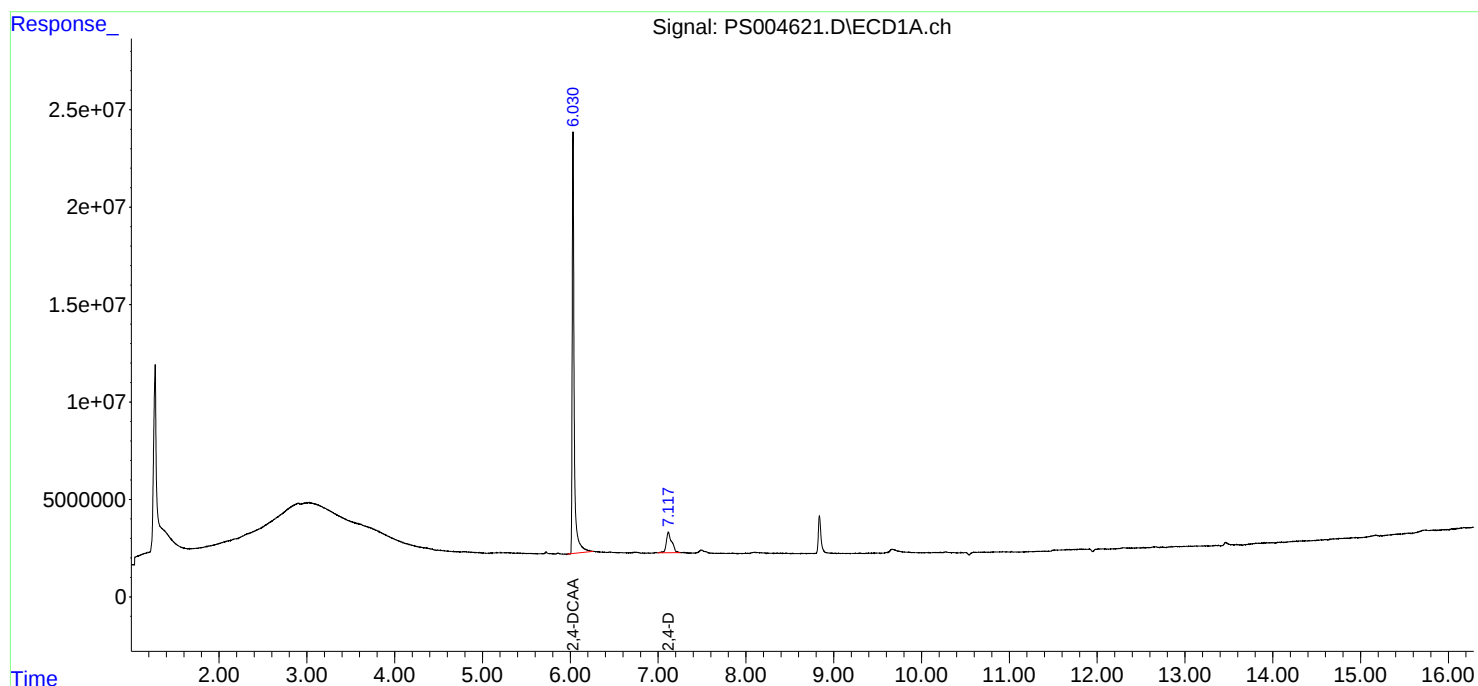


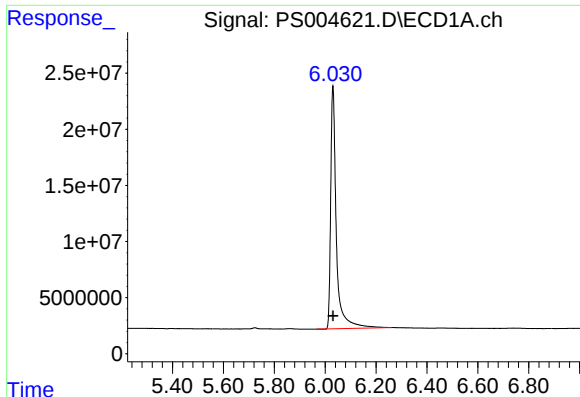

#4 2,4-DCAA


R.T.: 6.031 min
Delta R.T.: 0.000 min
Response: 333930565
Conc: 469.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

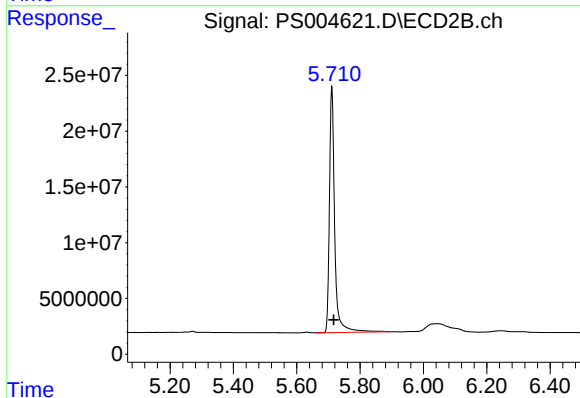


#4 2,4-DCAA

R.T.: 5.711 min
Delta R.T.: -0.006 min
Response: 254407371
Conc: 506.10 ng/ml

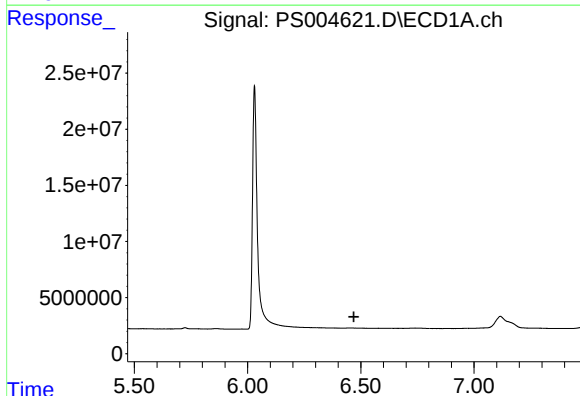


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 6.469 min
Response: 0
Conc: N.D.

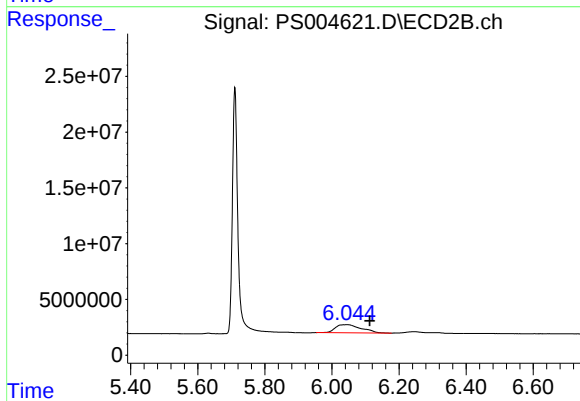

#7 MCPA


R.T.: 6.045 min
Delta R.T.: -0.068 min
Response: 39105337
Conc: 19.13 ug/ml

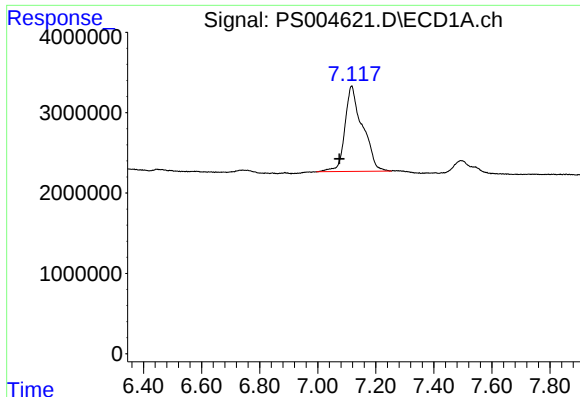

#9 2,4-D


R.T.: 7.117 min
Delta R.T.: 0.042 min
Response: 44820598
Conc: 61.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

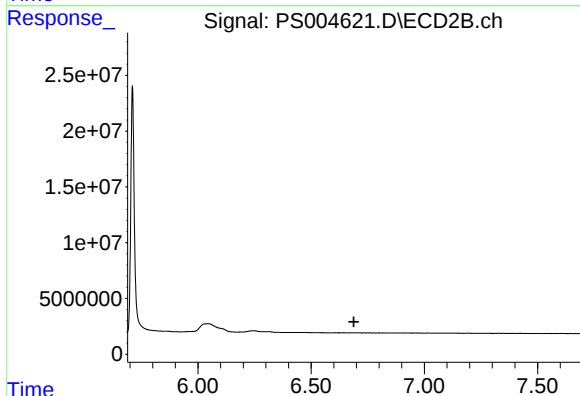


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

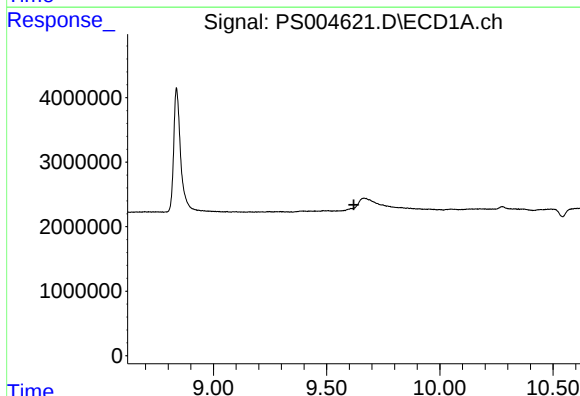


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.620 min
Response: 0
Conc: N.D.

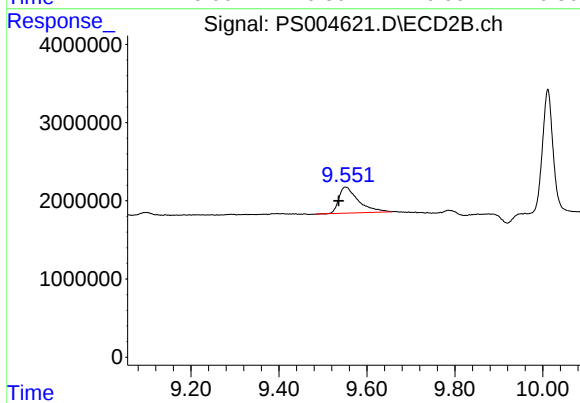

#15 Picloram


R.T.: 9.552 min
Delta R.T.: 0.016 min
Response: 10284167
Conc: 2.80 ng/ml

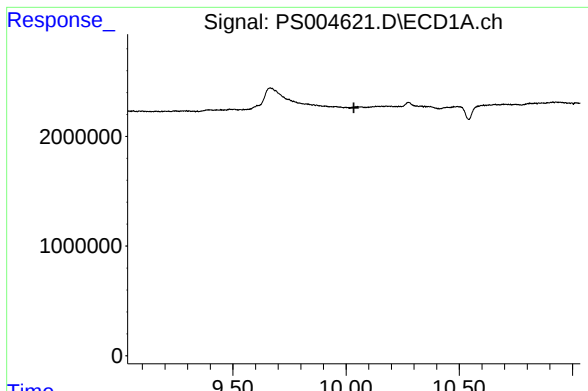

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

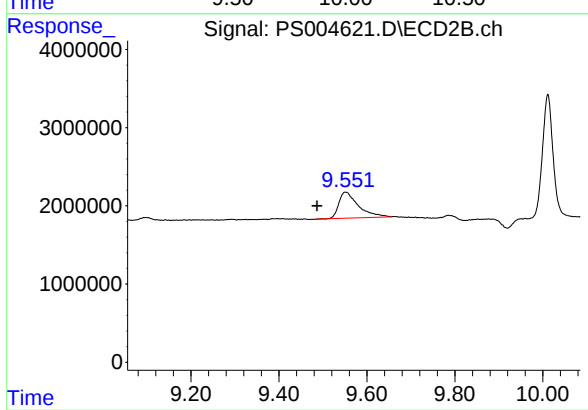

#16 DCPA

R.T.: 9.552 min
Delta R.T.: 0.065 min
Response: 10284167
Conc: 3.02 ng/ml