

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
 Data File : PS004635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 22:41
 Operator : EI\SJ
 Sample : K2637-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:06:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.012	5.714	85742059	67373323	120.640	134.027
Target Compounds							
1) T	Dalapon	2.382	2.051	56490802	100.3E6	59.789	143.105 #
2) T	3,5-DICHL...	5.425	4.985	3381018	7819341	3.992	11.886 #
3) T	4-Nitroph...	0.000	5.374	0	19037439	N.D.	86.104
5) T	DICAMBA	6.234	5.820	9146028	5611383	3.422	2.863
6) T	MCP	6.368	0.000	4018202	0	2.069	N.D. #
7) T	MCPA	0.000	6.049	0	41440220	N.D.	20.277
8) T	DICHLORPROP	0.000	6.406	0	3532902	N.D.	7.291
9) T	2,4-D	7.100	0.000	50249286	0	68.967	N.D. #
10) T	Pentachlo...	7.380	0.000	3942199	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	7.372	0	54332765	N.D.	20.282



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
Data File : PS004635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 22:41
Operator : EI\SJ
Sample : K2637-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:06:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

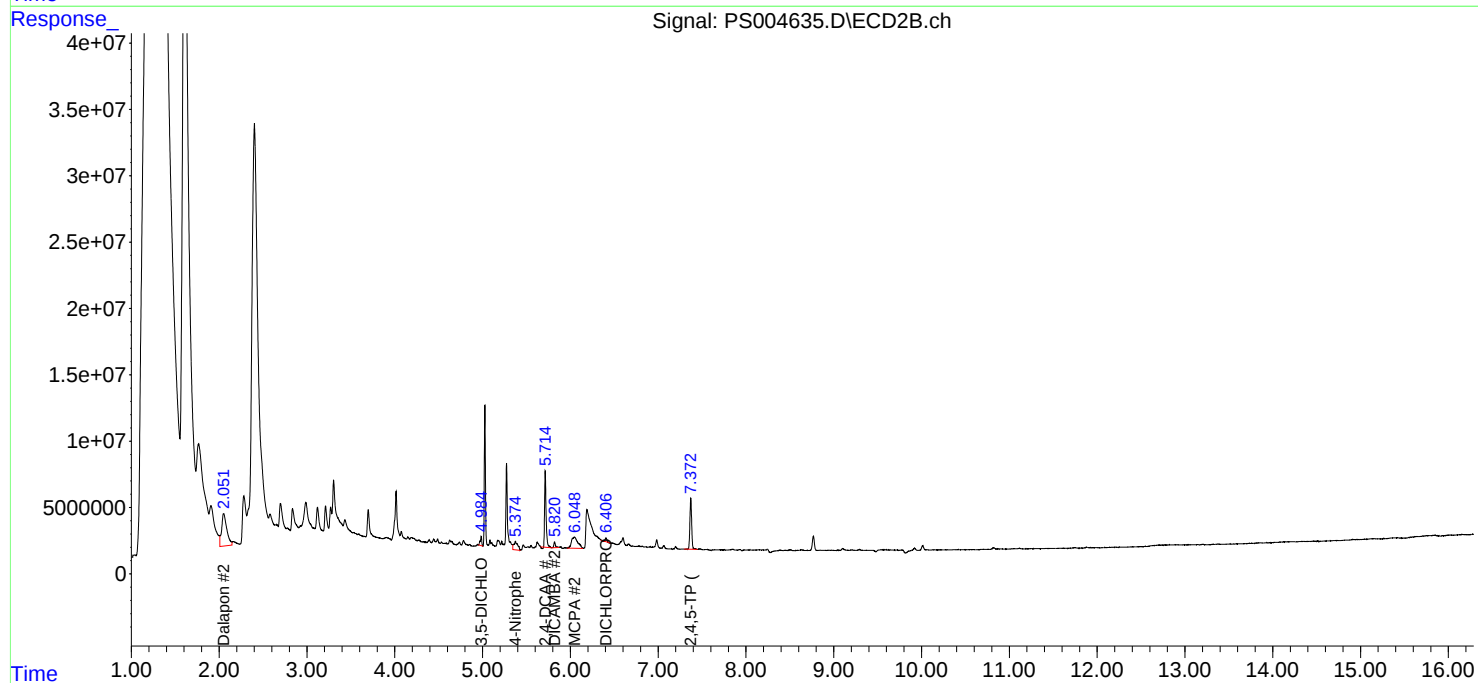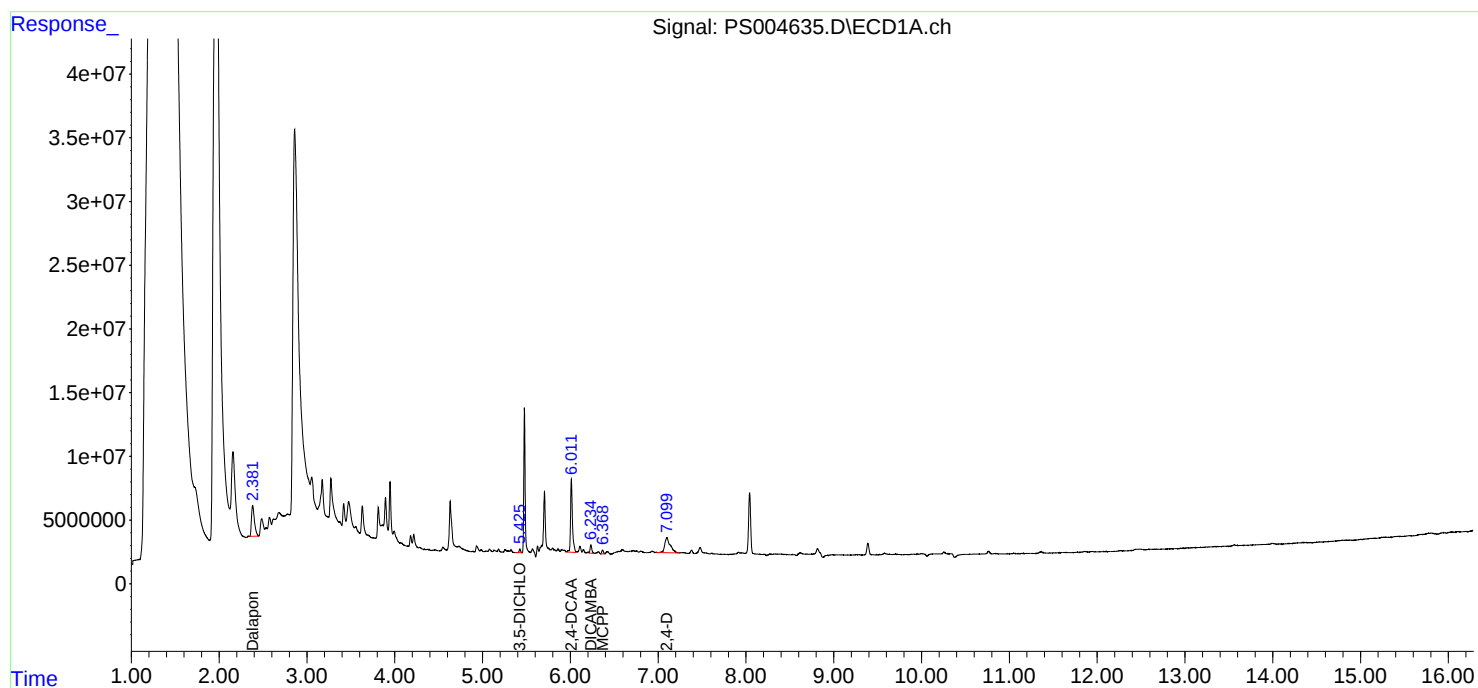


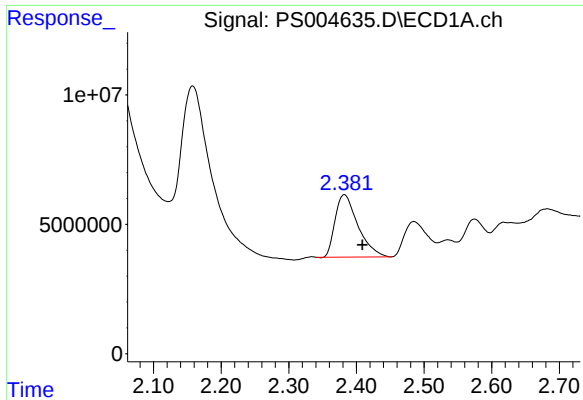

#1 Dalapon


R.T.: 2.382 min
Delta R.T.: -0.027 min
Response: 56490802
Conc: 59.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

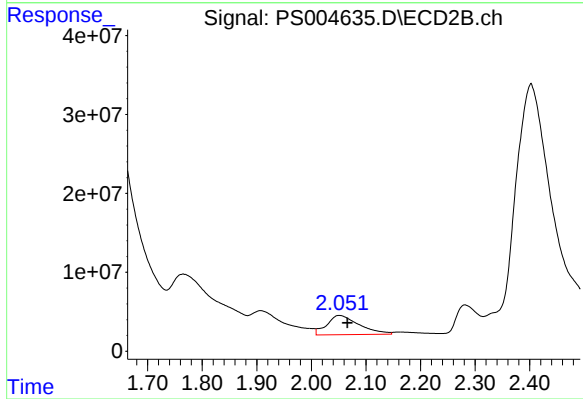


#1 Dalapon

R.T.: 2.051 min
Delta R.T.: -0.015 min
Response: 100316097
Conc: 143.10 ng/ml

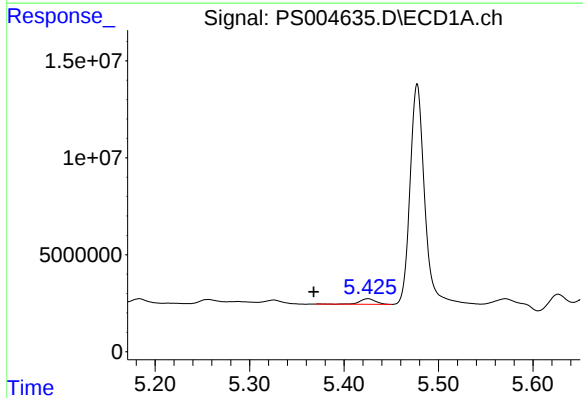


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.425 min
Delta R.T.: 0.057 min
Response: 3381018
Conc: 3.99 ng/ml

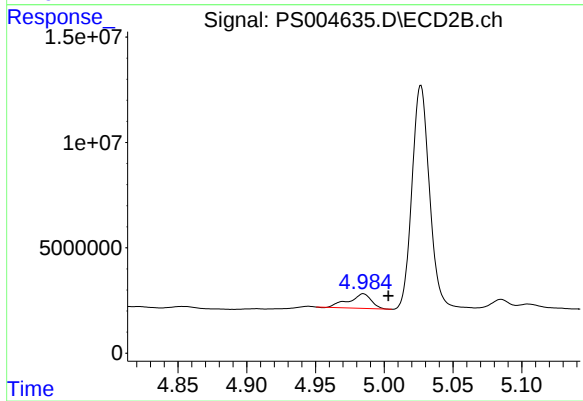

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.985 min
Delta R.T.: -0.018 min
Response: 7819341
Conc: 11.89 ng/ml

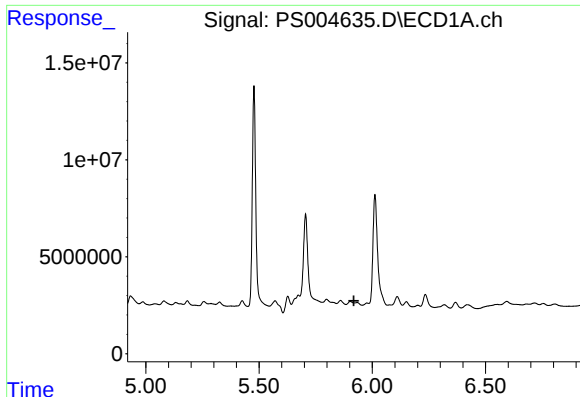

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

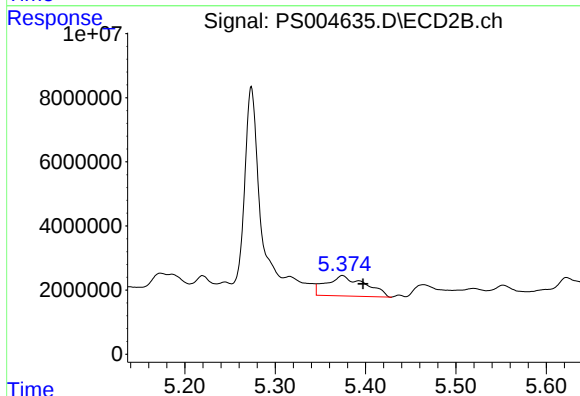


#3 4-Nitrophenol

R.T.: 5.374 min
Delta R.T.: -0.023 min
Response: 19037439
Conc: 86.10 ng/ml

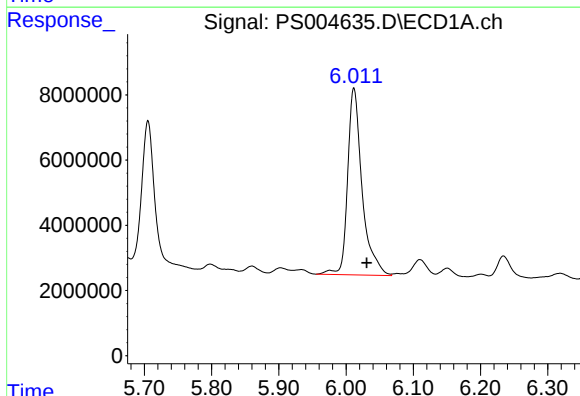


#4 2,4-DCAA

R.T.: 6.012 min
Delta R.T.: -0.019 min
Response: 85742059
Conc: 120.64 ng/ml

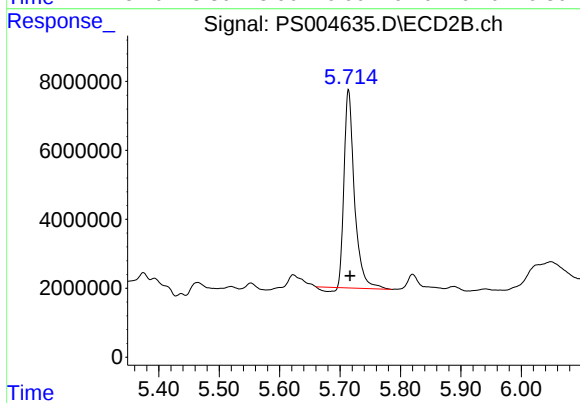

#4 2,4-DCAA


R.T.: 5.714 min
Delta R.T.: -0.002 min
Response: 67373323
Conc: 134.03 ng/ml

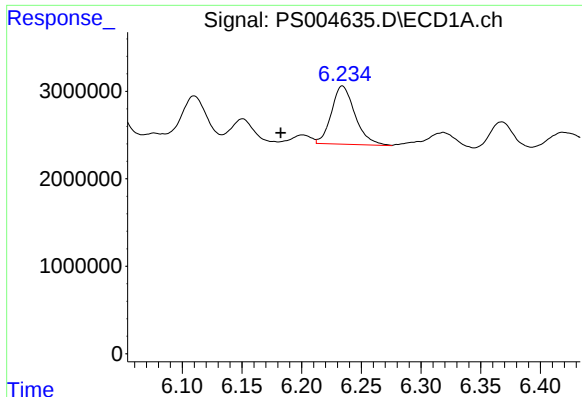

#5 DICAMBA


R.T.: 6.234 min
Delta R.T.: 0.052 min
Response: 9146028
Conc: 3.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

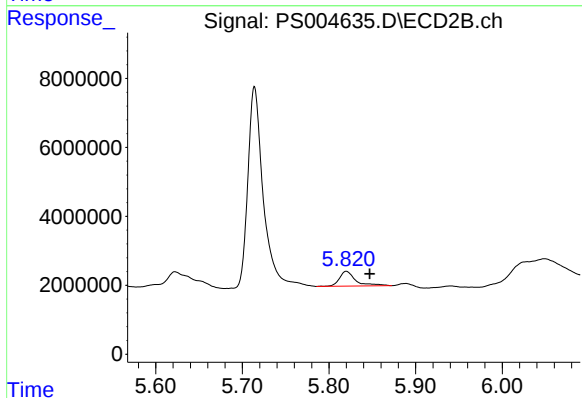


#5 DICAMBA

R.T.: 5.820 min
Delta R.T.: -0.027 min
Response: 5611383
Conc: 2.86 ng/ml

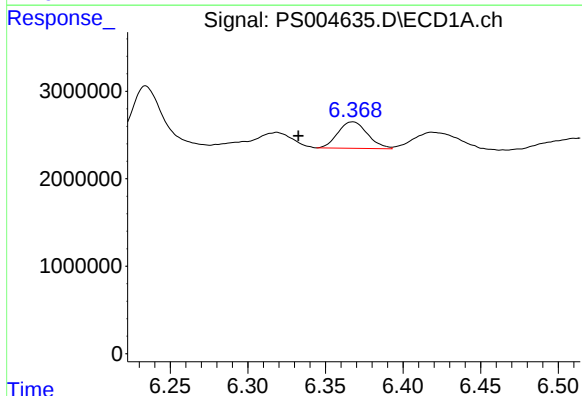


#6 MCP

R.T.: 6.368 min
Delta R.T.: 0.035 min
Response: 4018202
Conc: 2.07 ug/ml

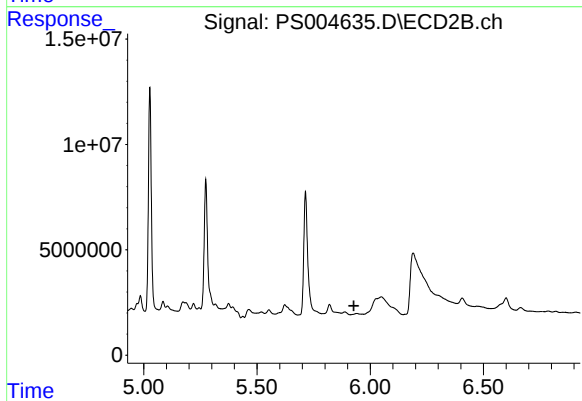

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.928 min
Response: 0
Conc: N.D.

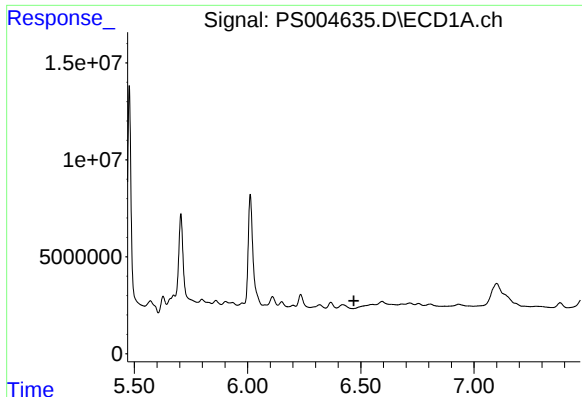

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.469 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

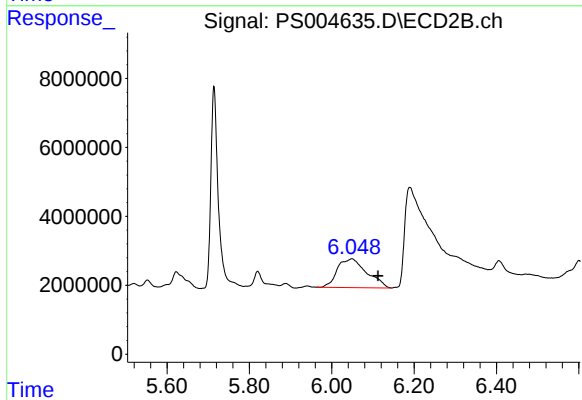


#7 MCPA

R.T.: 6.049 min
Delta R.T.: -0.064 min
Response: 41440220
Conc: 20.28 ug/ml

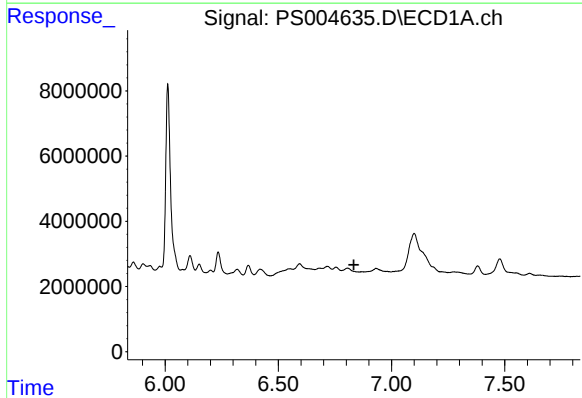


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.834 min
Response: 0
Conc: N.D.

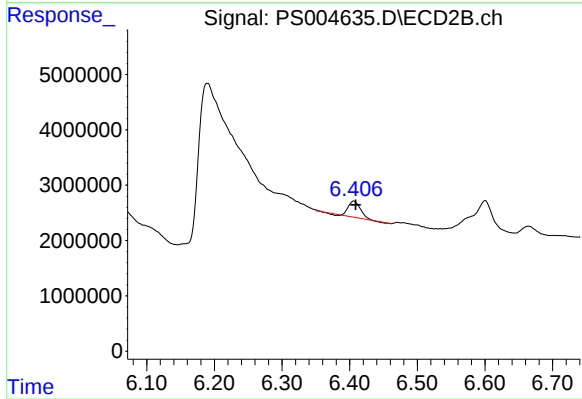

#8 DICHLORPROP


R.T.: 6.406 min
Delta R.T.: -0.003 min
Response: 3532902
Conc: 7.29 ng/ml

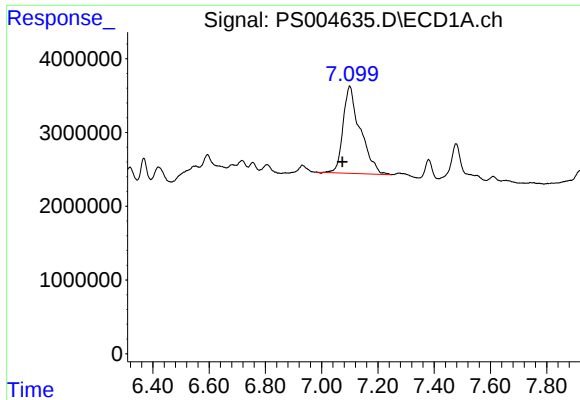

#9 2,4-D


R.T.: 7.100 min
Delta R.T.: 0.026 min
Response: 50249286
Conc: 68.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

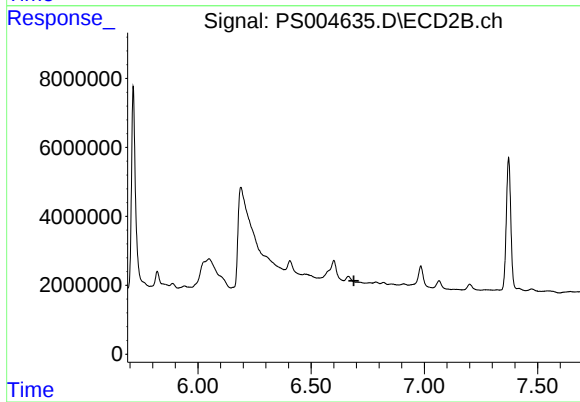


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

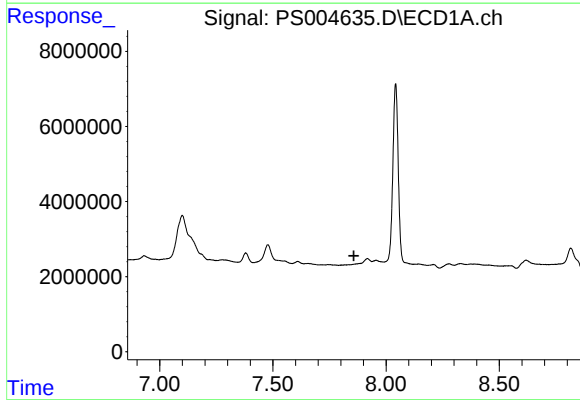

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.858 min
Response: 0
Conc: N.D.

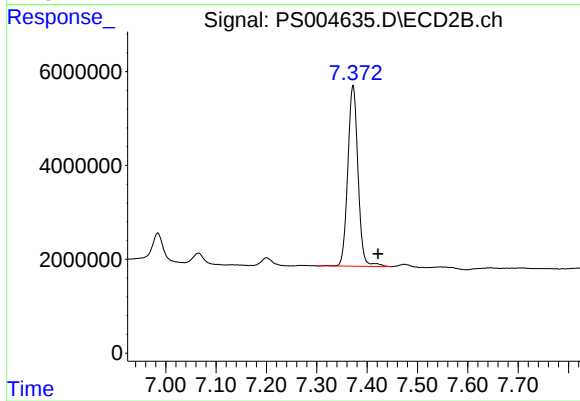

#11 2,4,5-TP (SILVEX)

R.T.: 7.372 min
Delta R.T.: -0.050 min
Response: 54332765
Conc: 20.28 ng/ml