

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
 Data File : PS004636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2019 23:11
 Operator : EI\SJ
 Sample : K2644-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:07:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.997	5.694	78259159	64610544	110.111	128.531
Target Compounds							
1) T	Dalapon	2.366	2.033	56360655	121.4E6	59.651	173.185 #
2) T	3,5-DICHL...	0.000	5.007	0	83483070	N.D.	126.903
3) T	4-Nitroph...	0.000	5.355	0	17207620	N.D.	77.828
5) T	DICAMBA	6.218	5.800	9006804	4655892	3.370	2.375 #
6) T	MCPD	6.351	0.000	3351857	0	1.726	N.D. #
7) T	MCPA	6.530	6.161	17441577	207.4E6	6.208	101.497 #
8) T	DICHLORPROP	0.000	6.385	0	4112356	N.D.	8.487
9) T	2,4-D	7.081	0.000	58141976	0	79.800	N.D. #
10) T	Pentachlo...	7.365	7.043	4905768	3553126	<MDL	<MDL #
11) T	2,4,5-TP ...	7.899	0.000	5725036	0	1.570	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
Data File : PS004636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2019 23:11
Operator : EI\SJ
Sample : K2644-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:07:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

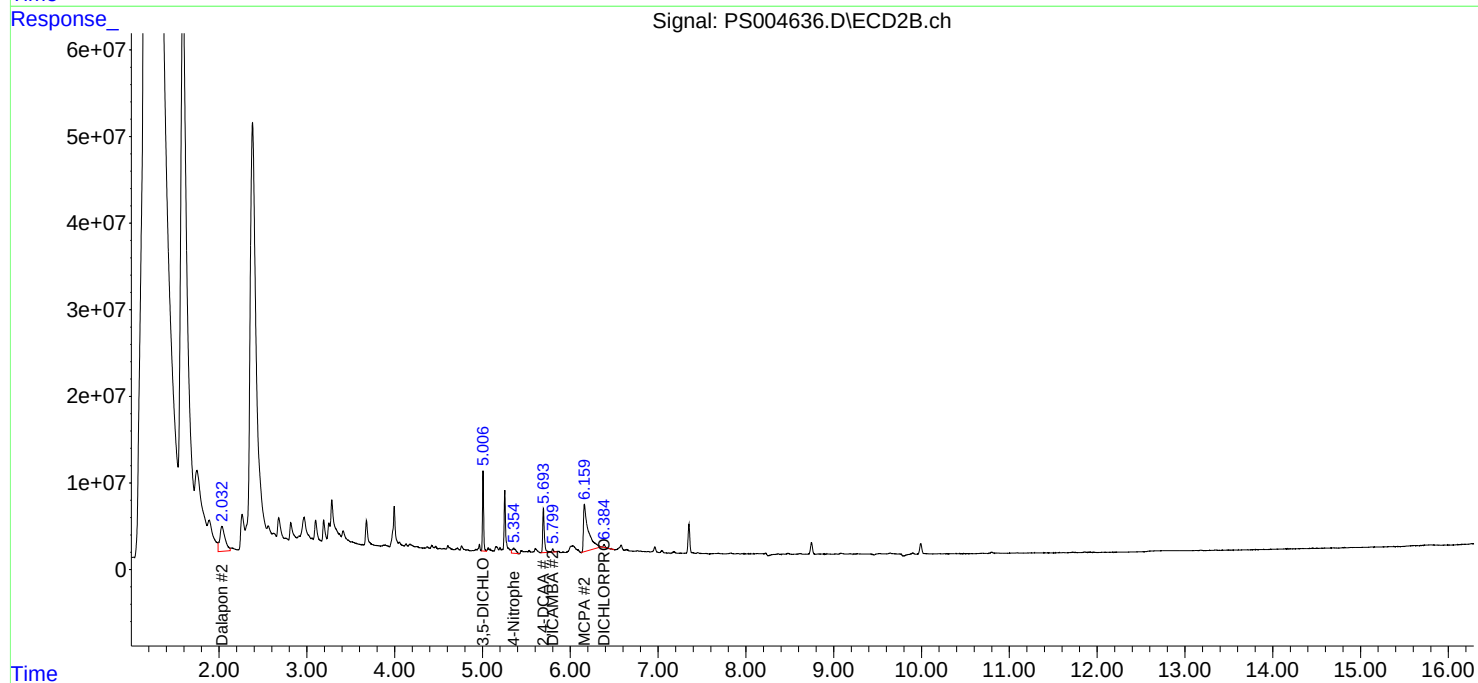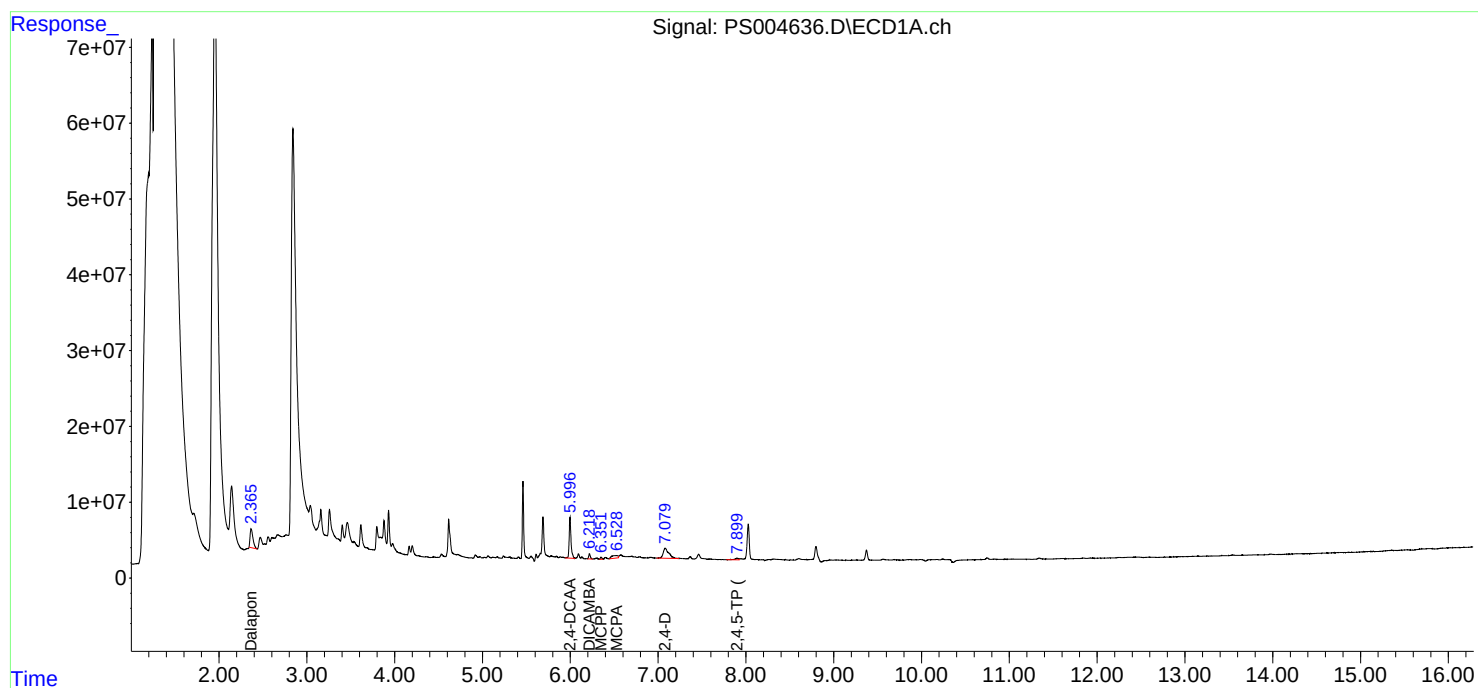


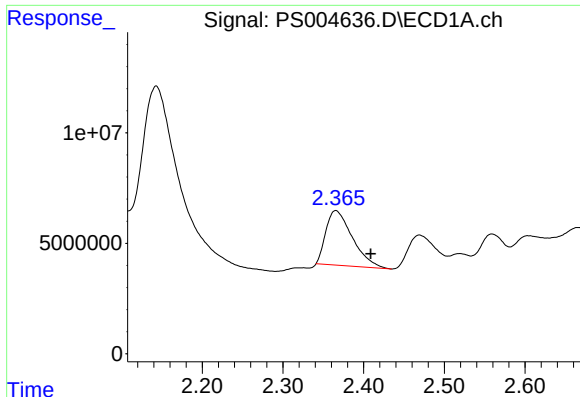

#1 Dalapon


R.T.: 2.366 min
Delta R.T.: -0.043 min
Response: 56360655
Conc: 59.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

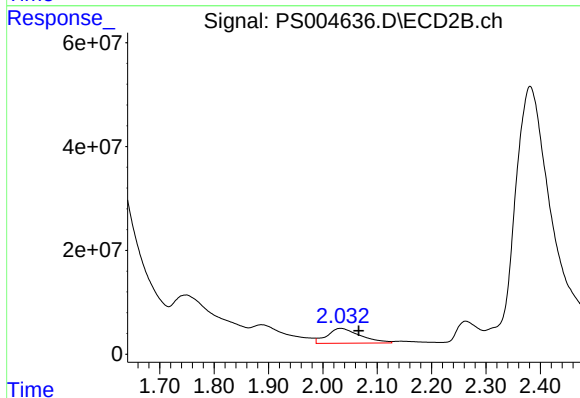


#1 Dalapon

R.T.: 2.033 min
Delta R.T.: -0.033 min
Response: 121402491
Conc: 173.19 ng/ml

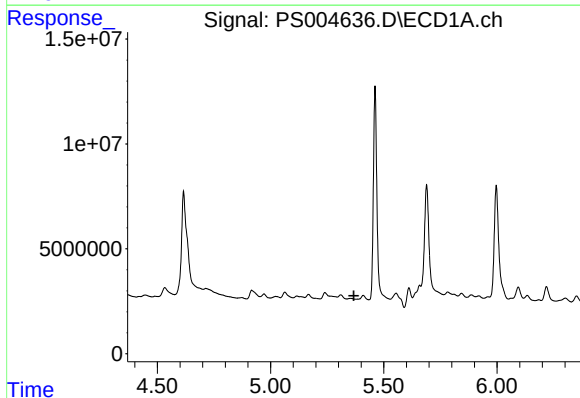


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.368 min
Response: 0
Conc: N.D.

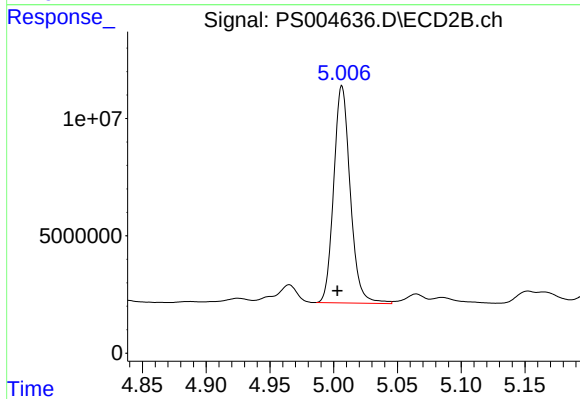

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.007 min
Delta R.T.: 0.004 min
Response: 83483070
Conc: 126.90 ng/ml

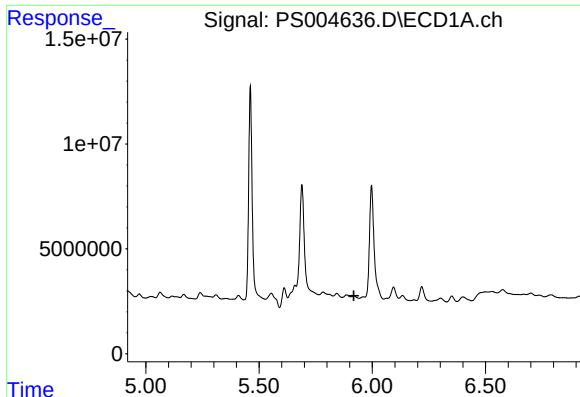

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

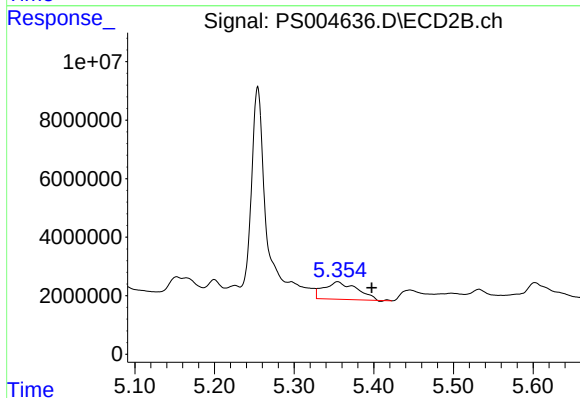


#3 4-Nitrophenol

R.T.: 5.355 min
Delta R.T.: -0.043 min
Response: 17207620
Conc: 77.83 ng/ml

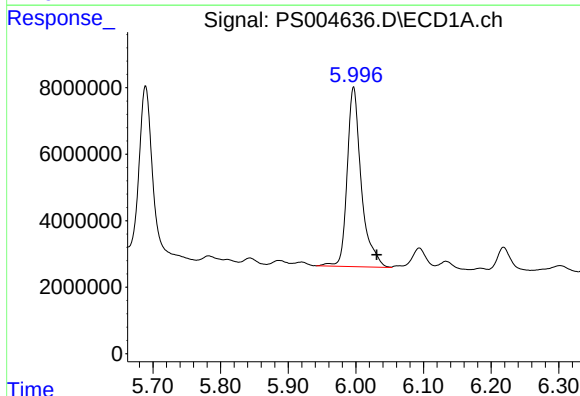


#4 2,4-DCAA

R.T.: 5.997 min
Delta R.T.: -0.034 min
Response: 78259159
Conc: 110.11 ng/ml

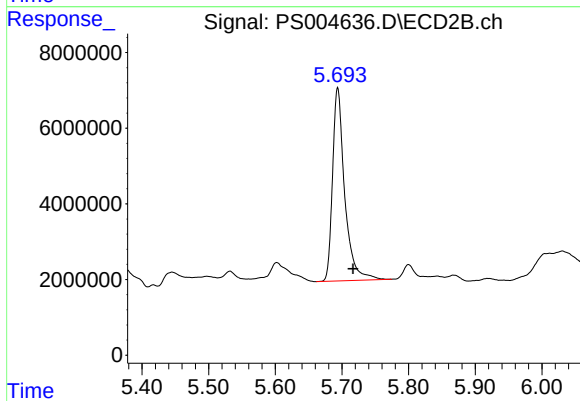

#4 2,4-DCAA


R.T.: 5.694 min
Delta R.T.: -0.023 min
Response: 64610544
Conc: 128.53 ng/ml

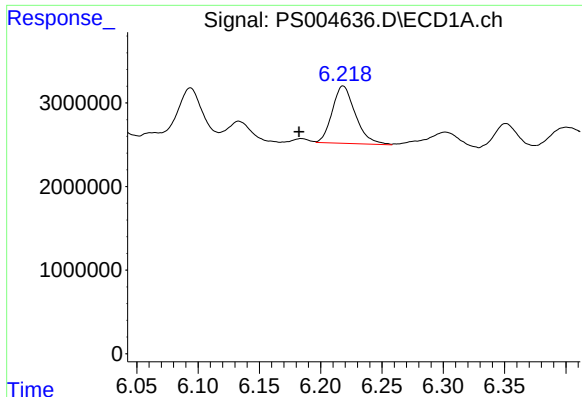

#5 DICAMBA


R.T.: 6.218 min
Delta R.T.: 0.036 min
Response: 9006804
Conc: 3.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

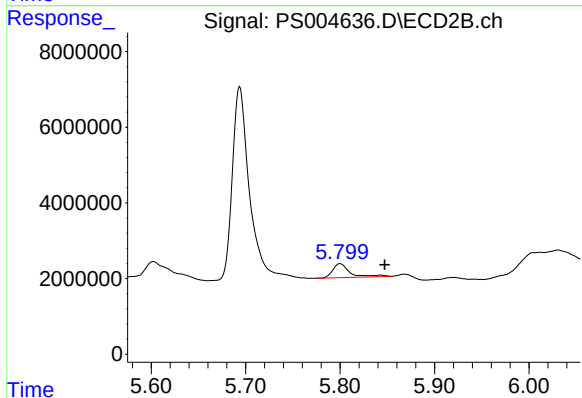


#5 DICAMBA

R.T.: 5.800 min
Delta R.T.: -0.047 min
Response: 4655892
Conc: 2.38 ng/ml

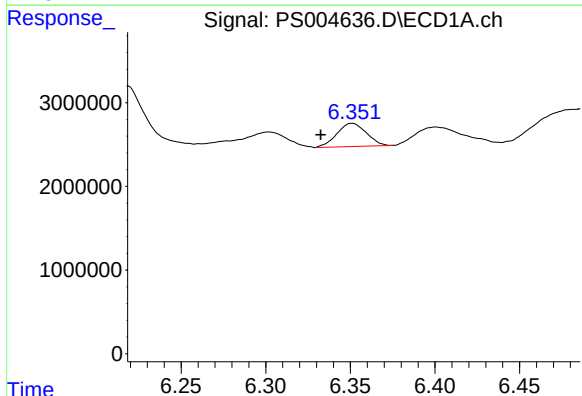


#6 MCP

R.T.: 6.351 min
Delta R.T.: 0.019 min
Response: 3351857
Conc: 1.73 ug/ml

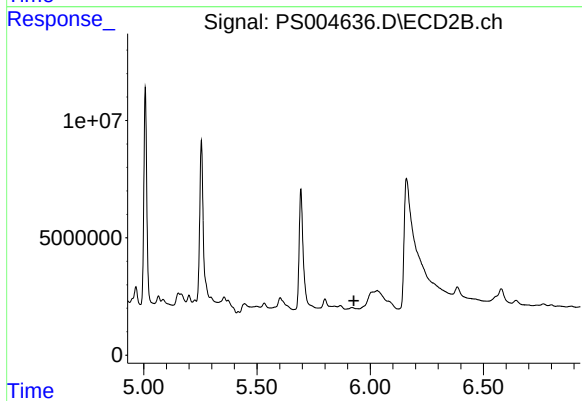

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

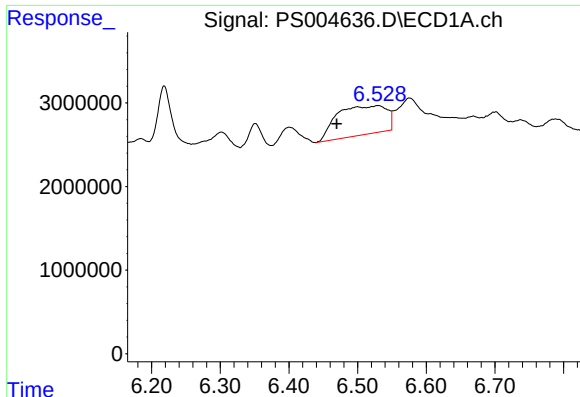

#7 MCPA


R.T.: 6.530 min
Delta R.T.: 0.060 min
Response: 17441577
Conc: 6.21 ug/ml

Instrument :
ECD_S
ClientSampleId :

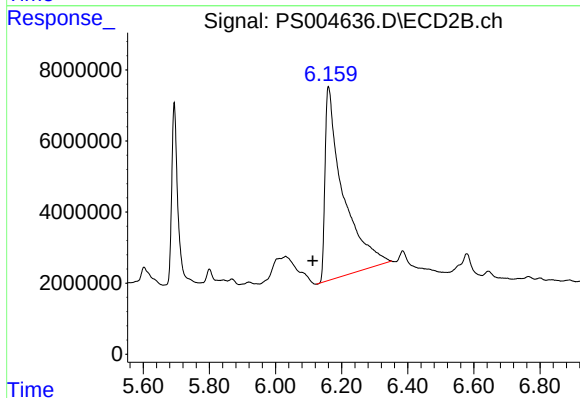


#7 MCPA

R.T.: 6.161 min
Delta R.T.: 0.048 min
Response: 207433390
Conc: 101.50 ug/ml

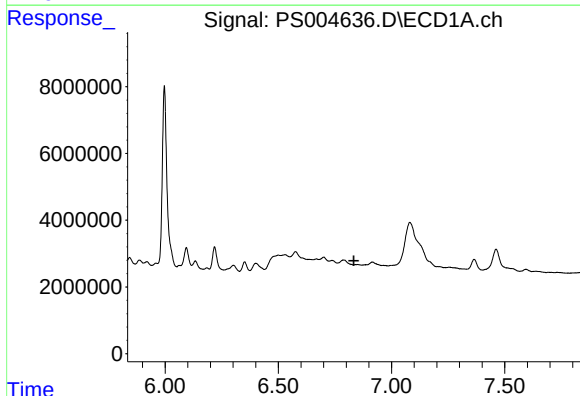


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.834 min
Response: 0
Conc: N.D.

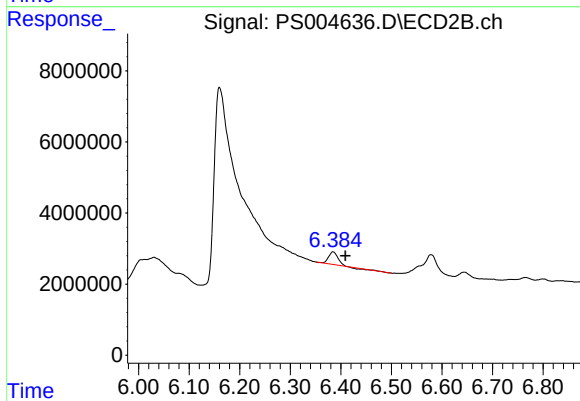

#8 DICHLORPROP


R.T.: 6.385 min
Delta R.T.: -0.024 min
Response: 4112356
Conc: 8.49 ng/ml

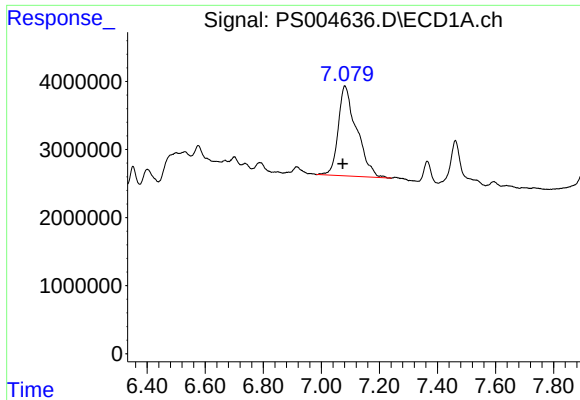

#9 2,4-D


R.T.: 7.081 min
Delta R.T.: 0.007 min
Response: 58141976
Conc: 79.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

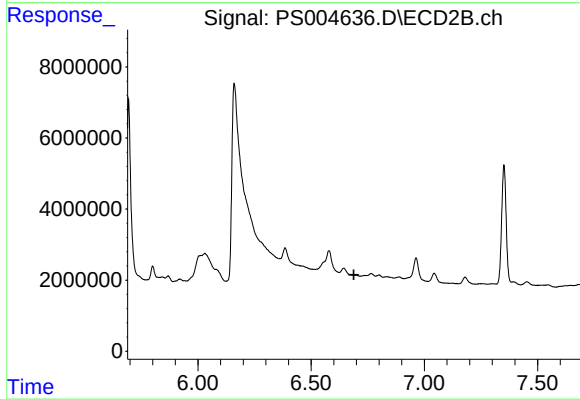


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

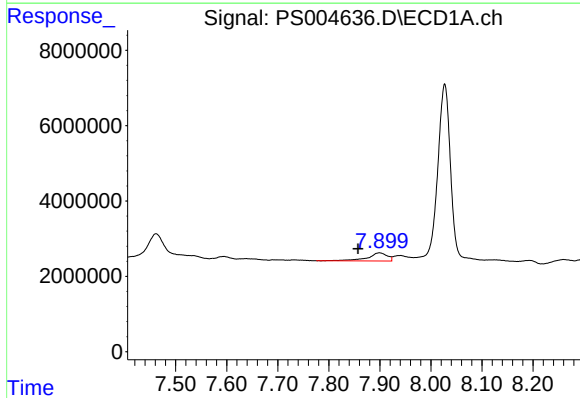

#11 2,4,5-TP (SILVEX)

R.T.: 7.899 min
Delta R.T.: 0.041 min
Response: 5725036
Conc: 1.57 ng/ml

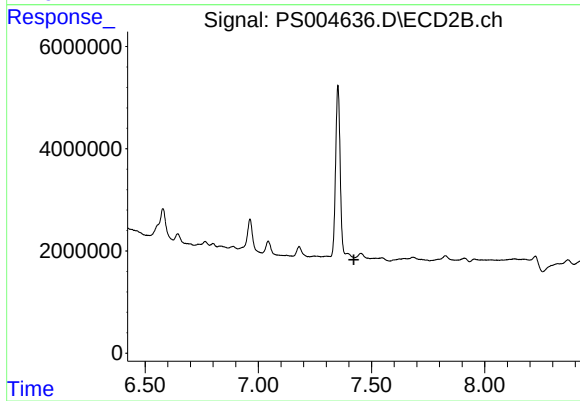

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.422 min
Response: 0
Conc: N.D.