

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
 Data File : PS004638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 00:15
 Operator : EI\SJ
 Sample : K2837-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 04:07:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.992	5.690	245.0E6	179.6E6	344.685	357.190
Target Compounds							
1) T	Dalapon	2.364	2.031	32542920	41824669	34.443	59.664 #
2) T	3,5-DICHL...	5.406	5.004	2888038	94554117	3.410	143.733 #
3) T	4-Nitroph...	5.886	5.441	6697717	4360119	26.374	19.720 #
5) T	DICAMBA	6.217	5.797	9563914	10240625	3.579	5.224 #
6) T	MCPD	6.349	0.000	5829512	0	3.002	N.D. #
7) T	MCPA	6.498	6.161	22583106	182.3E6	8.039	89.206 #
8) T	DICHLORPROP	0.000	6.383	0	5679335	N.D.	11.721
9) T	2,4-D	7.079	0.000	61178905	0	83.968	N.D. #
10) T	Pentachlo...	7.362	0.000	4008601	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
Data File : PS004638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 00:15
Operator : EI\SJ
Sample : K2837-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 04:07:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

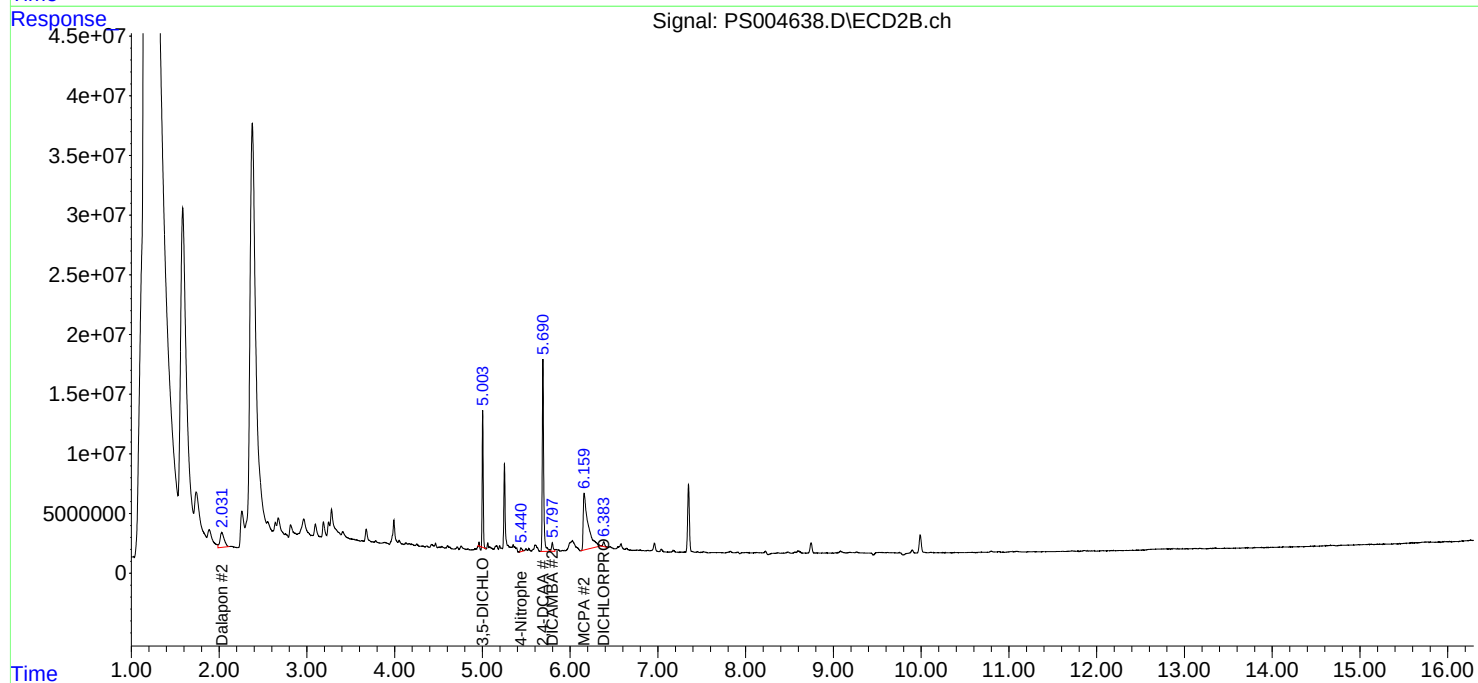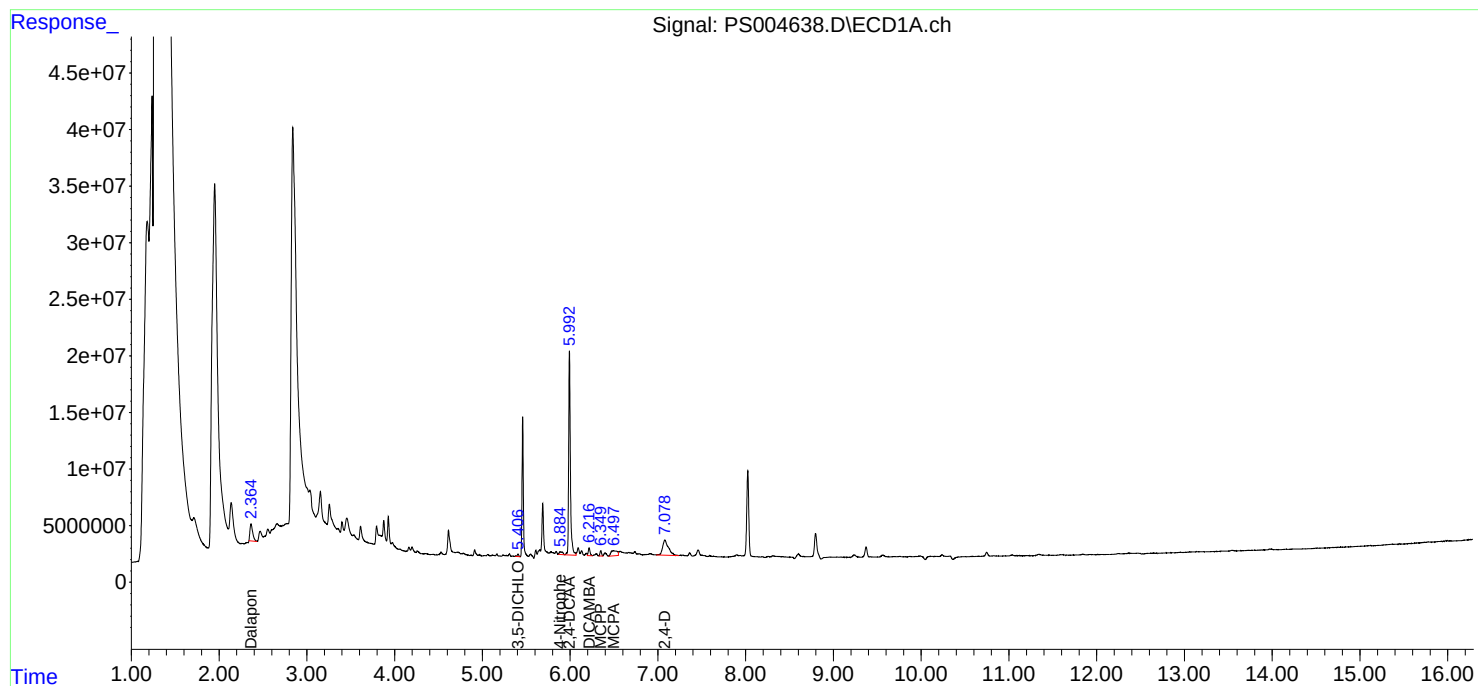


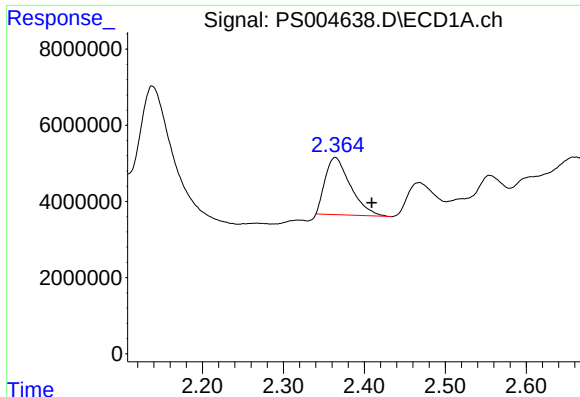

#1 Dalapon


R.T.: 2.364 min
Delta R.T.: -0.045 min
Response: 32542920
Conc: 34.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

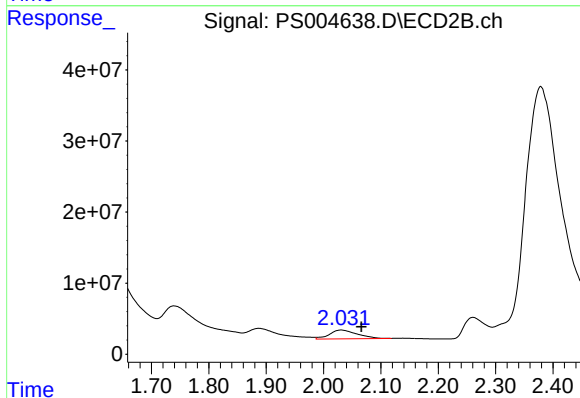


#1 Dalapon

R.T.: 2.031 min
Delta R.T.: -0.035 min
Response: 41824669
Conc: 59.66 ng/ml

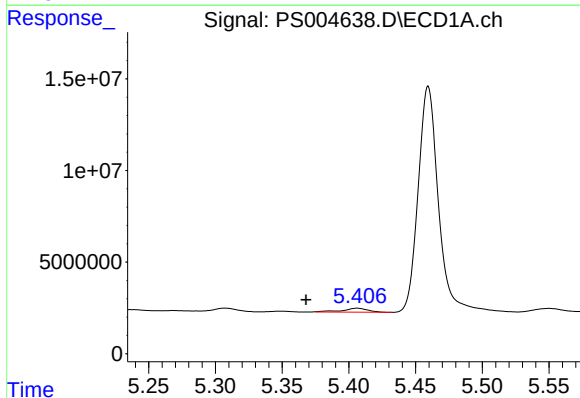


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.406 min
Delta R.T.: 0.038 min
Response: 2888038
Conc: 3.41 ng/ml

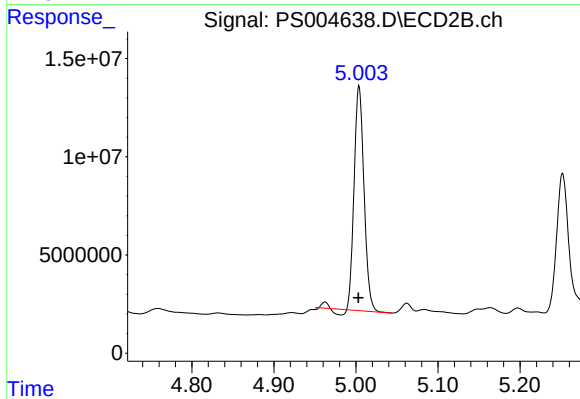

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.004 min
Delta R.T.: 0.001 min
Response: 94554117
Conc: 143.73 ng/ml

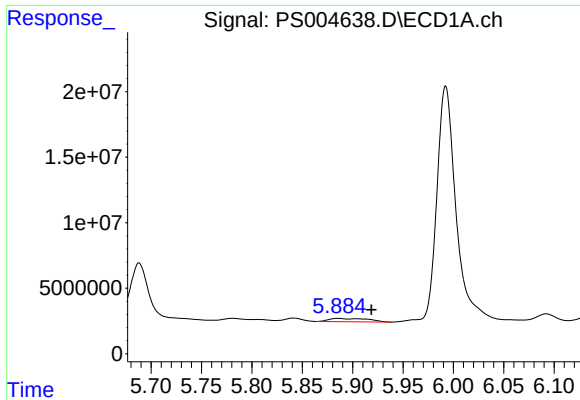

#3 4-Nitrophenol


R.T.: 5.886 min
Delta R.T.: -0.033 min
Response: 6697717
Conc: 26.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

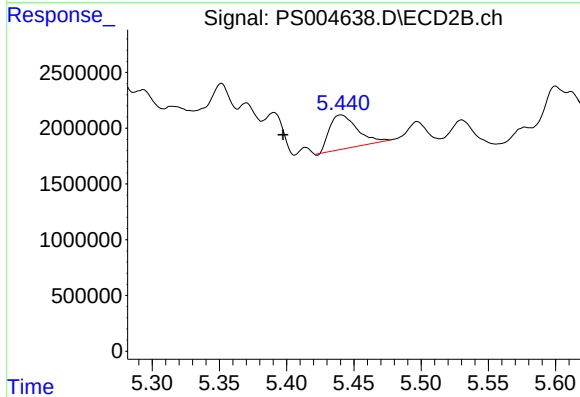


#3 4-Nitrophenol

R.T.: 5.441 min
Delta R.T.: 0.043 min
Response: 4360119
Conc: 19.72 ng/ml

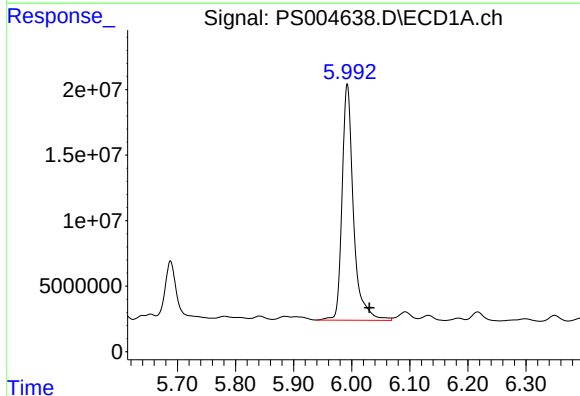


#4 2,4-DCAA

R.T.: 5.992 min
Delta R.T.: -0.038 min
Response: 244977230
Conc: 344.69 ng/ml

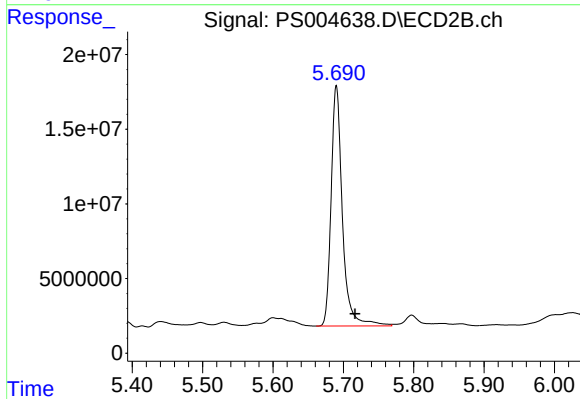

#4 2,4-DCAA


R.T.: 5.690 min
Delta R.T.: -0.026 min
Response: 179554252
Conc: 357.19 ng/ml

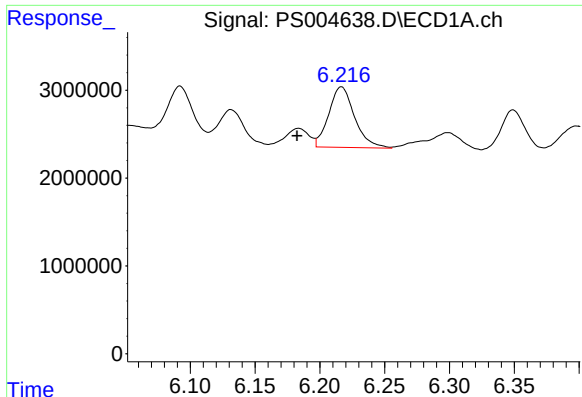

#5 DICAMBA


R.T.: 6.217 min
Delta R.T.: 0.034 min
Response: 9563914
Conc: 3.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

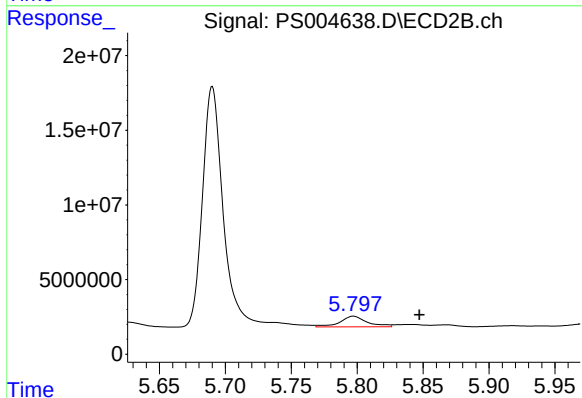


#5 DICAMBA

R.T.: 5.797 min
Delta R.T.: -0.050 min
Response: 10240625
Conc: 5.22 ng/ml

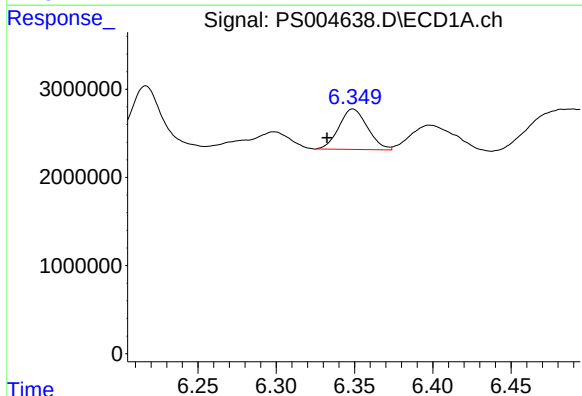


#6 MCP

R.T.: 6.349 min
Delta R.T.: 0.017 min
Response: 5829512
Conc: 3.00 ug/ml

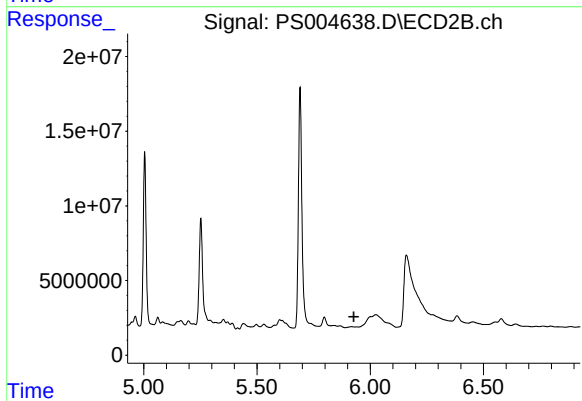

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

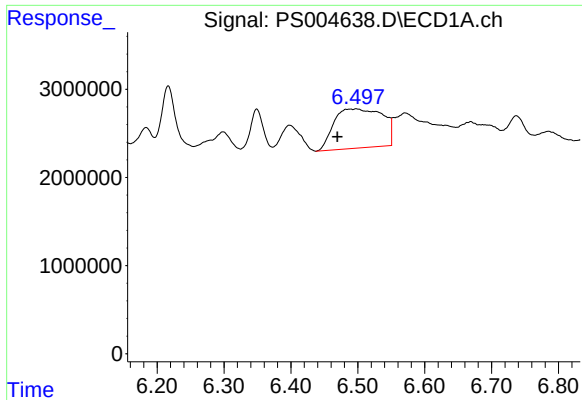

#7 MCPA


R.T.: 6.498 min
Delta R.T.: 0.029 min
Response: 22583106
Conc: 8.04 ug/ml

Instrument :
ECD_S
ClientSampleId :

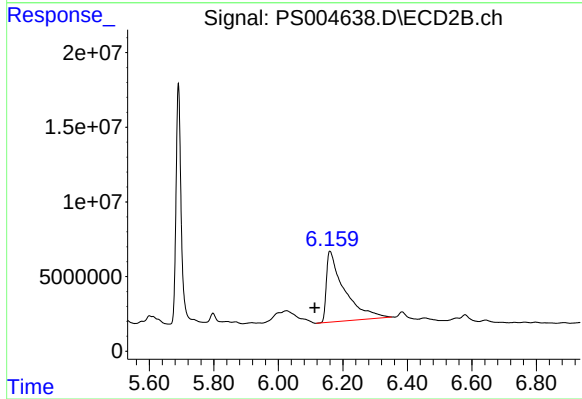


#7 MCPA

R.T.: 6.161 min
Delta R.T.: 0.048 min
Response: 182312423
Conc: 89.21 ug/ml

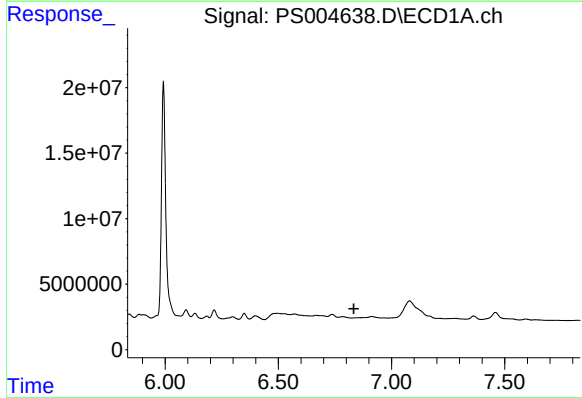


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.834 min
Response: 0
Conc: N.D.

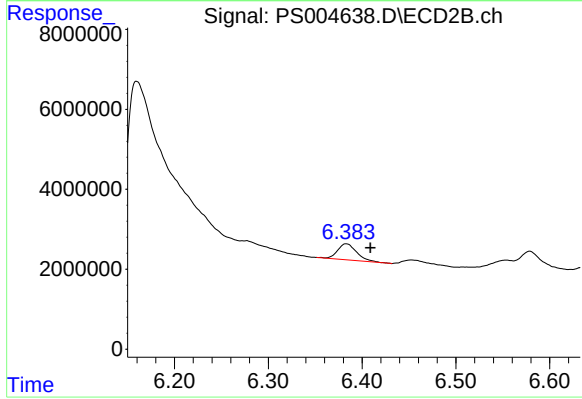

#8 DICHLORPROP


R.T.: 6.383 min
Delta R.T.: -0.026 min
Response: 5679335
Conc: 11.72 ng/ml

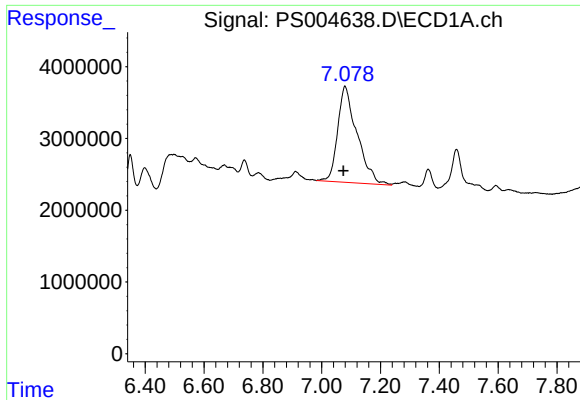

#9 2,4-D

R.T.: 7.079 min
Delta R.T.: 0.005 min
Response: 61178905
Conc: 83.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

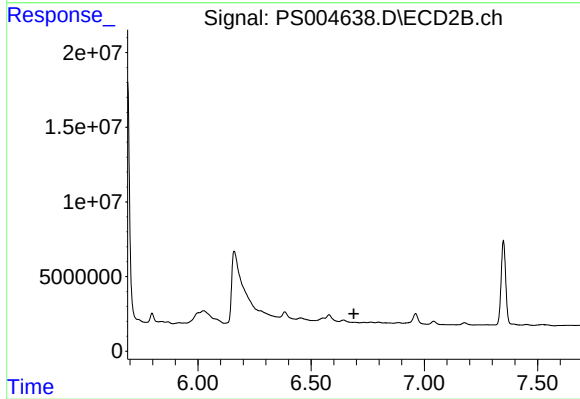

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.