

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
 Data File : PS004643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2019 03:25
 Operator : EI\SJ
 Sample : K2851-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 05:15:10 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
 Quant Title : 8080.M
 QLast Update : Mon May 13 15:36:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.999	5.696	228.5E6	167.6E6	321.493	333.391
Target Compounds							
1) T	Dalapon	2.370	2.035	33274794	40078064	35.217	57.173 #
2) T	3,5-DICHL...	0.000	5.010	0	89138603	N.D.	135.500
3) T	4-Nitroph...	0.000	5.357	0	20992793	N.D.	94.947
5) T	DICAMBA	6.222	5.803	7124537	7152938	2.666	3.649 #
6) T	MCPD	6.356	0.000	4294116	0	2.211	N.D. #
7) T	MCPA	6.406	6.182	6969020	98129073	2.481	48.015 #
8) T	DICHLORPROP	0.000	6.389	0	6371398	N.D.	13.149
9) T	2,4-D	7.085	0.000	55017237	0	75.511	N.D. #
10) T	Pentachlo...	7.368	7.045	3602680	3680943	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	7.355	0	68313583	N.D.	25.501
12) T	2,4,5-T	0.000	7.821	0	7692408	N.D.	3.197
15) T	Picloram	9.600	9.524	23532830	18388944	5.300	5.000
16) T	DCPA	0.000	9.524	0	18388944	N.D.	5.392



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051619\
Data File : PS004643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2019 03:25
Operator : EI\SJ
Sample : K2851-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:15:10 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051319.M
Quant Title : 8080.M
QLast Update : Mon May 13 15:36:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

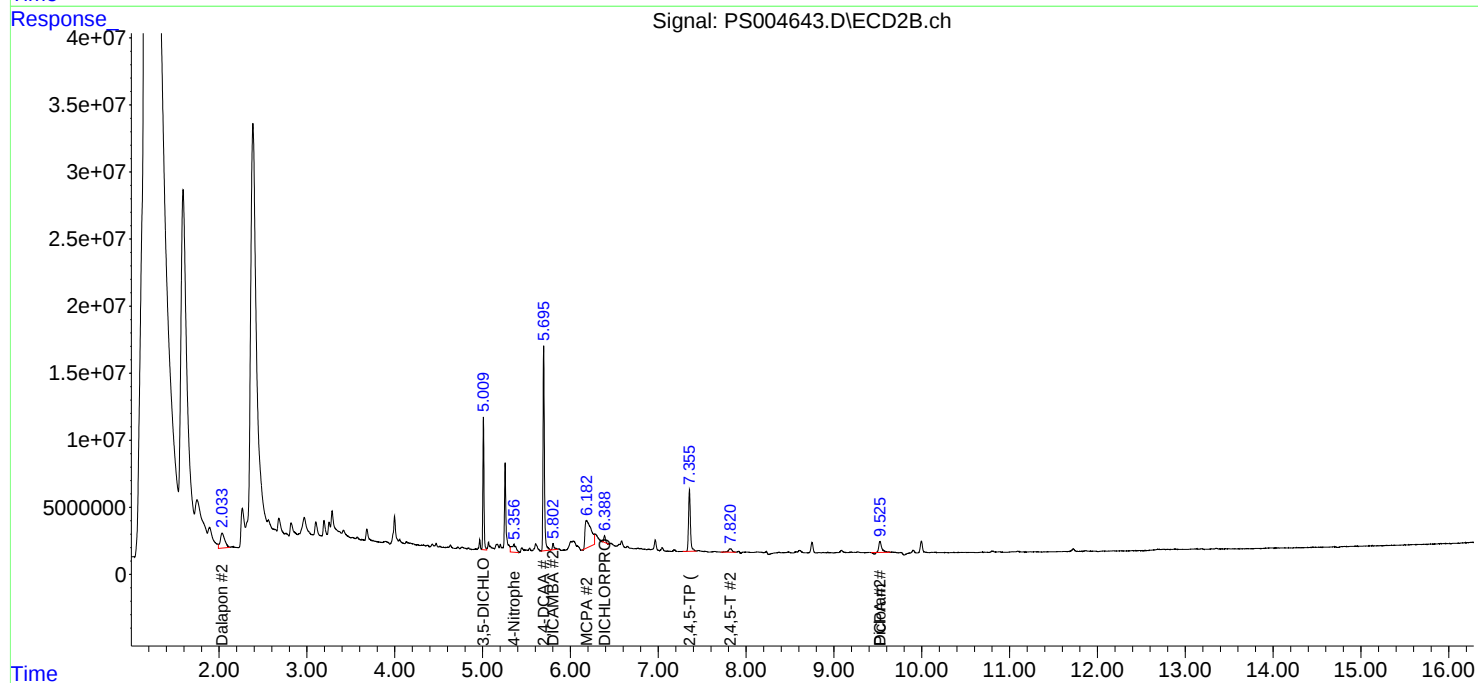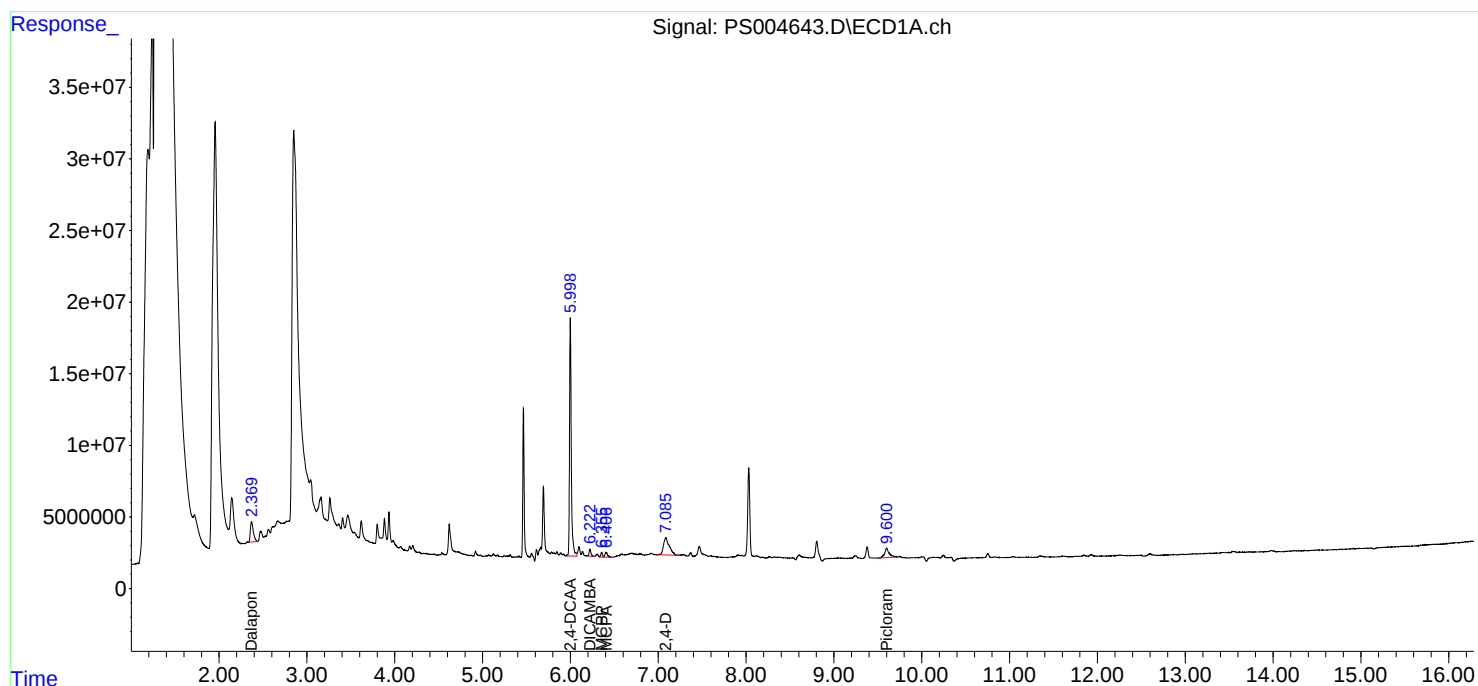


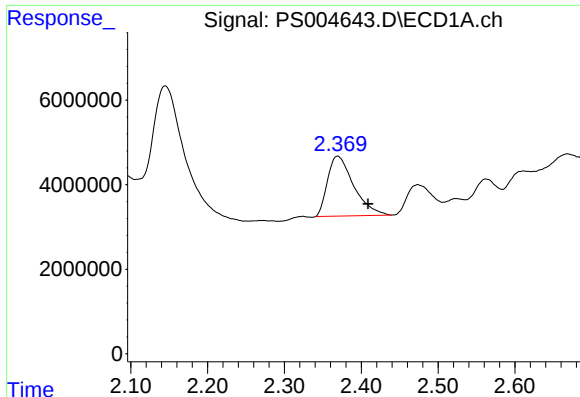

#1 Dalapon


R.T.: 2.370 min
Delta R.T.: -0.039 min
Response: 33274794
Conc: 35.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

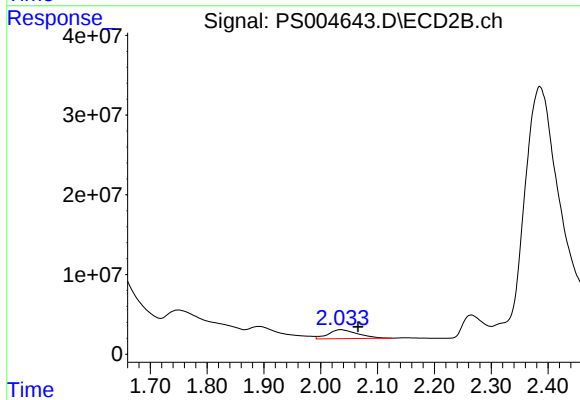


#1 Dalapon

R.T.: 2.035 min
Delta R.T.: -0.031 min
Response: 40078064
Conc: 57.17 ng/ml

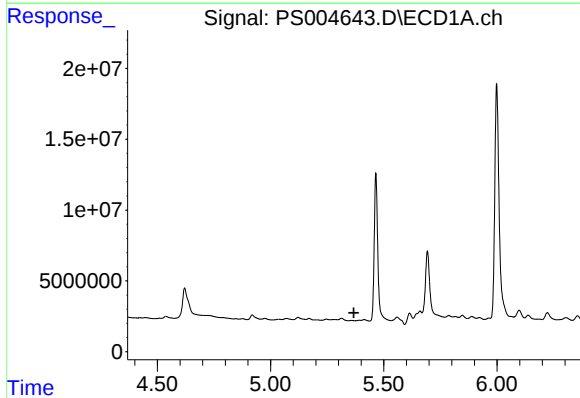


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.368 min
Response: 0
Conc: N.D.

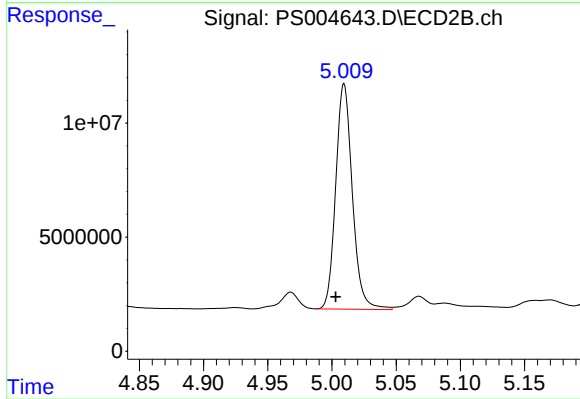

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.010 min
Delta R.T.: 0.007 min
Response: 89138603
Conc: 135.50 ng/ml

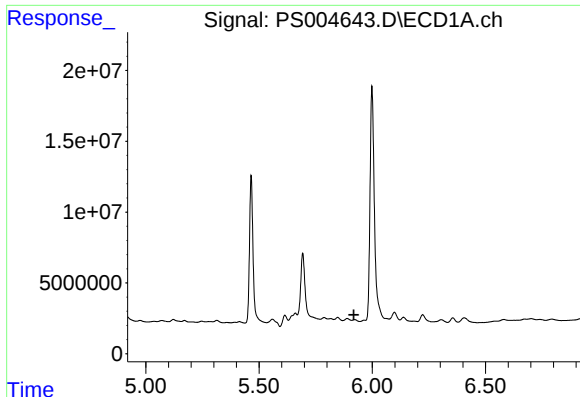

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

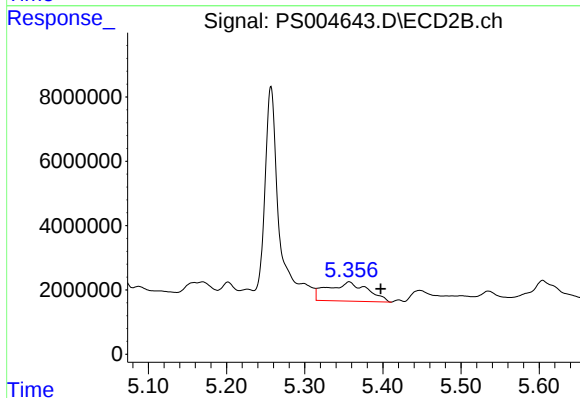


#3 4-Nitrophenol

R.T.: 5.357 min
Delta R.T.: -0.040 min
Response: 20992793
Conc: 94.95 ng/ml

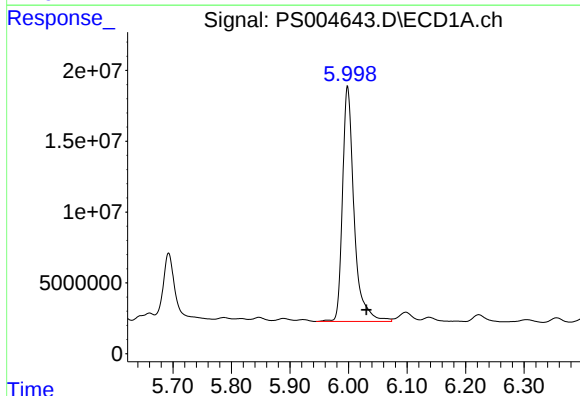


#4 2,4-DCAA

R.T.: 5.999 min
Delta R.T.: -0.032 min
Response: 228494193
Conc: 321.49 ng/ml

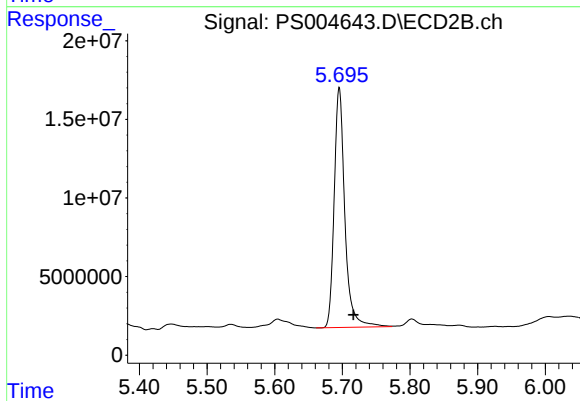

#4 2,4-DCAA


R.T.: 5.696 min
Delta R.T.: -0.021 min
Response: 167590812
Conc: 333.39 ng/ml

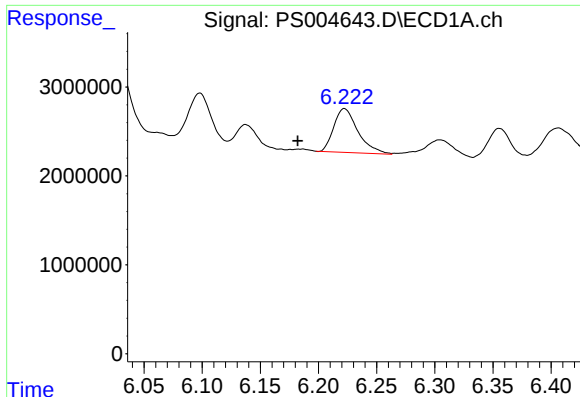

#5 DICAMBA


R.T.: 6.222 min
Delta R.T.: 0.040 min
Response: 7124537
Conc: 2.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

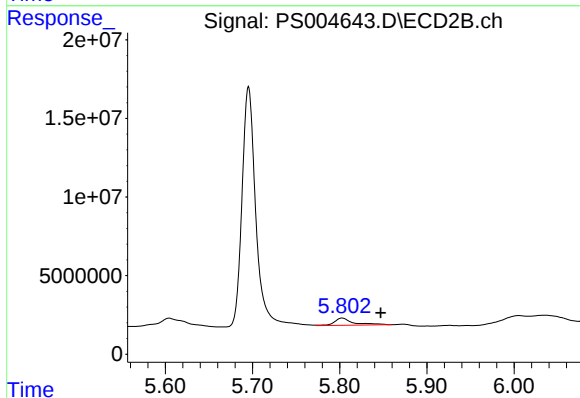


#5 DICAMBA

R.T.: 5.803 min
Delta R.T.: -0.044 min
Response: 7152938
Conc: 3.65 ng/ml

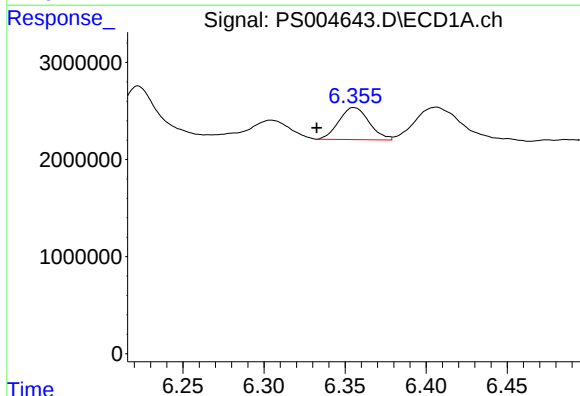


#6 MCP

R.T.: 6.356 min
Delta R.T.: 0.023 min
Response: 4294116
Conc: 2.21 ug/ml

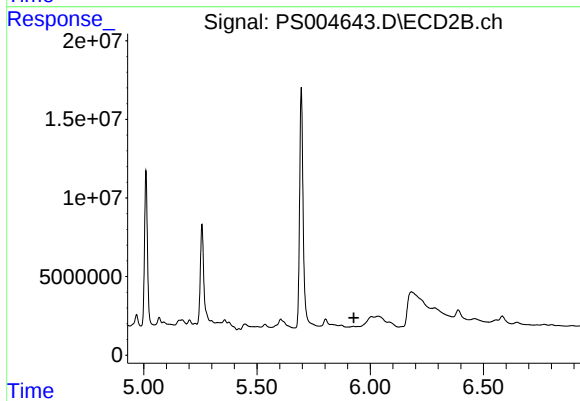

#6 MCP


R.T.: 0.000 min
Exp R.T. : 5.928 min
Response: 0
Conc: N.D.

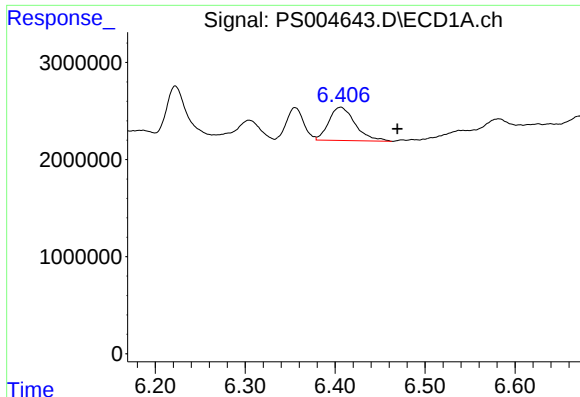

#7 MCPA


R.T.: 6.406 min
Delta R.T.: -0.063 min
Response: 6969020
Conc: 2.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

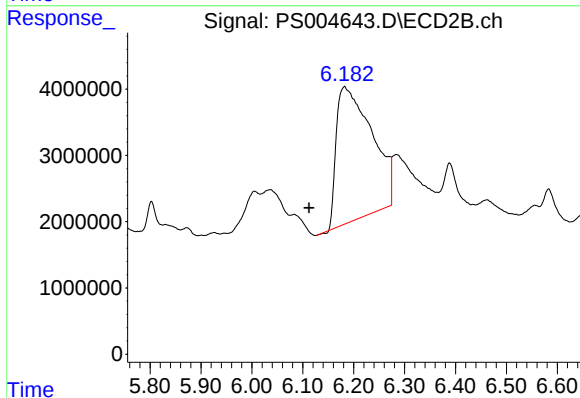


#7 MCPA

R.T.: 6.182 min
Delta R.T.: 0.070 min
Response: 98129073
Conc: 48.01 ug/ml

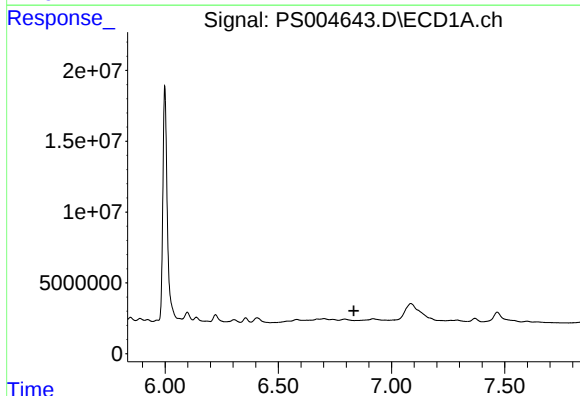


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.834 min
Response: 0
Conc: N.D.

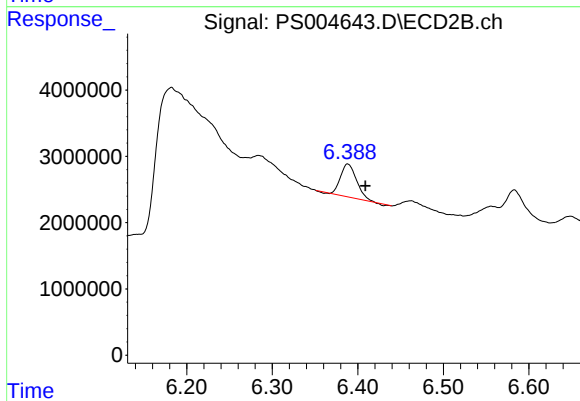

#8 DICHLORPROP


R.T.: 6.389 min
Delta R.T.: -0.020 min
Response: 6371398
Conc: 13.15 ng/ml

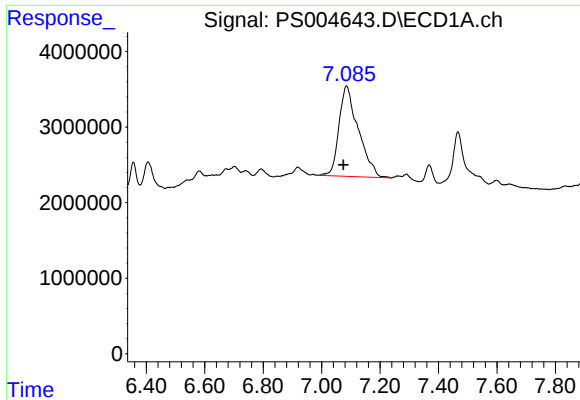

#9 2,4-D


R.T.: 7.085 min
Delta R.T.: 0.011 min
Response: 55017237
Conc: 75.51 ng/ml

Instrument :
ECD_S
ClientSampleId :

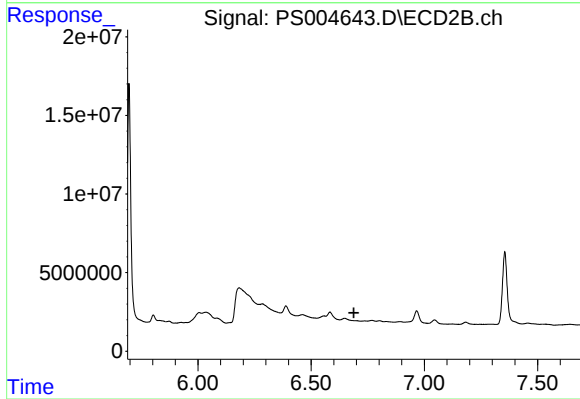


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.689 min
Response: 0
Conc: N.D.

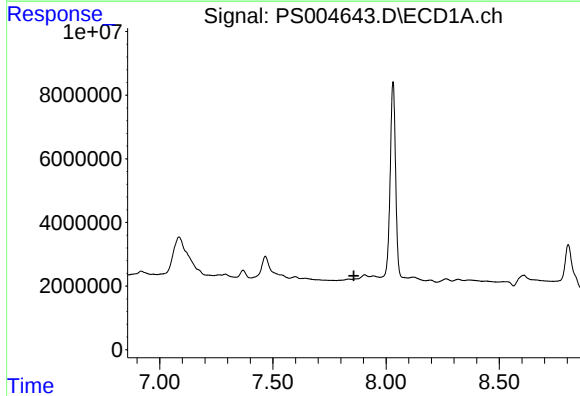


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.858 min
Response: 0
Conc: N.D.

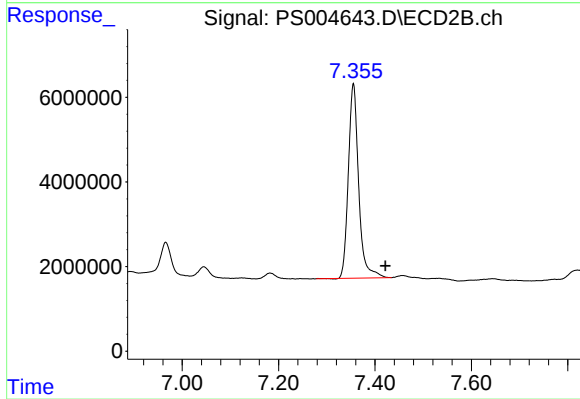

#11 2,4,5-TP (SILVEX)


R.T.: 7.355 min
Delta R.T.: -0.067 min
Response: 68313583
Conc: 25.50 ng/ml

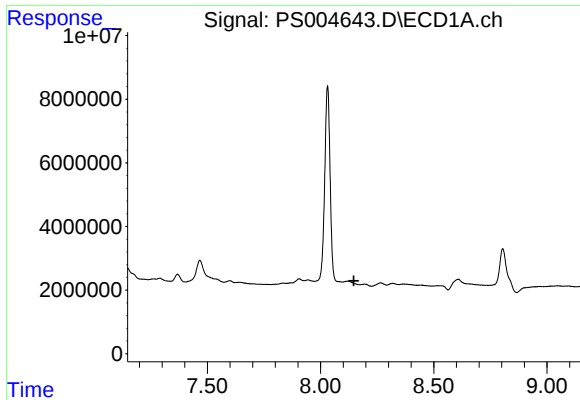

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

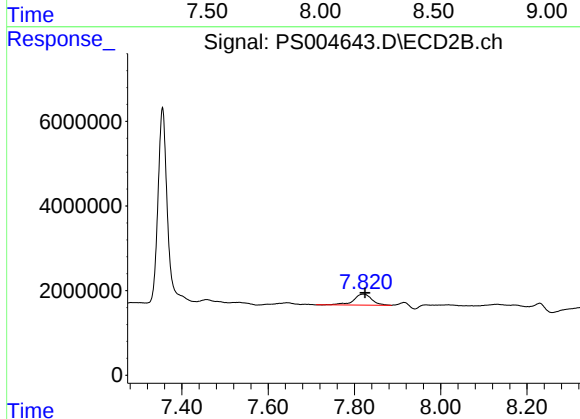


#12 2,4,5-T

R.T.: 7.821 min
Delta R.T.: -0.004 min
Response: 7692408
Conc: 3.20 ng/ml

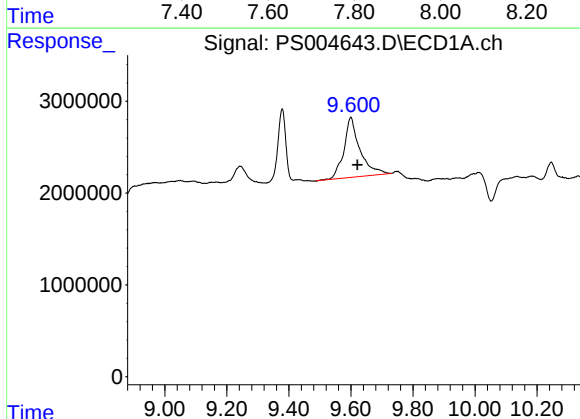


#15 Picloram

R.T.: 9.600 min
Delta R.T.: -0.021 min
Response: 23532830
Conc: 5.30 ng/ml

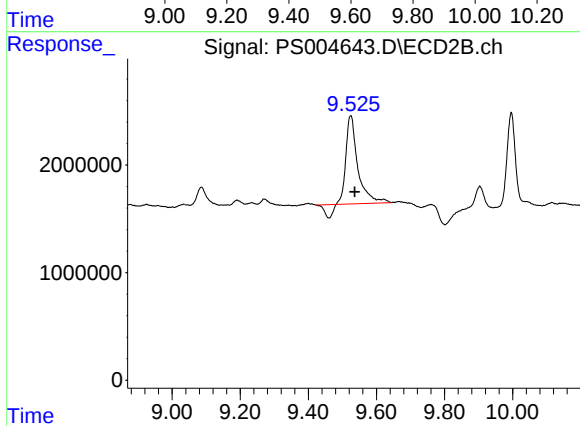

#15 Picloram


R.T.: 9.524 min
Delta R.T.: -0.012 min
Response: 18388944
Conc: 5.00 ng/ml

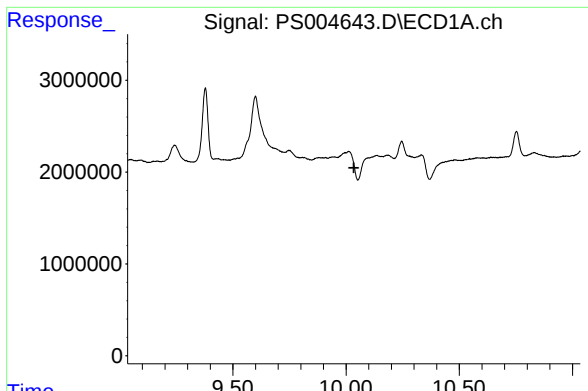

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.035 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

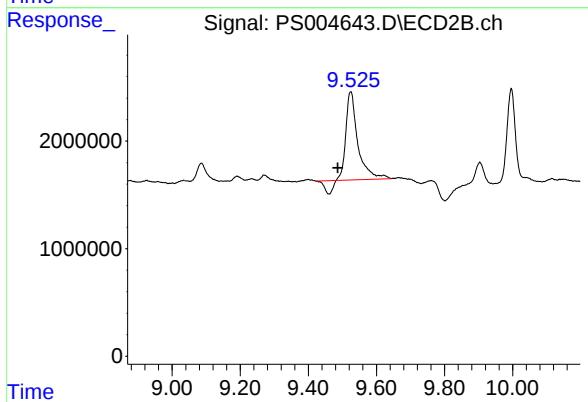

#16 DCPA

R.T.: 9.524 min
Delta R.T.: 0.038 min
Response: 18388944
Conc: 5.39 ng/ml