

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051622\
 Data File : PS019413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2022 09:28
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 19:45:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	0.000	34562	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.062	0.000	2715532	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.384f	0.000	169299	0	<MDL	N.D. #
3) T	4-Nitroph...	7.011	0.000	300852	0	<MDL	N.D. #
5) T	DICAMBA	7.421	6.970	1151299	421486	<MDL	<MDL #
8) T	DICHLORPROP	8.137	0.000	440895	0	<MDL	N.D. #
10) T	Pentachlo...	8.651	8.310	3851684	1714953	<MDL	<MDL #
11) T	2,4,5-TP ...	9.217	8.682	3090830	1408784	<MDL	<MDL #
12) T	2,4,5-T	9.524f	9.084	14658383	685633	<MDL	<MDL #
13) T	2,4-DB	0.000	9.494f	0	4461633	N.D.	7.847
14) T	DINOSEB	11.187	9.884	73832112	1324418	4.472	<MDL #
15) T	Picloram	11.017	10.810f	8516891	11282290	<MDL	1.886 #
16) T	DCPA	11.461	10.810	11909851	11282290	<MDL	1.922 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051622\
Data File : PS019413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2022 09:28
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 19:45:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

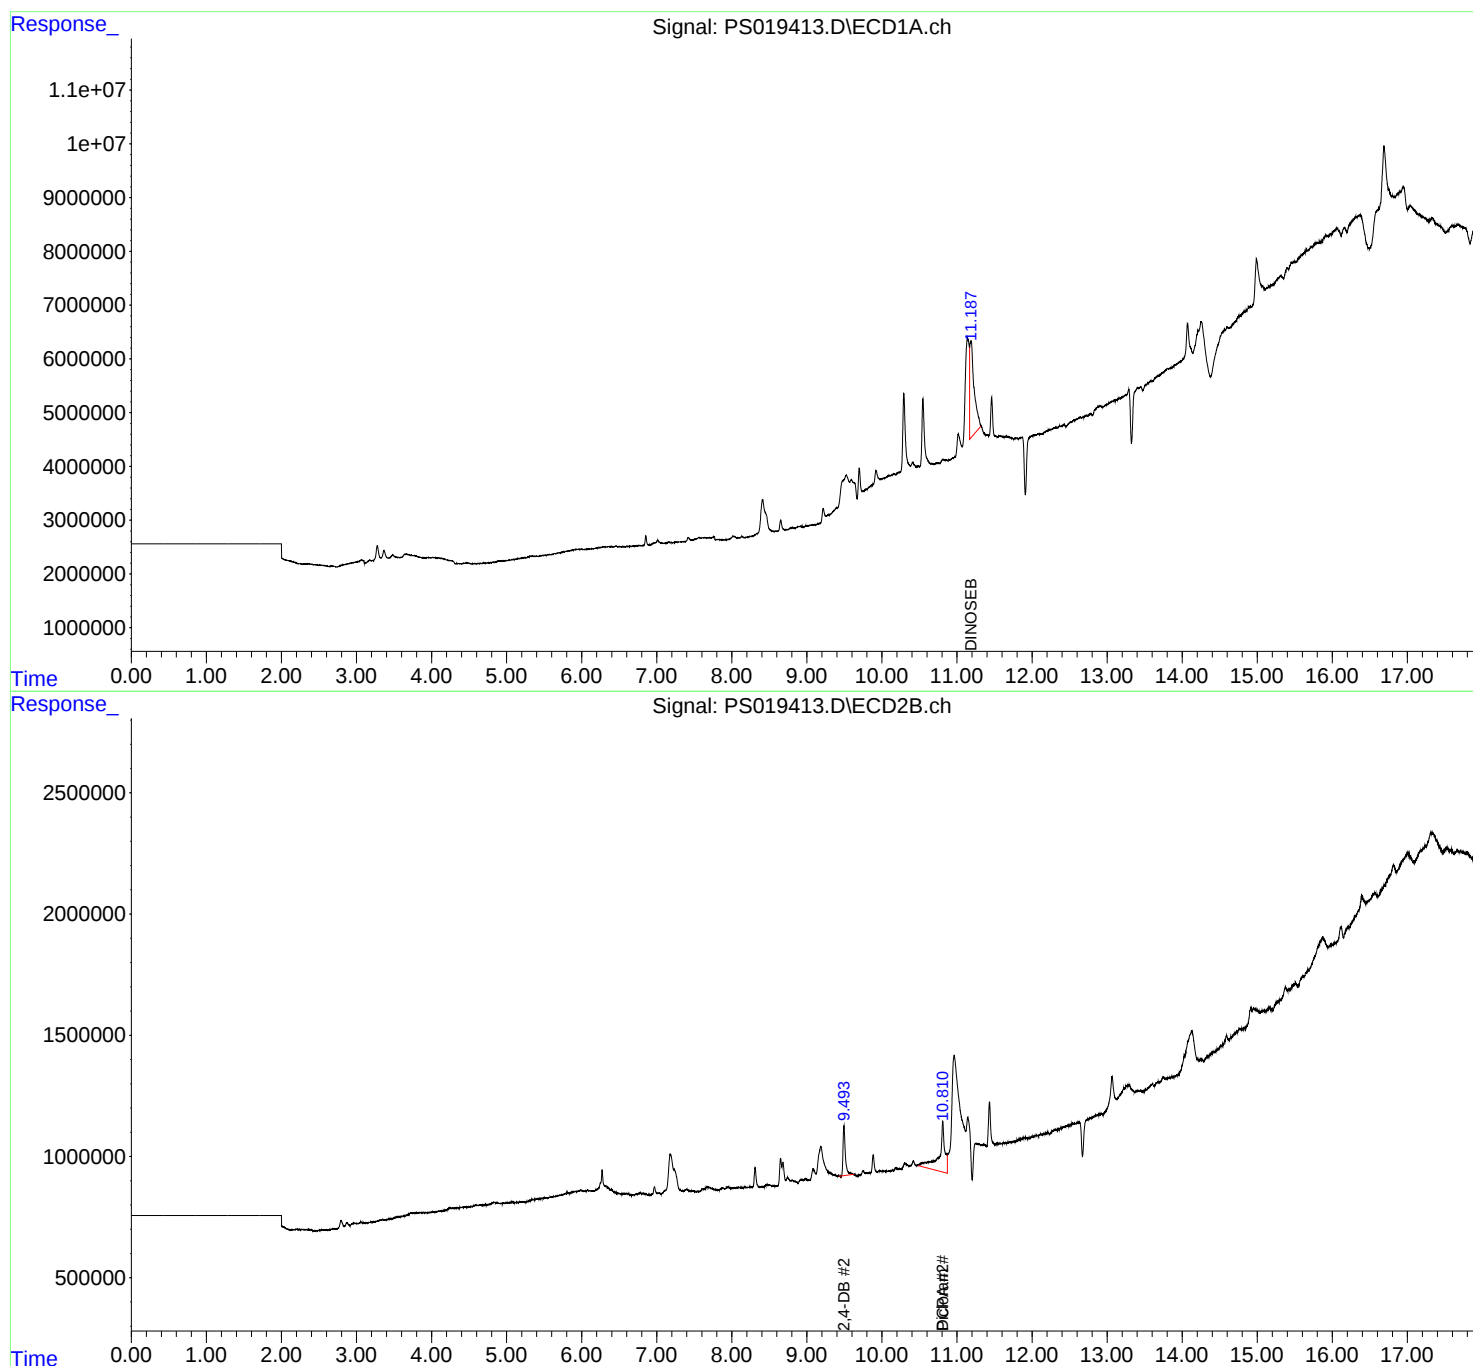


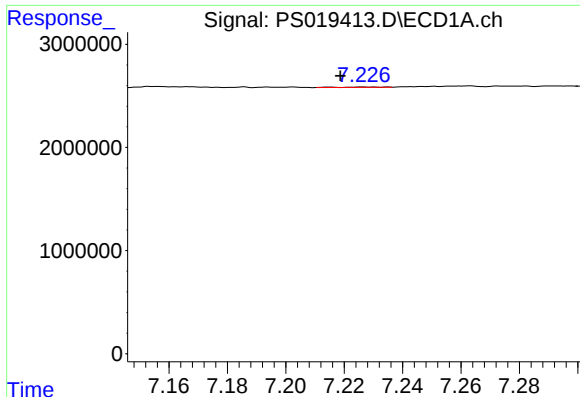

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.007 min
Response: 34562
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

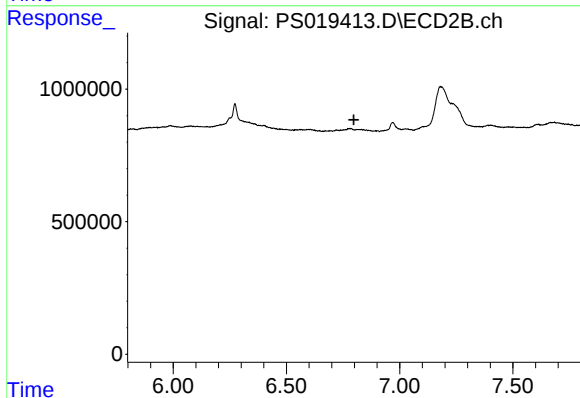


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.798 min
Response: 0
Conc: N.D.

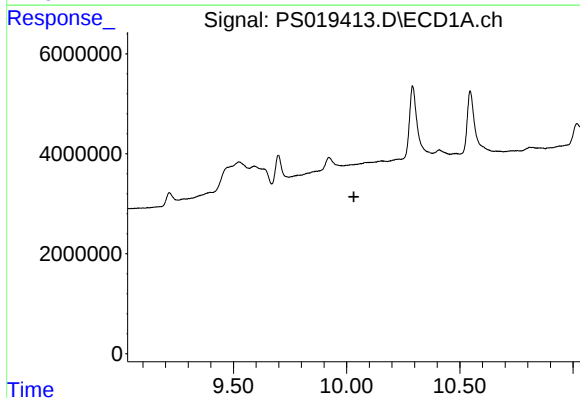


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.032 min
Response: 0
Conc: N.D.

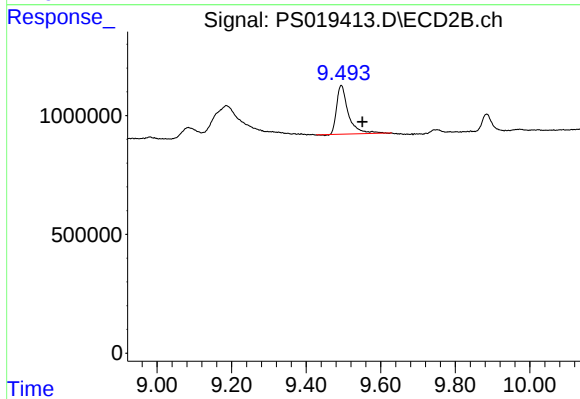

#13 2,4-DB


R.T.: 9.494 min
Delta R.T.: -0.057 min
Response: 4461633
Conc: 7.85 ng/ml

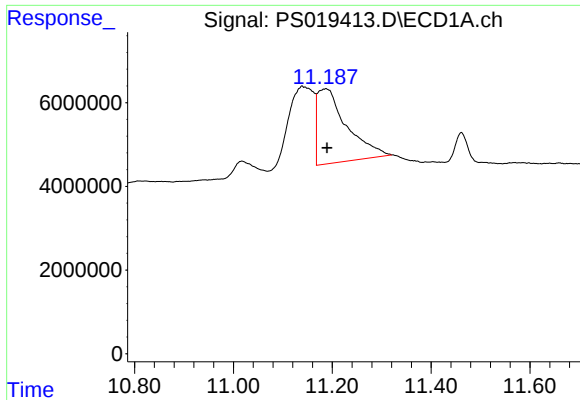

#14 DINOSEB


R.T.: 11.187 min
Delta R.T.: -0.002 min
Response: 73832112
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

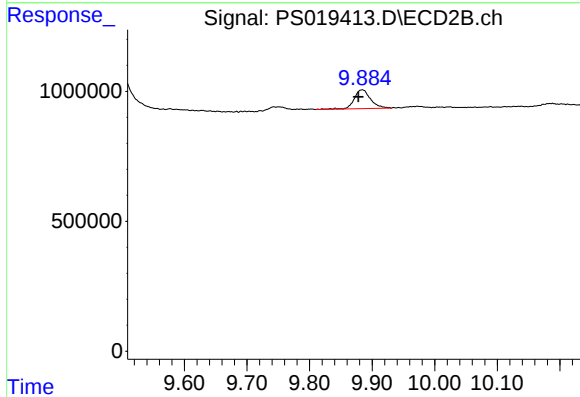


#14 DINOSEB

R.T.: 9.884 min
Delta R.T.: 0.006 min
Response: 1324418
Conc: N.D.

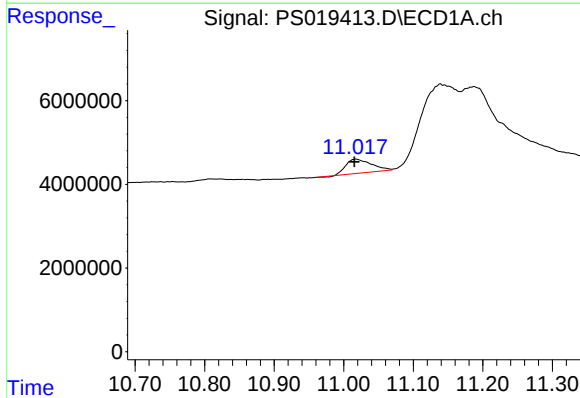


#15 Picloram

R.T.: 11.017 min
Delta R.T.: 0.002 min
Response: 8516891
Conc: N.D.

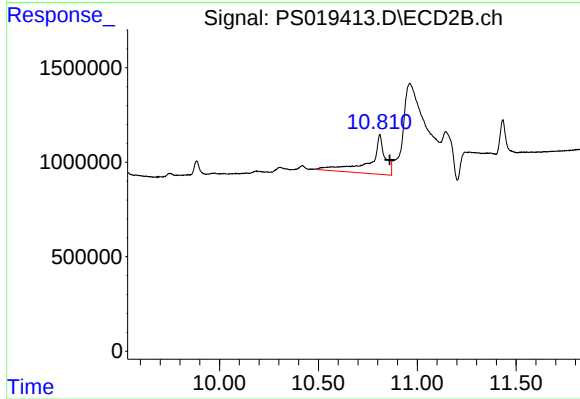

#15 Picloram


R.T.: 10.810 min
Delta R.T.: -0.051 min
Response: 11282290
Conc: 1.89 ng/ml

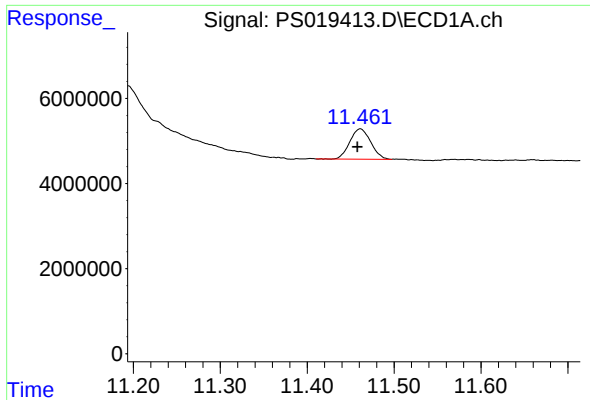

#16 DCPA

R.T.: 11.461 min
Delta R.T.: 0.003 min
Response: 11909851
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

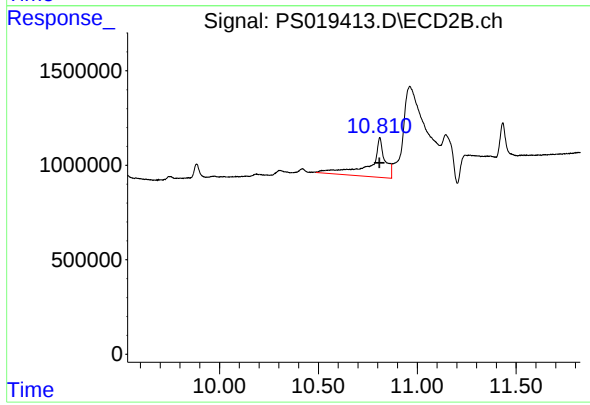

#16 DCPA

R.T.: 10.810 min
Delta R.T.: 0.002 min
Response: 11282290
Conc: 1.92 ng/ml