

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051622\
 Data File : PS019435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2022 01:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 02:40:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.223	6.800	1231.2E6	398.3E6	450.833	514.205
Target Compounds							
2) T	3,5-DICHL...	6.380f	5.923f	361659	168826	<MDL	<MDL #
3) T	4-Nitroph...	7.026	0.000	2106258	0	2.173	N.D. #
7) T	MCPA	7.684f	0.000	407021	0	<MDL	N.D. #
9) T	2,4-D	0.000	7.880	0	376941	N.D.	<MDL
10) T	Pentachlo...	8.650	8.312	797720	1312121	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	8.643	0	2656630	N.D.	<MDL
12) T	2,4,5-T	0.000	9.022	0	87316	N.D.	<MDL
13) T	2,4-DB	10.086f	9.502f	810879	9086119	<MDL	15.981 #
14) T	DINOSEB	11.192	9.901	31291990	478757	1.895	<MDL #
15) T	Picloram	11.023	10.815f	384041	346087	<MDL	<MDL #
16) T	DCPA	11.464	10.815	1551463	346087	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051622\
Data File : PS019435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2022 01:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 02:40:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

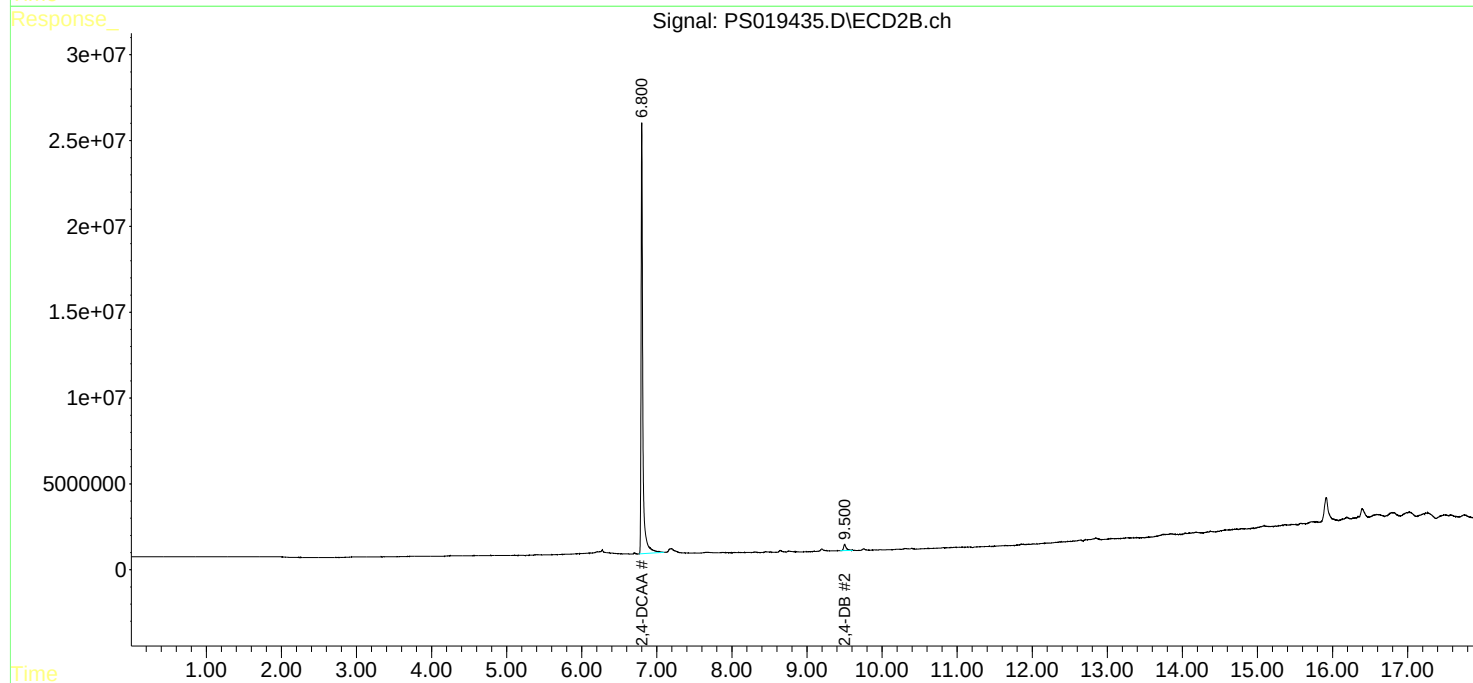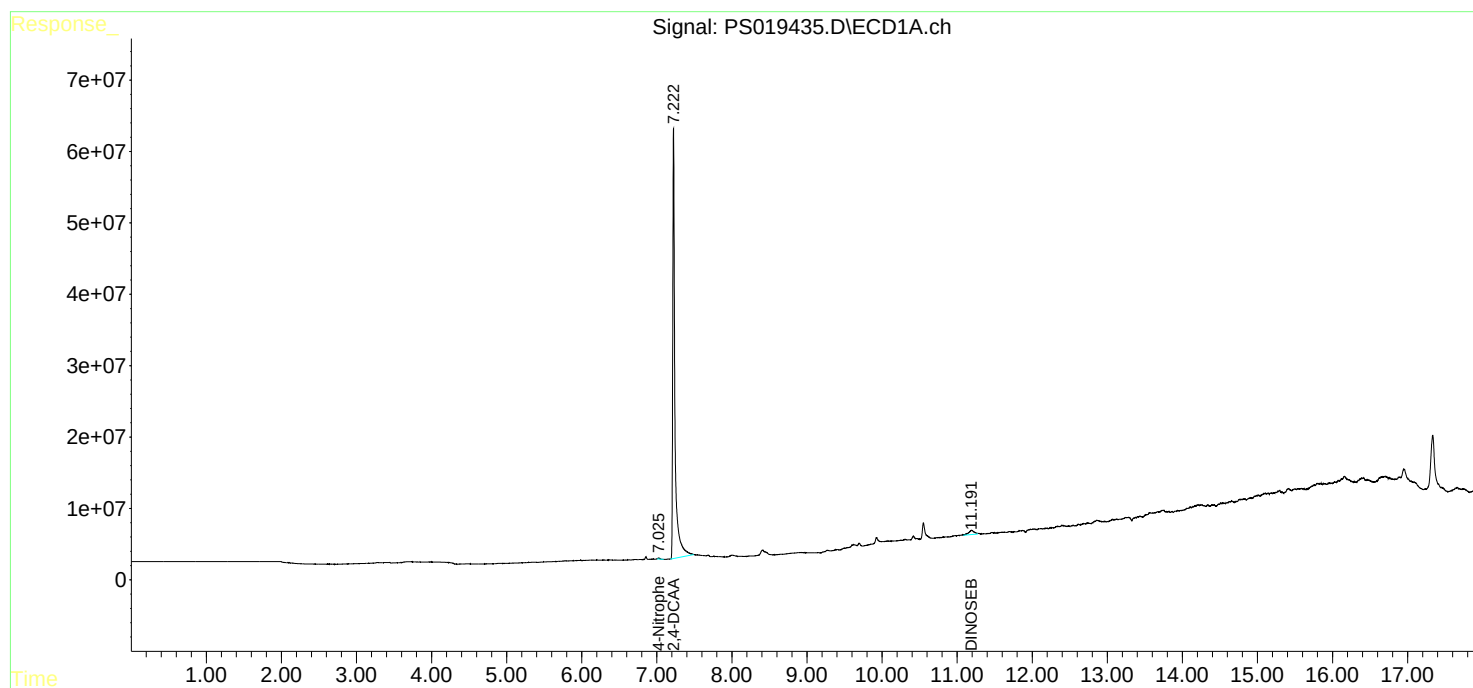


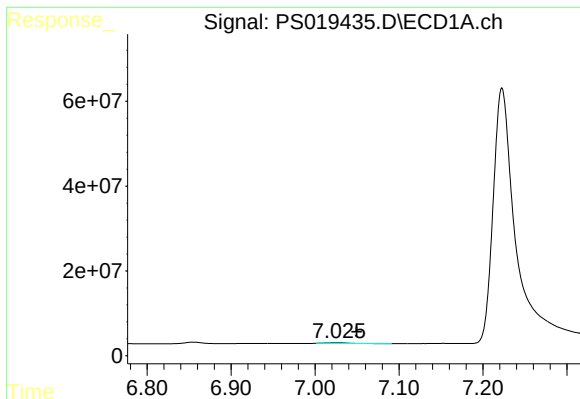

#3 4-Nitrophenol


R.T.: 7.026 min
Delta R.T.: -0.023 min
Response: 2106258
Conc: 2.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

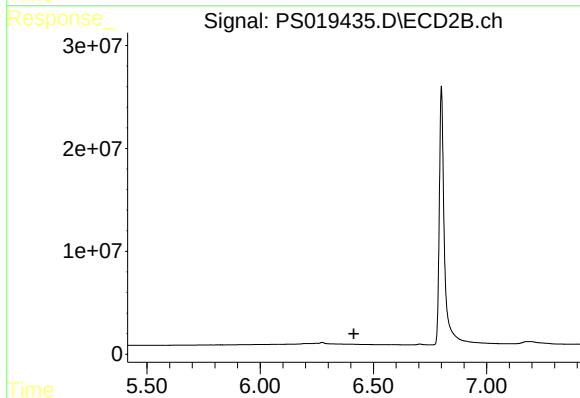


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

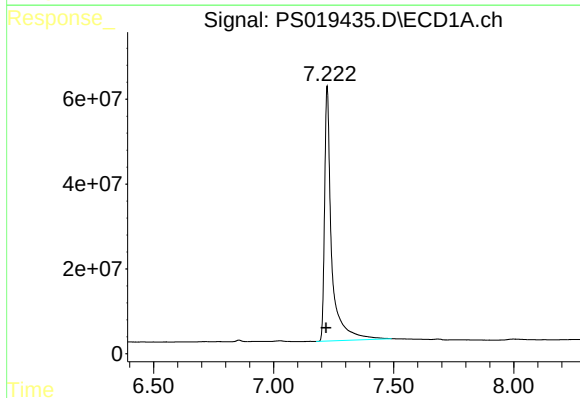


#4 2,4-DCAA

R.T.: 7.223 min
Delta R.T.: 0.004 min
Response: 1231168492
Conc: 450.83 ng/ml

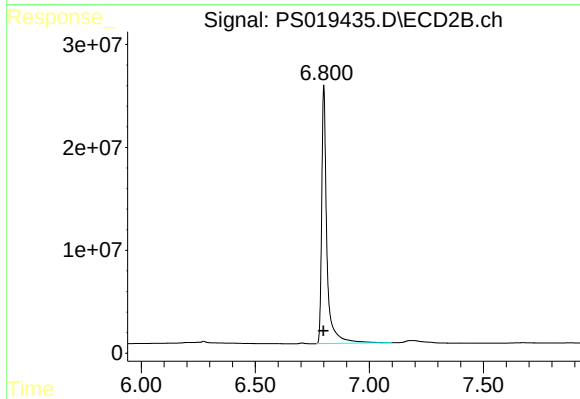

#4 2,4-DCAA


R.T.: 6.800 min
Delta R.T.: 0.002 min
Response: 398280387
Conc: 514.20 ng/ml

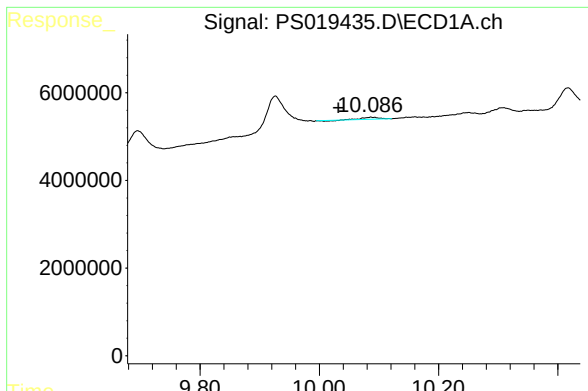

#13 2,4-DB


R.T.: 10.086 min
Delta R.T.: 0.054 min
Response: 810879
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

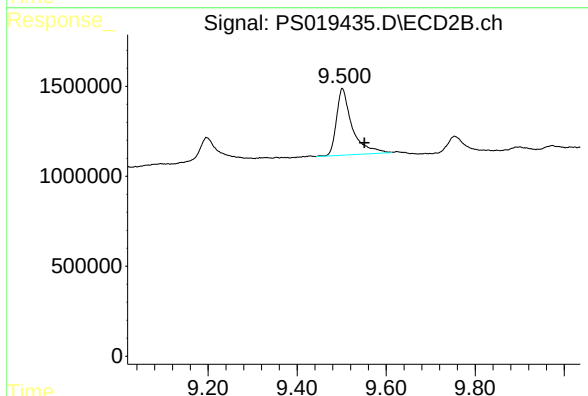


#13 2,4-DB

R.T.: 9.502 min
Delta R.T.: -0.050 min
Response: 9086119
Conc: 15.98 ng/ml

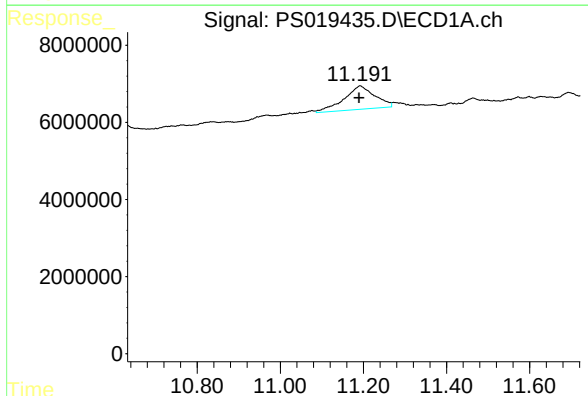

#14 DINOSEB

R.T.: 11.192 min
Delta R.T.: 0.003 min
Response: 31291990
Conc: 1.90 ng/ml

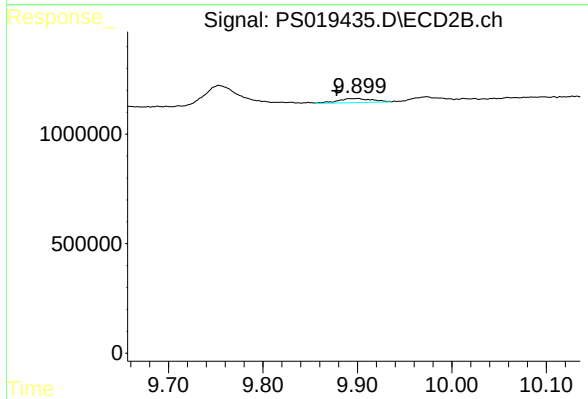

#14 DINOSEB

R.T.: 9.901 min
Delta R.T.: 0.022 min
Response: 478757
Conc: N.D.