

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
 Data File : PS010323.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 09:47
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 14:50:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.922	0	4899253	N.D.	9.135
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	965244	N.D.	<MDL
6) T	MCP	0.000	7.238	0	1224783	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.745	0	1274326	N.D.	2.257
9) T	2,4-D	8.418	8.014	7567862	1559079	10.712	2.248 #
10) T	Pentachlo...	0.000	8.441	0	1152825	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.801	0	2129599	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	4487151	N.D.	1.543
13) T	2,4-DB	0.000	9.703	0	2192039	N.D.	5.500
14) T	DINOSEB	0.000	10.022	0	1284858	N.D.	<MDL
15) T	Picloram	11.030	11.006	36221478	45961615	7.900	10.886 #
16) T	DCPA	0.000	10.951	0	3385066	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
Data File : PS010323.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 09:47
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 14:50:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

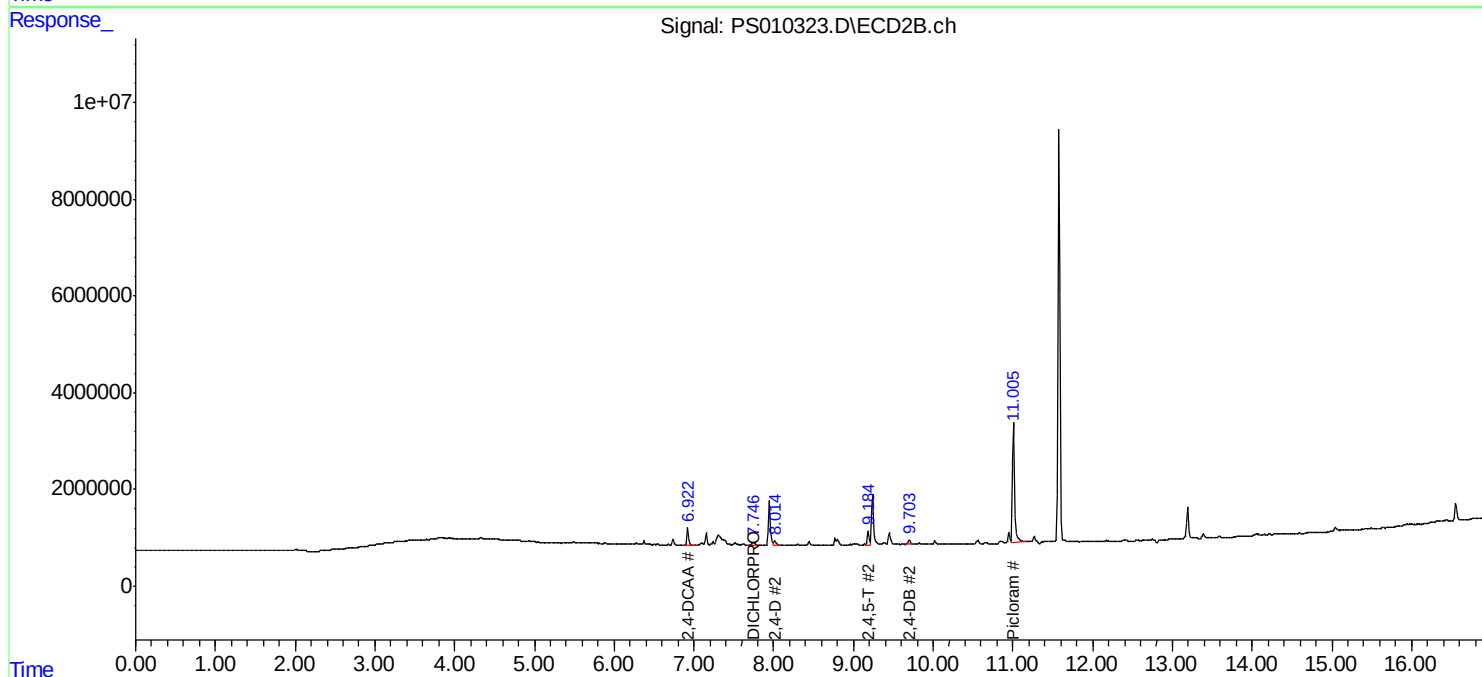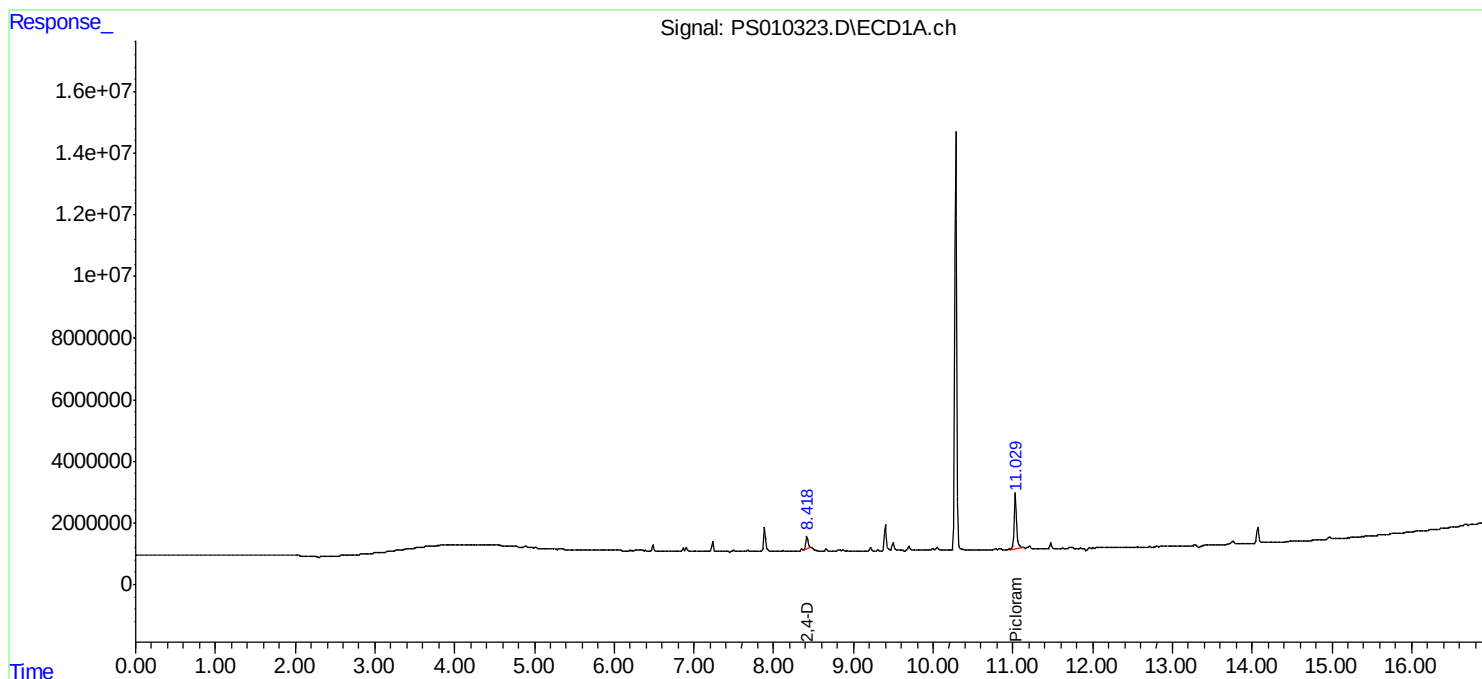


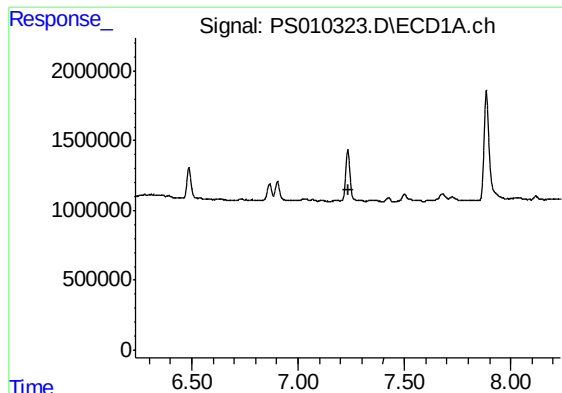

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

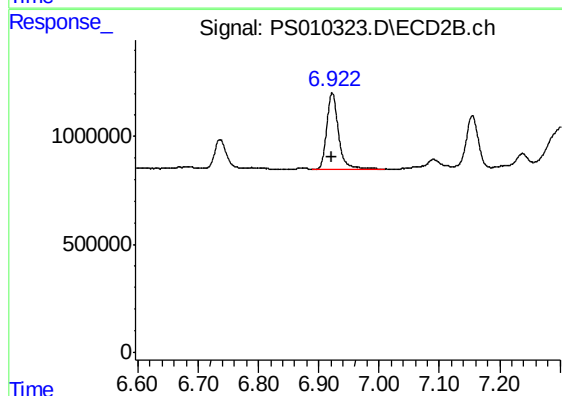


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 4899253
Conc: 9.14 ng/ml

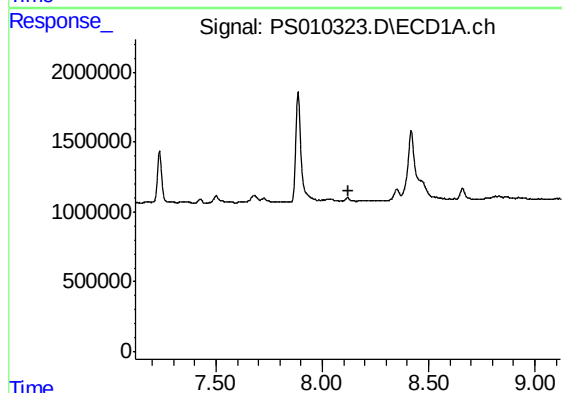


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

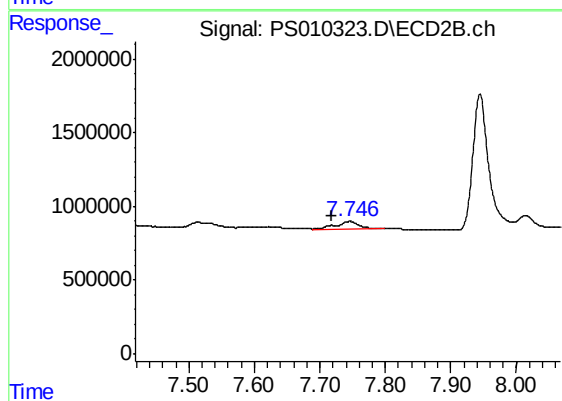

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.027 min
Response: 1274326
Conc: 2.26 ng/ml

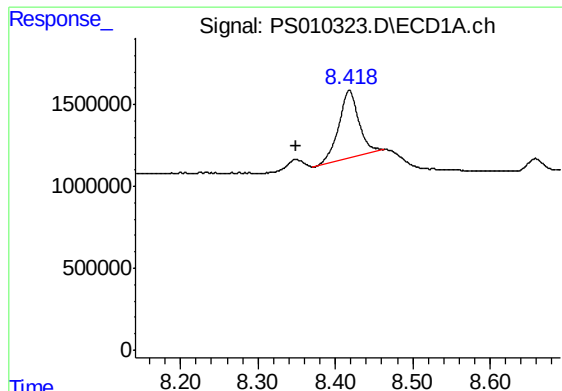

#9 2,4-D


R.T.: 8.418 min
Delta R.T.: 0.069 min
Response: 7567862
Conc: 10.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

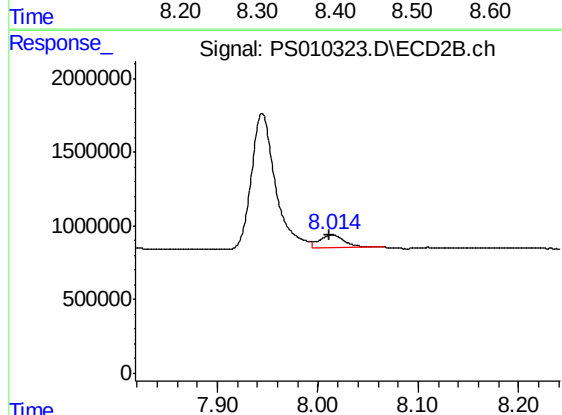


#9 2,4-D

R.T.: 8.014 min
Delta R.T.: 0.003 min
Response: 1559079
Conc: 2.25 ng/ml

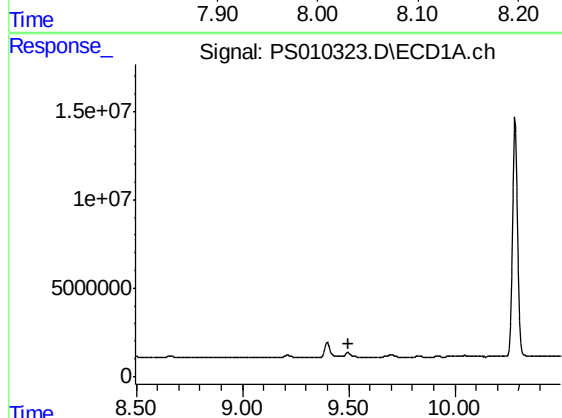


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.497 min
Response: 0
Conc: N.D.

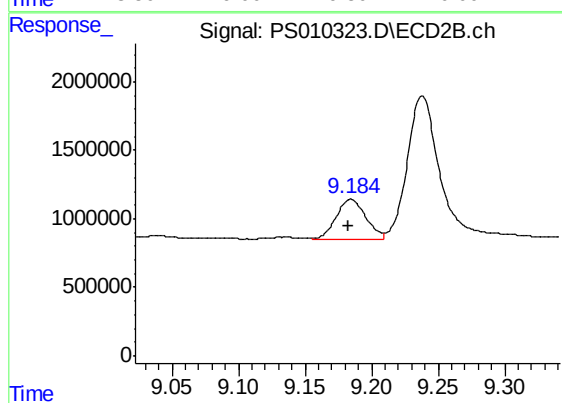

#12 2,4,5-T


R.T.: 9.184 min
Delta R.T.: 0.002 min
Response: 4487151
Conc: 1.54 ng/ml

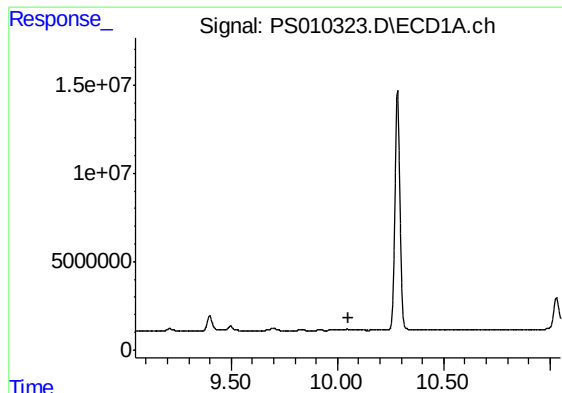

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

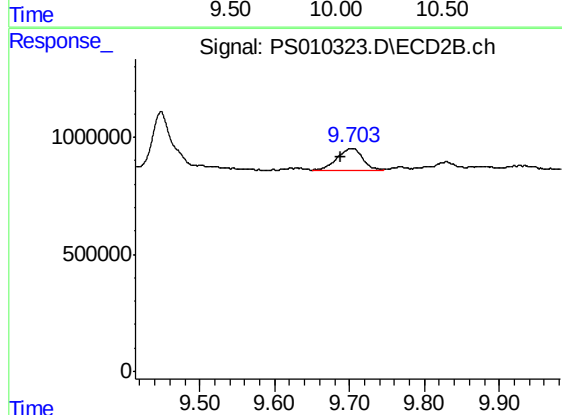


#13 2,4-DB

R.T.: 9.703 min
Delta R.T.: 0.014 min
Response: 2192039
Conc: 5.50 ng/ml

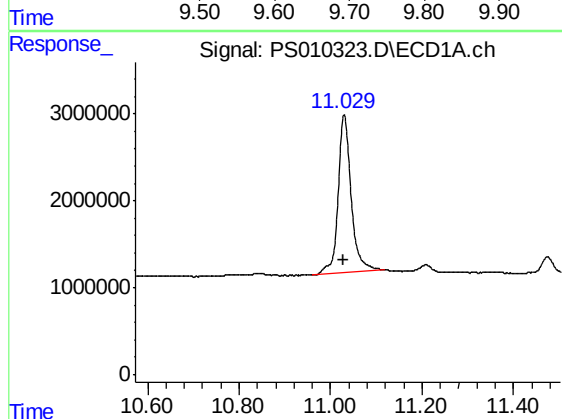

#15 Picloram

R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 36221478
Conc: 7.90 ng/ml

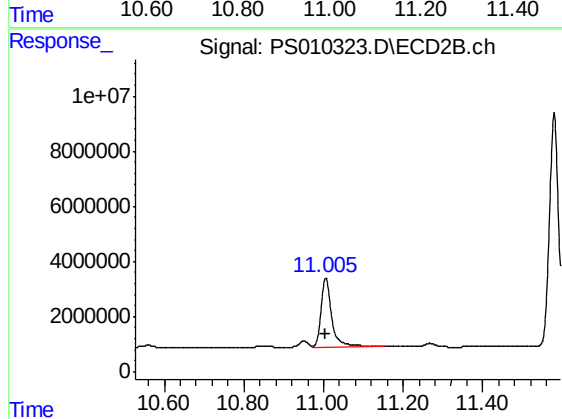

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.002 min
Response: 45961615
Conc: 10.89 ng/ml