

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
 Data File : PS010324.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 10:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 14:51:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.921	308.6E6	264.8E6	438.895	493.721
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	1655937	N.D.	<MDL
6) T	MCP	0.000	7.153	0	816437	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.713	0	592493	N.D.	1.049
9) T	2,4-D	0.000	8.016	0	909429	N.D.	1.312
11) T	2,4,5-TP ...	0.000	8.801	0	1363341	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	3519594	N.D.	1.211
13) T	2,4-DB	0.000	9.694	0	838225	N.D.	2.103
14) T	DINOSEB	0.000	10.022	0	624513	N.D.	<MDL
15) T	Picloram	11.031	11.006	25475320	35327033	5.557	8.368 #
16) T	DCPA	0.000	10.950	0	2353459	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
Data File : PS010324.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 10:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 14:51:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

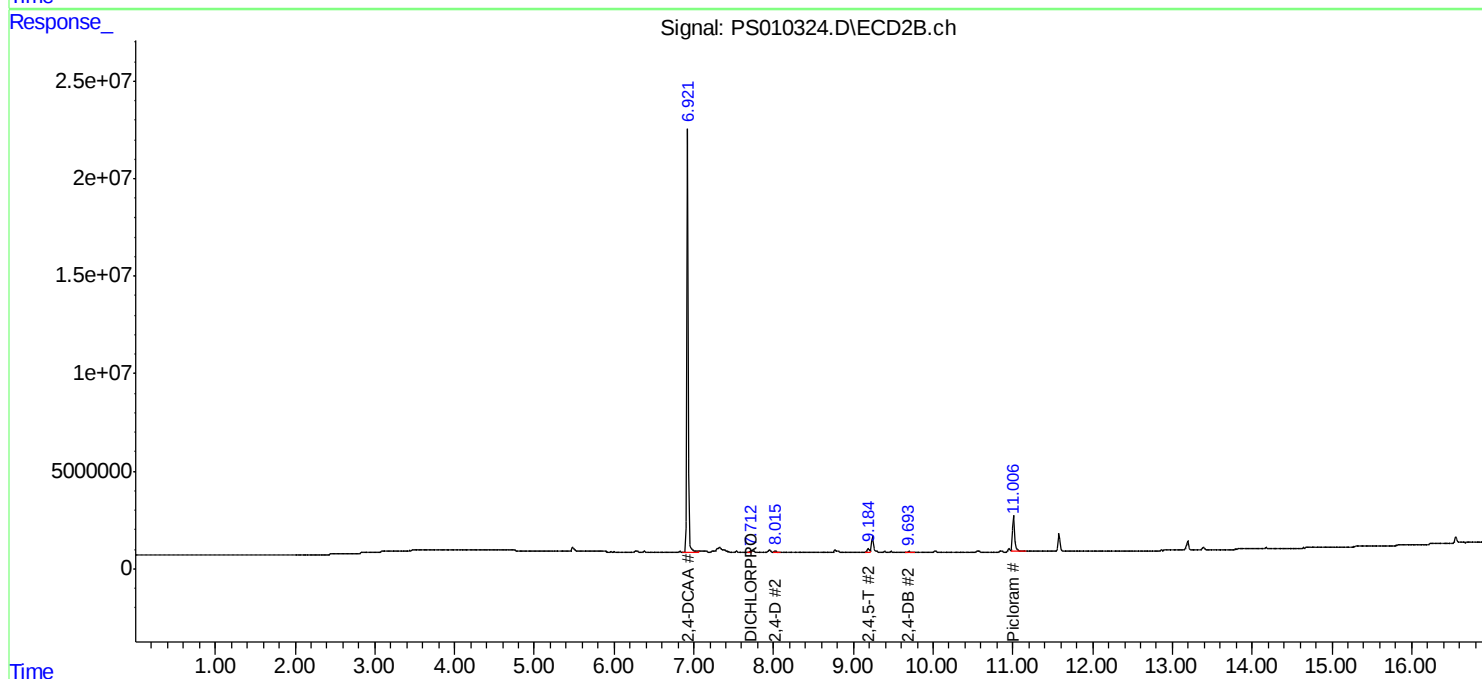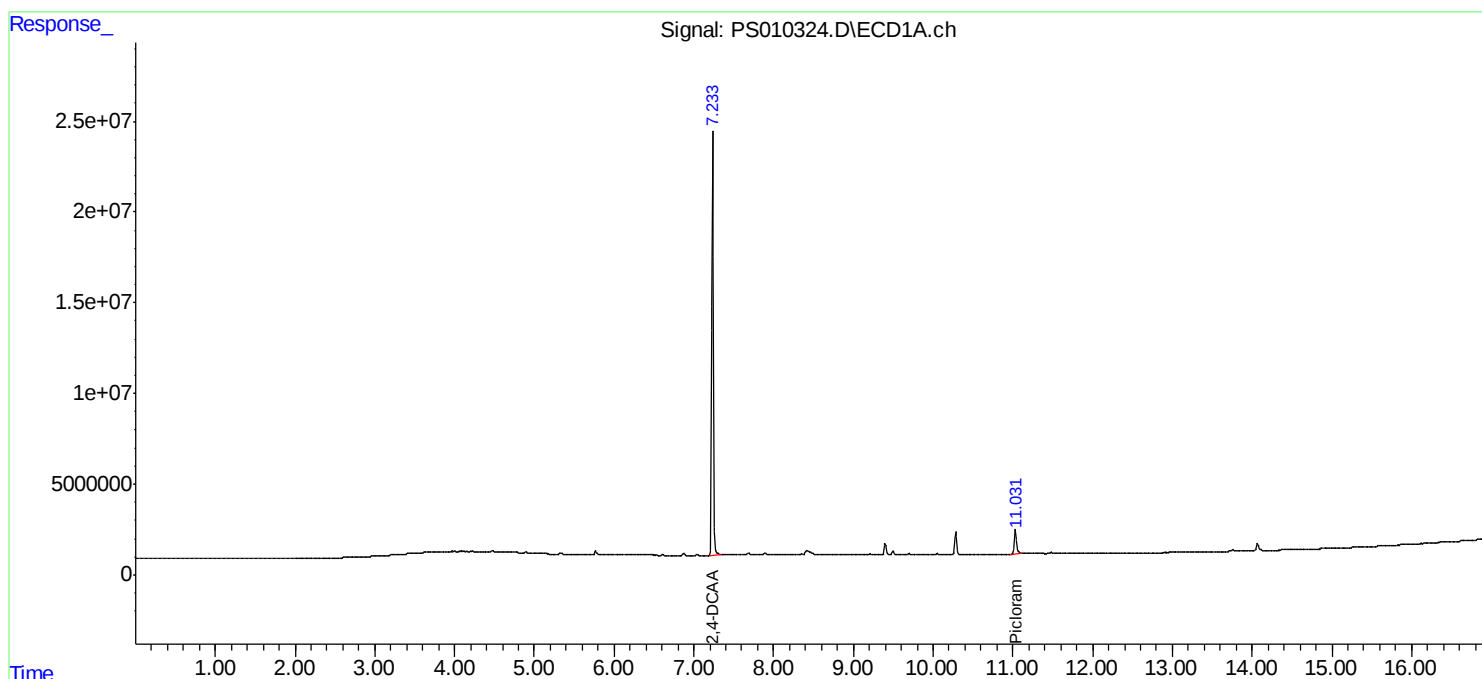


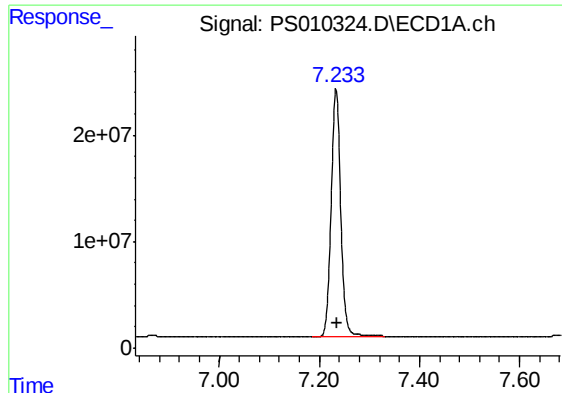

#4 2,4-DCAA


R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 308585013
Conc: 438.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

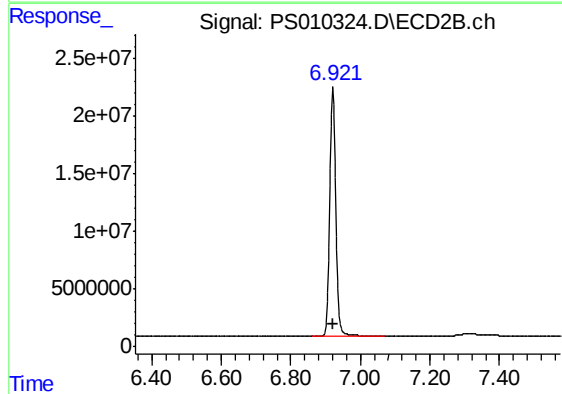


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 264778469
Conc: 493.72 ng/ml

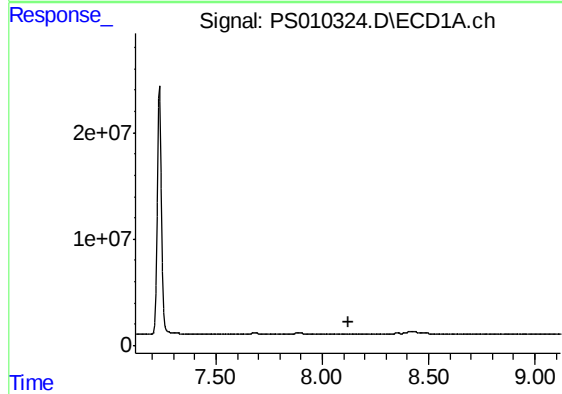


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

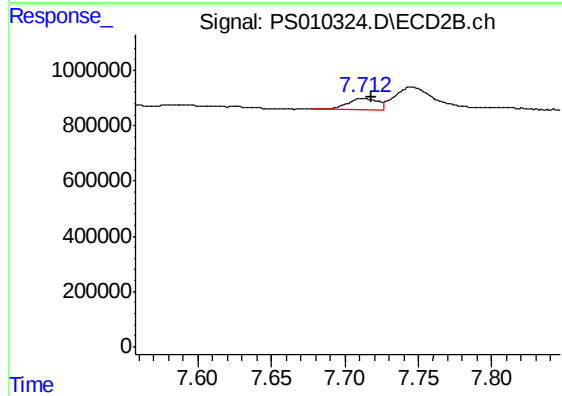

#8 DICHLORPROP


R.T.: 7.713 min
Delta R.T.: -0.005 min
Response: 592493
Conc: 1.05 ng/ml

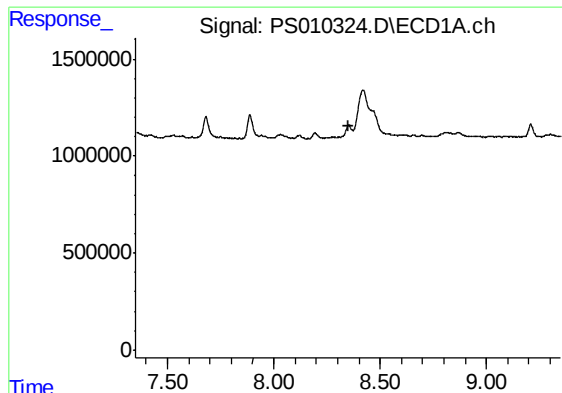

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 8.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

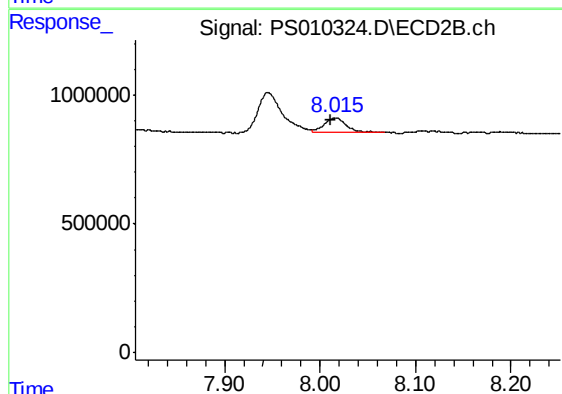


#9 2,4-D

R.T.: 8.016 min
Delta R.T.: 0.005 min
Response: 909429
Conc: 1.31 ng/ml

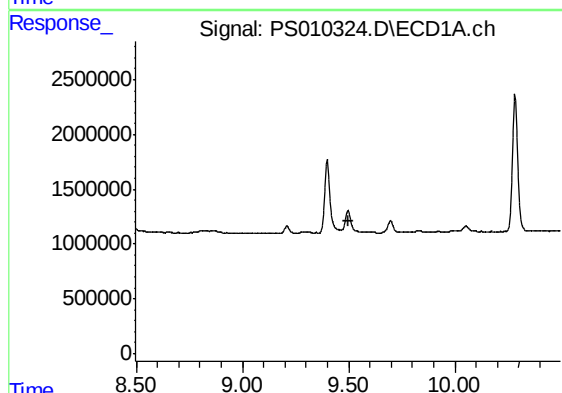


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.497 min
Response: 0
Conc: N.D.

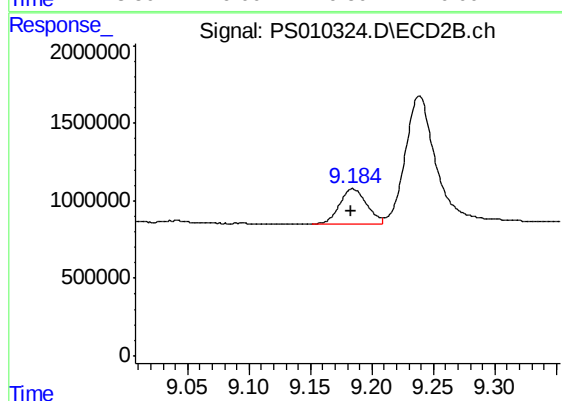

#12 2,4,5-T


R.T.: 9.185 min
Delta R.T.: 0.002 min
Response: 3519594
Conc: 1.21 ng/ml

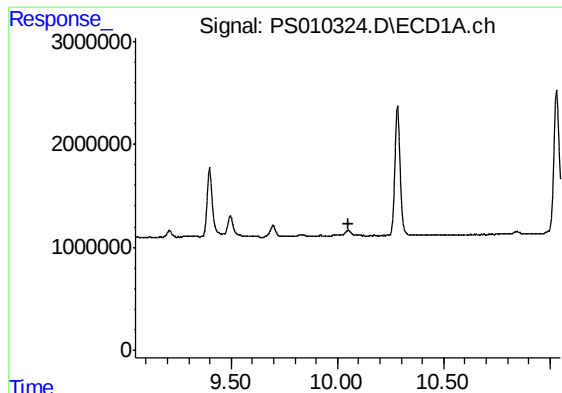

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

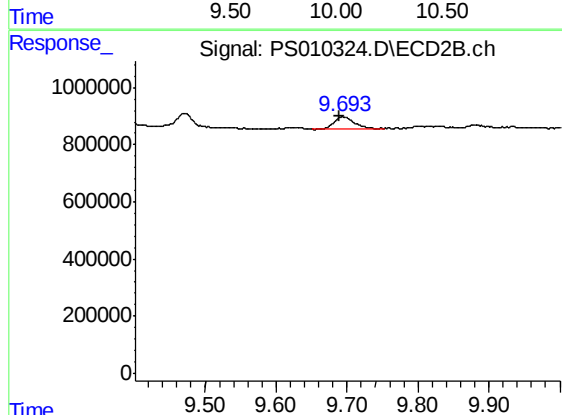


#13 2,4-DB

R.T.: 9.694 min
Delta R.T.: 0.004 min
Response: 838225
Conc: 2.10 ng/ml

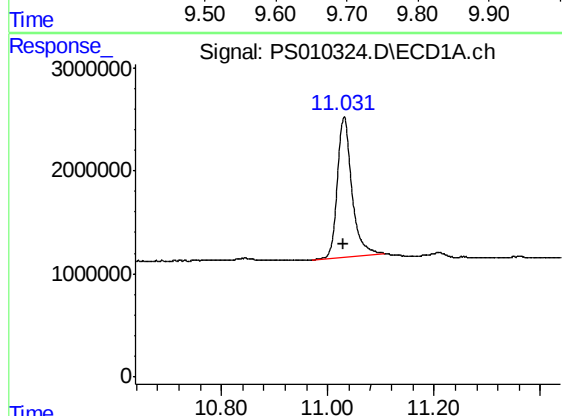

#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.002 min
Response: 25475320
Conc: 5.56 ng/ml

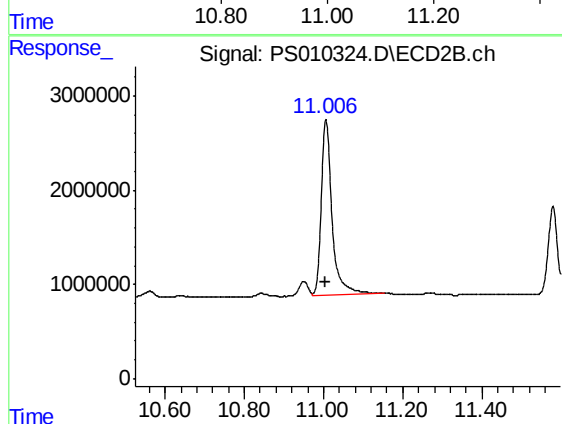

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.003 min
Response: 35327033
Conc: 8.37 ng/ml