

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
 Data File : PS010330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2020 15:37
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 16:22:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.921	316.1E6	270.2E6	449.550	503.798
Target Compounds							
2) T	3,5-DICHL...	0.000	6.099	0	221166	N.D.	<MDL
5) T	DICAMBA	0.000	7.088	0	1181473	N.D.	<MDL
6) T	MCPD	0.000	7.234	0	4275079	N.D.	2.329
7) T	MCPA	0.000	7.482	0	271255	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	1048684	N.D.	1.857
11) T	2,4,5-TP ...	0.000	8.773	0	438453	N.D.	<MDL
12) T	2,4,5-T	0.000	9.244	0	499318	N.D.	<MDL
13) T	2,4-DB	0.000	9.709	0	261137	N.D.	<MDL
15) T	Picloram	0.000	11.012	0	852807	N.D.	<MDL
16) T	DCPA	0.000	10.951	0	212421	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051820\
Data File : PS010330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2020 15:37
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 16:22:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

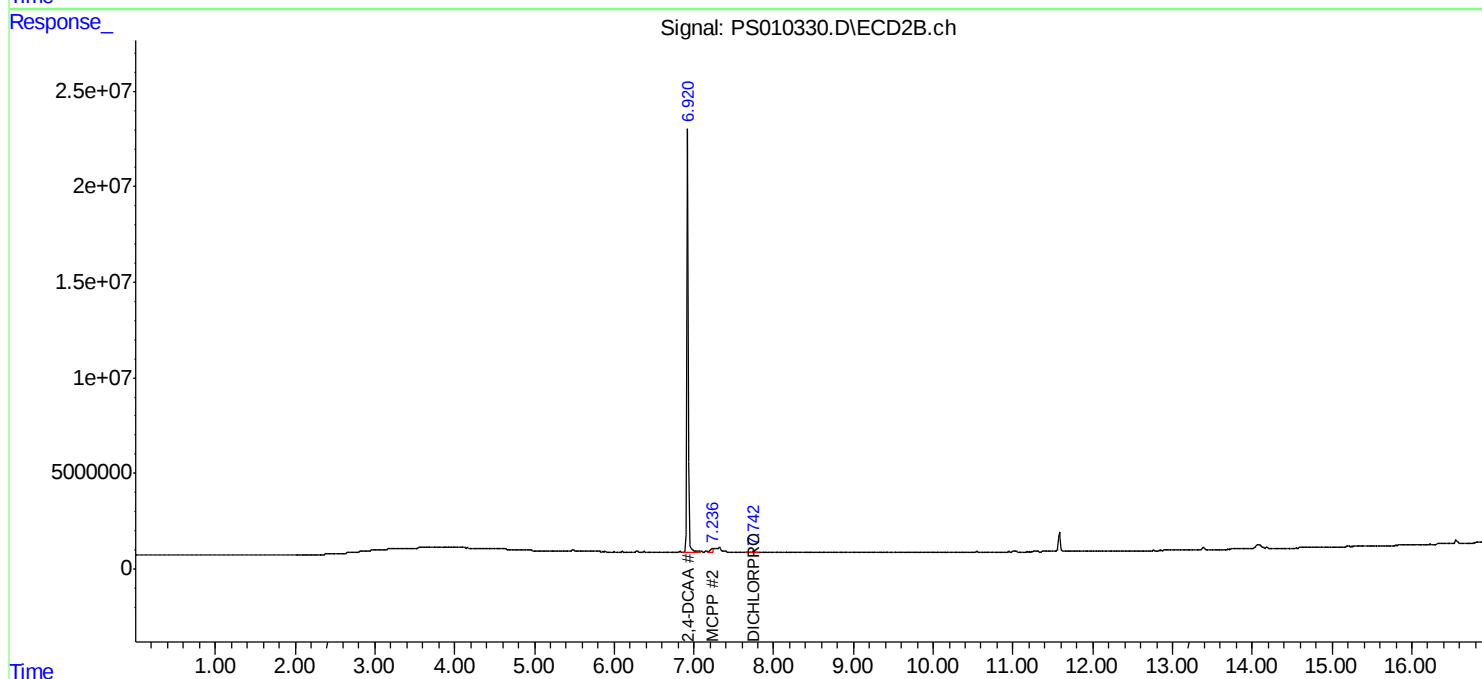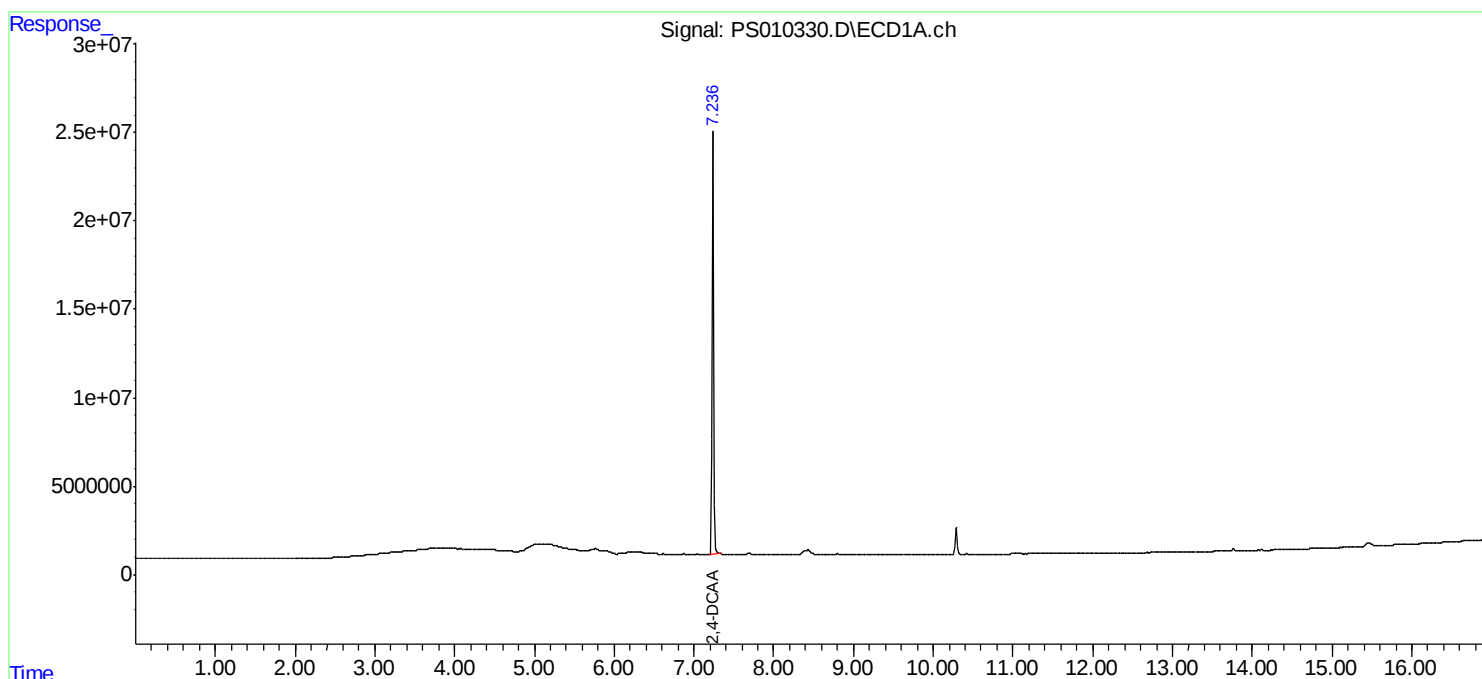


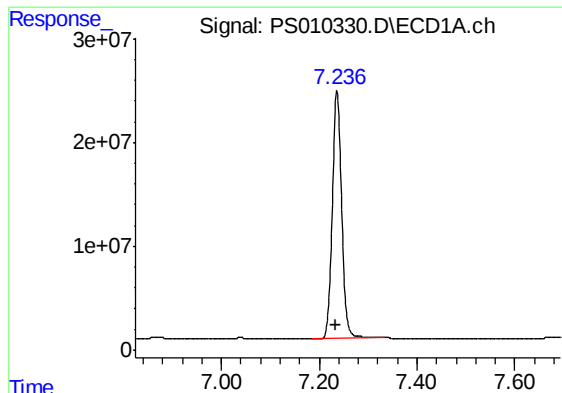

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: 0.002 min
Response: 316076192
Conc: 449.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

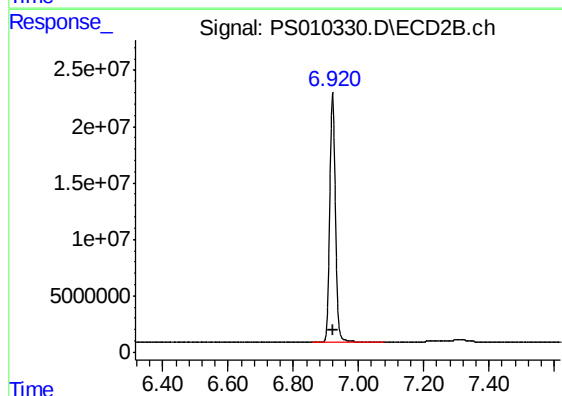


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: -0.001 min
Response: 270182337
Conc: 503.80 ng/ml

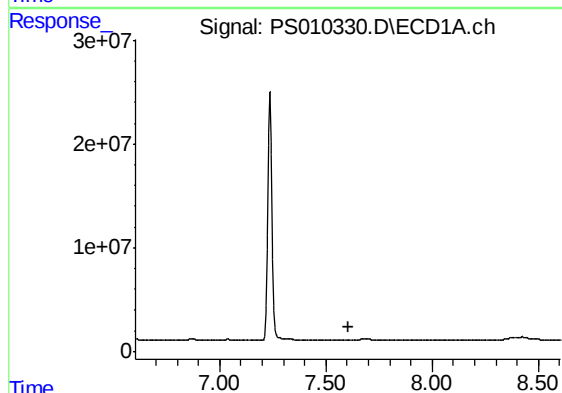


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.604 min
Response: 0
Conc: N.D.

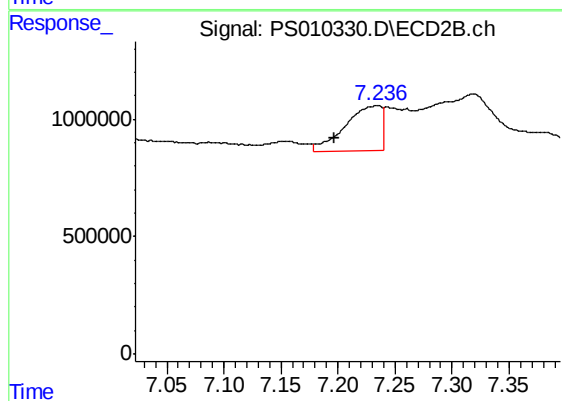

#6 MCPP


R.T.: 7.234 min
Delta R.T.: 0.037 min
Response: 4275079
Conc: 2.33 ug/ml

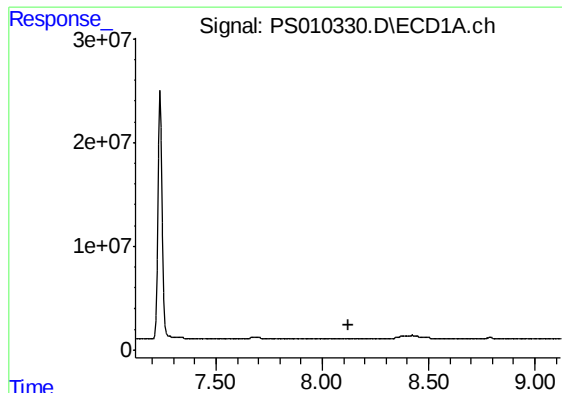

#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

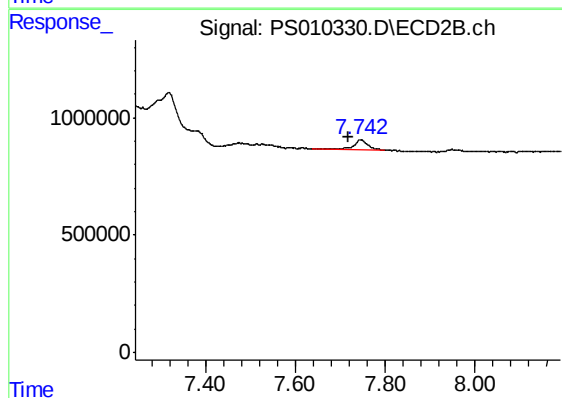

#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.025 min
Response: 1048684
Conc: 1.86 ng/ml