

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051821\
 Data File : PS015027.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 May 2021 17:48
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 18:48:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.887	694.7E6	267.7E6	415.204	553.111 #
Target Compounds							
5) T	DICAMBA	7.349	7.055	6556607	5004308	1.001	2.337 #
9) T	2,4-D	8.325f	0.000	41960068	0	23.579	N.D. #
10) T	Pentachlo...	8.577	0.000	4052962	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.129	0.000	6507892	0	<MDL	N.D. #
12) T	2,4,5-T	9.448f	0.000	18417831	0	2.014	N.D. #
15) T	Picloram	10.980f	11.004f	129.5E6	45240660	10.664	11.354



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051821\
Data File : PS015027.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 May 2021 17:48
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 18:48:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

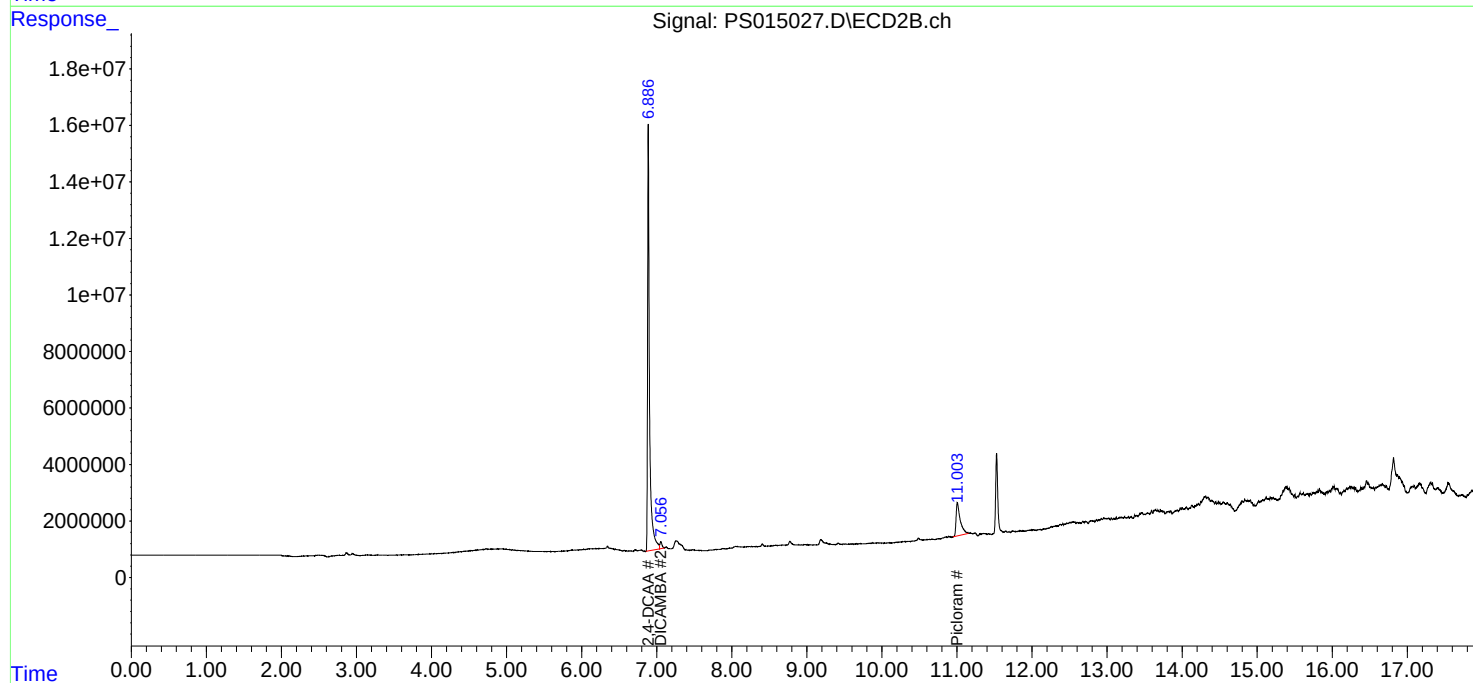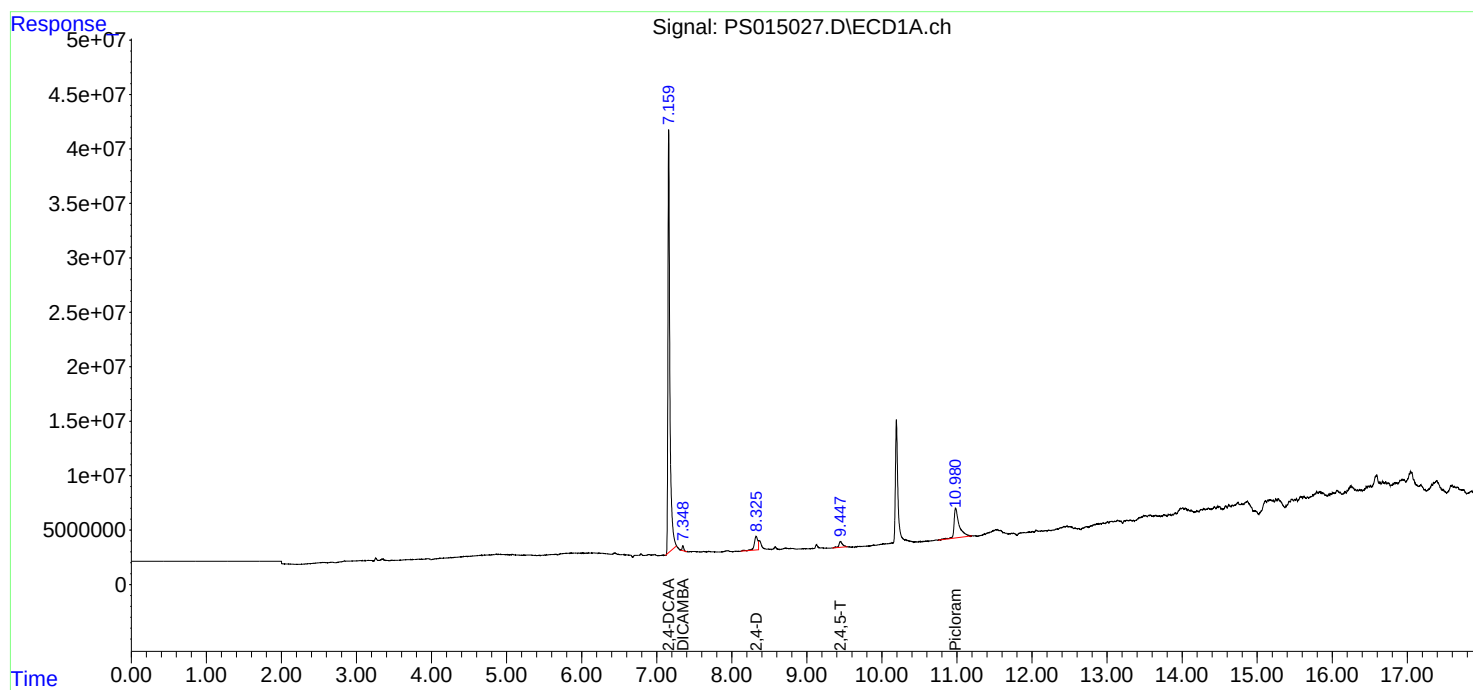


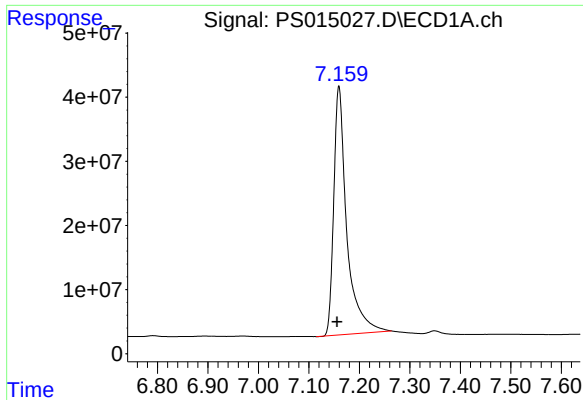

#4 2,4-DCAA


R.T.: 7.159 min
Delta R.T.: 0.004 min
Response: 694739867
Conc: 415.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

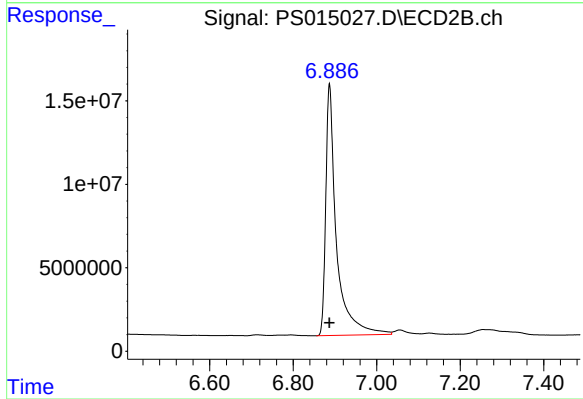


#4 2,4-DCAA

R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 267657693
Conc: 553.11 ng/ml

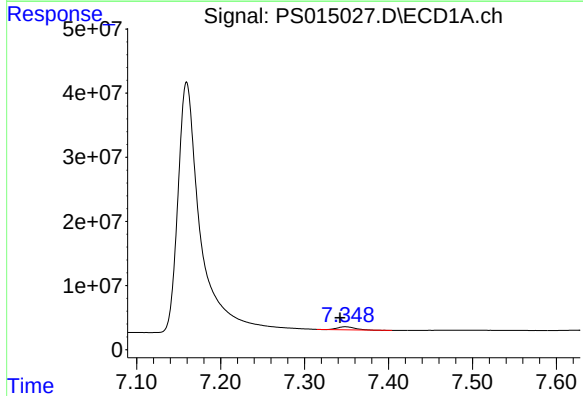


#5 DICAMBA

R.T.: 7.349 min
Delta R.T.: 0.006 min
Response: 6556607
Conc: 1.00 ng/ml

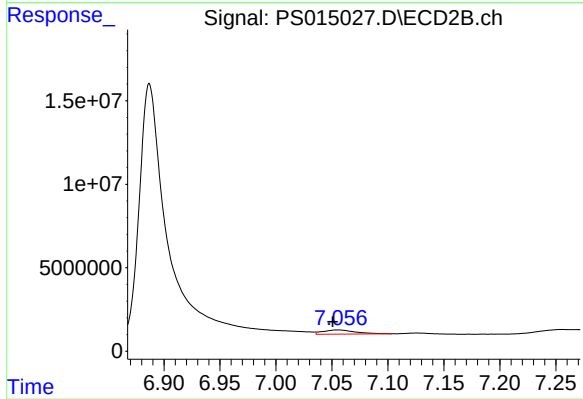

#5 DICAMBA


R.T.: 7.055 min
Delta R.T.: 0.004 min
Response: 5004308
Conc: 2.34 ng/ml

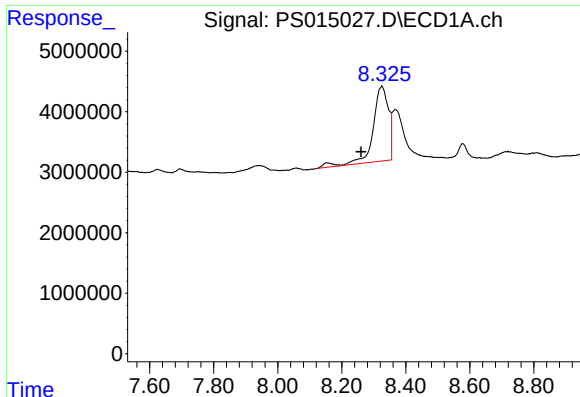

#9 2,4-D


R.T.: 8.325 min
Delta R.T.: 0.065 min
Response: 41960068
Conc: 23.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

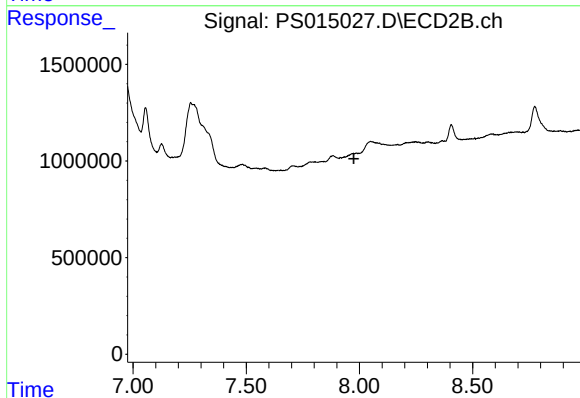


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.975 min
Response: 0
Conc: N.D.

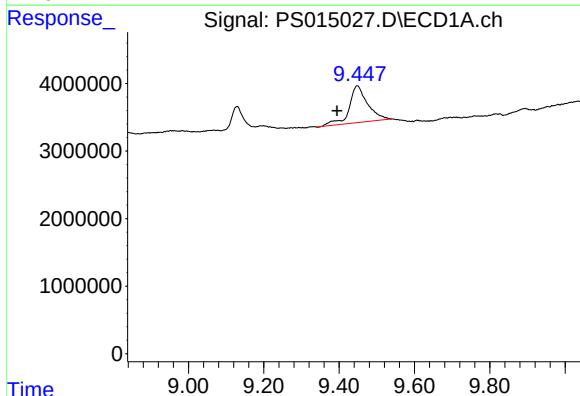


#12 2,4,5-T

R.T.: 9.448 min
Delta R.T.: 0.054 min
Response: 18417831
Conc: 2.01 ng/ml

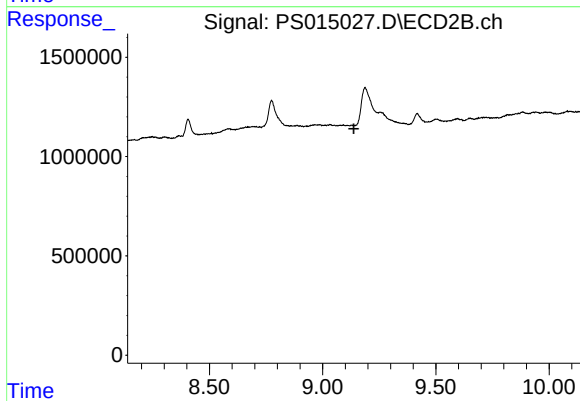

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 9.138 min
Response: 0
Conc: N.D.

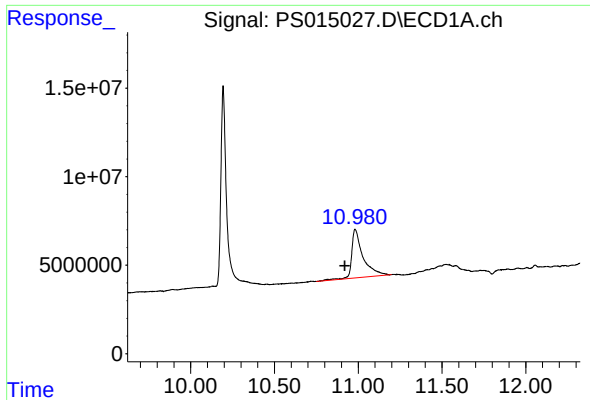

#15 Picloram

R.T.: 10.980 min
Delta R.T.: 0.062 min
Response: 129540614
Conc: 10.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

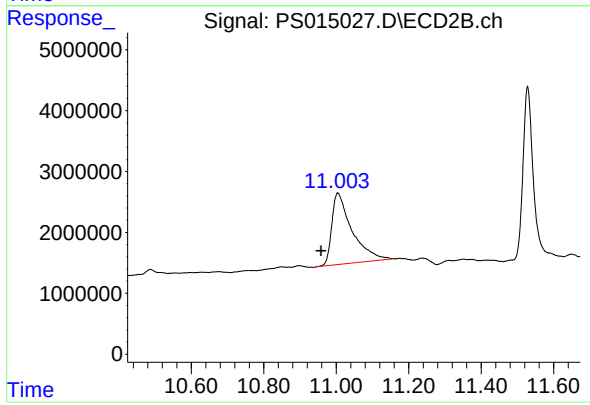

#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.046 min
Response: 45240660
Conc: 11.35 ng/ml