

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051822\
 Data File : PS019466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2022 02:15
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 02:31:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.798	2113.9E6	685.8E6	774.077	885.395
Target Compounds							
1) T	Dalapon	3.026	2.534	3247.1E6	639.6E6	672.590	719.561
2) T	3,5-DICHL...	6.431	5.975	2389.2E6	860.2E6	675.918	737.609
3) T	4-Nitroph...	7.056	6.418	783.4E6	272.5E6	808.337	772.402
5) T	DICAMBA	7.409	6.963	7450.2E6	2519.5E6	674.572	751.899
6) T	MCPD	7.579	7.061	599.4E6	199.9E6	67.052	75.177
7) T	MCPA	7.729	7.274	777.3E6	274.8E6	62.369	73.770
8) T	DICHLORPROP	8.103	7.586	1822.9E6	635.4E6	651.592	741.429
9) T	2,4-D	8.336	7.879	2086.4E6	746.6E6	661.347	747.632
10) T	Pentachlo...	8.640	8.305	25876.0E6	8431.8E6	658.646	750.060
11) T	2,4,5-TP ...	9.193	8.667	11854.8E6	3651.1E6	655.862	758.654
12) T	2,4,5-T	9.480	9.045	14033.6E6	3288.1E6	663.494	759.359
13) T	2,4-DB	10.037	9.552	2712.8E6	416.1E6	632.609	731.808
14) T	DINOSEB	11.186	9.876	12293.7E6	2430.8E6	744.563	838.815
15) T	Picloram	11.036	10.873	17884.3E6	4069.5E6	611.846	680.425
16) T	DCPA	11.454	10.806	17785.4E6	4454.4E6	679.586	758.783



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051822\
Data File : PS019466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2022 02:15
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 02:31:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

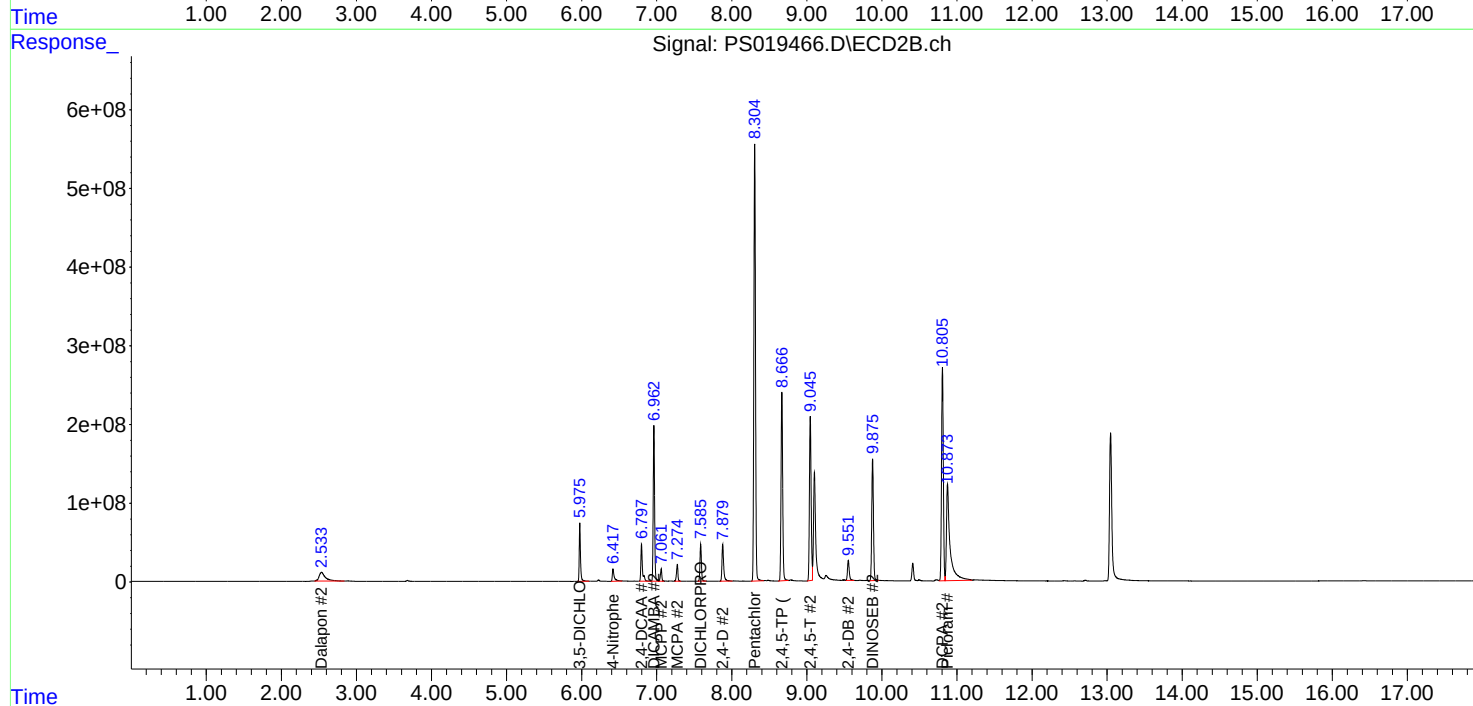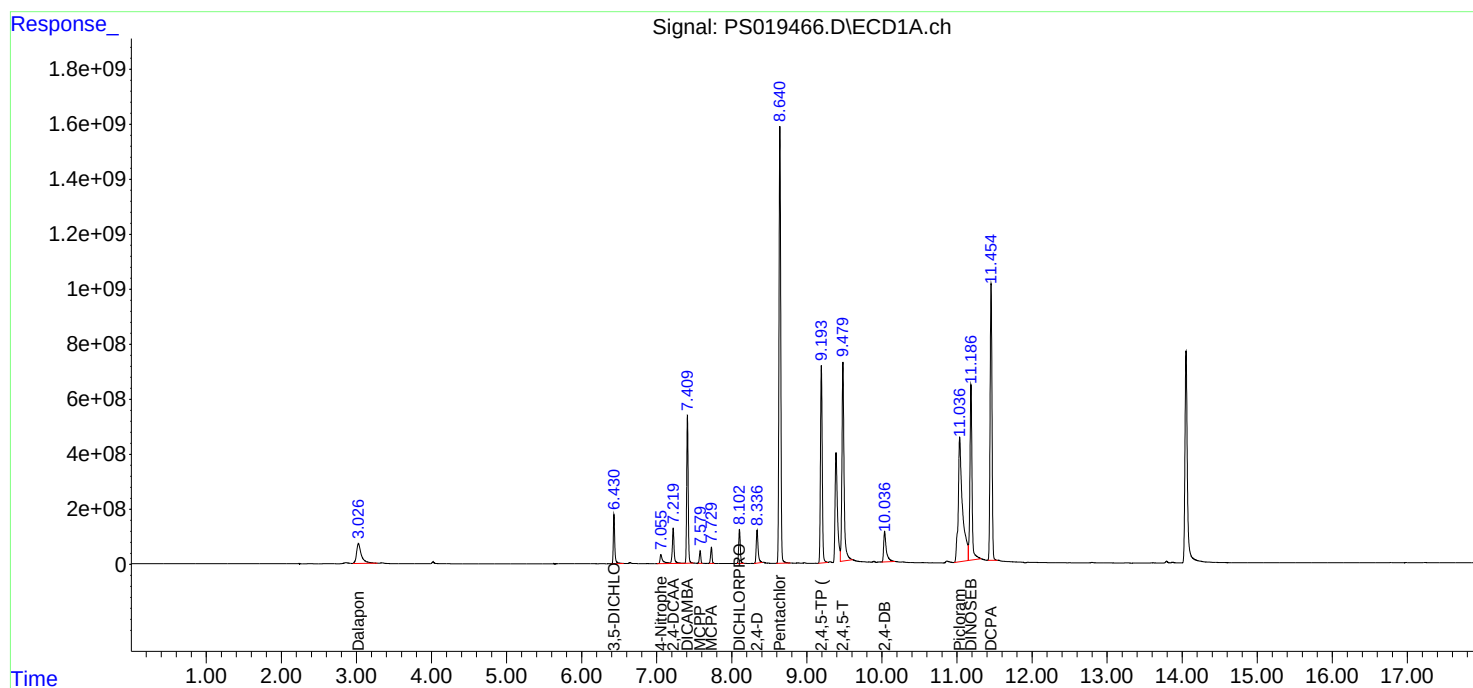


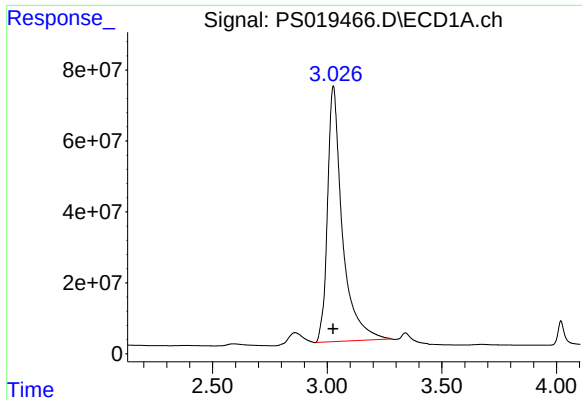

#1 Dalapon


R.T.: 3.026 min
Delta R.T.: 0.000 min
Response: 3247060772
Conc: 672.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

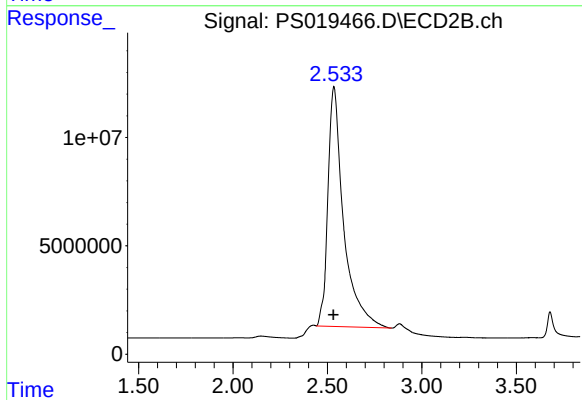


#1 Dalapon

R.T.: 2.534 min
Delta R.T.: 0.003 min
Response: 639633328
Conc: 719.56 ng/ml

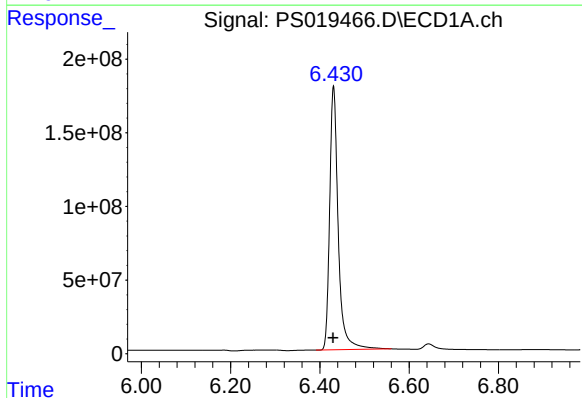


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.431 min
Delta R.T.: 0.000 min
Response: 2389152842
Conc: 675.92 ng/ml

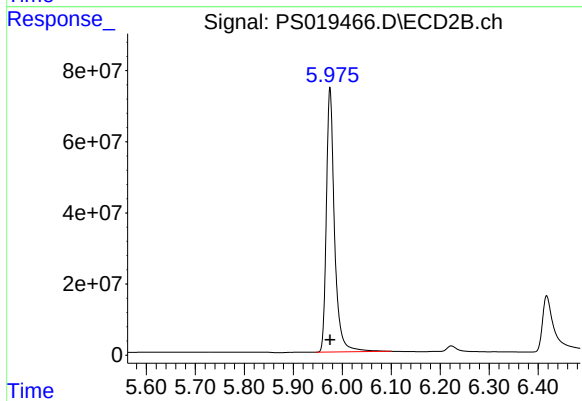

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.975 min
Delta R.T.: 0.000 min
Response: 860232009
Conc: 737.61 ng/ml

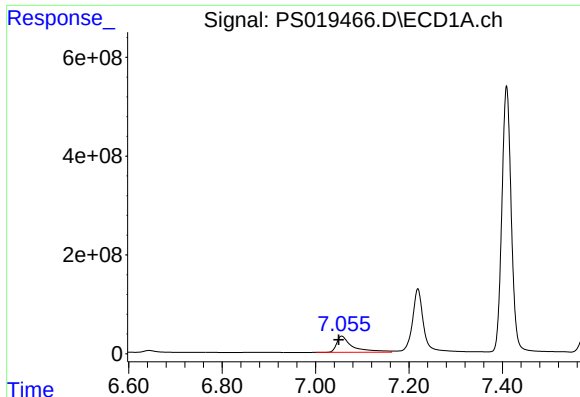

#3 4-Nitrophenol


R.T.: 7.056 min
Delta R.T.: 0.007 min
Response: 783350441
Conc: 808.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

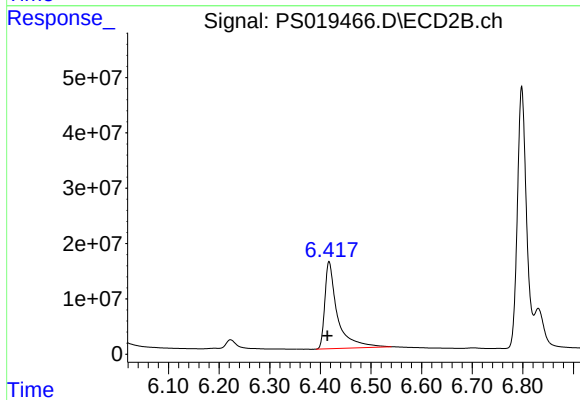


#3 4-Nitrophenol

R.T.: 6.418 min
Delta R.T.: 0.004 min
Response: 272529455
Conc: 772.40 ng/ml

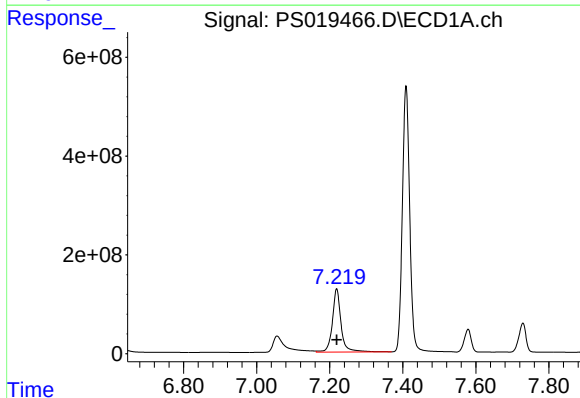


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 2113908729
Conc: 774.08 ng/ml

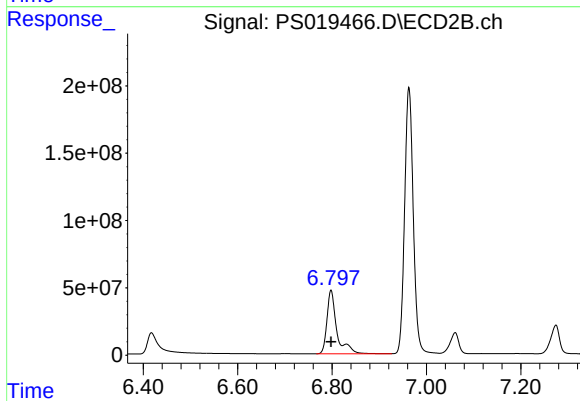

#4 2,4-DCAA


R.T.: 6.798 min
Delta R.T.: 0.000 min
Response: 685787882
Conc: 885.40 ng/ml

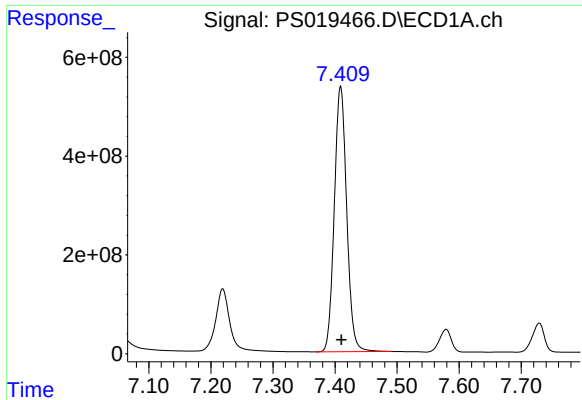

#5 DICAMBA


R.T.: 7.409 min
Delta R.T.: -0.001 min
Response: 7450174782
Conc: 674.57 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

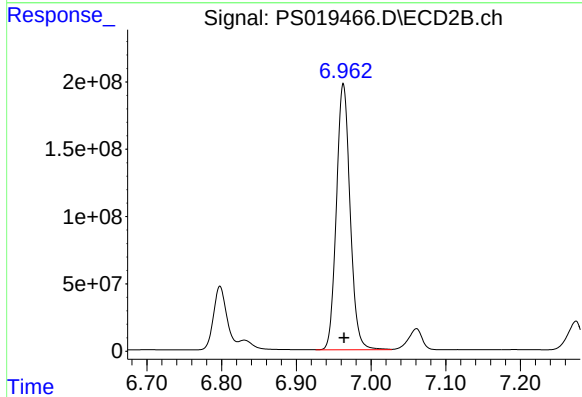


#5 DICAMBA

R.T.: 6.963 min
Delta R.T.: -0.001 min
Response: 2519476295
Conc: 751.90 ng/ml

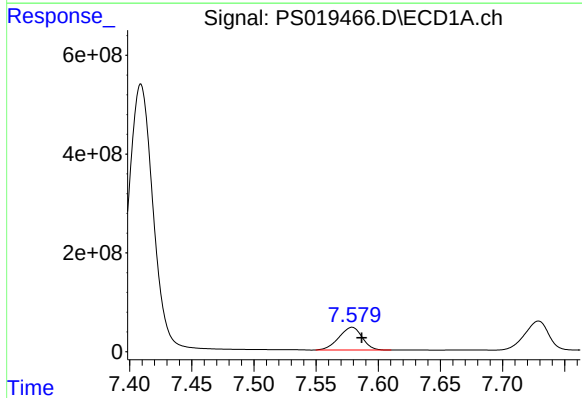


#6 MCP

R.T.: 7.579 min
Delta R.T.: -0.008 min
Response: 599393916
Conc: 67.05 ug/ml

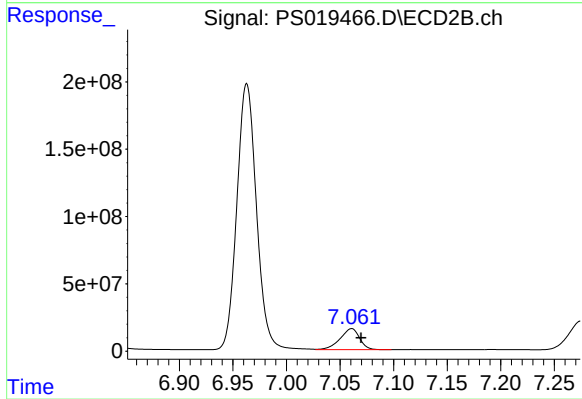

#6 MCP


R.T.: 7.061 min
Delta R.T.: -0.009 min
Response: 199919397
Conc: 75.18 ug/ml

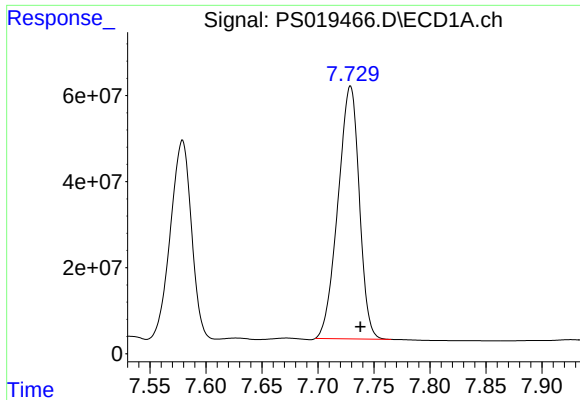

#7 MCPA


R.T.: 7.729 min
Delta R.T.: -0.009 min
Response: 777309459
Conc: 62.37 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

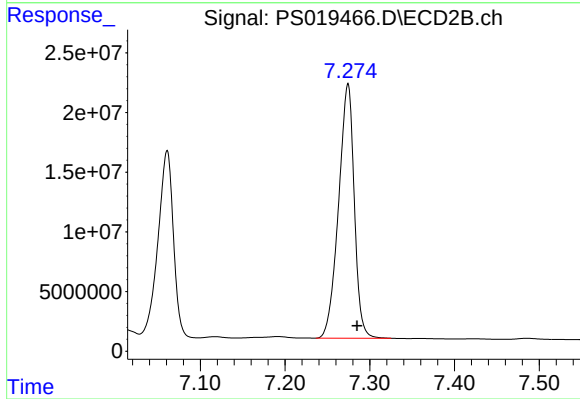


#7 MCPA

R.T.: 7.274 min
Delta R.T.: -0.011 min
Response: 274767000
Conc: 73.77 ug/ml

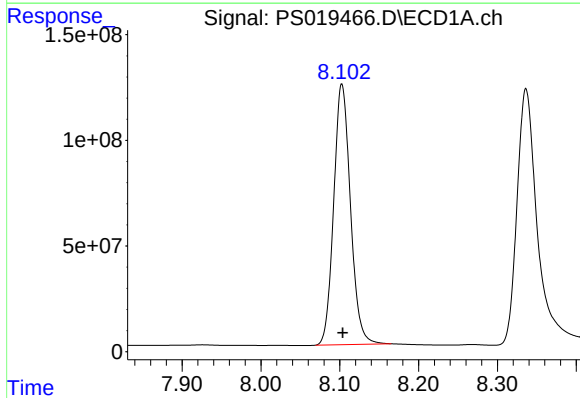


#8 DICHLORPROP

R.T.: 8.103 min
Delta R.T.: 0.000 min
Response: 1822880016
Conc: 651.59 ng/ml

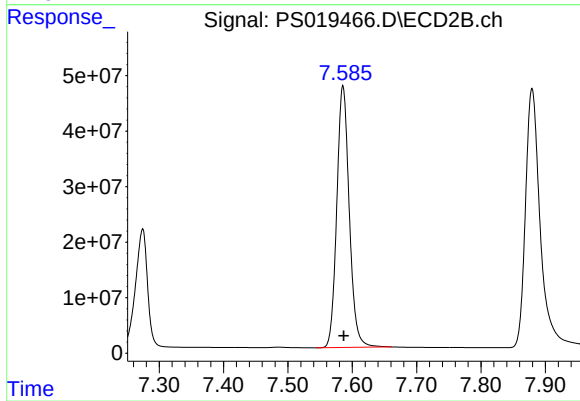

#8 DICHLORPROP


R.T.: 7.586 min
Delta R.T.: -0.001 min
Response: 635403041
Conc: 741.43 ng/ml

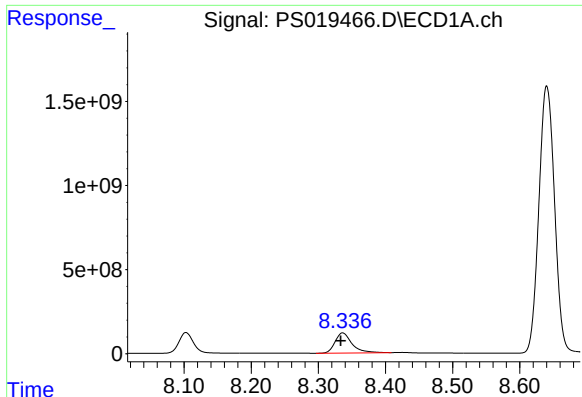

#9 2,4-D


R.T.: 8.336 min
Delta R.T.: 0.003 min
Response: 2086410301
Conc: 661.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

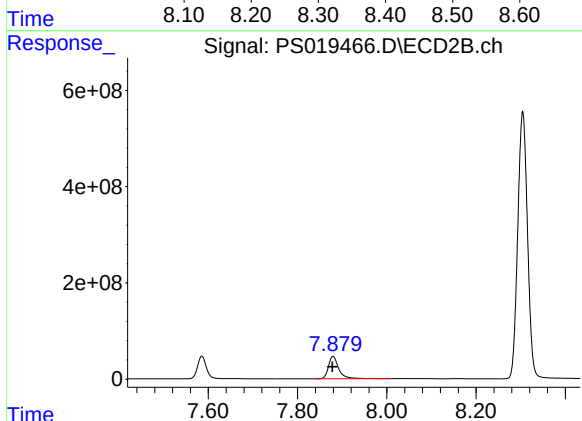


#9 2,4-D

R.T.: 7.879 min
Delta R.T.: 0.001 min
Response: 746609638
Conc: 747.63 ng/ml

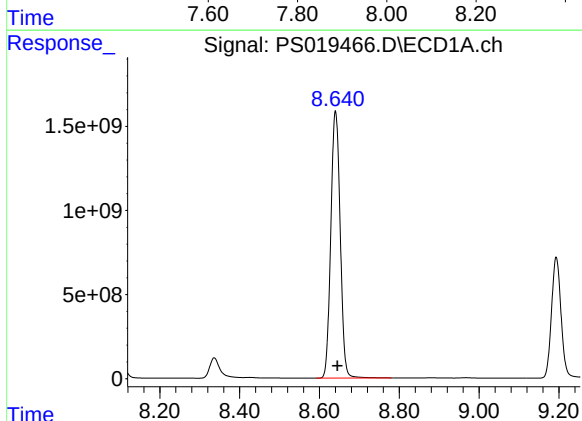


#10 Pentachlorophenol

R.T.: 8.640 min
Delta R.T.: -0.004 min
Response: 25875961550
Conc: 658.65 ng/ml

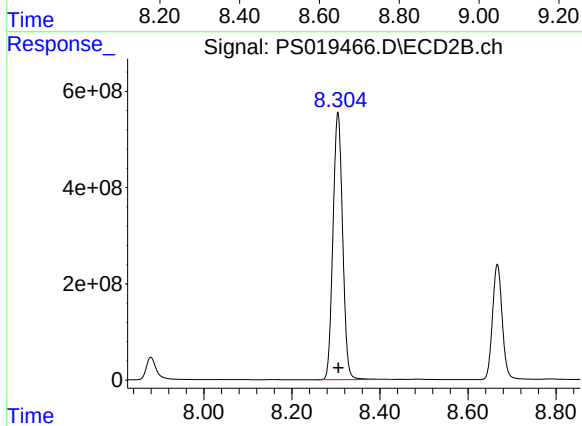

#10 Pentachlorophenol


R.T.: 8.305 min
Delta R.T.: -0.001 min
Response: 8431760684
Conc: 750.06 ng/ml

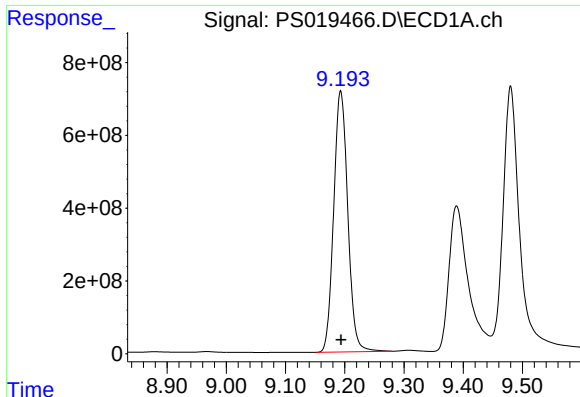

#11 2,4,5-TP (SILVEX)


R.T.: 9.193 min
Delta R.T.: 0.000 min
Response: 11854789408
Conc: 655.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

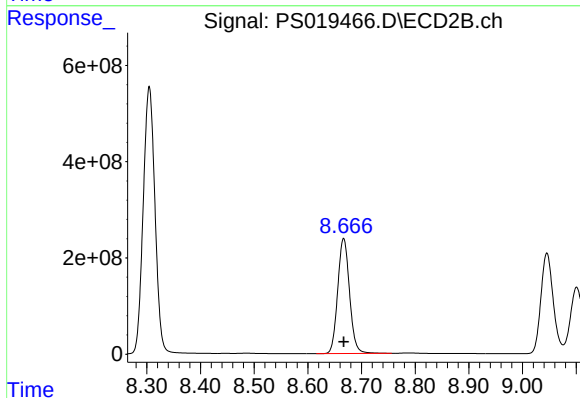


#11 2,4,5-TP (SILVEX)

R.T.: 8.667 min
Delta R.T.: 0.000 min
Response: 3651057108
Conc: 758.65 ng/ml

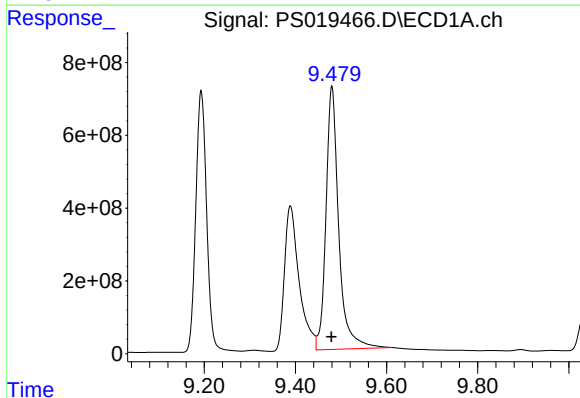


#12 2,4,5-T

R.T.: 9.480 min
Delta R.T.: 0.001 min
Response: 14033611810
Conc: 663.49 ng/ml

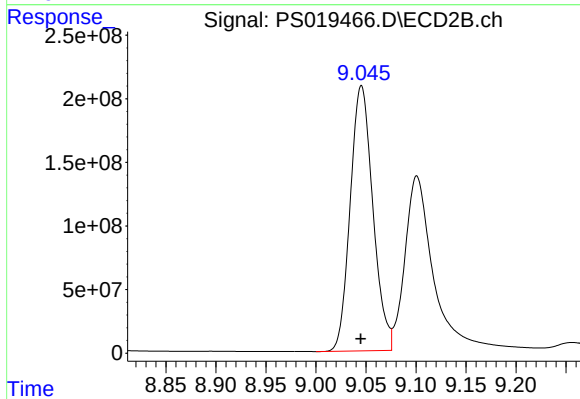

#12 2,4,5-T


R.T.: 9.045 min
Delta R.T.: 0.000 min
Response: 3288069120
Conc: 759.36 ng/ml

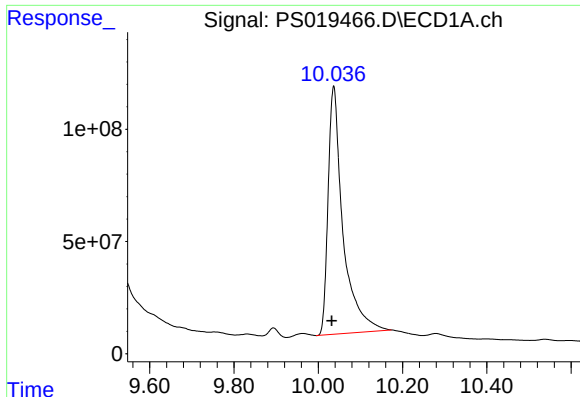

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: 0.005 min
Response: 2712790579
Conc: 632.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

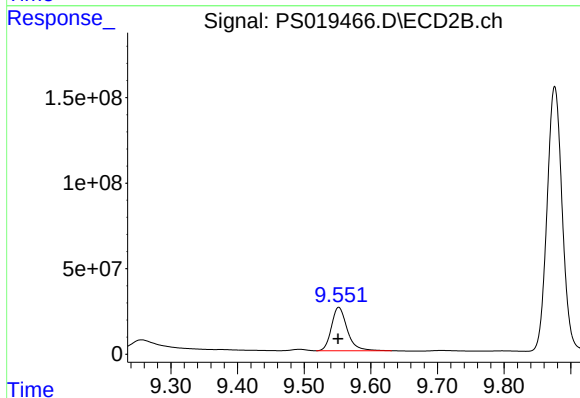


#13 2,4-DB

R.T.: 9.552 min
Delta R.T.: 0.000 min
Response: 416078056
Conc: 731.81 ng/ml

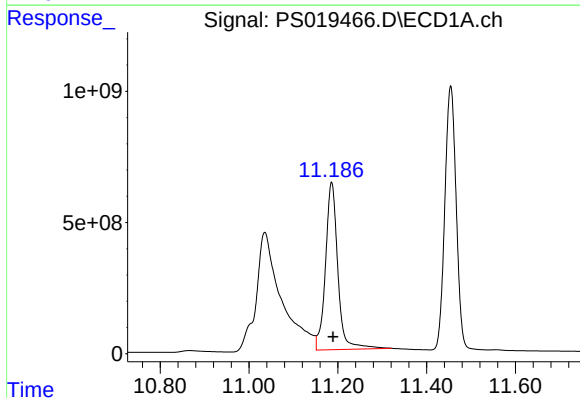


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.003 min
Response: 12293740863
Conc: 744.56 ng/ml

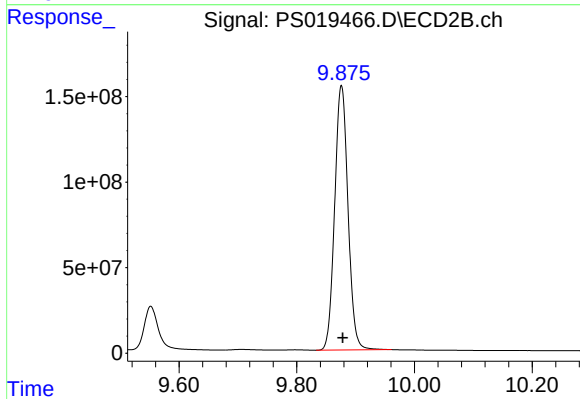

#14 DINOSEB


R.T.: 9.876 min
Delta R.T.: -0.002 min
Response: 2430784673
Conc: 838.81 ng/ml

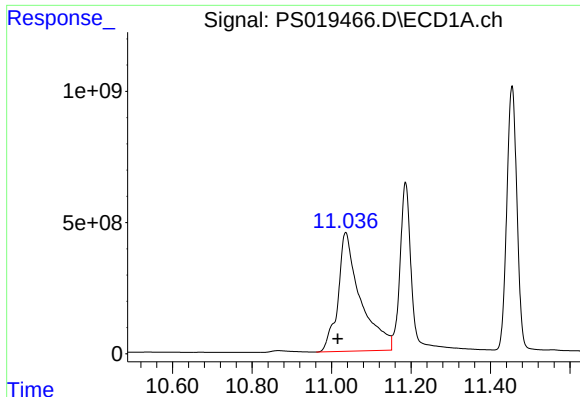

#15 Picloram


R.T.: 11.036 min
Delta R.T.: 0.020 min
Response: 17884332167
Conc: 611.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

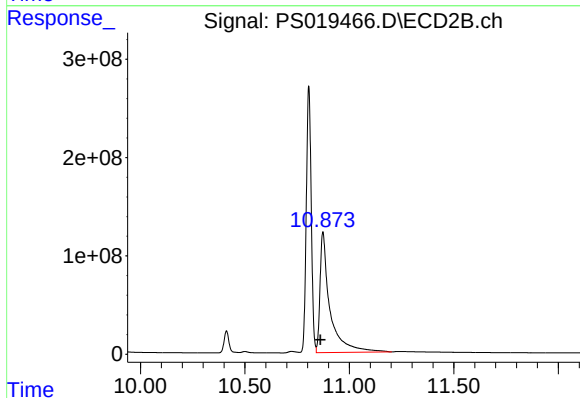


#15 Picloram

R.T.: 10.873 min
Delta R.T.: 0.012 min
Response: 4069482567
Conc: 680.43 ng/ml

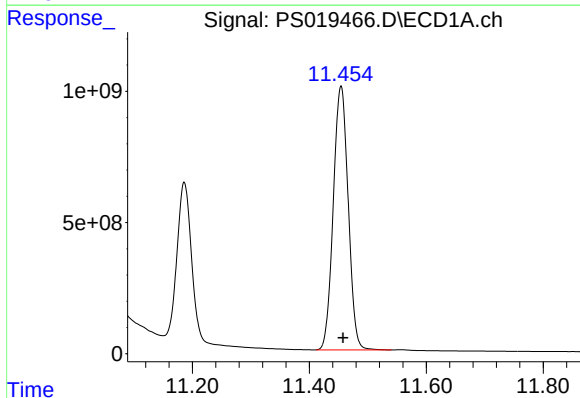

#16 DCPA

R.T.: 11.454 min
Delta R.T.: -0.004 min
Response: 17785422898
Conc: 679.59 ng/ml

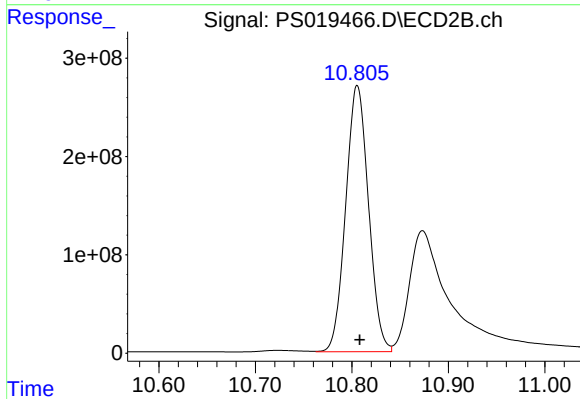

#16 DCPA

R.T.: 10.806 min
Delta R.T.: -0.002 min
Response: 4454410328
Conc: 758.78 ng/ml