

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051920\
 Data File : PS010342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2020 08:58
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 17:31:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.235	6.923	5676073	5679442	8.073	10.590 #
Target Compounds							
2) T	3,5-DICHL...	6.485	6.034	207.3E6	171916	214.909	<MDL #
3) T	4-Nitroph...	0.000	6.538	0	263197	N.D.	<MDL
5) T	DICAMBA	0.000	7.091	0	1655209	N.D.	<MDL
6) T	MCP	0.000	7.237	0	2851844	N.D.	1.554
7) T	MCPA	0.000	7.385	0	2441753	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	3534831	N.D.	6.261
9) T	2,4-D	8.417	8.016	232.5E6	2322704	329.134	3.350 #
10) T	Pentachlo...	0.000	8.441	0	1316422	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	3999266	N.D.	1.381
12) T	2,4,5-T	0.000	9.184	0	6819049	N.D.	2.345
13) T	2,4-DB	0.000	9.698	0	2768384	N.D.	6.946
14) T	DINOSEB	0.000	10.022	0	2104091	N.D.	<MDL
15) T	Picloram	11.030	11.006	35093504	43710640	7.654	10.353 #
16) T	DCPA	0.000	10.950	0	5372255	N.D.	1.503



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051920\
Data File : PS010342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2020 08:58
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 17:31:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

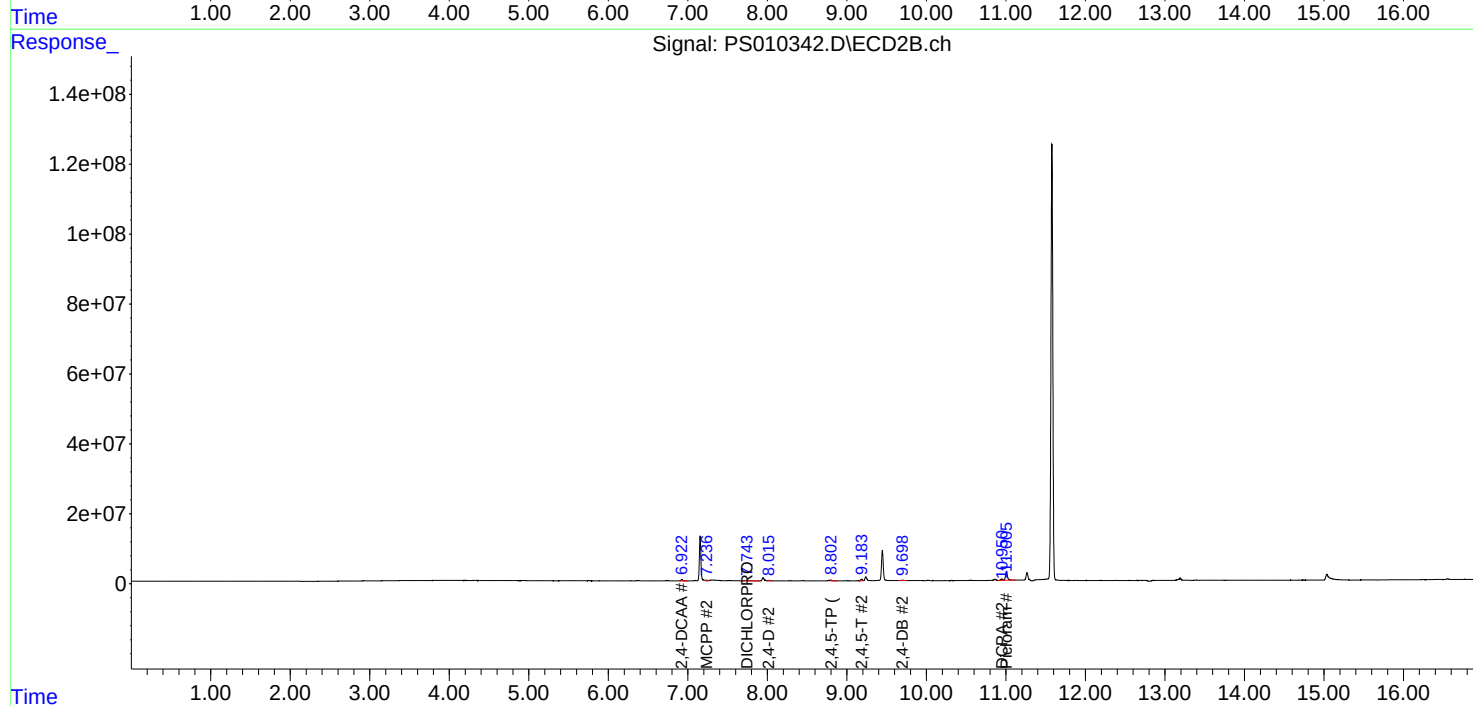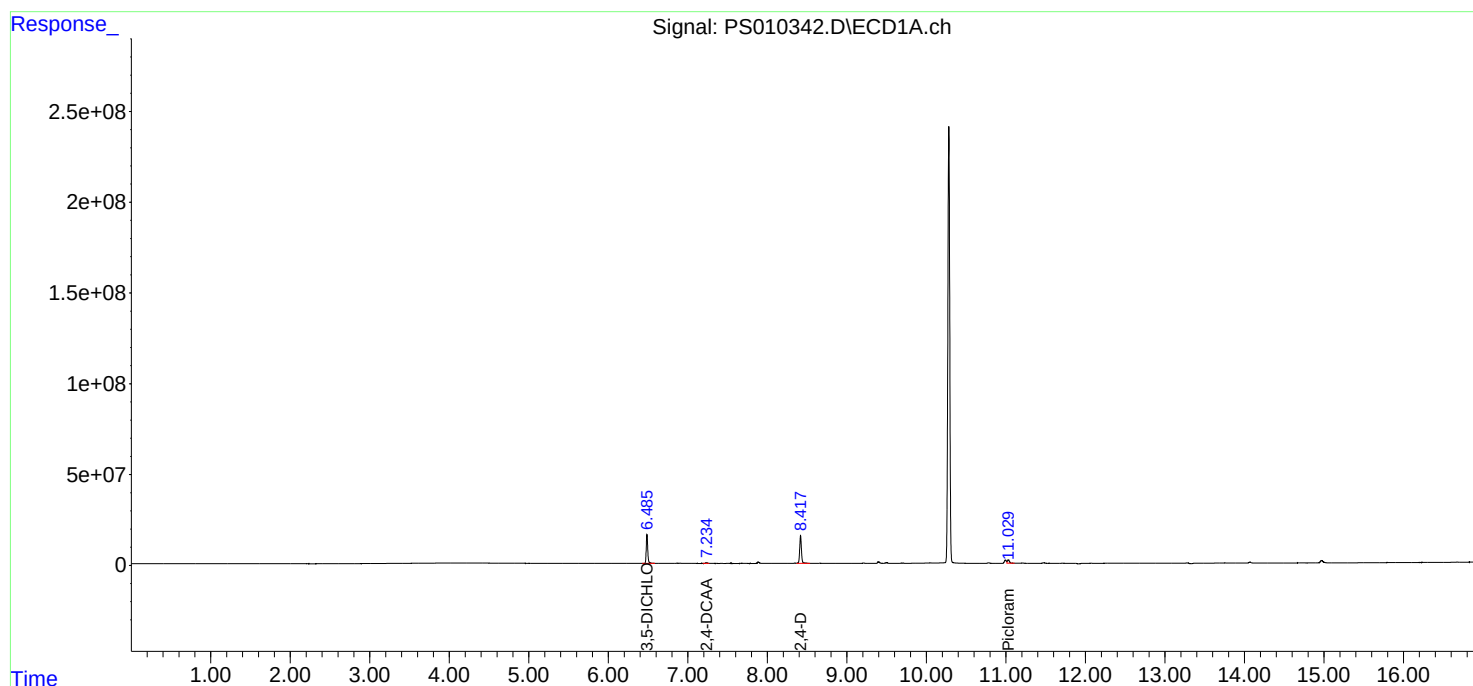


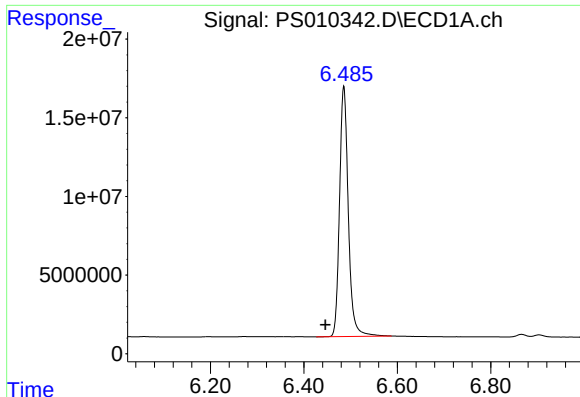

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.485 min
Delta R.T.: 0.039 min
Response: 207331868
Conc: 214.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

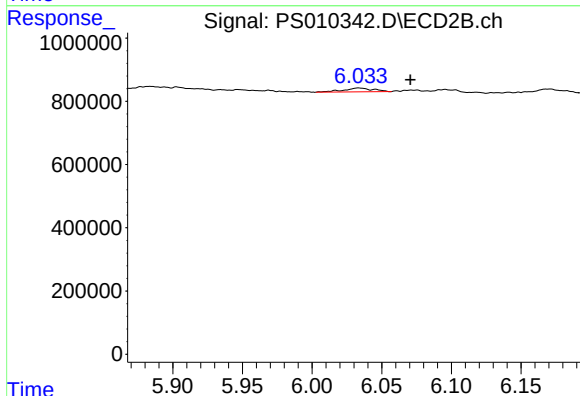


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.034 min
Delta R.T.: -0.037 min
Response: 171916
Conc: N.D.

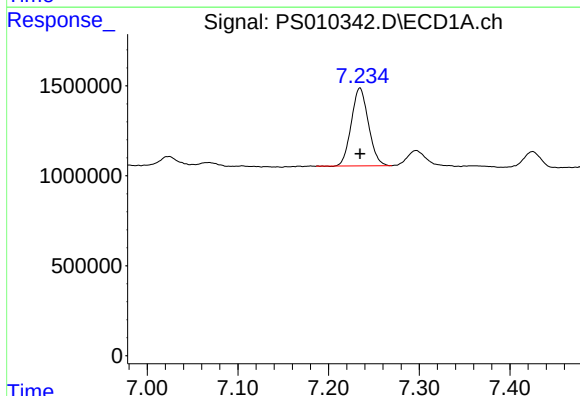


#4 2,4-DCAA

R.T.: 7.235 min
Delta R.T.: 0.000 min
Response: 5676073
Conc: 8.07 ng/ml

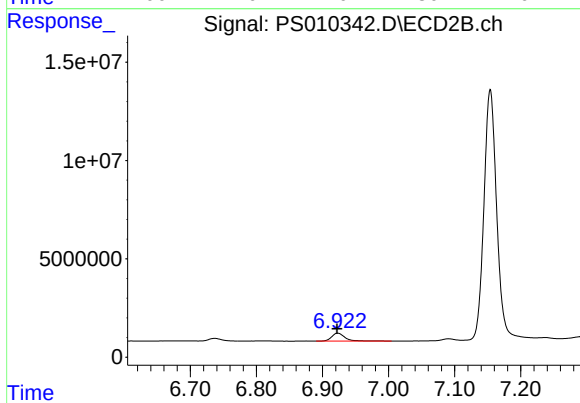

#4 2,4-DCAA


R.T.: 6.923 min
Delta R.T.: 0.001 min
Response: 5679442
Conc: 10.59 ng/ml

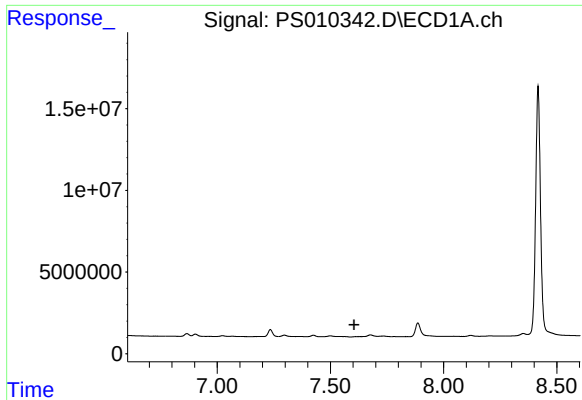

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

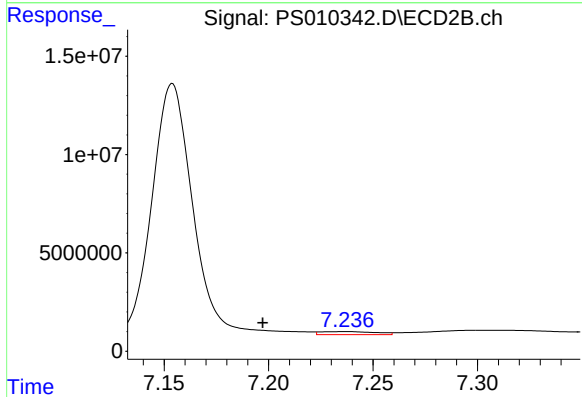


#6 MCP

R.T.: 7.237 min
Delta R.T.: 0.039 min
Response: 2851844
Conc: 1.55 ug/ml

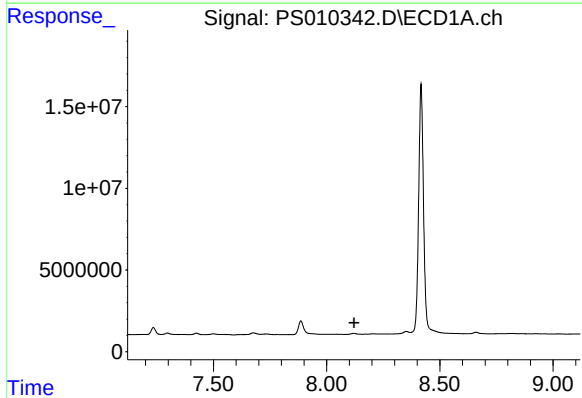


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

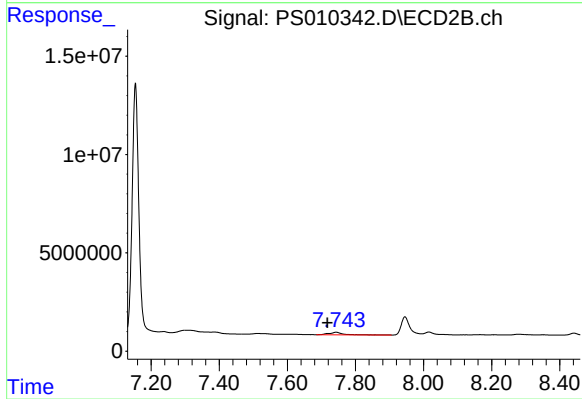

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.025 min
Response: 3534831
Conc: 6.26 ng/ml

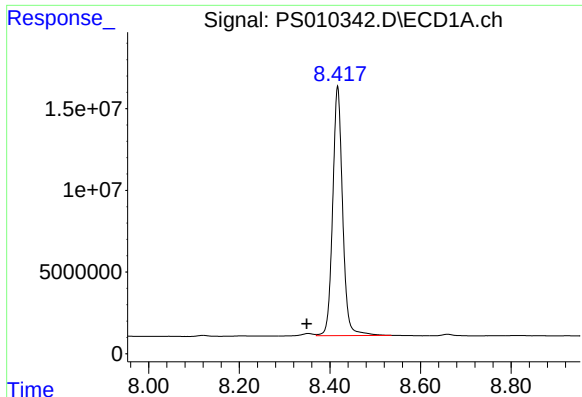

#9 2,4-D


R.T.: 8.417 min
Delta R.T.: 0.068 min
Response: 232517965
Conc: 329.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

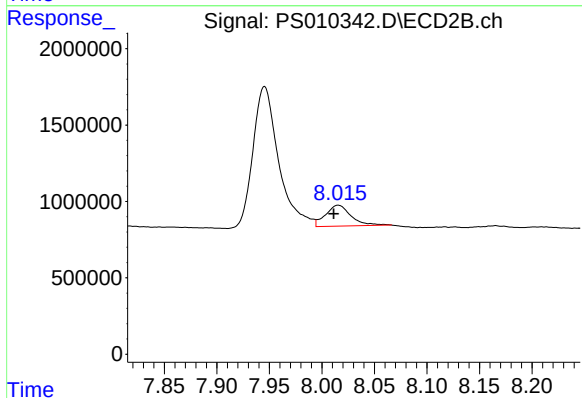


#9 2,4-D

R.T.: 8.016 min
Delta R.T.: 0.004 min
Response: 2322704
Conc: 3.35 ng/ml

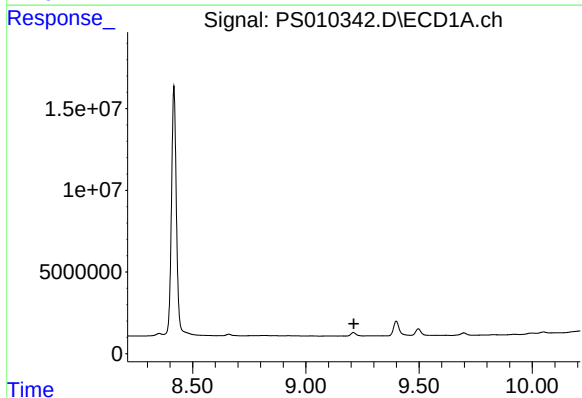


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.212 min
Response: 0
Conc: N.D.

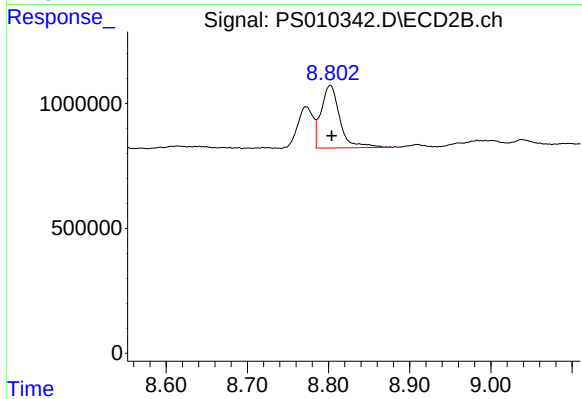

#11 2,4,5-TP (SILVEX)


R.T.: 8.802 min
Delta R.T.: -0.002 min
Response: 3999266
Conc: 1.38 ng/ml

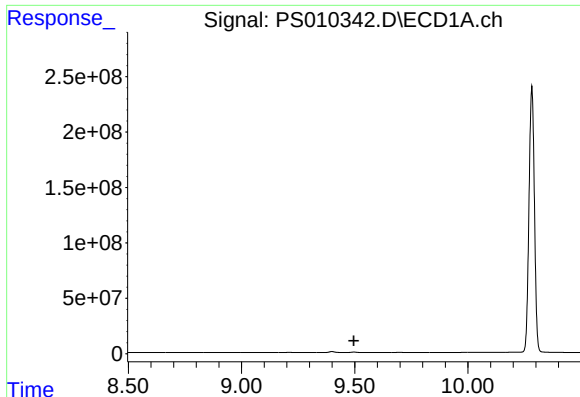

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

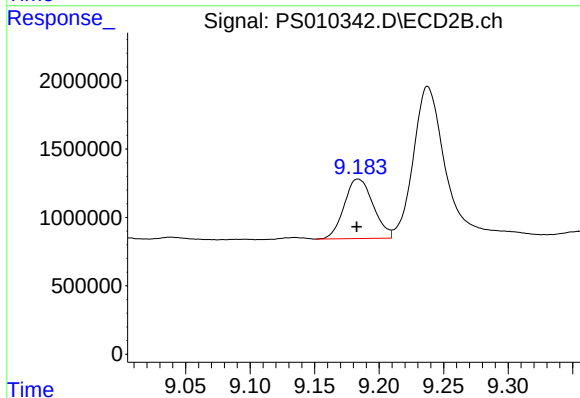


#12 2,4,5-T

R.T.: 9.184 min
Delta R.T.: 0.001 min
Response: 6819049
Conc: 2.35 ng/ml

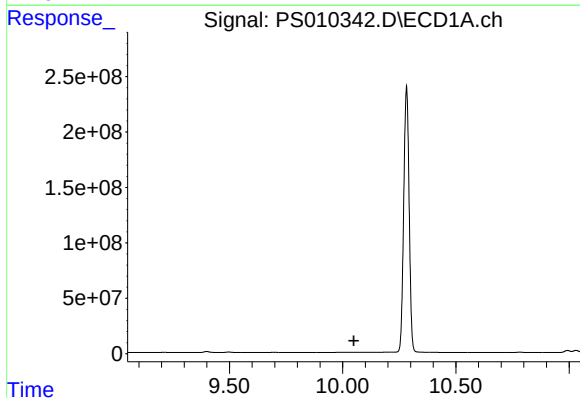


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

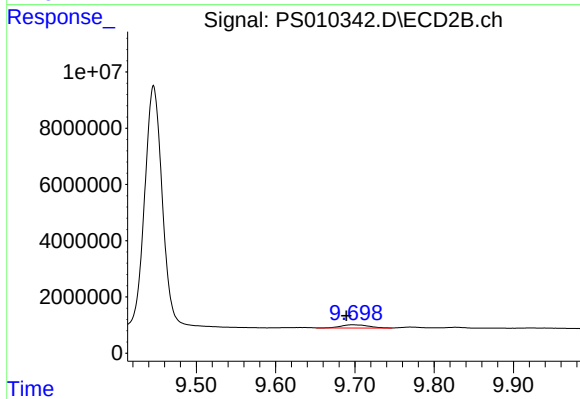

#13 2,4-DB


R.T.: 9.698 min
Delta R.T.: 0.008 min
Response: 2768384
Conc: 6.95 ng/ml

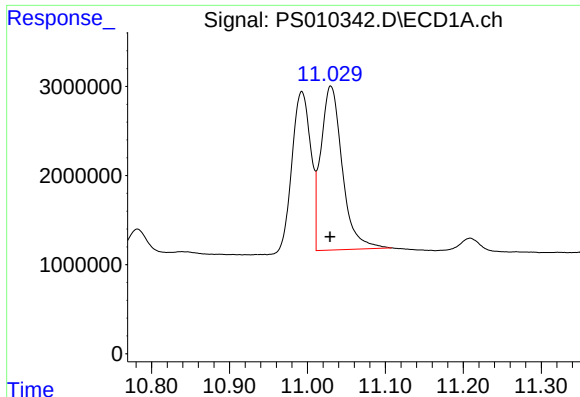

#15 Picloram


R.T.: 11.030 min
Delta R.T.: 0.000 min
Response: 35093504
Conc: 7.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

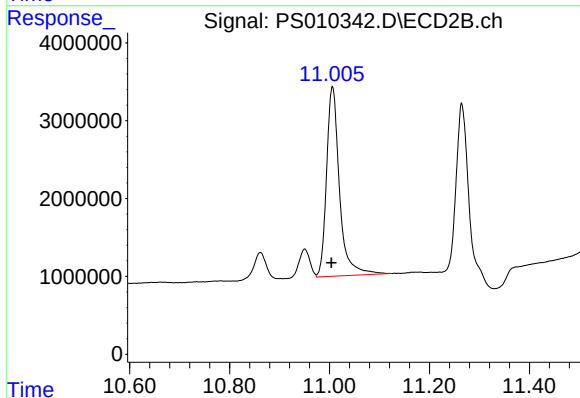


#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.002 min
Response: 43710640
Conc: 10.35 ng/ml

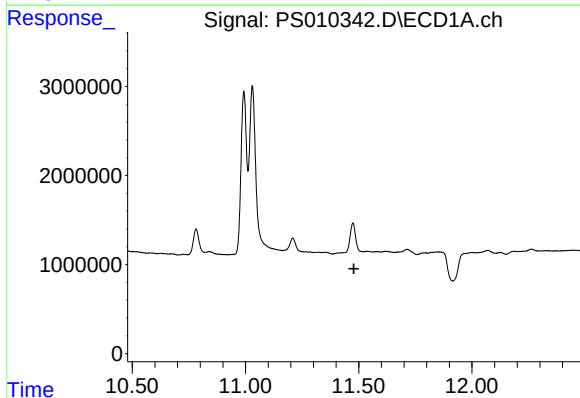

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.479 min
Response: 0
Conc: N.D.

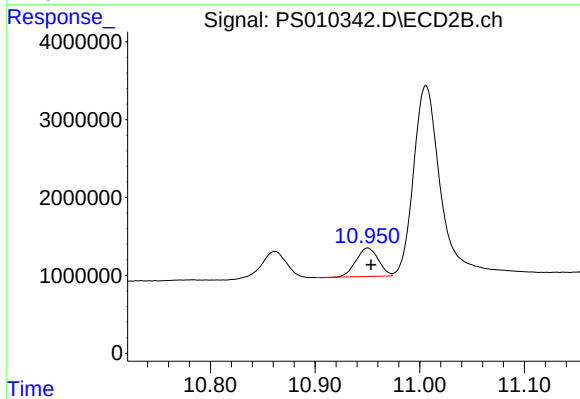

#16 DCPA

R.T.: 10.950 min
Delta R.T.: -0.003 min
Response: 5372255
Conc: 1.50 ng/ml