

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051920\
 Data File : PS010343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2020 09:21
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 17:31:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.233	6.920	323.0E6	276.7E6	459.345	515.905
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	2301956	N.D.	1.051
6) T	MCPD	0.000	7.154	0	1613034	N.D.	<MDL
7) T	MCPA	0.000	7.362	0	3450435	N.D.	1.268
8) T	DICHLORPROP	0.000	7.716	0	867109	N.D.	1.536
9) T	2,4-D	0.000	8.018	0	1599389	N.D.	2.307
11) T	2,4,5-TP ...	0.000	8.802	0	2669823	N.D.	<MDL
12) T	2,4,5-T	0.000	9.186	0	5817483	N.D.	2.001
13) T	2,4-DB	0.000	9.694	0	1307691	N.D.	3.281
14) T	DINOSEB	0.000	10.022	0	1543153	N.D.	<MDL
15) T	Picloram	11.033	11.009	27320877	35997274	5.959	8.526 #
16) T	DCPA	0.000	10.951	0	4657405	N.D.	1.303



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051920\
Data File : PS010343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2020 09:21
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 17:31:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

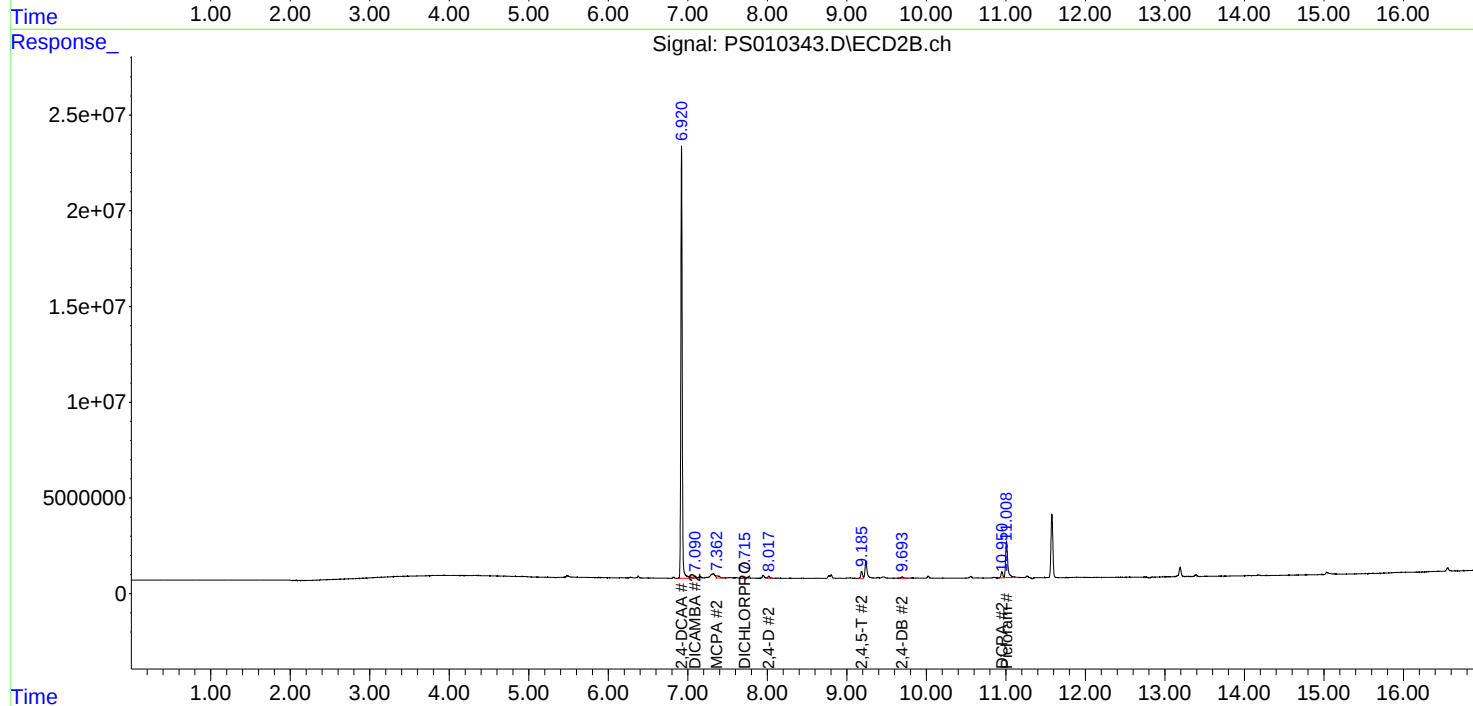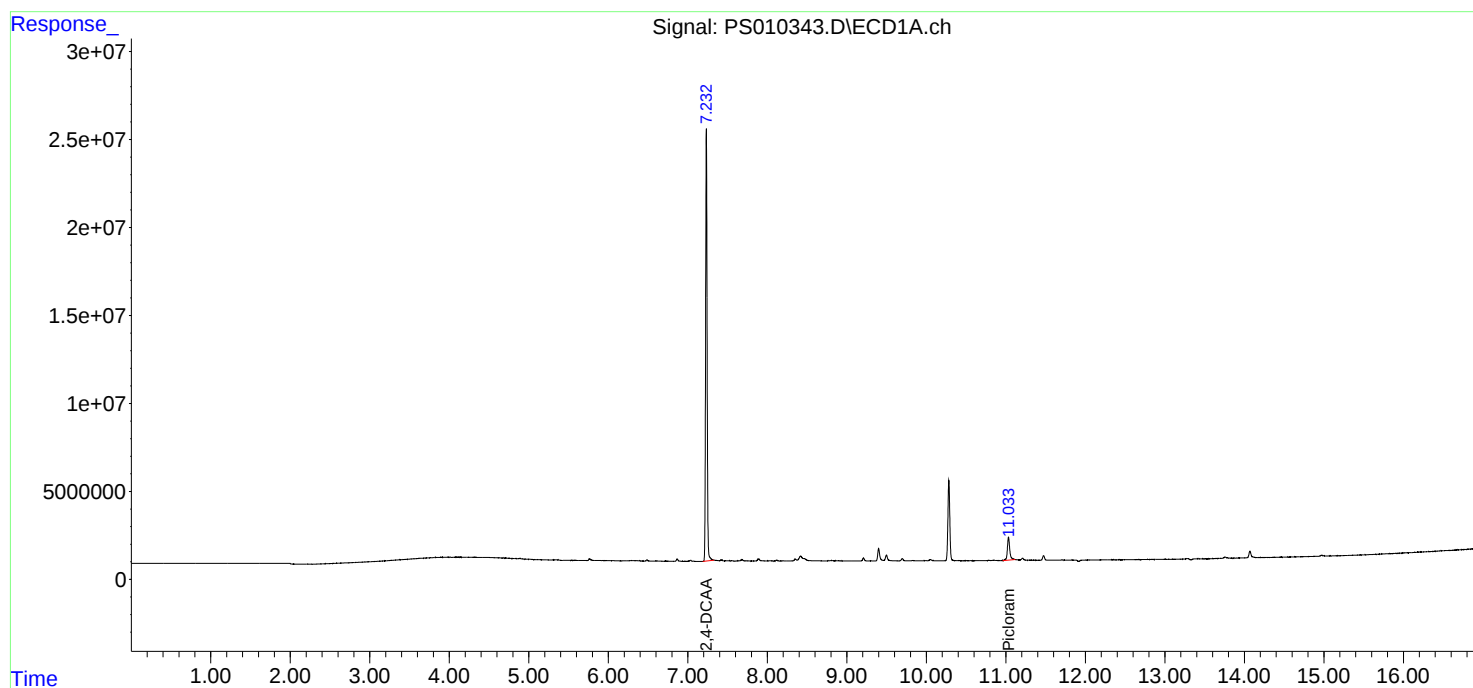


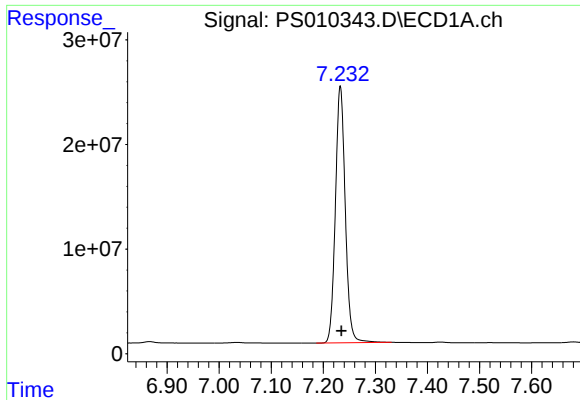

#4 2,4-DCAA


R.T.: 7.233 min
Delta R.T.: -0.002 min
Response: 322963009
Conc: 459.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

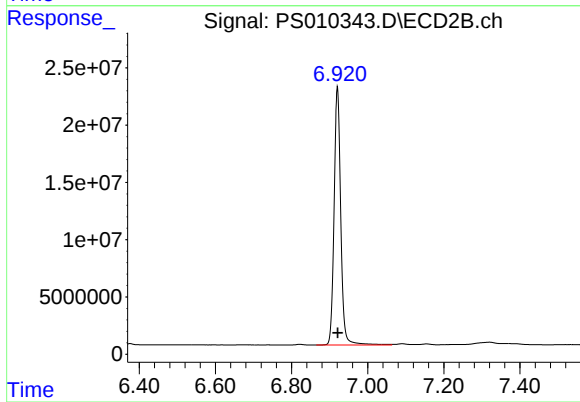


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.001 min
Response: 276675185
Conc: 515.90 ng/ml

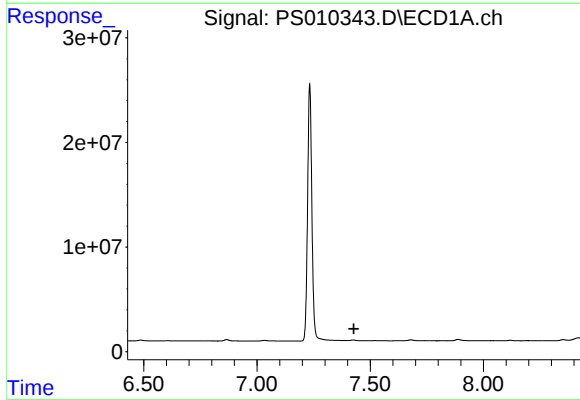


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

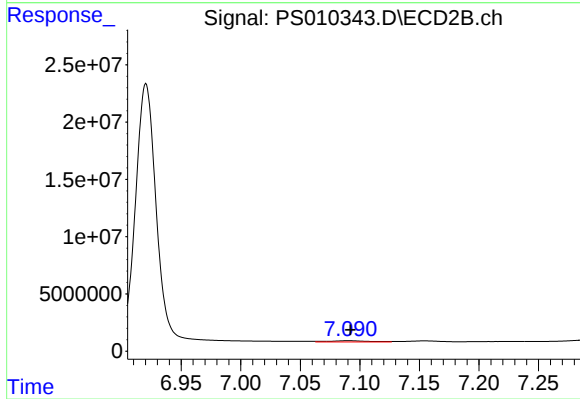

#5 DICAMBA


R.T.: 7.090 min
Delta R.T.: -0.002 min
Response: 2301956
Conc: 1.05 ng/ml

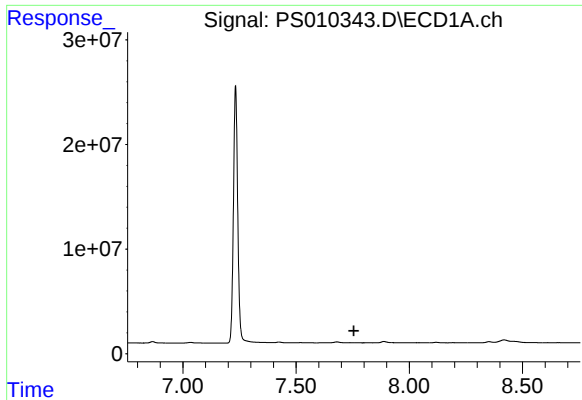

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

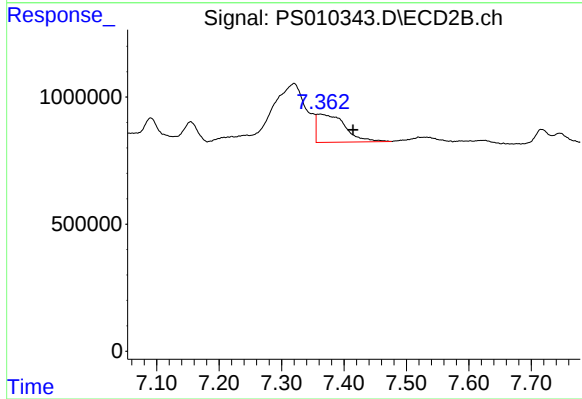


#7 MCPA

R.T.: 7.362 min
Delta R.T.: -0.052 min
Response: 3450435
Conc: 1.27 ug/ml

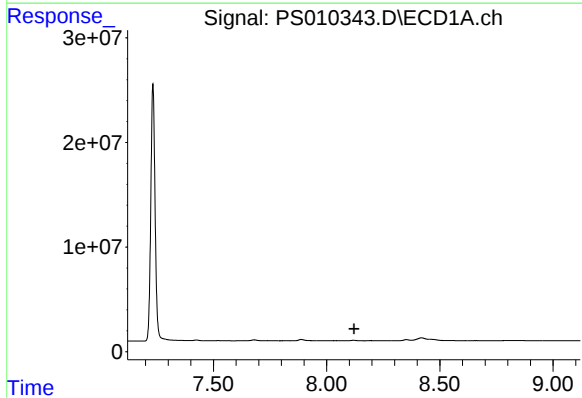


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

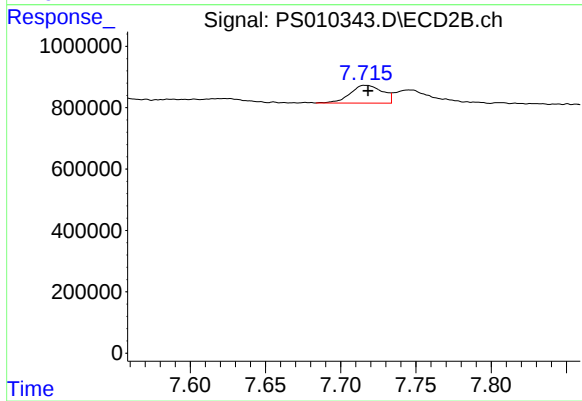

#8 DICHLORPROP


R.T.: 7.716 min
Delta R.T.: -0.002 min
Response: 867109
Conc: 1.54 ng/ml

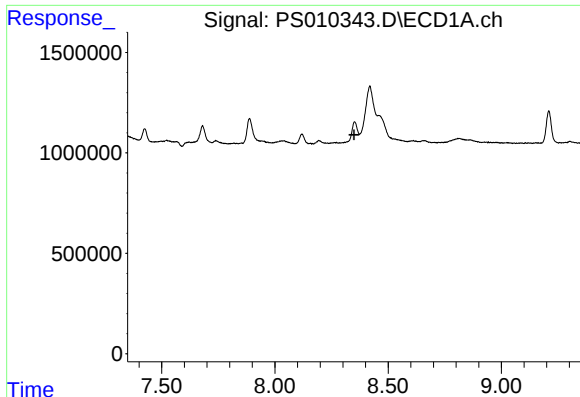

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

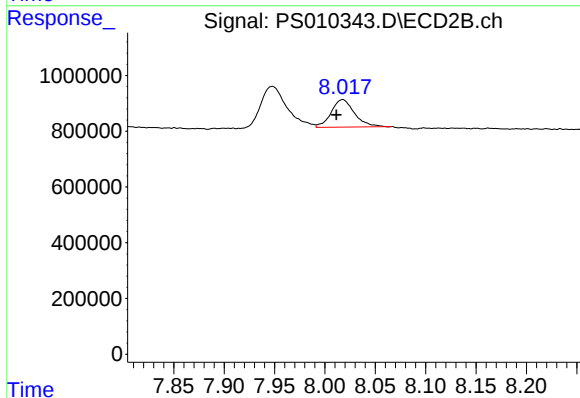


#9 2,4-D

R.T.: 8.018 min
Delta R.T.: 0.006 min
Response: 1599389
Conc: 2.31 ng/ml

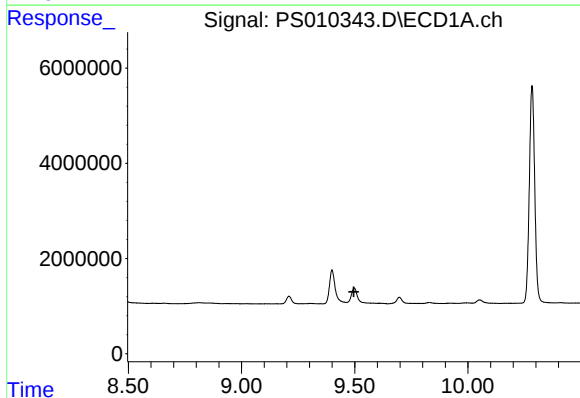


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 9.497 min
Response: 0
Conc: N.D.

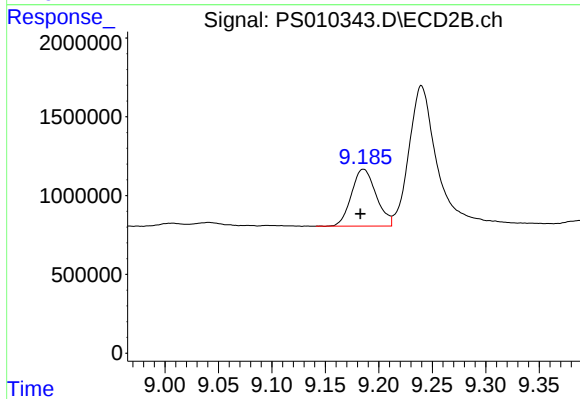

#12 2,4,5-T


R.T.: 9.186 min
Delta R.T.: 0.003 min
Response: 5817483
Conc: 2.00 ng/ml

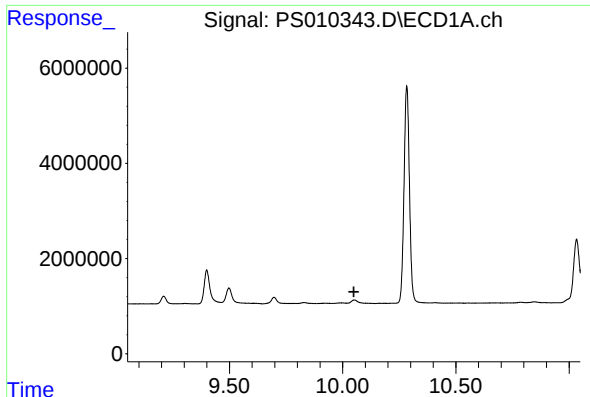

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

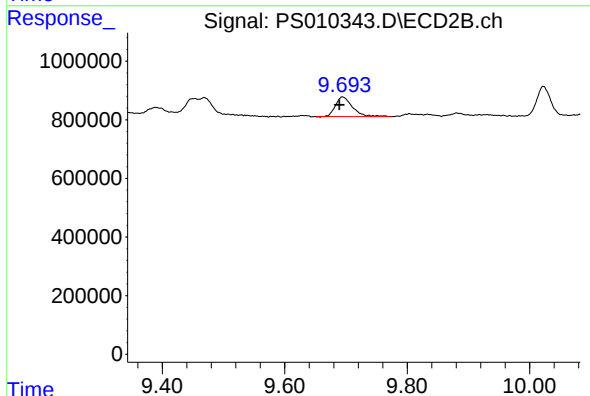


#13 2,4-DB

R.T.: 9.694 min
Delta R.T.: 0.005 min
Response: 1307691
Conc: 3.28 ng/ml

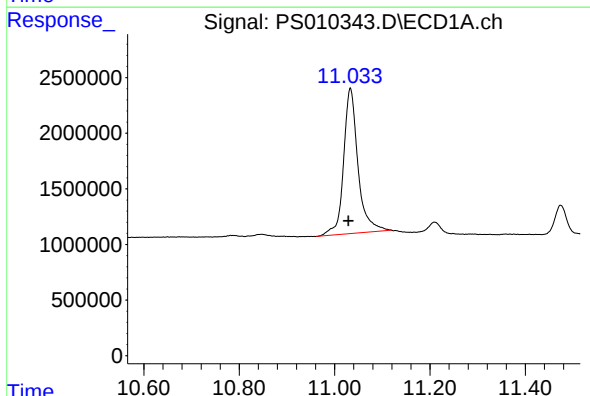


#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.004 min
Response: 27320877
Conc: 5.96 ng/ml

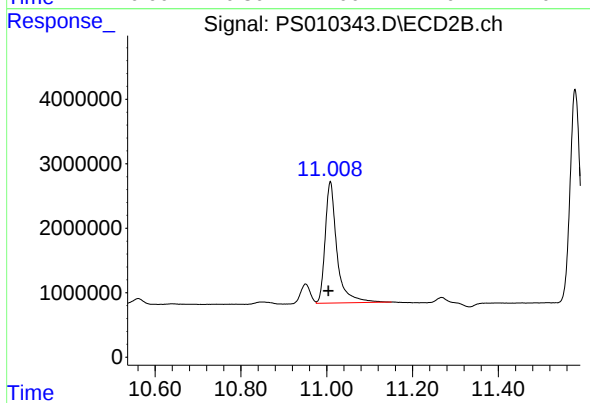

#15 Picloram


R.T.: 11.009 min
Delta R.T.: 0.005 min
Response: 35997274
Conc: 8.53 ng/ml

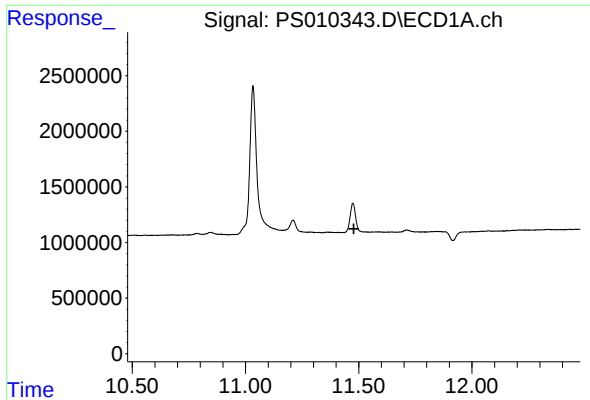

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

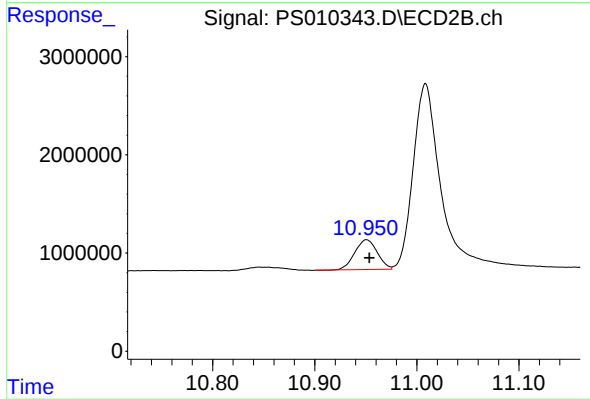

#16 DCPA

R.T.: 10.951 min
Delta R.T.: -0.003 min
Response: 4657405
Conc: 1.30 ng/ml