

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051921\
 Data File : PS015029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 10:52
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 14:20:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.428f	0.000	7272560	0	3.103	N.D. #
5) T	DICAMBA	7.346	0.000	4435438	0	<MDL	N.D. #
7) T	MCPA	7.635	0.000	3695549	0	<MDL	N.D. #
10) T	Pentachlo...	8.567	8.394	12816557	4525615	<MDL	<MDL #
11) T	2,4,5-TP ...	9.114	8.760	9803036	3274724	1.073	1.136
12) T	2,4,5-T	9.417	9.158	19352669	4344871	2.116	1.628
14) T	DINOSEB	11.090	0.000	12884439	0	1.797	N.D. #
15) T	Picloram	10.899	10.980	16326782	47620189	1.344	11.951 #
16) T	DCPA	11.355	10.893	17556473	6793705	1.285	1.594



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051921\
Data File : PS015029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 10:52
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 14:20:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

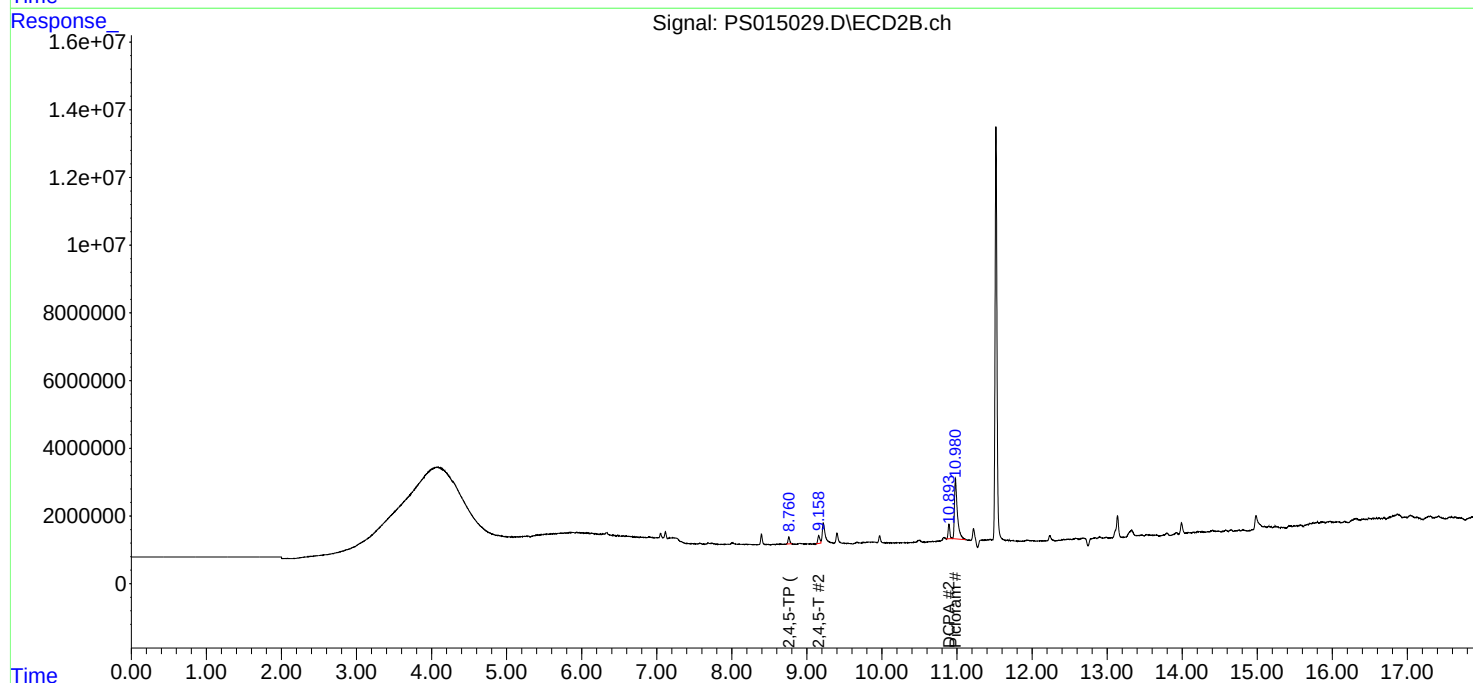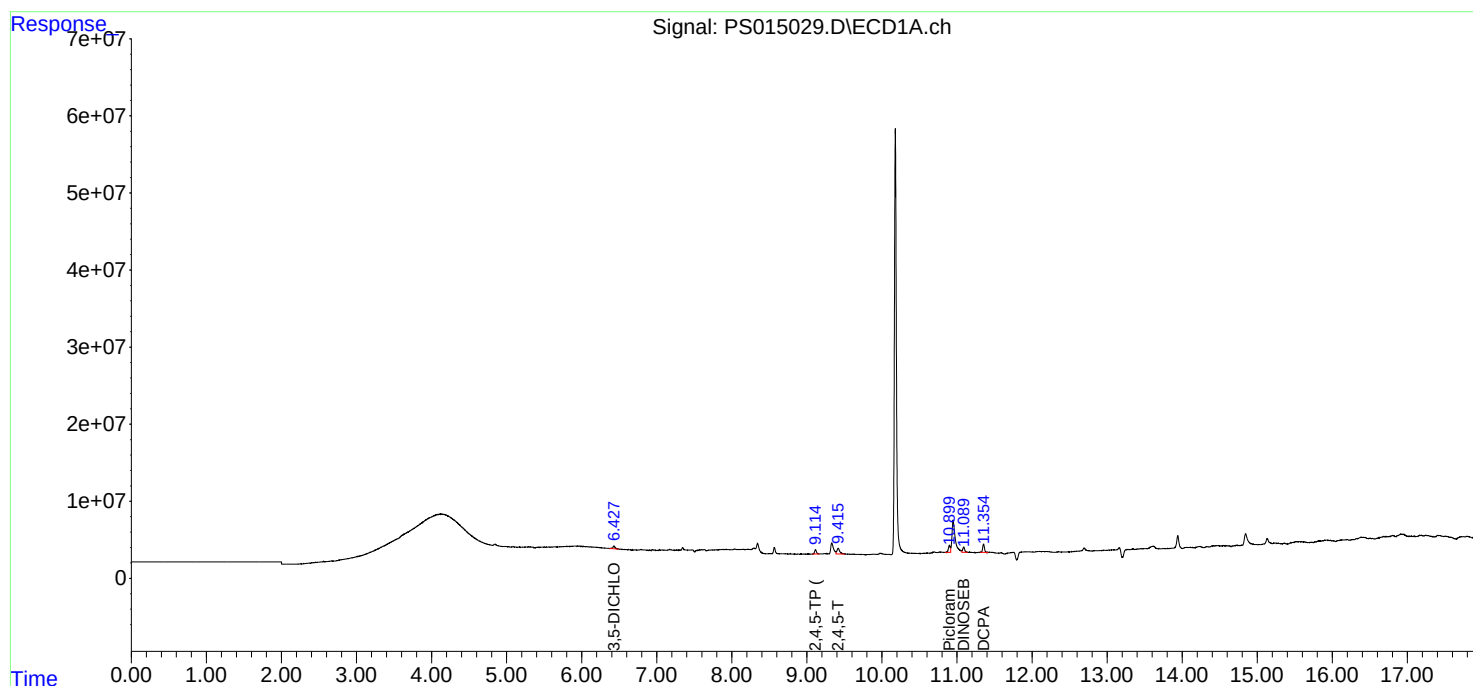


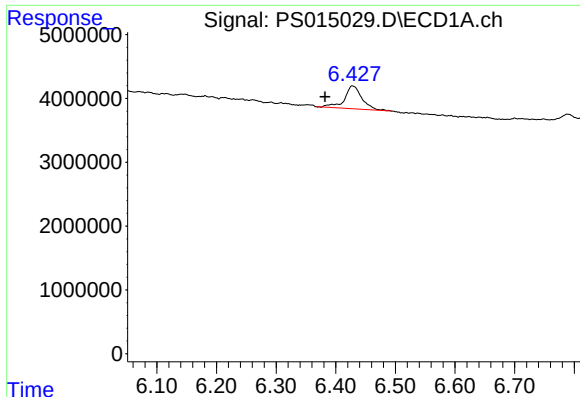

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.428 min
Delta R.T.: 0.046 min
Response: 7272560
Conc: 3.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

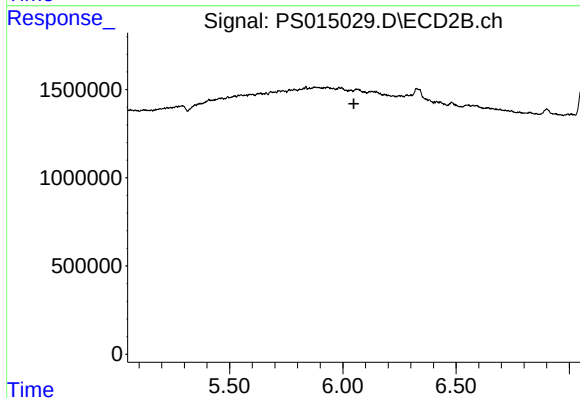


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

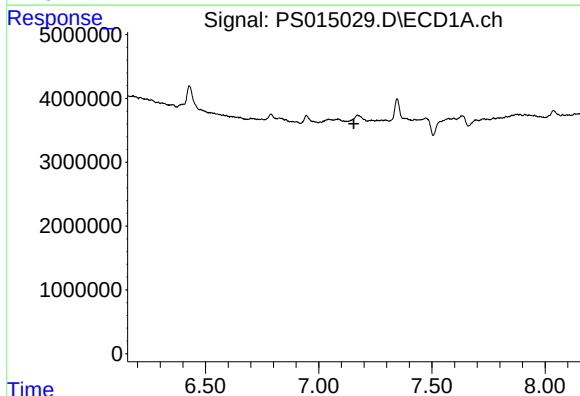


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.156 min
Response: 0
Conc: N.D.

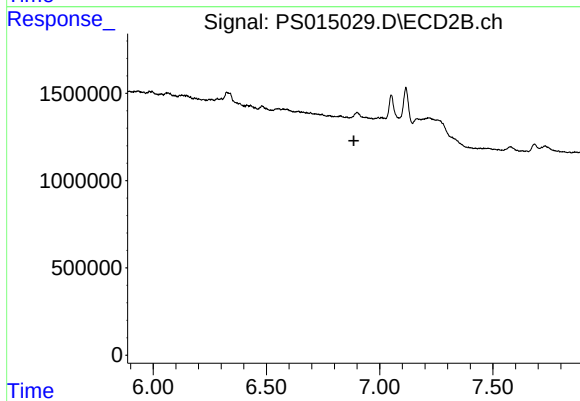

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.886 min
Response: 0
Conc: N.D.

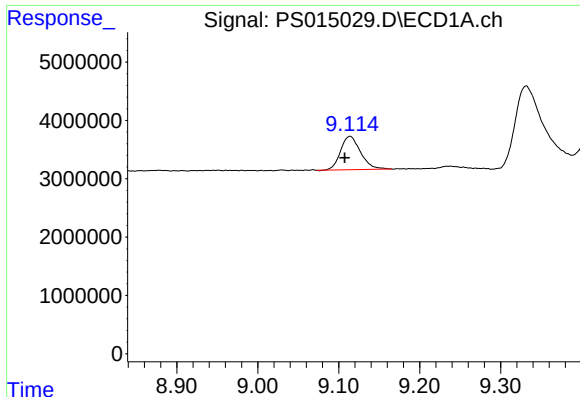

#11 2,4,5-TP (SILVEX)


R.T.: 9.114 min
Delta R.T.: 0.007 min
Response: 9803036
Conc: 1.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

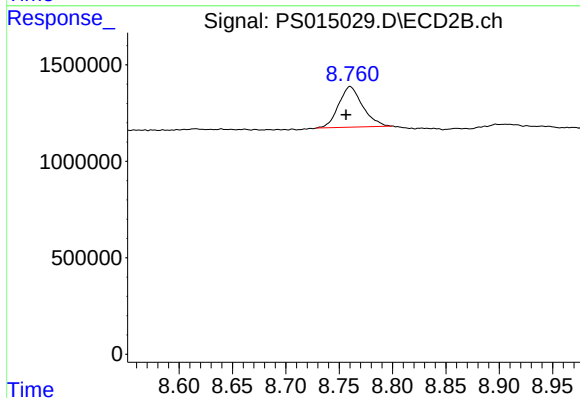


#11 2,4,5-TP (SILVEX)

R.T.: 8.760 min
Delta R.T.: 0.004 min
Response: 3274724
Conc: 1.14 ng/ml

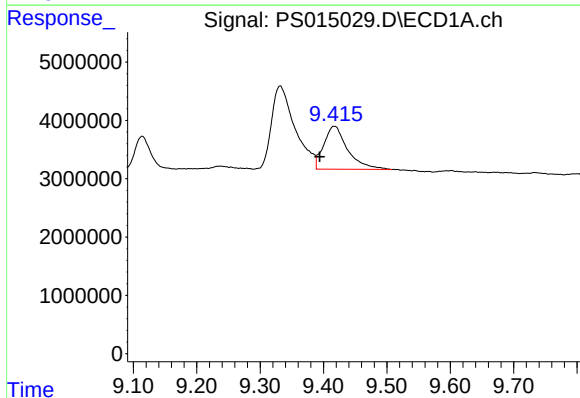


#12 2,4,5-T

R.T.: 9.417 min
Delta R.T.: 0.023 min
Response: 19352669
Conc: 2.12 ng/ml

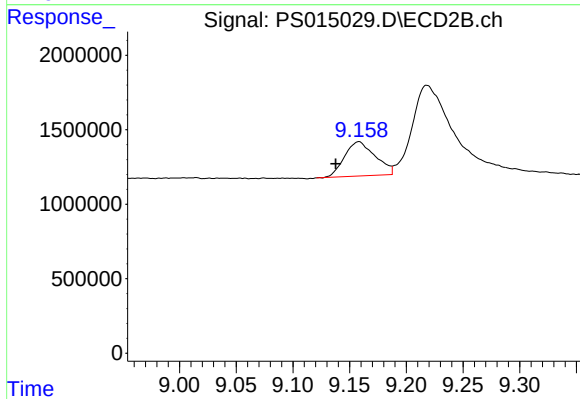

#12 2,4,5-T


R.T.: 9.158 min
Delta R.T.: 0.021 min
Response: 4344871
Conc: 1.63 ng/ml

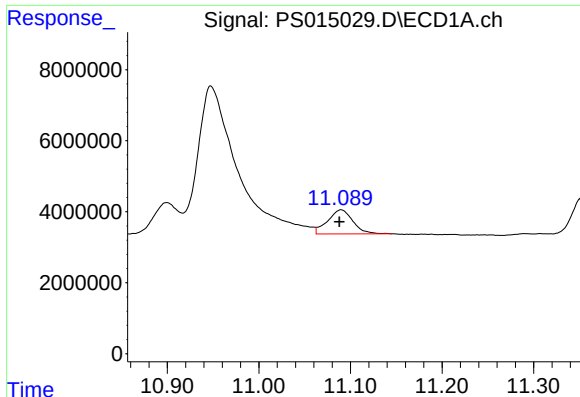

#14 DINoseb


R.T.: 11.090 min
Delta R.T.: 0.002 min
Response: 12884439
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

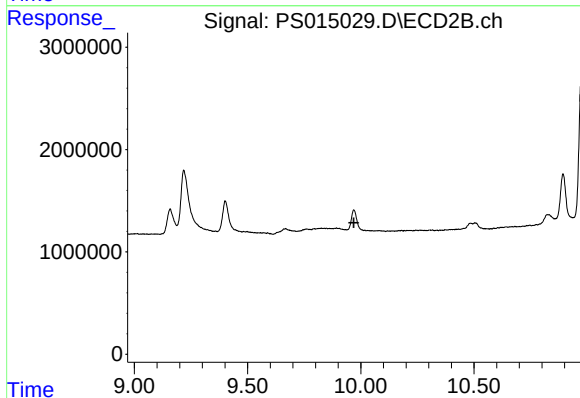


#14 DINoseb

R.T.: 0.000 min
Exp R.T. : 9.970 min
Response: 0
Conc: N.D.

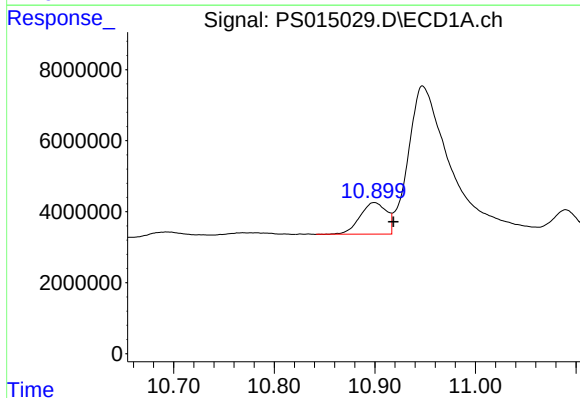


#15 Picloram

R.T.: 10.899 min
Delta R.T.: -0.019 min
Response: 16326782
Conc: 1.34 ng/ml

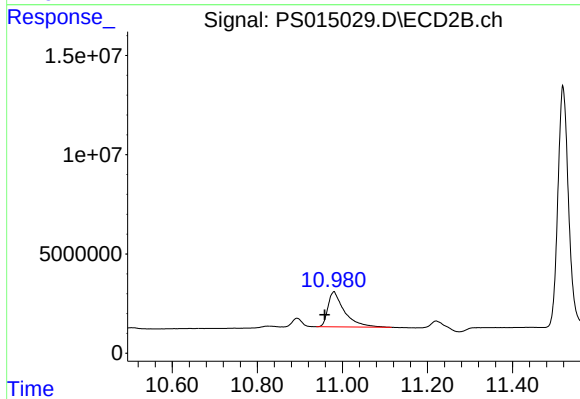

#15 Picloram


R.T.: 10.980 min
Delta R.T.: 0.022 min
Response: 47620189
Conc: 11.95 ng/ml

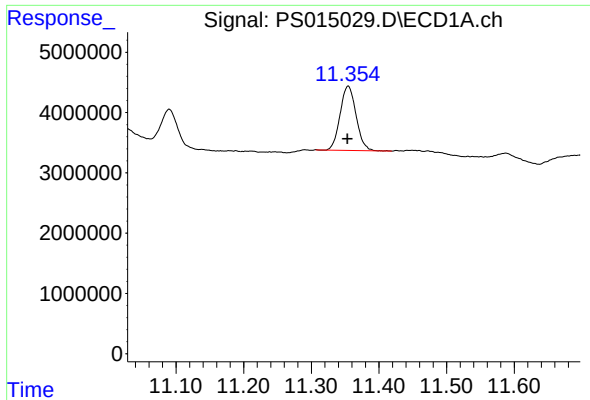

#16 DCPA

R.T.: 11.355 min
Delta R.T.: 0.000 min
Response: 17556473
Conc: 1.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

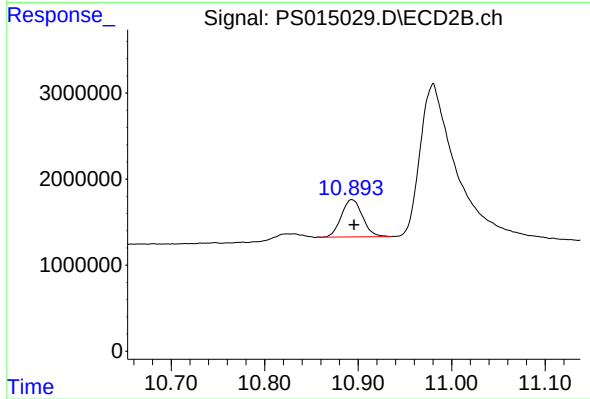

#16 DCPA

R.T.: 10.893 min
Delta R.T.: -0.003 min
Response: 6793705
Conc: 1.59 ng/ml