

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051921\
 Data File : PS015033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 May 2021 15:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 19 19:05:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.159	6.887	706.3E6	273.7E6	422.137	565.597 #
Target Compounds							
2) T	3,5-DICHL...	6.441f	0.000	6983051	0	2.979	N.D. #
5) T	DICAMBA	7.349	7.055	4811512	4090801	<MDL	1.910 #
9) T	2,4-D	8.325f	0.000	27826277	0	15.637	N.D. #
11) T	2,4,5-TP ...	9.129	0.000	5221676	0	<MDL	N.D. #
12) T	2,4,5-T	9.450f	0.000	17669083	0	1.932	N.D. #
15) T	Picloram	10.980f	11.004f	125.1E6	43805037	10.302	10.993



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051921\
Data File : PS015033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 May 2021 15:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 19 19:05:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

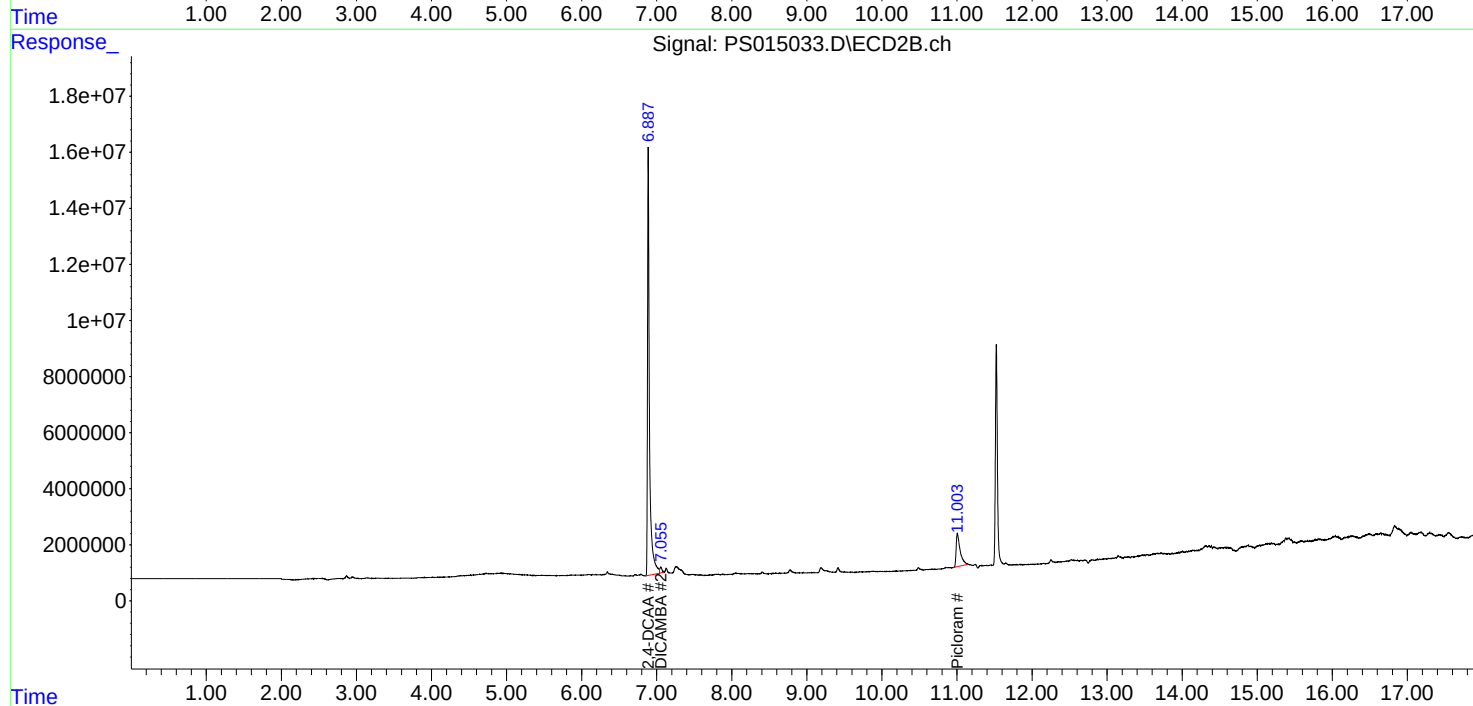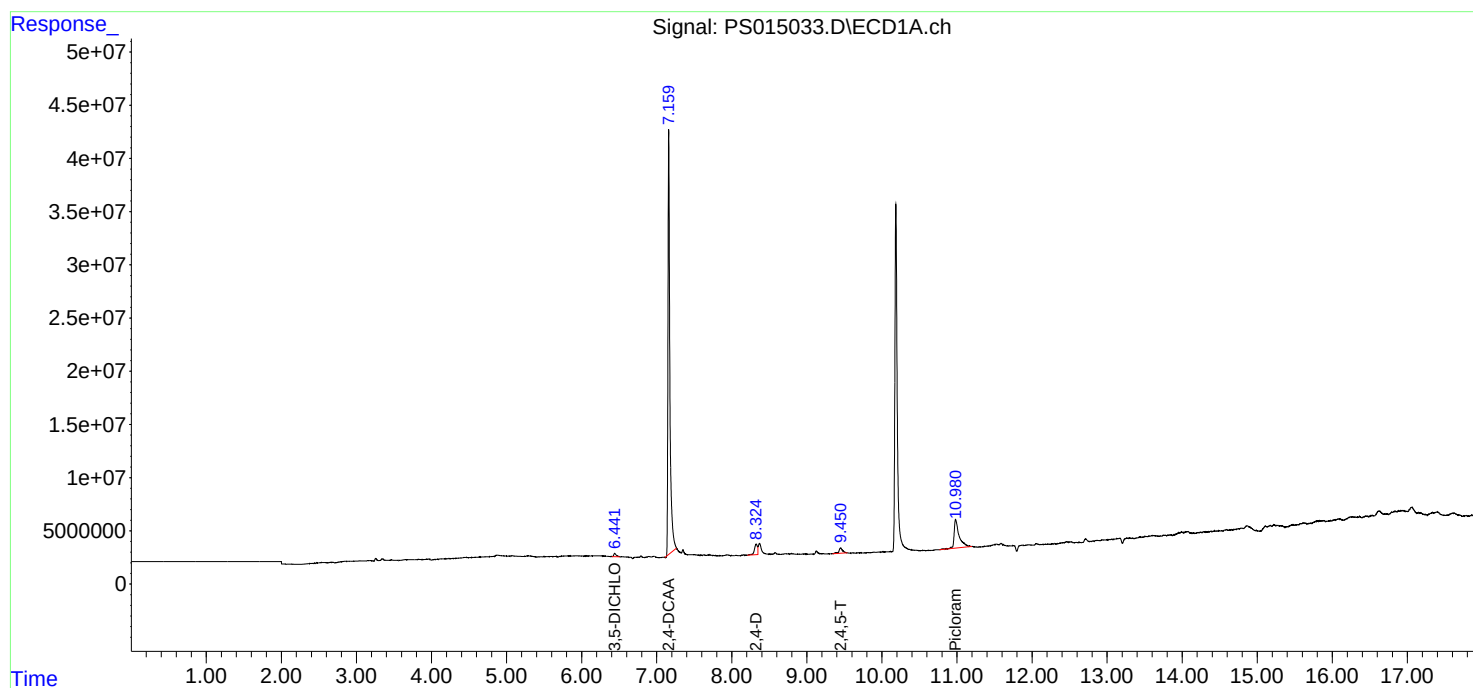


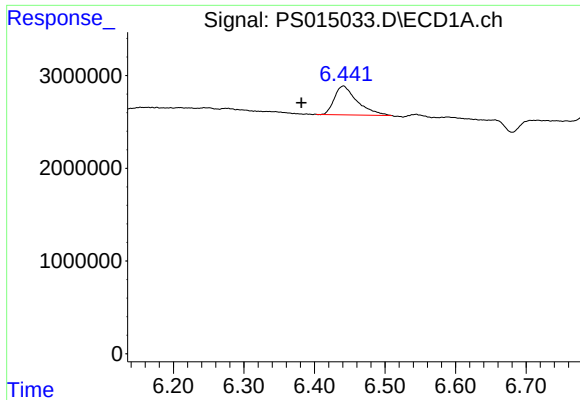

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.441 min
Delta R.T.: 0.060 min
Response: 6983051
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

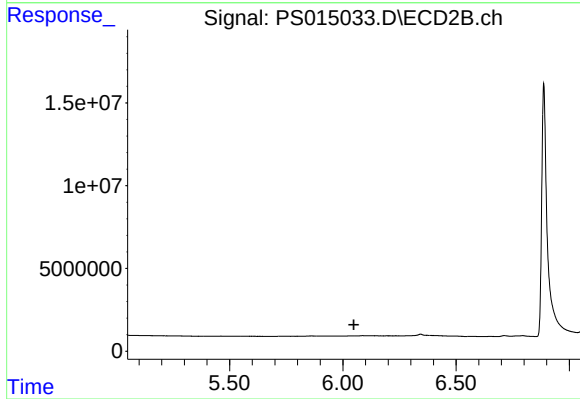


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

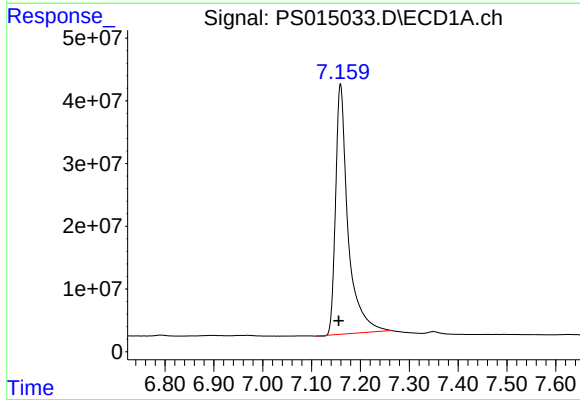


#4 2,4-DCAA

R.T.: 7.159 min
Delta R.T.: 0.004 min
Response: 706340865
Conc: 422.14 ng/ml

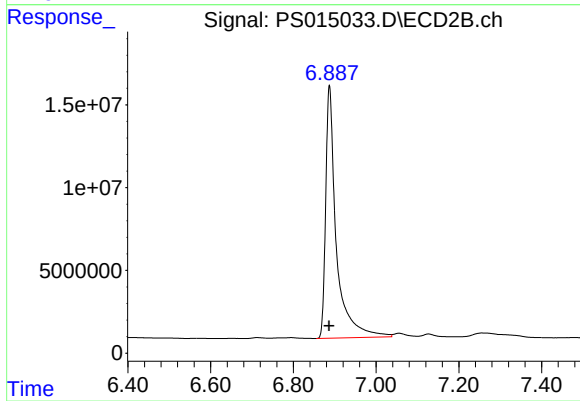

#4 2,4-DCAA


R.T.: 6.887 min
Delta R.T.: 0.000 min
Response: 273699937
Conc: 565.60 ng/ml

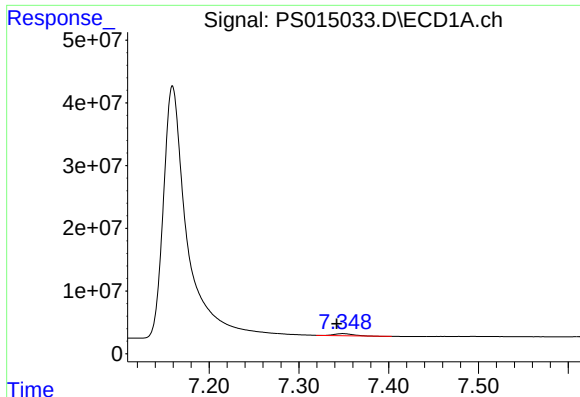

#5 DICAMBA


R.T.: 7.349 min
Delta R.T.: 0.007 min
Response: 4811512
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

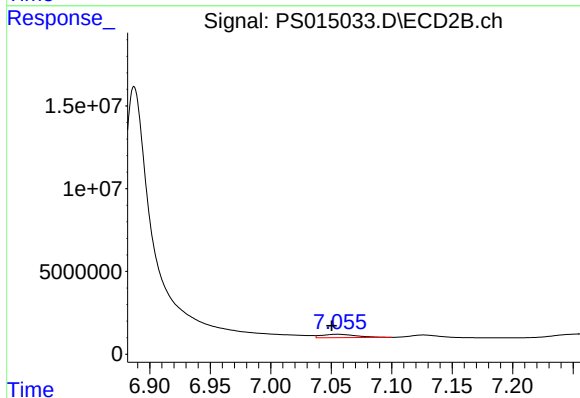


#5 DICAMBA

R.T.: 7.055 min
Delta R.T.: 0.005 min
Response: 4090801
Conc: 1.91 ng/ml

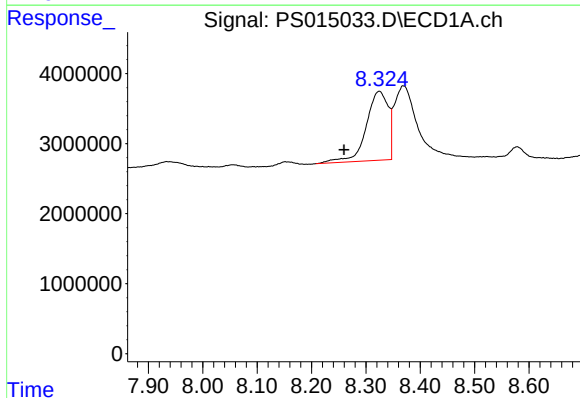


#9 2,4-D

R.T.: 8.325 min
Delta R.T.: 0.065 min
Response: 27826277
Conc: 15.64 ng/ml

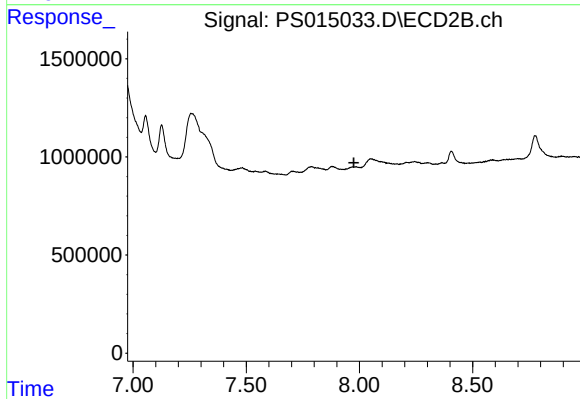

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.975 min
Response: 0
Conc: N.D.

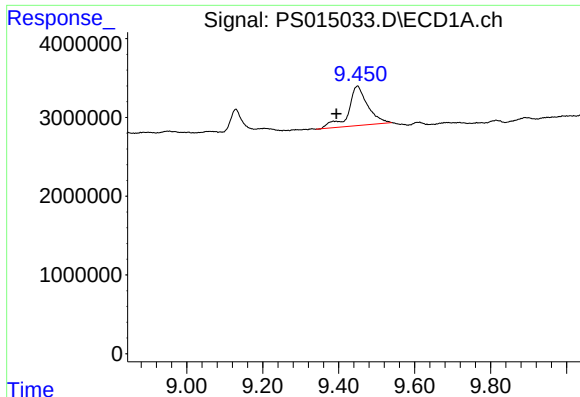

#12 2,4,5-T


R.T.: 9.450 min
Delta R.T.: 0.056 min
Response: 17669083
Conc: 1.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

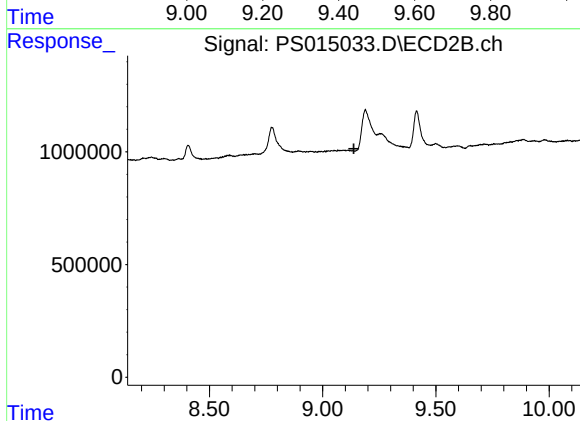


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.138 min
Response: 0
Conc: N.D.

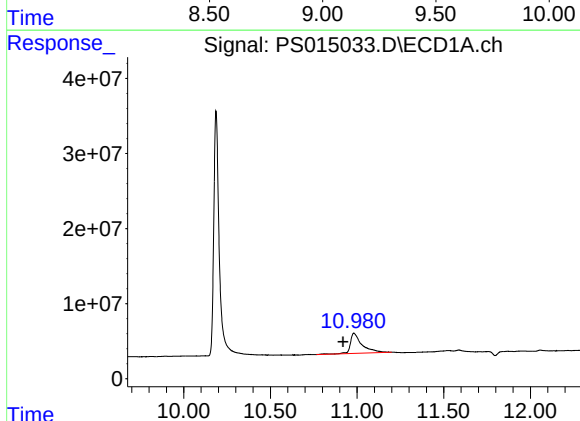

#15 Picloram

R.T.: 10.980 min
Delta R.T.: 0.062 min
Response: 125143825
Conc: 10.30 ng/ml

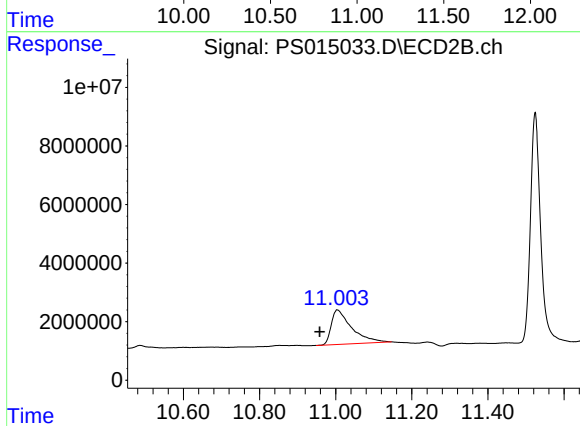

#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.046 min
Response: 43805037
Conc: 10.99 ng/ml