

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052021\
 Data File : PL066841.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 18:42
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PSTDICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 06:40:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052021.M
 Quant Title : GC Extractables
 QLast Update : Fri May 21 06:38:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.853	0.000	2929992	0	1.514	N.D.	#
6) B	beta-BHC	0.000	5.021	0	4836284	N.D.	3.530	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052021\
Data File : PL066841.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 18:42
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PSTDICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 06:40:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052021.M
Quant Title : GC Extractables
QLast Update : Fri May 21 06:38:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

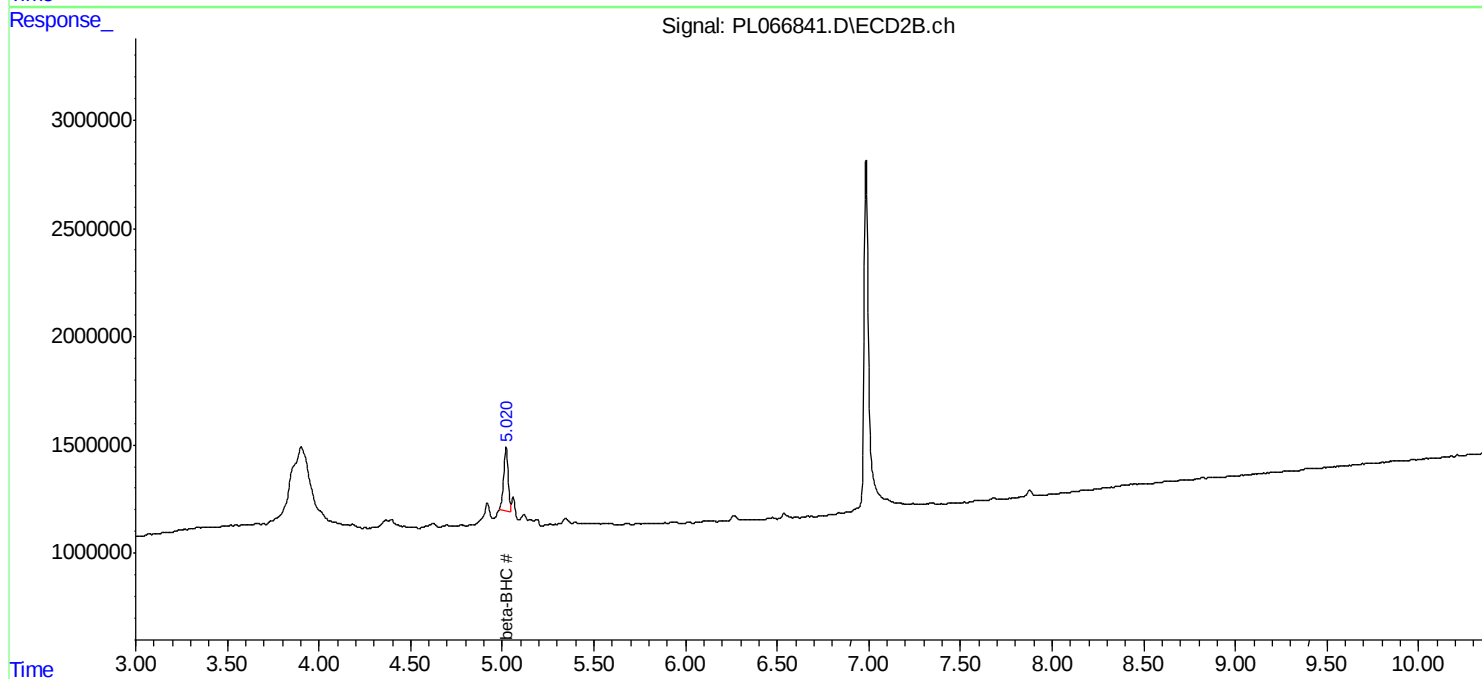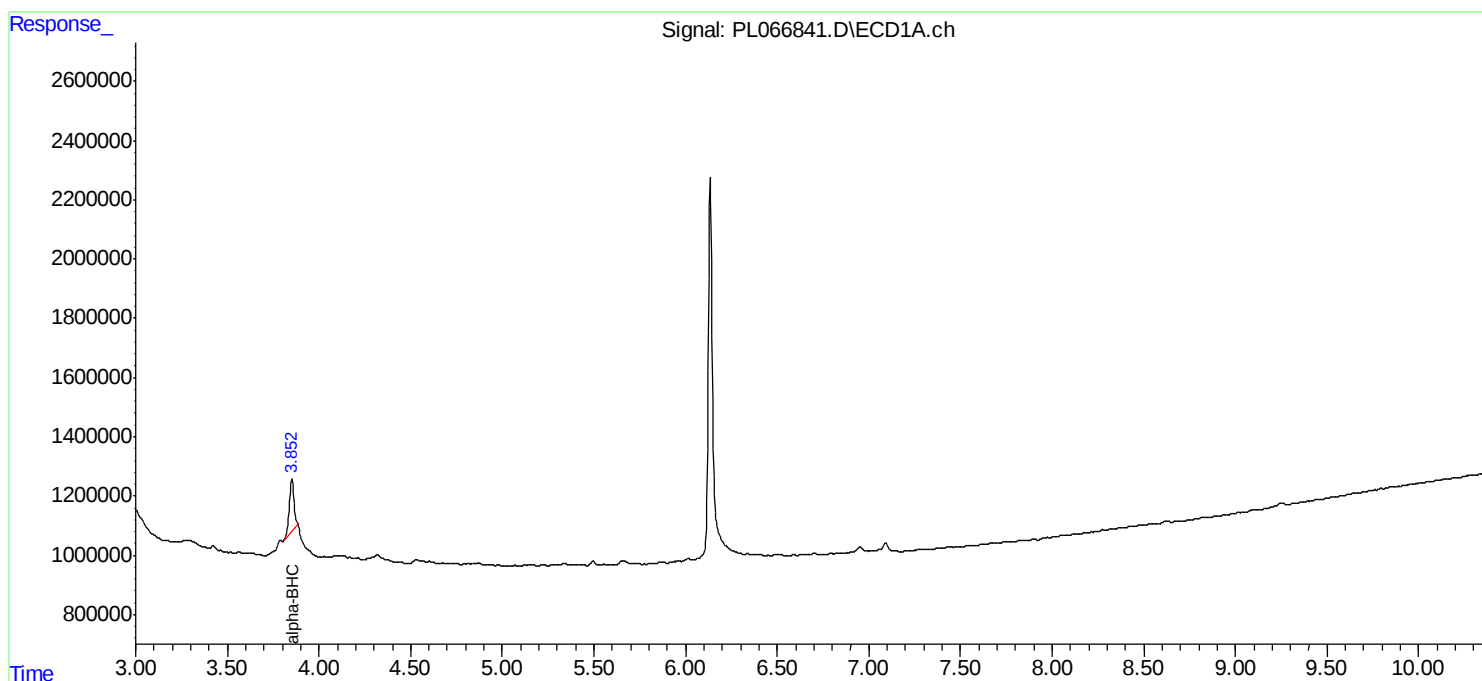


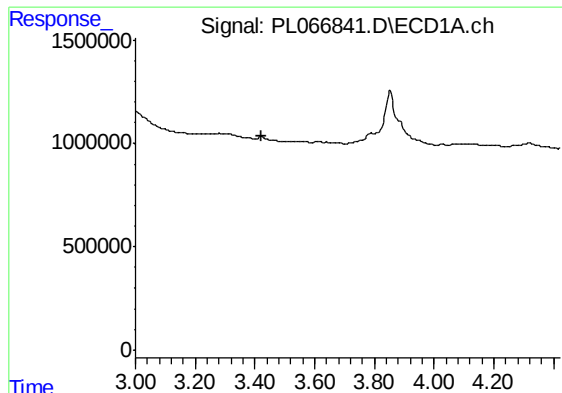

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PSTDICC050

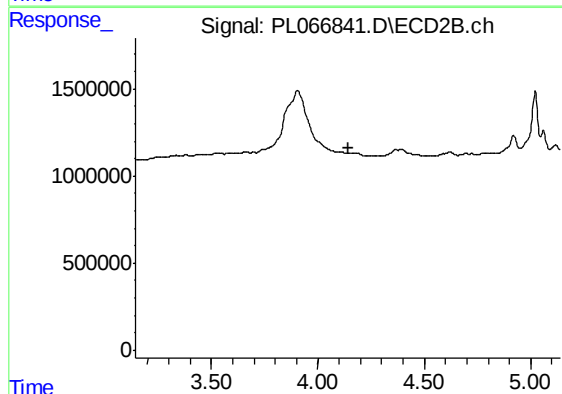


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.143 min
Response: 0
Conc: N.D.

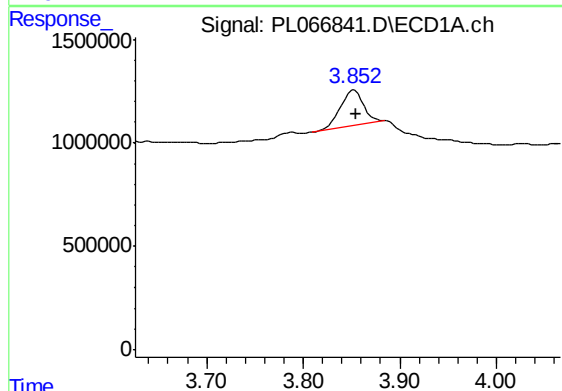


#2 alpha-BHC

R.T.: 3.853 min
Delta R.T.: -0.002 min
Response: 2929992
Conc: 1.51 ng/ml

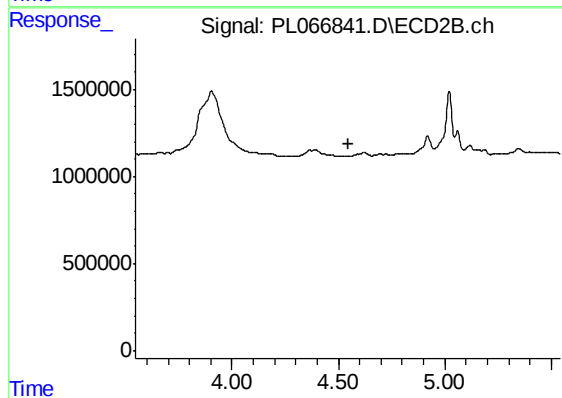

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.546 min
Response: 0
Conc: N.D.

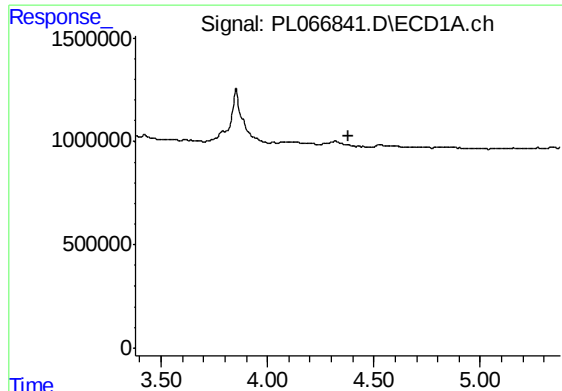

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PSTDICC050

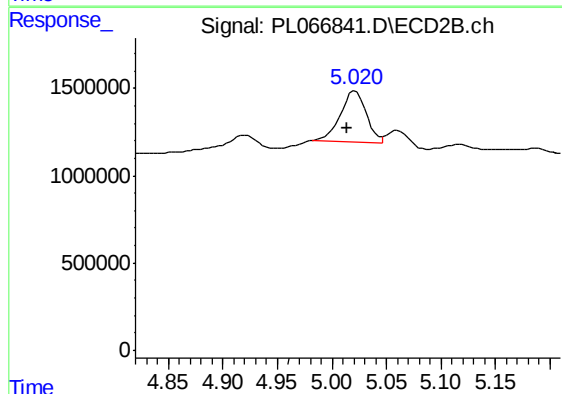


#6 beta-BHC

R.T.: 5.021 min
Delta R.T.: 0.007 min
Response: 4836284
Conc: 3.53 ng/ml

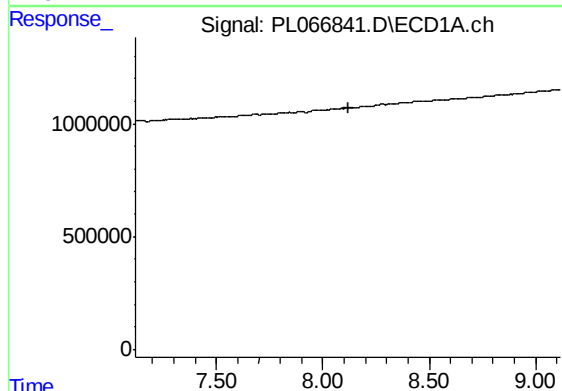

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.118 min
Response: 0
Conc: N.D.

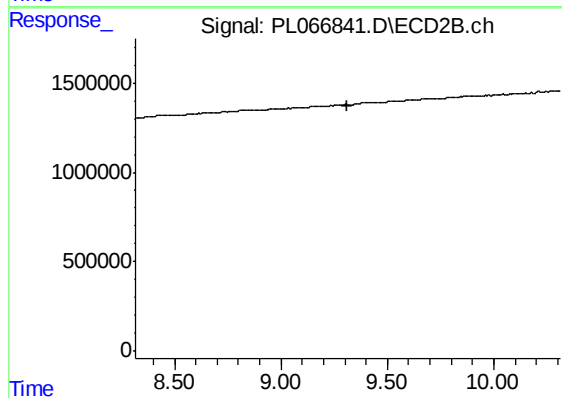

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.314 min
Response: 0
Conc: N.D.