

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052021\
 Data File : PL066843.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 19:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PSTDICC005

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 06:41:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052021.M
 Quant Title : GC Extractables
 QLast Update : Fri May 21 06:38:18 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.423	4.143	7609795	11415400	6.209	6.380
28) SA Decachlor...	8.119	9.315	10162939	12899554	6.174	6.625
Target Compounds						
2) A alpha-BHC	3.851	0.000	2949816	0	1.524	N.D. #
6) B beta-BHC	0.000	5.022	0	4699190	N.D.	3.430 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL052021\
Data File : PL066843.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 19:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PSTDIC005

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 06:41:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL052021.M
Quant Title : GC Extractables
QLast Update : Fri May 21 06:38:18 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

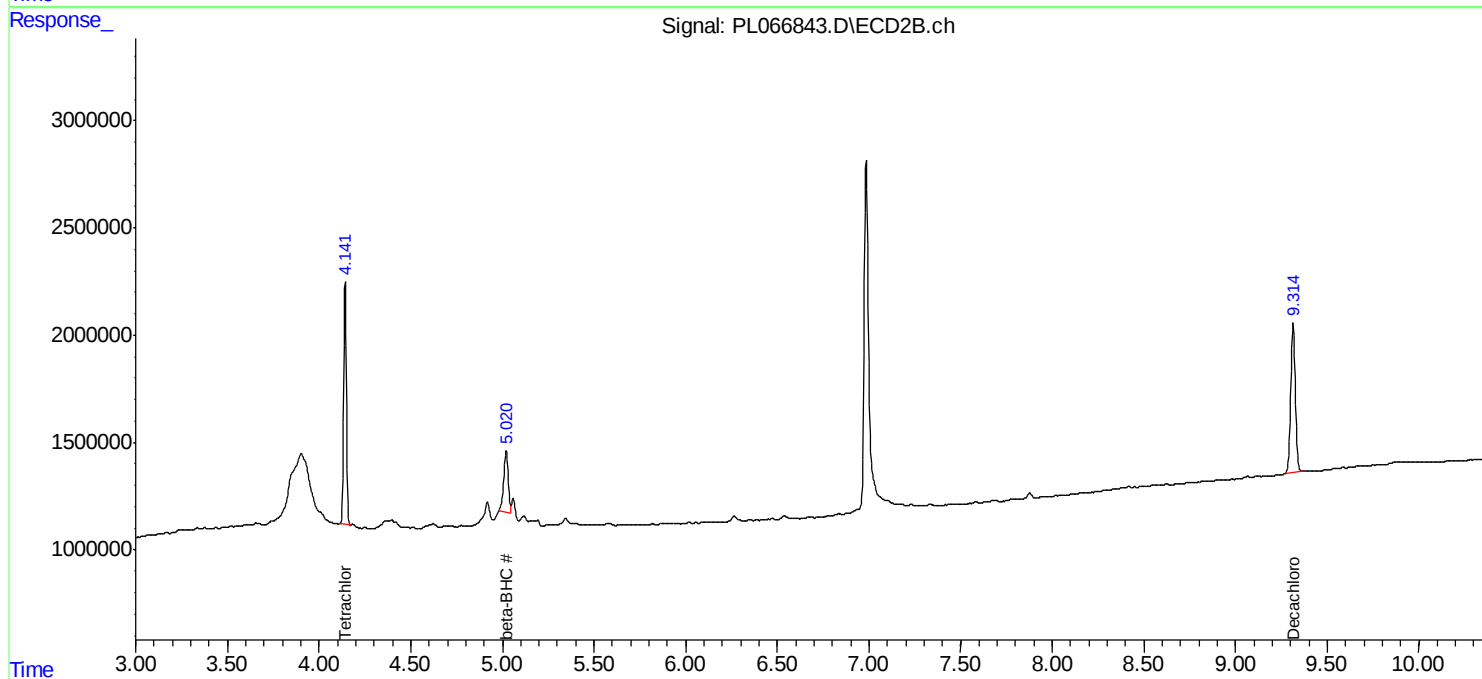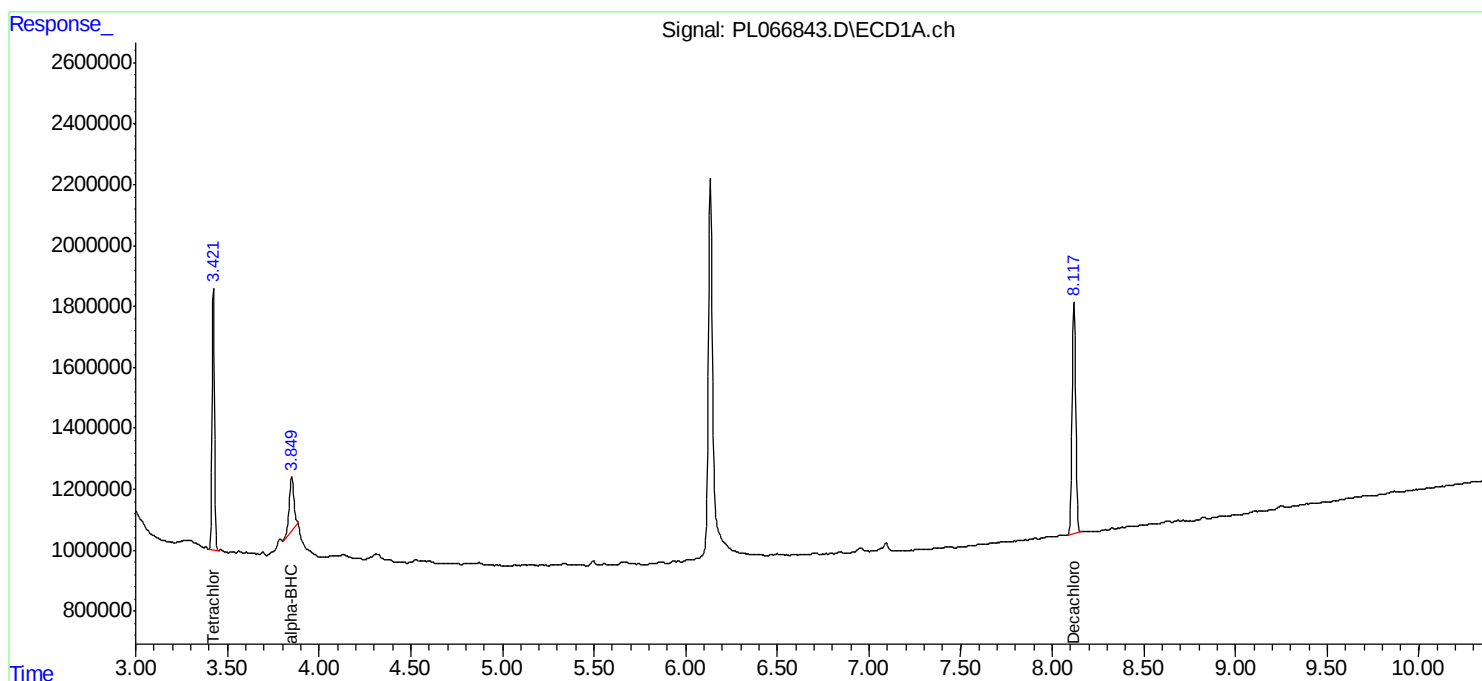


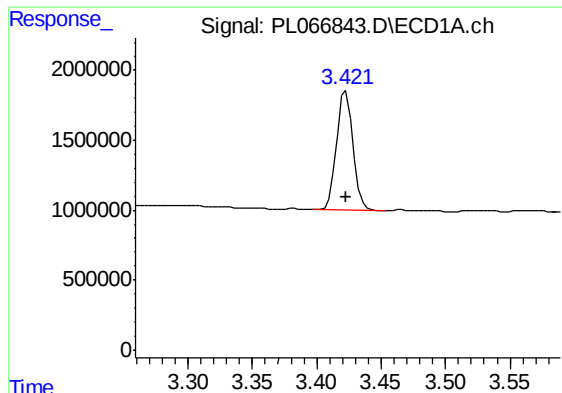

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: 0.000 min
Response: 7609795
Conc: 6.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
PSTDIC005

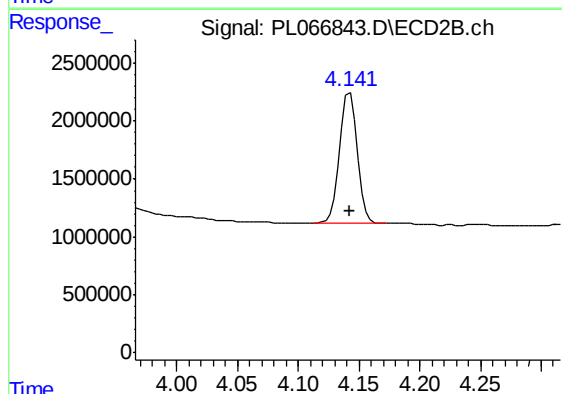


#1 Tetrachloro-m-xylene

R.T.: 4.143 min
Delta R.T.: 0.000 min
Response: 11415400
Conc: 6.38 ng/ml

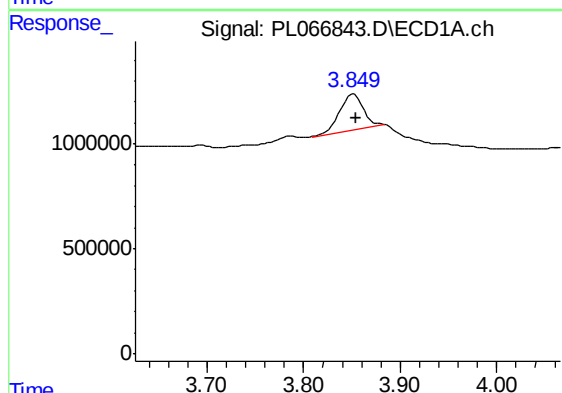


#2 alpha-BHC

R.T.: 3.851 min
Delta R.T.: -0.003 min
Response: 2949816
Conc: 1.52 ng/ml

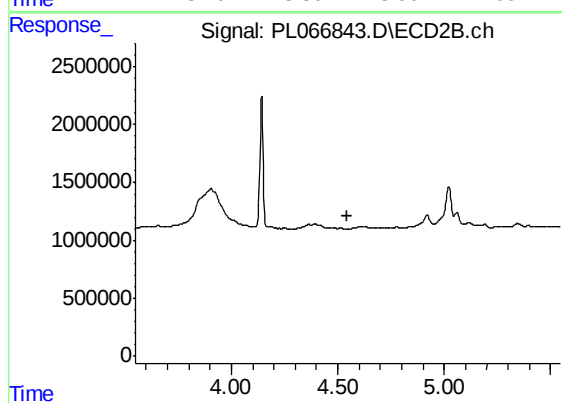

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.546 min
Response: 0
Conc: N.D.

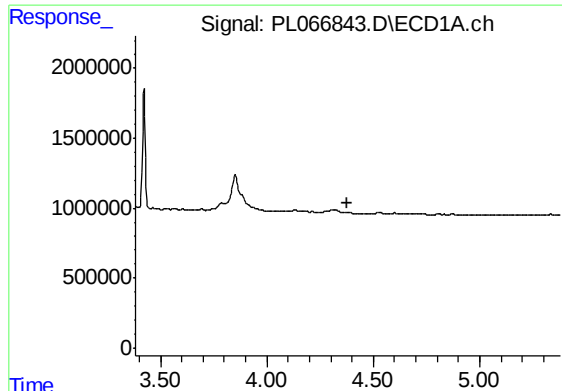

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PSTDICC005

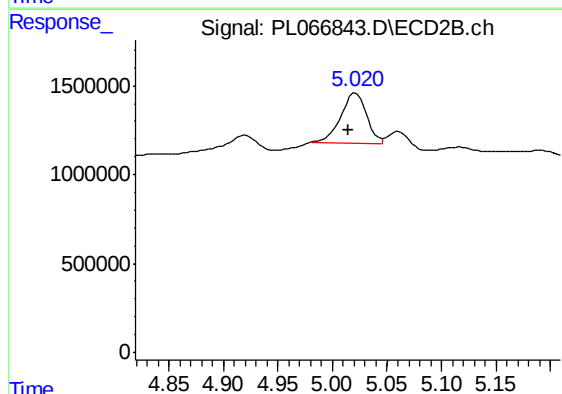


#6 beta-BHC

R.T.: 5.022 min
Delta R.T.: 0.007 min
Response: 4699190
Conc: 3.43 ng/ml

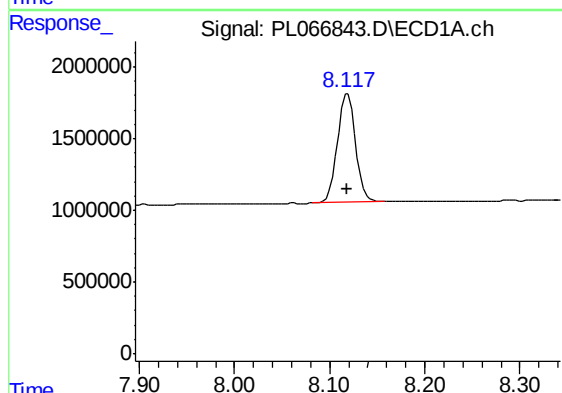

#28 Decachlorobiphenyl

R.T.: 8.119 min
Delta R.T.: 0.000 min
Response: 10162939
Conc: 6.17 ng/ml

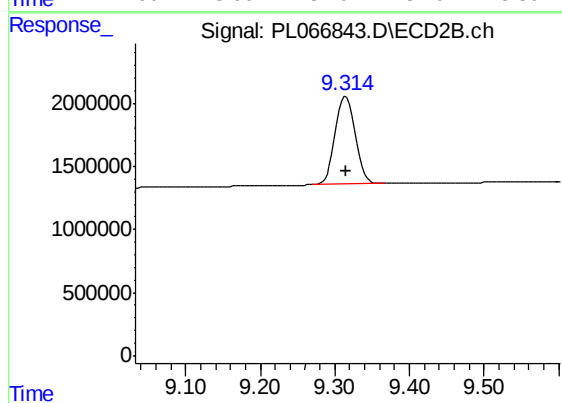

#28 Decachlorobiphenyl

R.T.: 9.315 min
Delta R.T.: 0.000 min
Response: 12899554
Conc: 6.62 ng/ml