

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052021\
 Data File : PS015053.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2021 17:26
 Operator : DD\AJ
 Sample : PB136572BS
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB136572BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 04:59:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
 Quant Title : 8080.M
 QLast Update : Tue May 11 00:04:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.155	6.884	843.2E6	250.6E6	503.944	517.902
Target Compounds							
1) T	Dalapon	3.005	2.602	888.5E6	308.2E6	434.415	456.038
2) T	3,5-DICHL...	6.382	6.048	1111.3E6	378.4E6	474.124	489.816
3) T	4-Nitroph...	6.993	6.506	371.1E6	143.2E6	446.259	482.266
5) T	DICAMBA	7.342	7.049	3155.3E6	1079.6E6	481.532	504.080
6) T	MCPD	7.506	7.140	231.0E6	89664082	47.239	50.731
7) T	MCPA	7.653	7.355	324.6E6	121.9E6	46.723	48.549
8) T	DICHLORPROP	8.027	7.674	755.0E6	266.8E6	473.378	493.417
9) T	2,4-D	8.260	7.973	824.0E6	301.4E6	463.064	494.974
10) T	Pentachlo...	8.561	8.392	11795.5E6	3819.8E6	501.703	529.775
11) T	2,4,5-TP ...	9.106	8.754	4473.2E6	1475.9E6	489.465	512.088
12) T	2,4,5-T	9.393	9.135	4425.9E6	1372.8E6	483.949	514.376
13) T	2,4-DB	9.941	9.641	771.0E6	176.9E6	444.344	501.521
14) T	DINOSEB	11.086	9.967	3432.3E6	1049.3E6	478.642	512.282
15) T	Picloram	10.919	10.957	5051.2E6	1734.5E6	415.833	435.306
16) T	DCPA	11.351	10.892	6796.2E6	2262.5E6	497.549	530.823



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052021\
Data File : PS015053.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2021 17:26
Operator : DD\AJ
Sample : PB136572BS
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB136572BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 04:59:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051021.M
Quant Title : 8080.M
QLast Update : Tue May 11 00:04:04 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

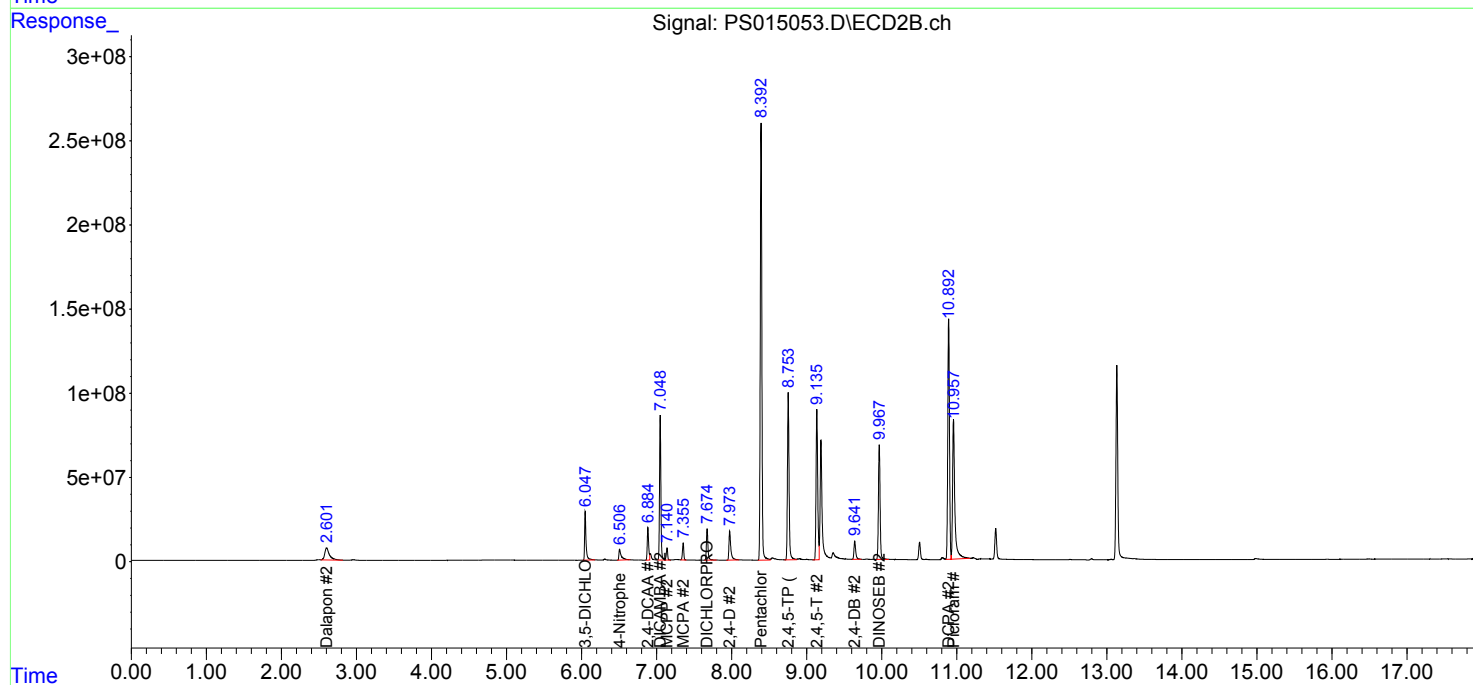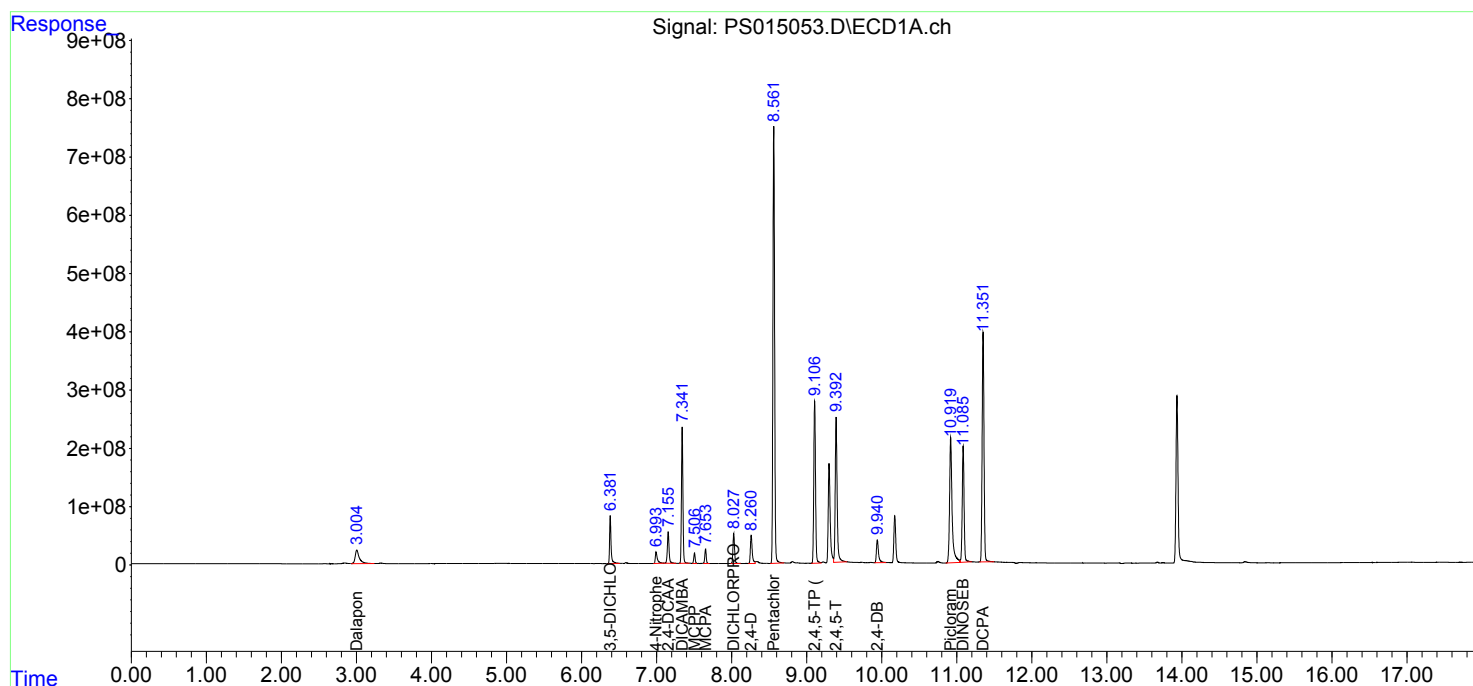


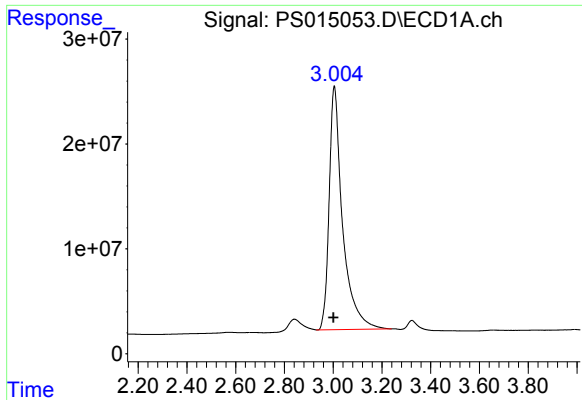

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: 0.004 min
Response: 888548790
Conc: 434.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

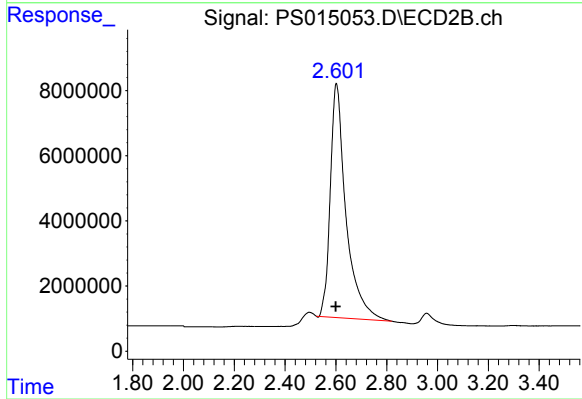


#1 Dalapon

R.T.: 2.602 min
Delta R.T.: 0.003 min
Response: 308241624
Conc: 456.04 ng/ml

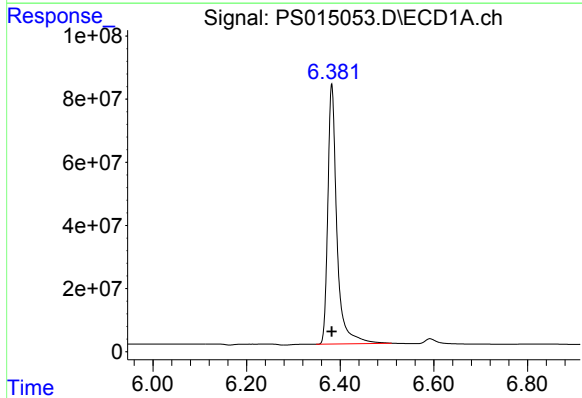


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.382 min
Delta R.T.: 0.000 min
Response: 1111259560
Conc: 474.12 ng/ml

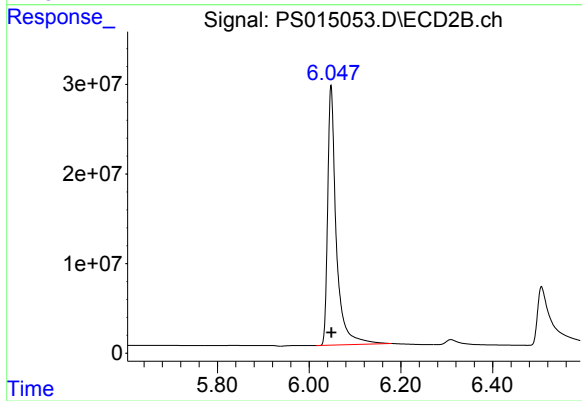

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.048 min
Delta R.T.: 0.000 min
Response: 378392699
Conc: 489.82 ng/ml

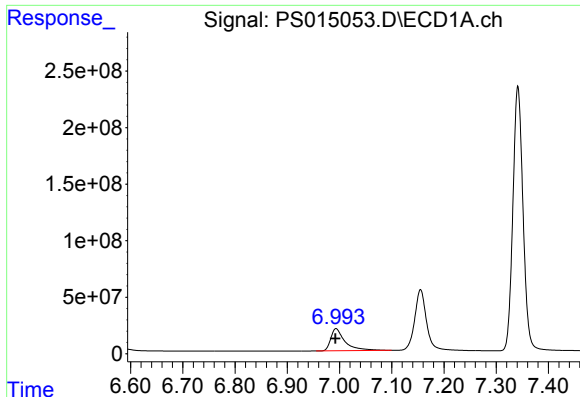

#3 4-Nitrophenol


R.T.: 6.993 min
Delta R.T.: 0.001 min
Response: 371067148
Conc: 446.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

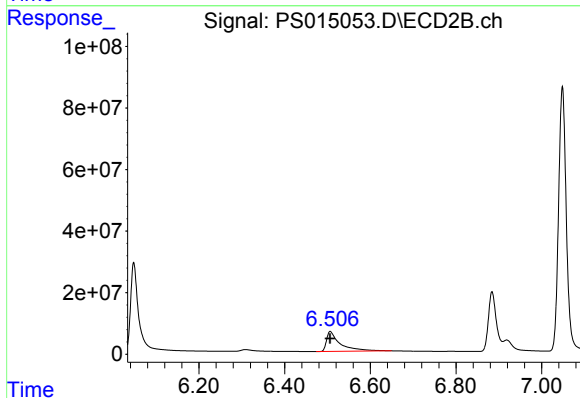


#3 4-Nitrophenol

R.T.: 6.506 min
Delta R.T.: 0.000 min
Response: 143229144
Conc: 482.27 ng/ml

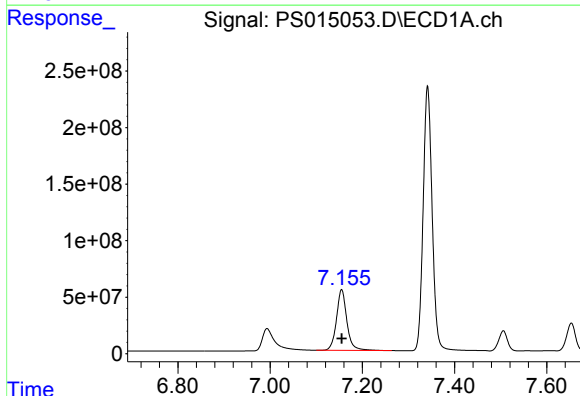


#4 2,4-DCAA

R.T.: 7.155 min
Delta R.T.: 0.000 min
Response: 843223727
Conc: 503.94 ng/ml

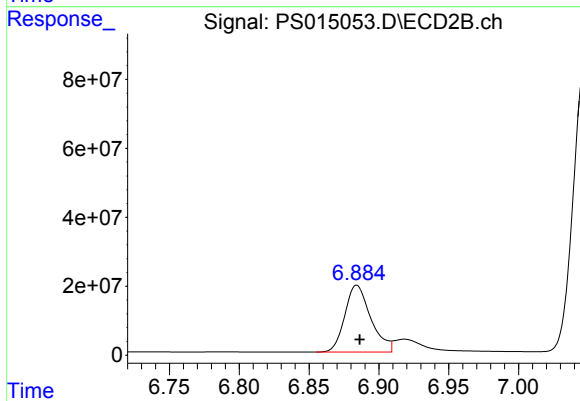

#4 2,4-DCAA


R.T.: 6.884 min
Delta R.T.: -0.002 min
Response: 250619459
Conc: 517.90 ng/ml

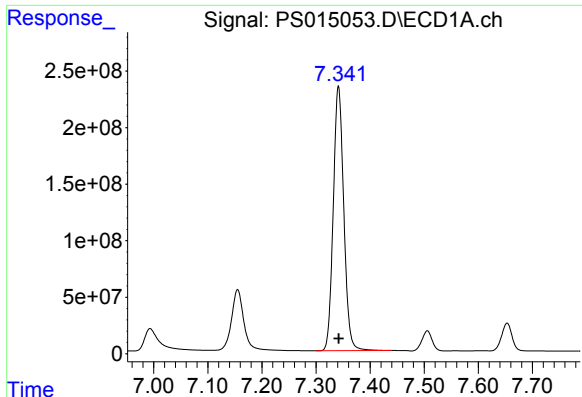

#5 DICAMBA


R.T.: 7.342 min
Delta R.T.: 0.000 min
Response: 3155290221
Conc: 481.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

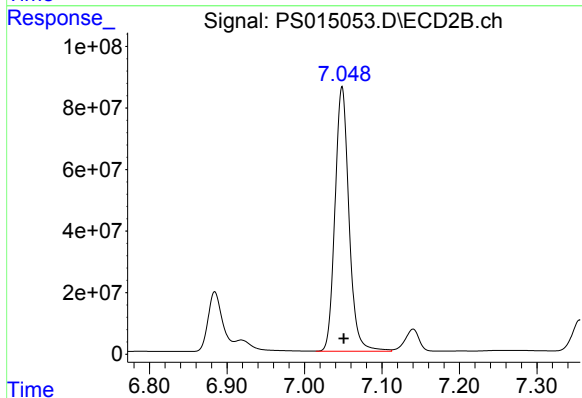


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.002 min
Response: 1079608246
Conc: 504.08 ng/ml

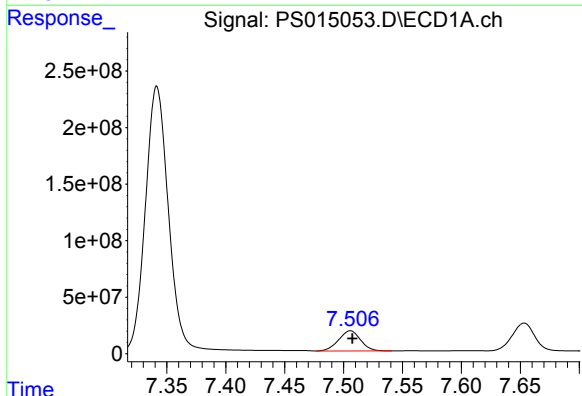


#6 MCP

R.T.: 7.506 min
Delta R.T.: -0.002 min
Response: 230986286
Conc: 47.24 ug/ml

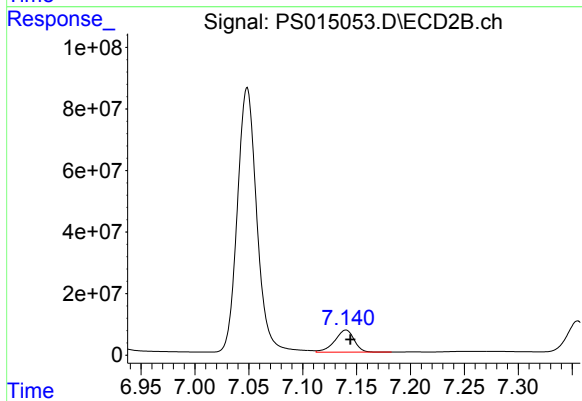

#6 MCP


R.T.: 7.140 min
Delta R.T.: -0.004 min
Response: 89664082
Conc: 50.73 ug/ml

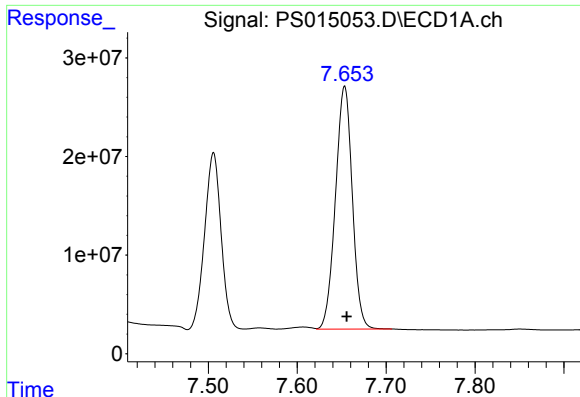

#7 MCPA


R.T.: 7.653 min
Delta R.T.: -0.002 min
Response: 324589921
Conc: 46.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

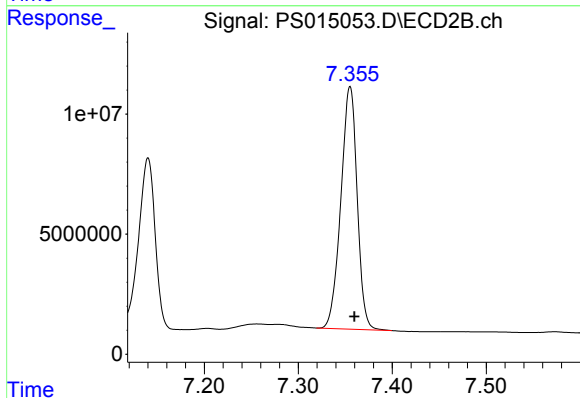


#7 MCPA

R.T.: 7.355 min
Delta R.T.: -0.005 min
Response: 121948972
Conc: 48.55 ug/ml

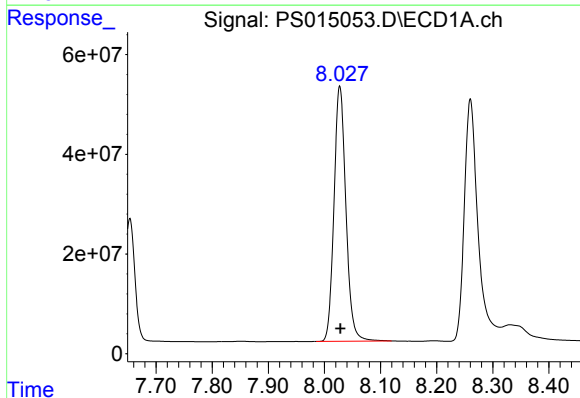


#8 DICHLORPROP

R.T.: 8.027 min
Delta R.T.: 0.000 min
Response: 754993688
Conc: 473.38 ng/ml

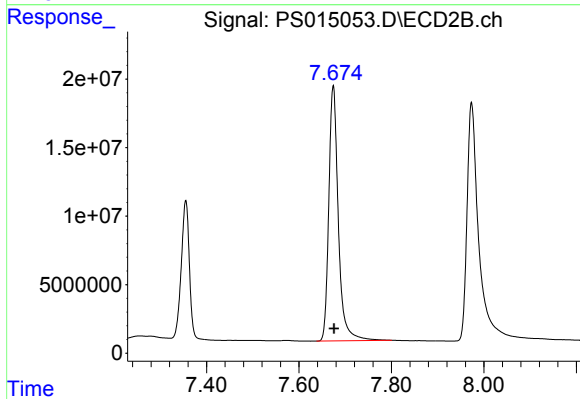

#8 DICHLORPROP


R.T.: 7.674 min
Delta R.T.: -0.002 min
Response: 266836294
Conc: 493.42 ng/ml

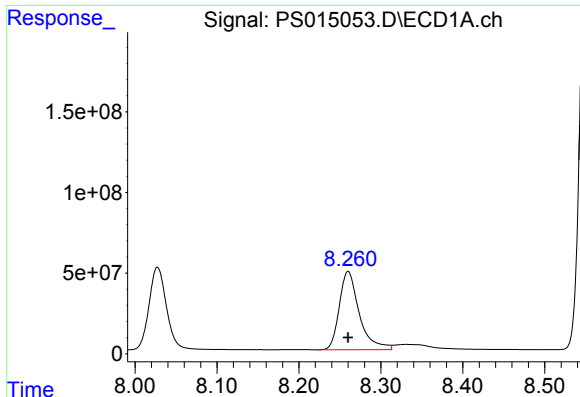

#9 2,4-D


R.T.: 8.260 min
Delta R.T.: 0.000 min
Response: 824036434
Conc: 463.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

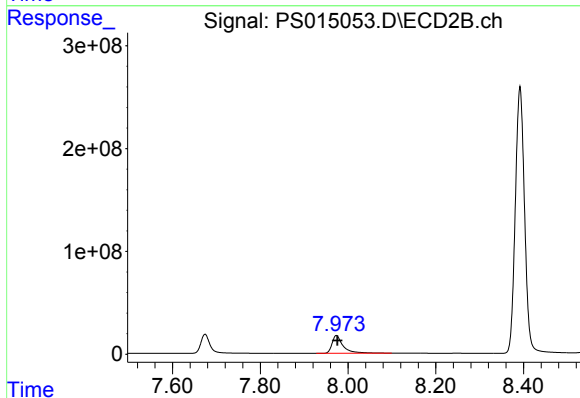


#9 2,4-D

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 301403519
Conc: 494.97 ng/ml

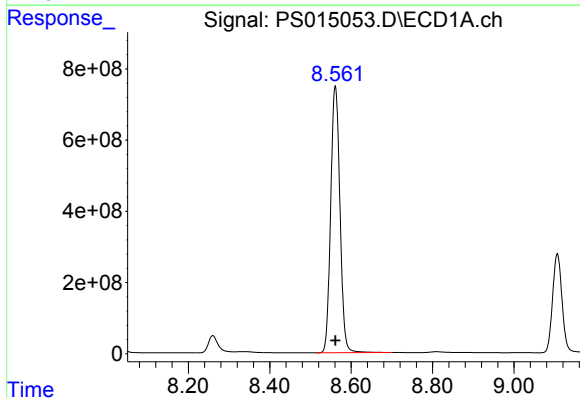


#10 Pentachlorophenol

R.T.: 8.561 min
Delta R.T.: 0.000 min
Response: 11795456648
Conc: 501.70 ng/ml

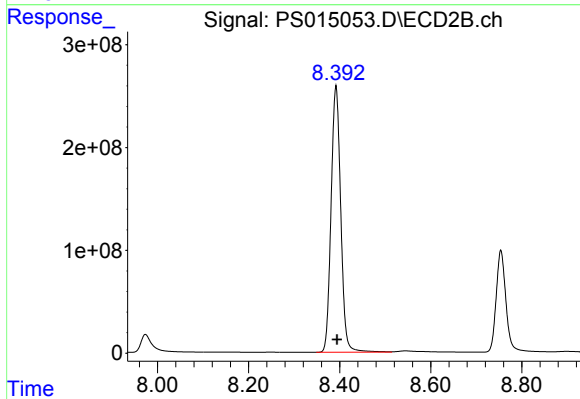

#10 Pentachlorophenol


R.T.: 8.392 min
Delta R.T.: -0.002 min
Response: 3819804574
Conc: 529.77 ng/ml

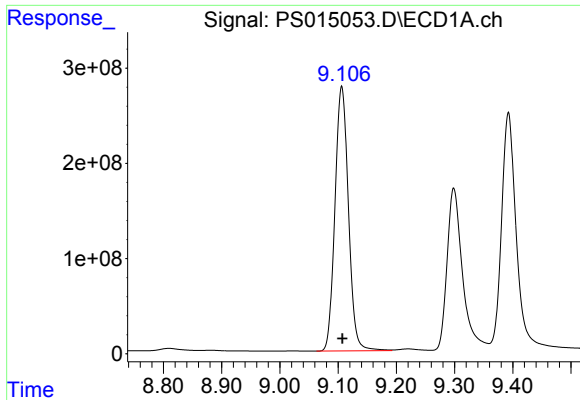

#11 2,4,5-TP (SILVEX)


R.T.: 9.106 min
Delta R.T.: -0.001 min
Response: 4473249330
Conc: 489.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

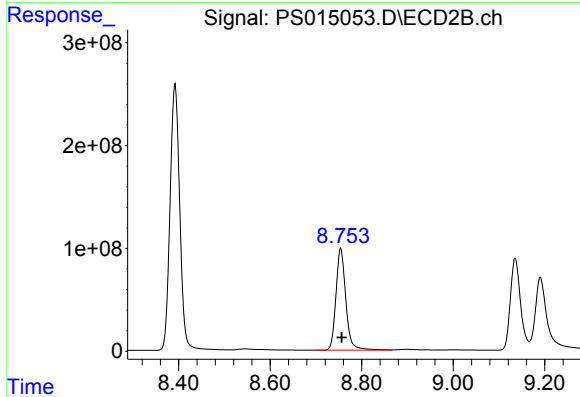


#11 2,4,5-TP (SILVEX)

R.T.: 8.754 min
Delta R.T.: -0.002 min
Response: 1475866090
Conc: 512.09 ng/ml

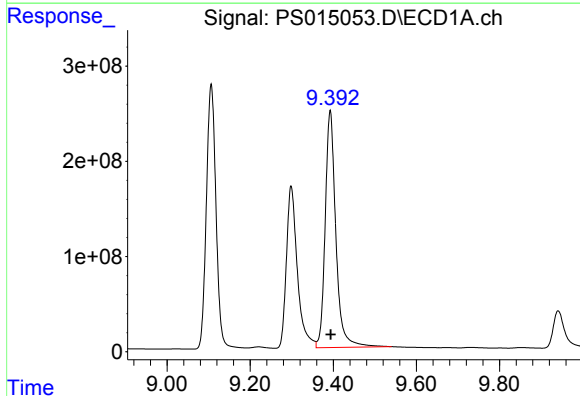


#12 2,4,5-T

R.T.: 9.393 min
Delta R.T.: -0.001 min
Response: 4425907590
Conc: 483.95 ng/ml

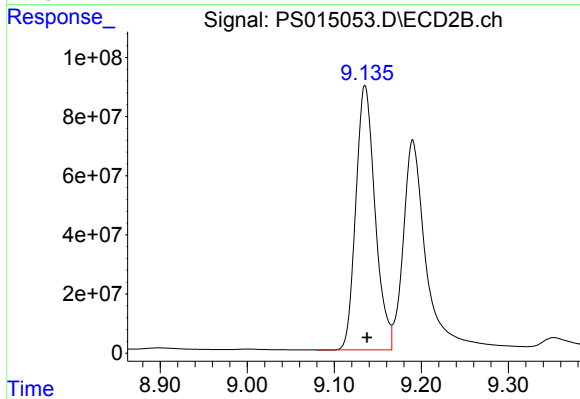

#12 2,4,5-T


R.T.: 9.135 min
Delta R.T.: -0.002 min
Response: 1372804149
Conc: 514.38 ng/ml

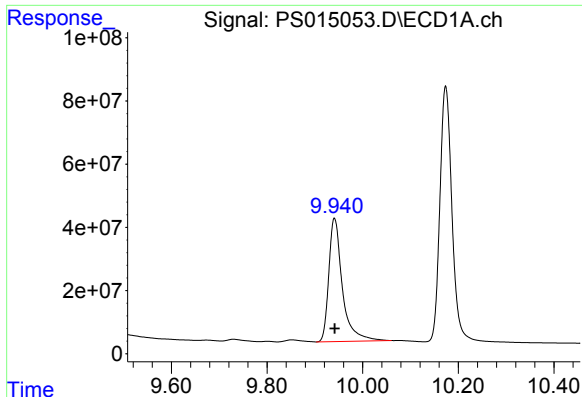

#13 2,4-DB


R.T.: 9.941 min
Delta R.T.: 0.000 min
Response: 771014994
Conc: 444.34 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

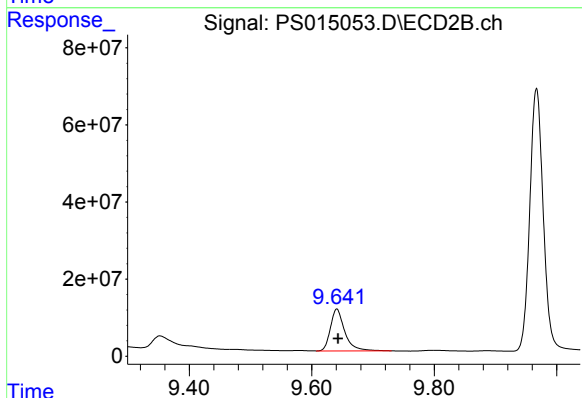


#13 2,4-DB

R.T.: 9.641 min
Delta R.T.: -0.002 min
Response: 176918960
Conc: 501.52 ng/ml

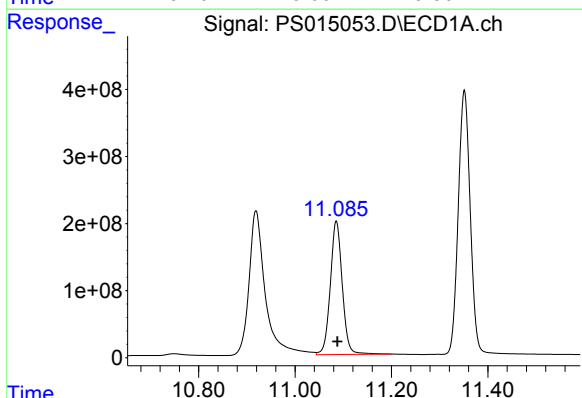


#14 DINOSEB

R.T.: 11.086 min
Delta R.T.: -0.002 min
Response: 3432342998
Conc: 478.64 ng/ml

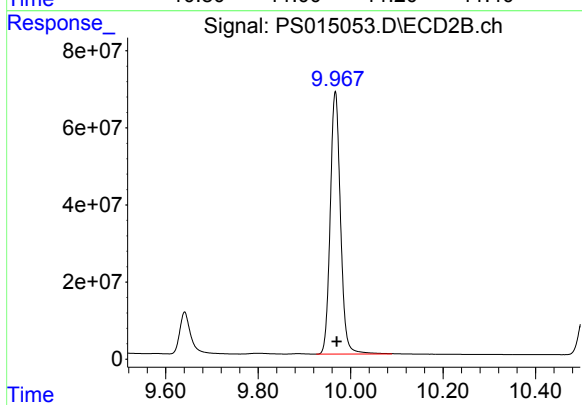

#14 DINOSEB


R.T.: 9.967 min
Delta R.T.: -0.003 min
Response: 1049257444
Conc: 512.28 ng/ml

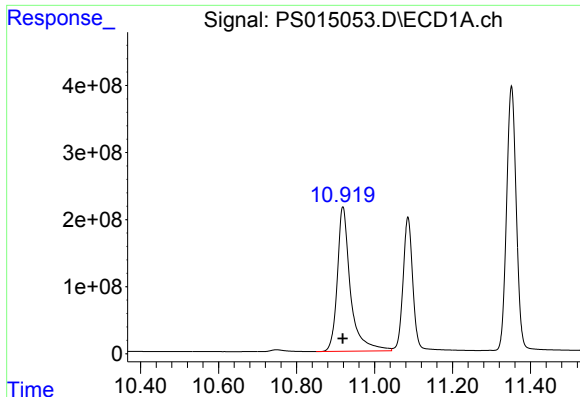

#15 Picloram


R.T.: 10.919 min
Delta R.T.: 0.000 min
Response: 5051240922
Conc: 415.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB136572BS

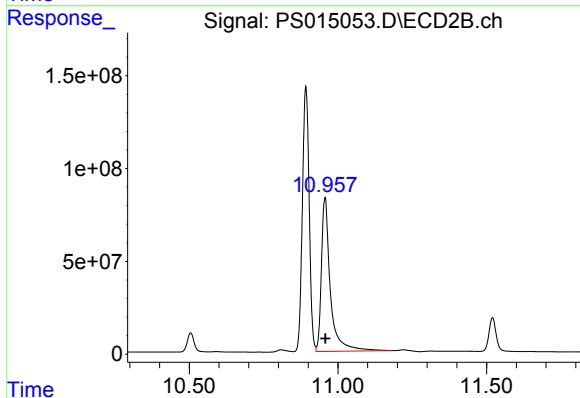


#15 Picloram

R.T.: 10.957 min
Delta R.T.: -0.001 min
Response: 1734548969
Conc: 435.31 ng/ml

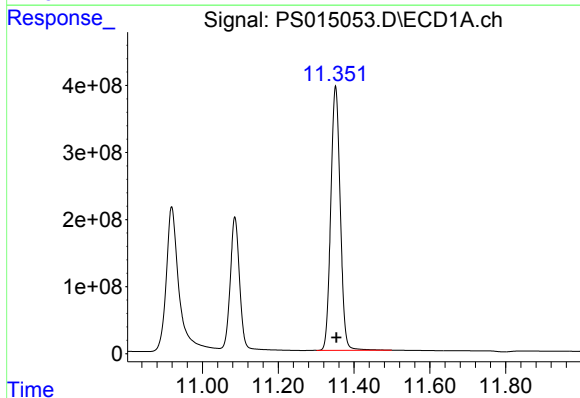

#16 DCPA

R.T.: 11.351 min
Delta R.T.: -0.002 min
Response: 6796232095
Conc: 497.55 ng/ml

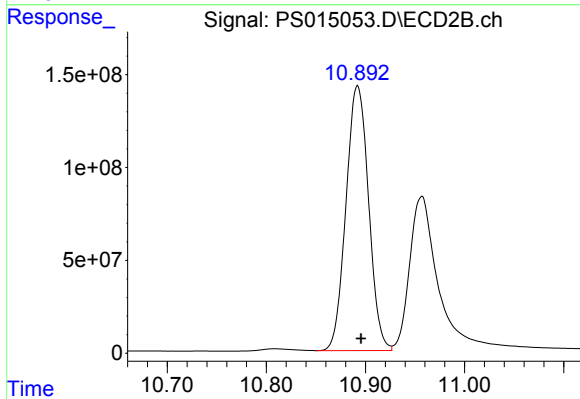

#16 DCPA

R.T.: 10.892 min
Delta R.T.: -0.004 min
Response: 2262544586
Conc: 530.82 ng/ml