

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052022\
 Data File : PS019490.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 May 2022 09:40
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 20 22:38:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
 Quant Title : 8080.M
 QLast Update : Wed May 04 16:27:11 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.247	0.000	846146	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	3.071f	0.000	317952	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.461	5.931f	663249	90530	<MDL	<MDL #
3) T	4-Nitroph...	0.000	6.401	0	215544	N.D.	<MDL
5) T	DICAMBA	7.423	0.000	2525637	0	<MDL	N.D. #
6) T	MCPD	7.601	0.000	160168	0	<MDL	N.D. #
7) T	MCPA	7.750	0.000	2803925	0	<MDL	N.D. #
10) T	Pentachlo...	8.654	8.307	5240545	1303968	<MDL	<MDL #
11) T	2,4,5-TP ...	9.212	8.674	4891627	1099536	<MDL	<MDL #
12) T	2,4,5-T	9.468	9.076	15515567	2070133	<MDL	<MDL #
13) T	2,4-DB	10.019	9.580	666242	778400	<MDL	1.369 #
14) T	DINOSEB	11.184	9.877	51419433	1543881	3.114	<MDL #
15) T	Picloram	10.998	10.801f	415.6E6	14800852	14.219	2.475 #
16) T	DCPA	11.457	10.801	17068793	14800852	<MDL	2.521 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052022\
Data File : PS019490.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 May 2022 09:40
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 20 22:38:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS050422.M
Quant Title : 8080.M
QLast Update : Wed May 04 16:27:11 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

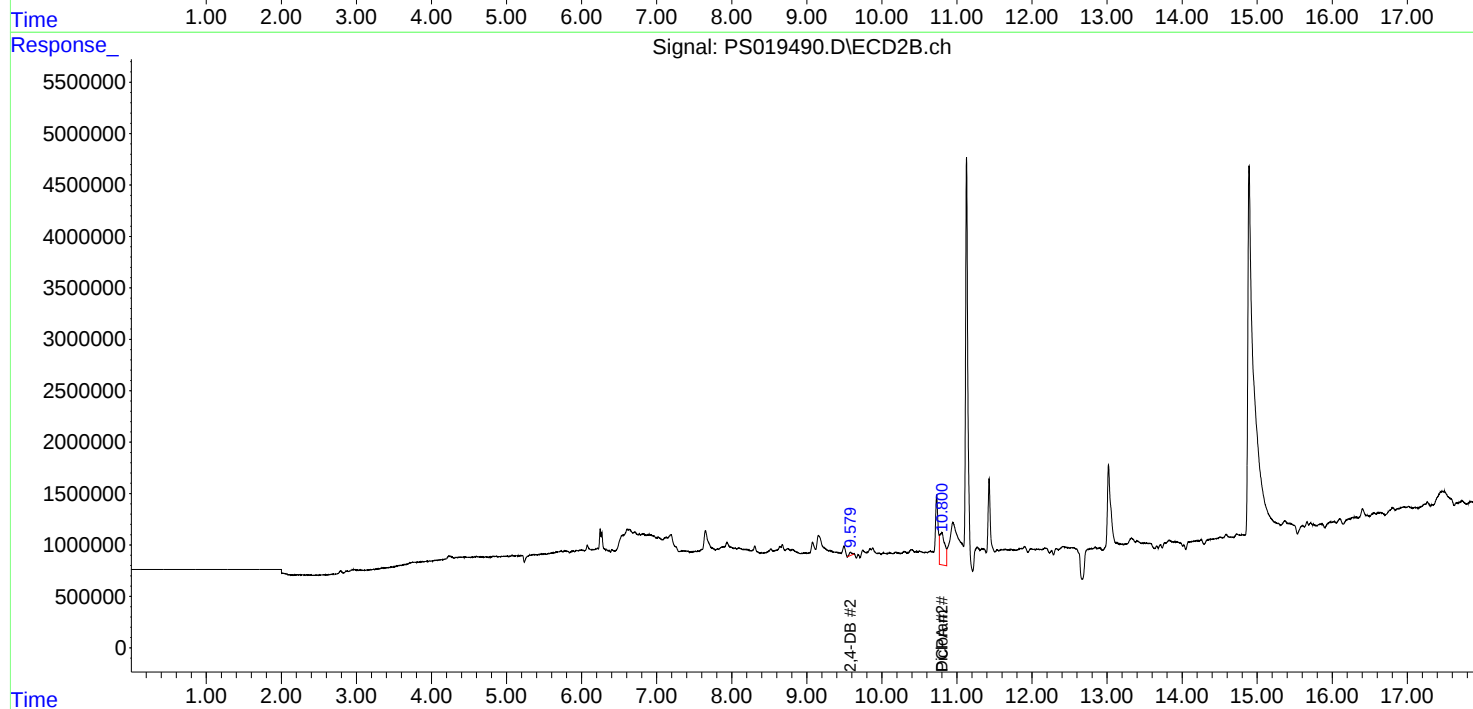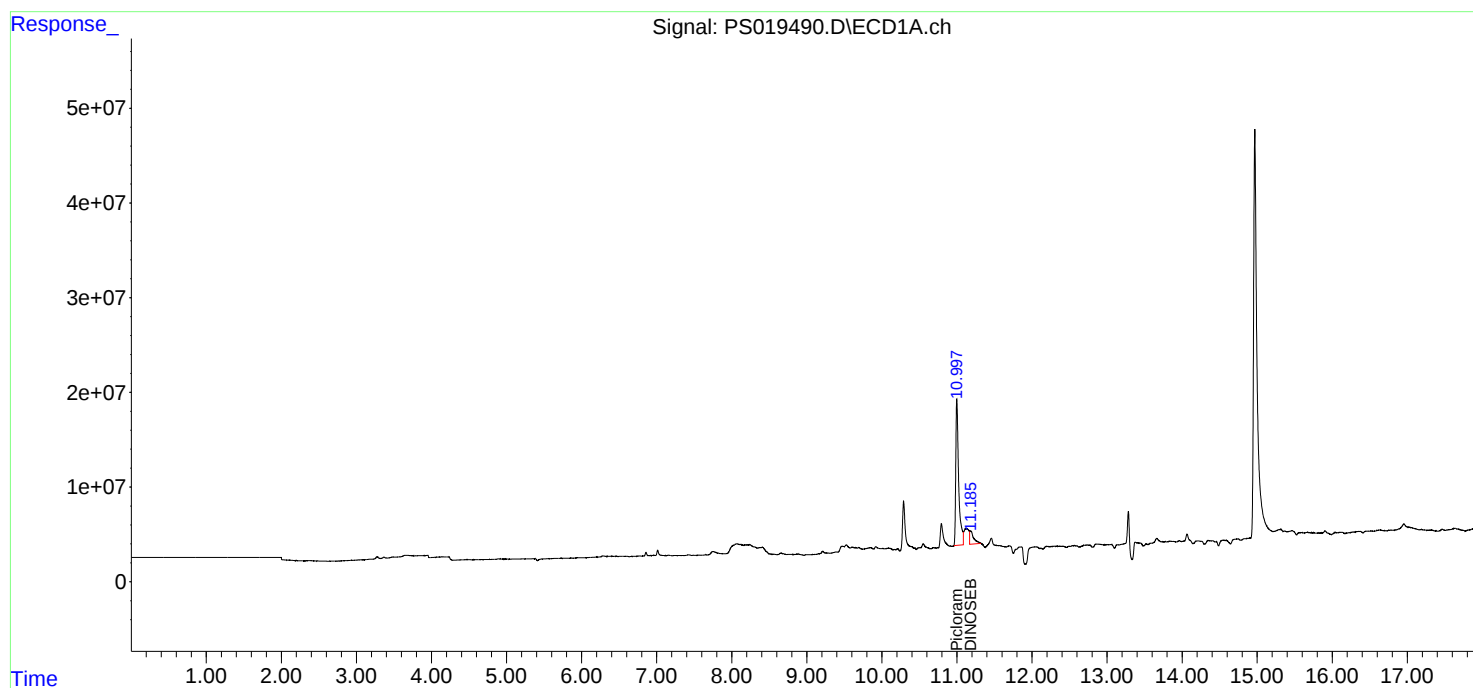


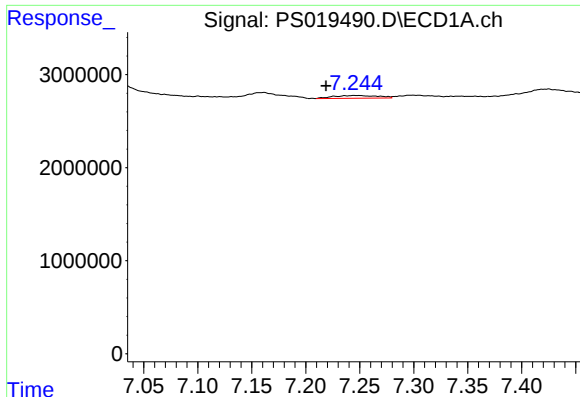

#4 2,4-DCAA


R.T.: 7.247 min
Delta R.T.: 0.028 min
Response: 846146
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

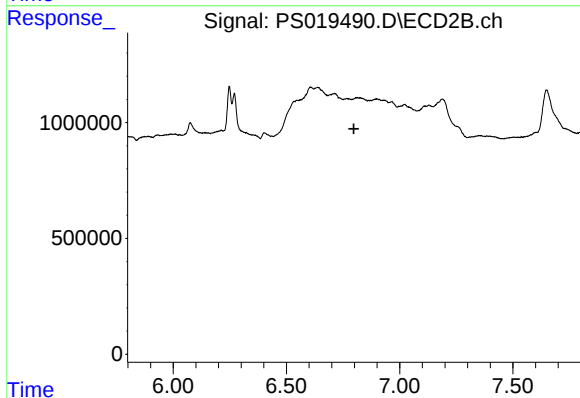


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.798 min
Response: 0
Conc: N.D.

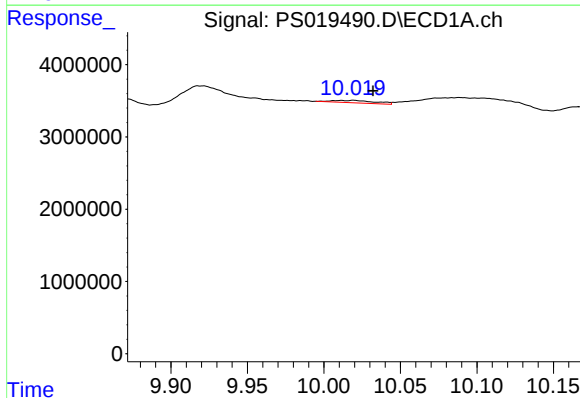


#13 2,4-DB

R.T.: 10.019 min
Delta R.T.: -0.013 min
Response: 666242
Conc: N.D.

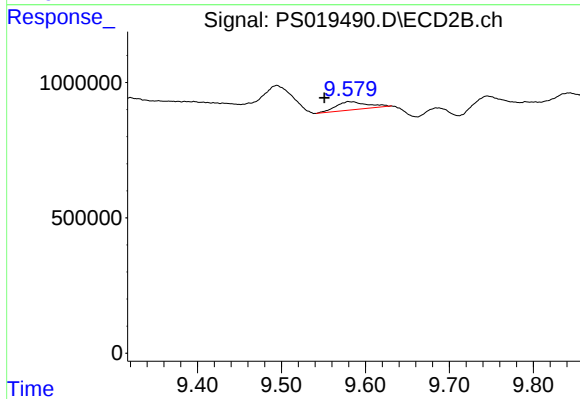

#13 2,4-DB


R.T.: 9.580 min
Delta R.T.: 0.029 min
Response: 778400
Conc: 1.37 ng/ml

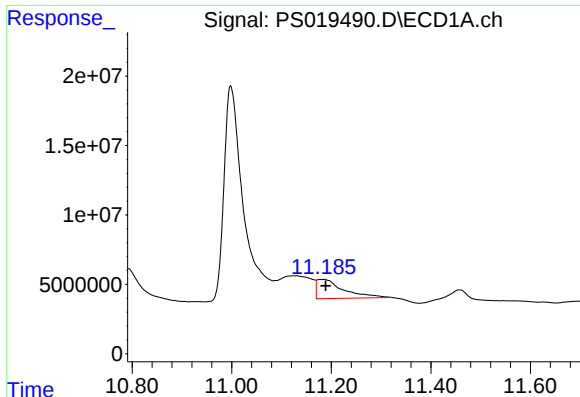

#14 DINOSEB


R.T.: 11.184 min
Delta R.T.: -0.006 min
Response: 51419433
Conc: 3.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

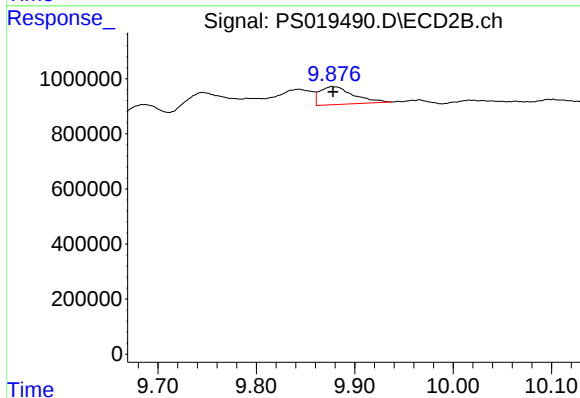


#14 DINOSEB

R.T.: 9.877 min
Delta R.T.: -0.001 min
Response: 1543881
Conc: N.D.

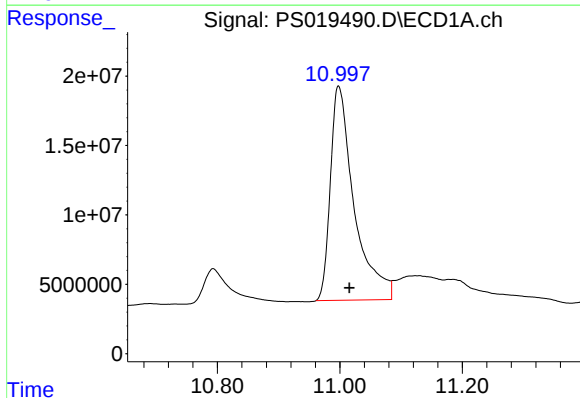


#15 Picloram

R.T.: 10.998 min
Delta R.T.: -0.017 min
Response: 415637073
Conc: 14.22 ng/ml

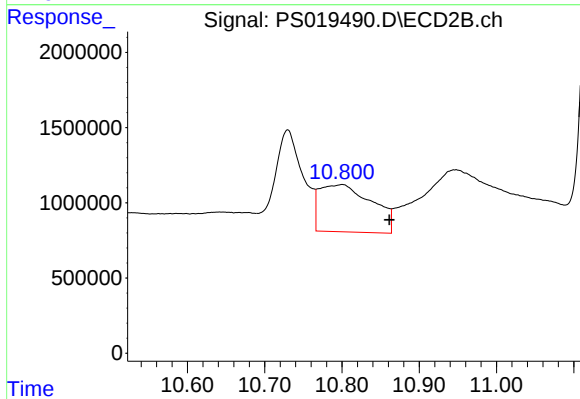

#15 Picloram


R.T.: 10.801 min
Delta R.T.: -0.061 min
Response: 14800852
Conc: 2.47 ng/ml

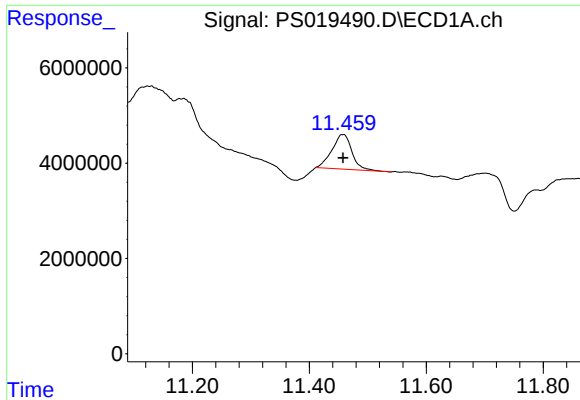

#16 DCPA

R.T.: 11.457 min
Delta R.T.: 0.000 min
Response: 17068793
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

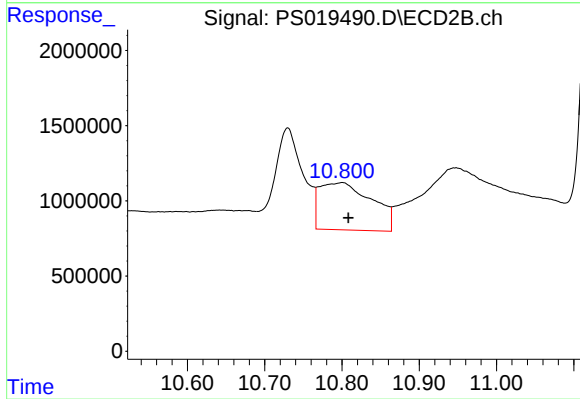

#16 DCPA

R.T.: 10.801 min
Delta R.T.: -0.007 min
Response: 14800852
Conc: 2.52 ng/ml