

Data Path : P:\HPCHEM1\ECD_S\Data\PS052118\
 Data File : PS000129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2018 17:48
 Operator : UA
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:40:21 2018
 Quant Method : P:\HPCHEM1\ECD_S\Method\PS052118.M
 Quant Title : 8080.M
 QLast Update : Tue May 22 01:38:24 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.807	11.171	264.7E6	233.7E6	750.000	750.000
Target Compounds							
1) T	Dalapon	3.151	2.525	322.3E6	267.8E6	682.500	682.500
2) T	3,5-DICHL...	10.219	9.316	370.9E6	305.9E6	697.500	697.500
3) T	4-Nitroph...	11.403	10.318	156.8E6	124.6E6	682.500	682.500
5) T	DICAMBA	12.126	11.461	922.8E6	784.6E6	705.000	705.000
6) T	MCPD	12.466	11.687	79835150	65772830	70.500	70.500
7) T	MCPA	12.718	12.065	132.2E6	101.9E6	69.750	69.750
8) T	DICHLORPROP	13.320	12.585	241.5E6	200.3E6	705.000	705.000
9) T	2,4-D	13.677	13.056	316.5E6	270.2E6	705.000	705.000
10) T	Pentachlo...	14.077	13.620	3559.7E6	3164.4E6	712.500	712.500
11) T	2,4,5-TP ...	14.944	14.229	1415.3E6	1232.6E6	712.500	712.500
12) T	2,4,5-T	15.341	14.760	1406.3E6	1184.8E6	712.500	715.079
13) T	2,4-DB	16.096	15.449	193.7E6	150.9E6	712.500	712.500
14) T	DINOSEB	17.610	15.881	1034.8E6	879.0E6	705.000	705.000
15) T	Picloram	17.366	17.128	1883.3E6	1562.5E6	712.500	712.500
16) T	DCPA	17.950	17.069	1747.0E6	1501.0E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : P:\HPCHEM1\ECD_S\Data\PS052118\
Data File : PS000129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2018 17:48
Operator : UA
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:40:21 2018
Quant Method : P:\HPCHEM1\ECD_S\Method\PS052118.M
Quant Title : 8080.M
QLast Update : Tue May 22 01:38:24 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

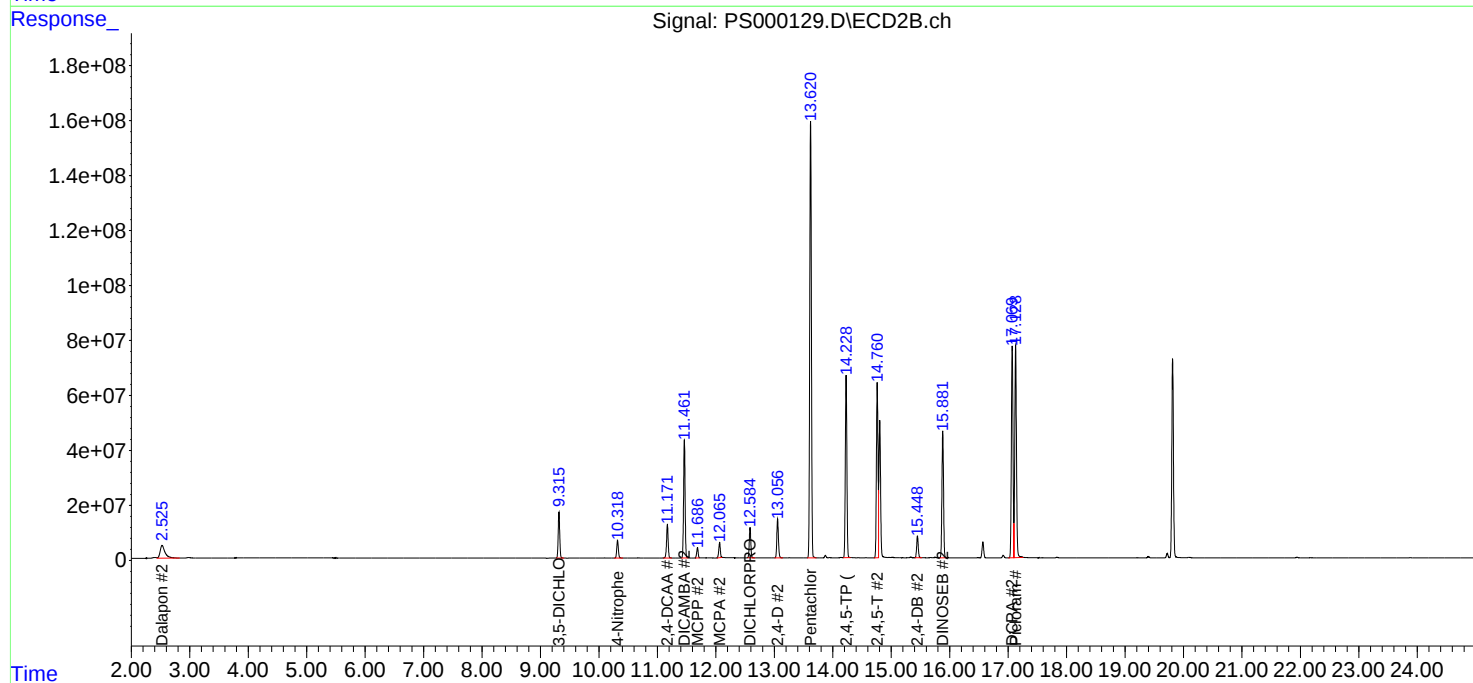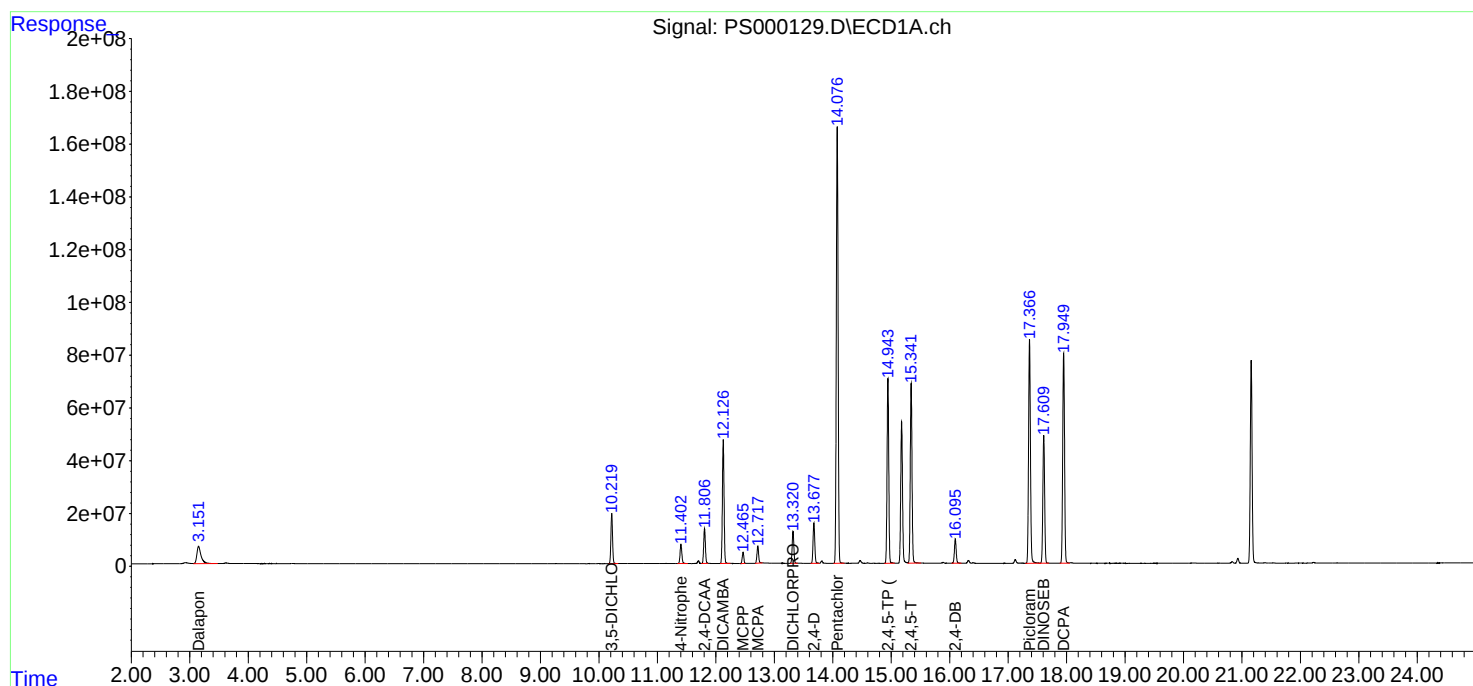


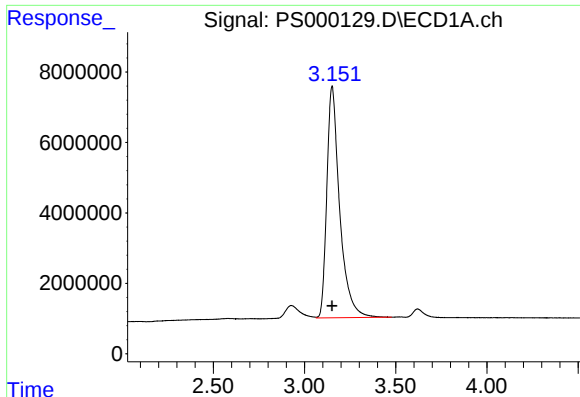

#1 Dalapon


R.T.: 3.151 min
Delta R.T.: 0.000 min
Response: 322289802
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

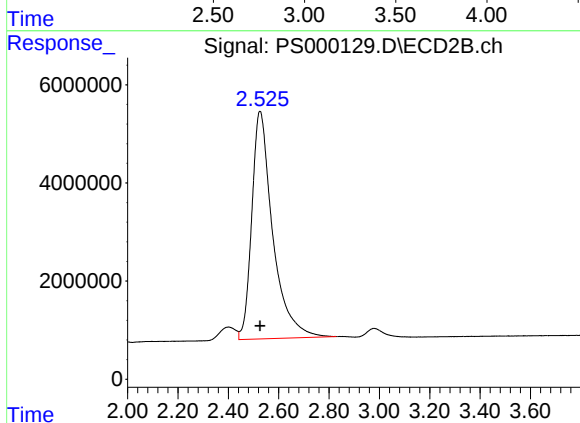


#1 Dalapon

R.T.: 2.525 min
Delta R.T.: 0.000 min
Response: 267773228
Conc: 682.50 ng/ml

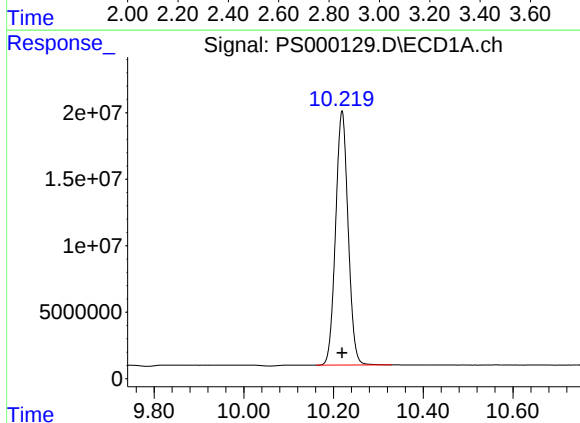


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.219 min
Delta R.T.: 0.000 min
Response: 370859975
Conc: 697.50 ng/ml

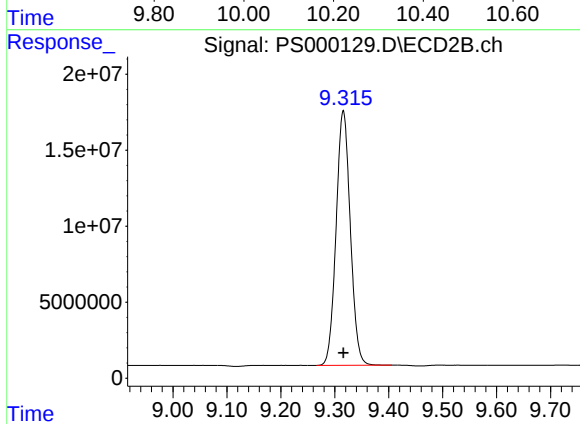

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.316 min
Delta R.T.: 0.000 min
Response: 305918347
Conc: 697.50 ng/ml

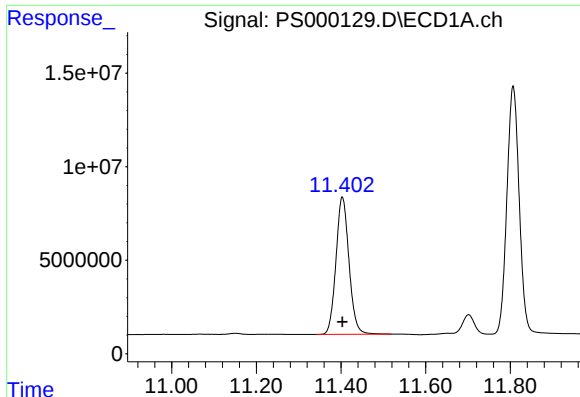

#3 4-Nitrophenol


R.T.: 11.403 min
Delta R.T.: 0.000 min
Response: 156782330
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

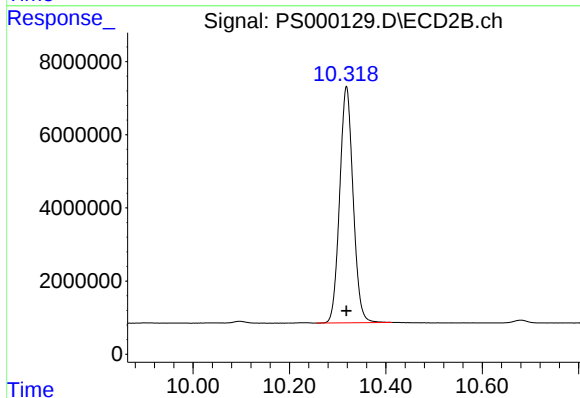


#3 4-Nitrophenol

R.T.: 10.318 min
Delta R.T.: 0.000 min
Response: 124576947
Conc: 682.50 ng/ml

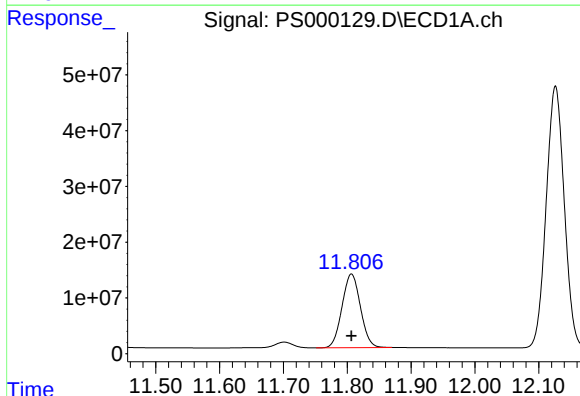


#4 2,4-DCAA

R.T.: 11.807 min
Delta R.T.: 0.000 min
Response: 264674020
Conc: 750.00 ng/ml

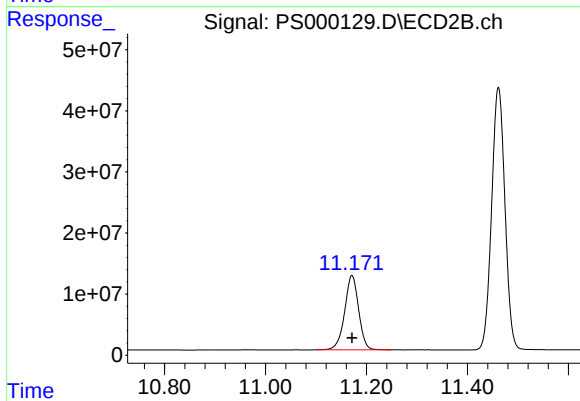

#4 2,4-DCAA


R.T.: 11.171 min
Delta R.T.: 0.000 min
Response: 233731338
Conc: 750.00 ng/ml

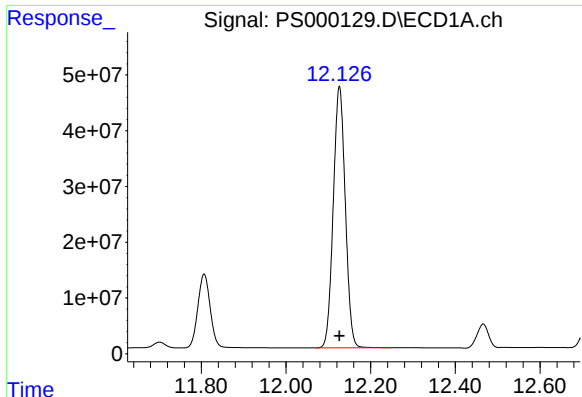

#5 DICAMBA


R.T.: 12.126 min
Delta R.T.: 0.000 min
Response: 922848186
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

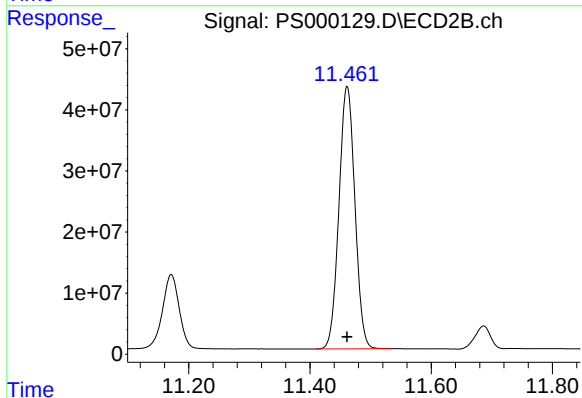


#5 DICAMBA

R.T.: 11.461 min
Delta R.T.: 0.000 min
Response: 784553601
Conc: 705.00 ng/ml

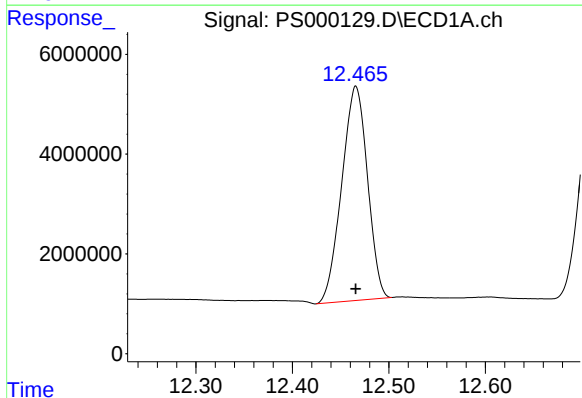


#6 MCP

R.T.: 12.466 min
Delta R.T.: 0.000 min
Response: 79835150
Conc: 70.50 ug/ml

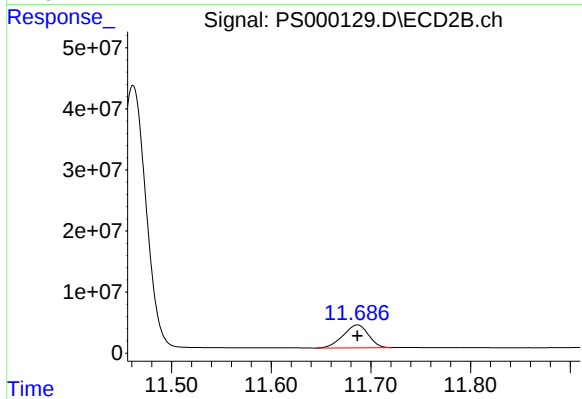

#6 MCP


R.T.: 11.687 min
Delta R.T.: 0.000 min
Response: 65772830
Conc: 70.50 ug/ml

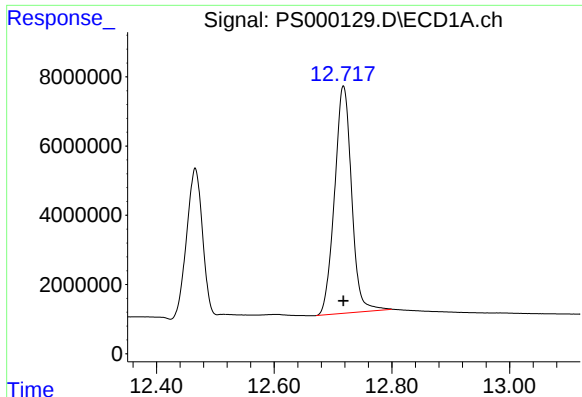

#7 MCPA


R.T.: 12.718 min
Delta R.T.: 0.000 min
Response: 132240412
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

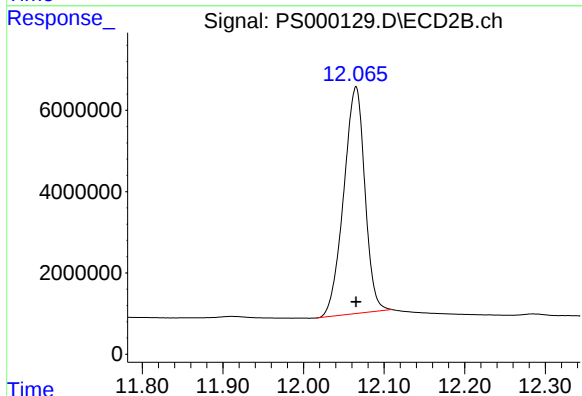


#7 MCPA

R.T.: 12.065 min
Delta R.T.: 0.000 min
Response: 101894862
Conc: 69.75 ug/ml

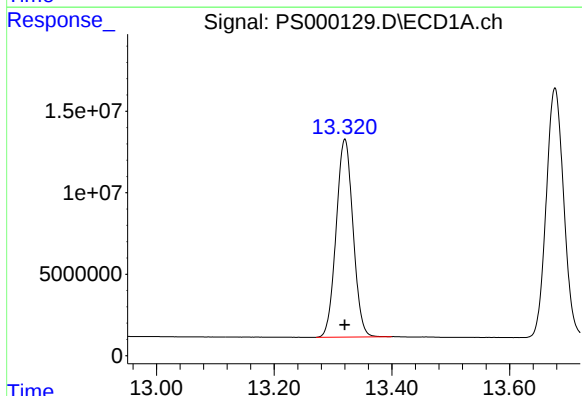


#8 DICHLORPROP

R.T.: 13.320 min
Delta R.T.: 0.000 min
Response: 241512985
Conc: 705.00 ng/ml

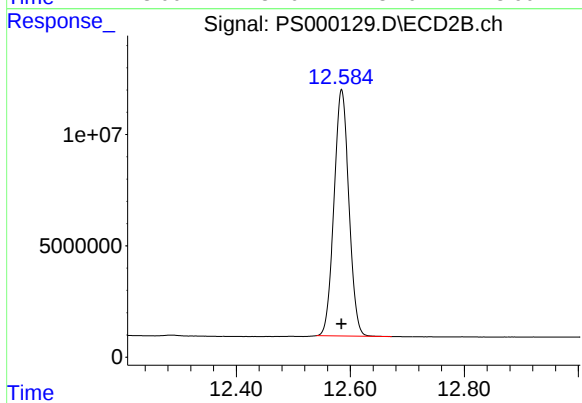

#8 DICHLORPROP


R.T.: 12.585 min
Delta R.T.: 0.000 min
Response: 200250613
Conc: 705.00 ng/ml

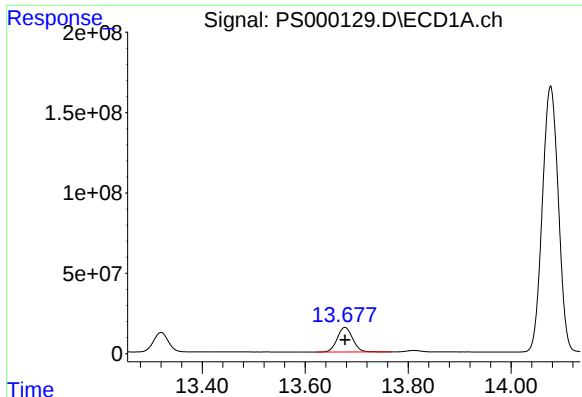

#9 2,4-D


R.T.: 13.677 min
Delta R.T.: 0.000 min
Response: 316526924
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

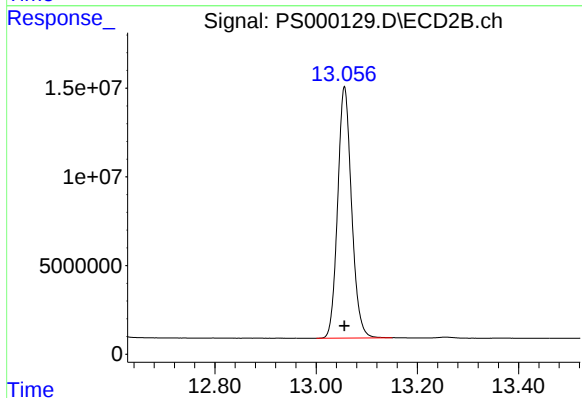


#9 2,4-D

R.T.: 13.056 min
Delta R.T.: 0.000 min
Response: 270182803
Conc: 705.00 ng/ml

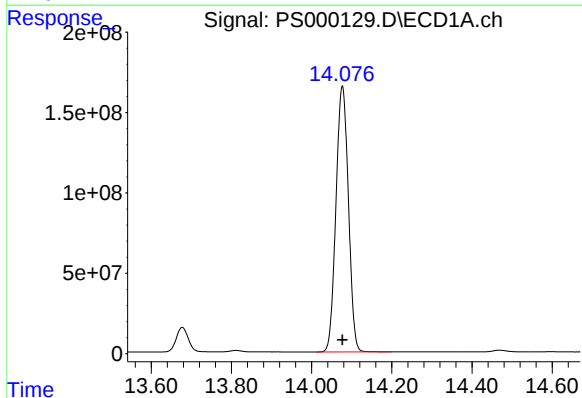


#10 Pentachlorophenol

R.T.: 14.077 min
Delta R.T.: 0.000 min
Response: 3559698217
Conc: 712.50 ng/ml

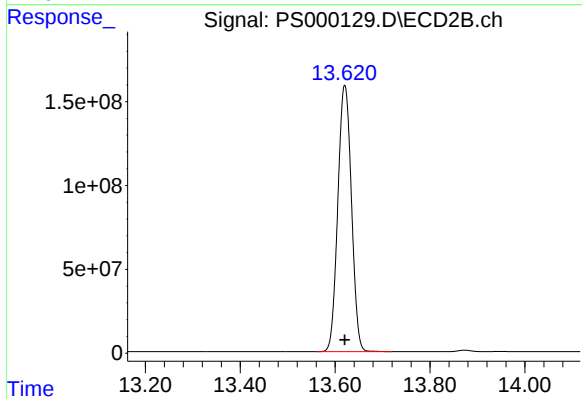

#10 Pentachlorophenol


R.T.: 13.620 min
Delta R.T.: 0.000 min
Response: 3164414536
Conc: 712.50 ng/ml

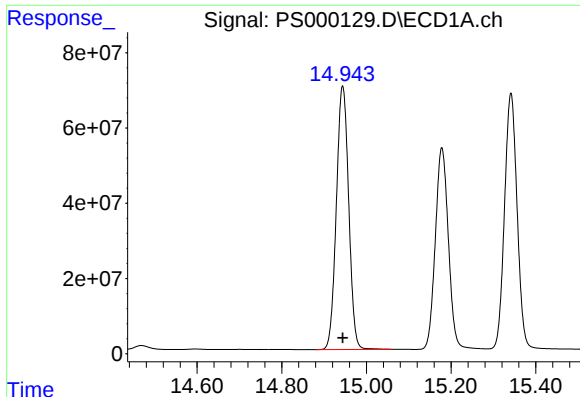

#11 2,4,5-TP (SILVEX)


R.T.: 14.944 min
Delta R.T.: 0.000 min
Response: 1415348496
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

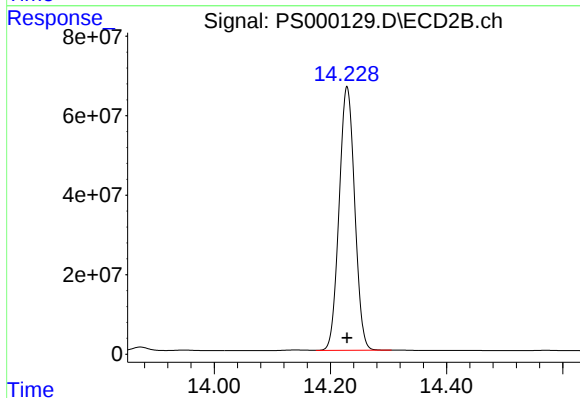


#11 2,4,5-TP (SILVEX)

R.T.: 14.229 min
Delta R.T.: 0.000 min
Response: 1232570144
Conc: 712.50 ng/ml

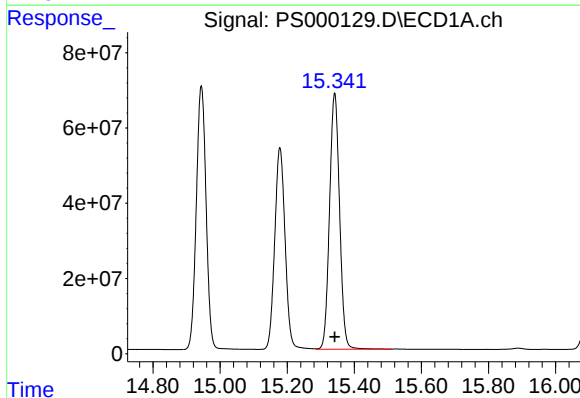


#12 2,4,5-T

R.T.: 15.341 min
Delta R.T.: 0.000 min
Response: 1406299035
Conc: 712.50 ng/ml

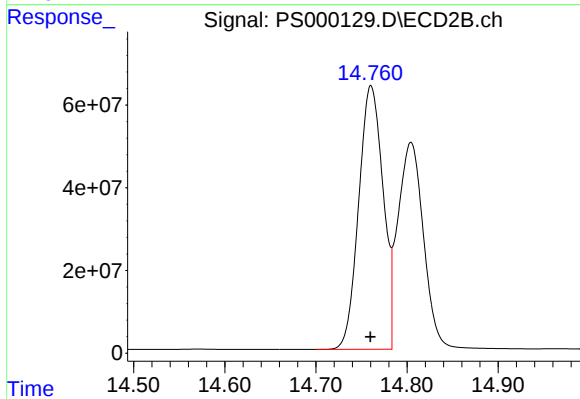

#12 2,4,5-T


R.T.: 14.760 min
Delta R.T.: 0.000 min
Response: 1184779007
Conc: 715.08 ng/ml

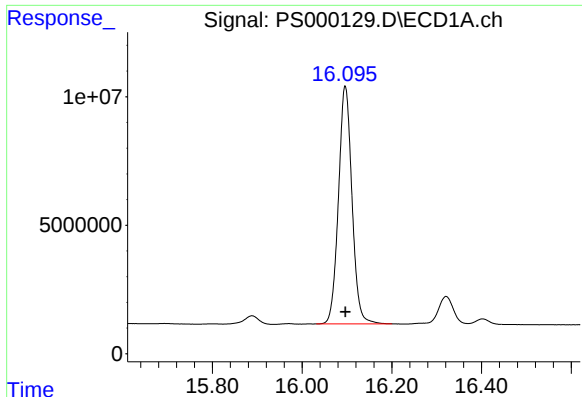

#13 2,4-DB


R.T.: 16.096 min
Delta R.T.: 0.000 min
Response: 193726241
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

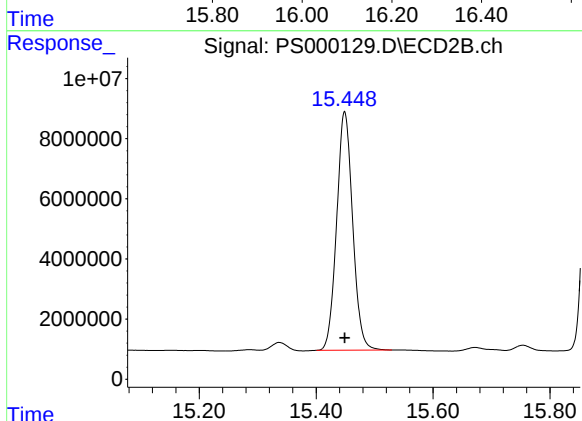


#13 2,4-DB

R.T.: 15.449 min
Delta R.T.: 0.000 min
Response: 150859454
Conc: 712.50 ng/ml

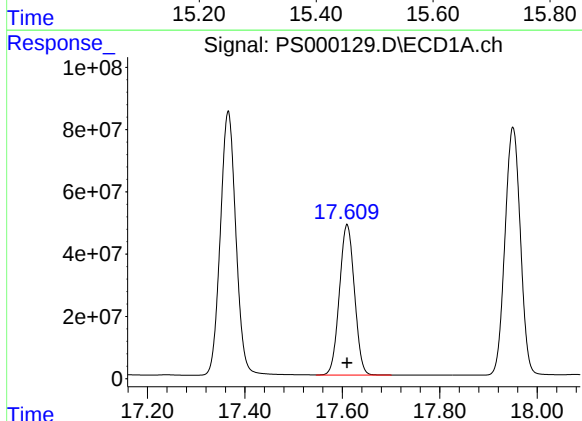


#14 DINOSEB

R.T.: 17.610 min
Delta R.T.: 0.000 min
Response: 1034750889
Conc: 705.00 ng/ml

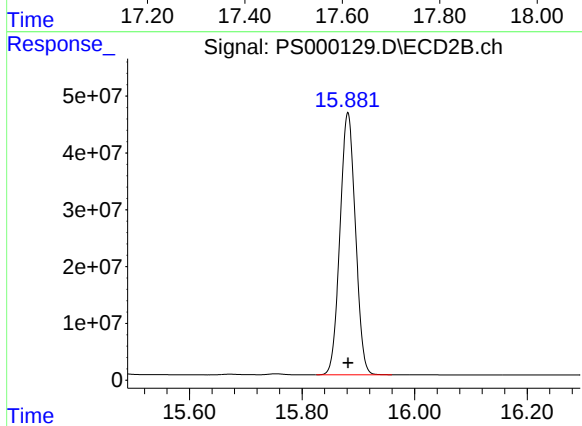

#14 DINOSEB


R.T.: 15.881 min
Delta R.T.: 0.000 min
Response: 878951591
Conc: 705.00 ng/ml

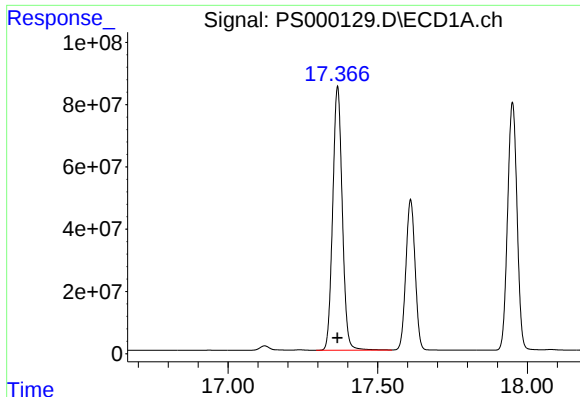

#15 Picloram


R.T.: 17.366 min
Delta R.T.: 0.000 min
Response: 1883308711
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

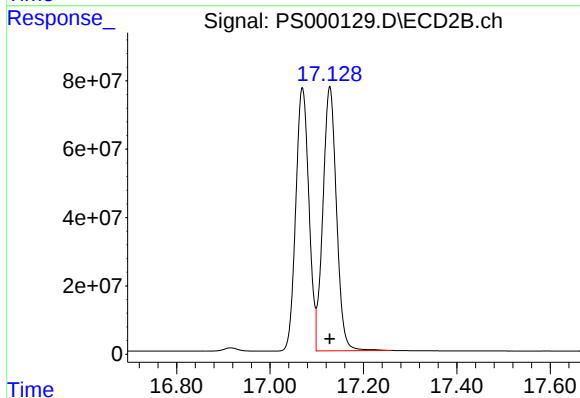


#15 Picloram

R.T.: 17.128 min
Delta R.T.: 0.000 min
Response: 1562543630
Conc: 712.50 ng/ml

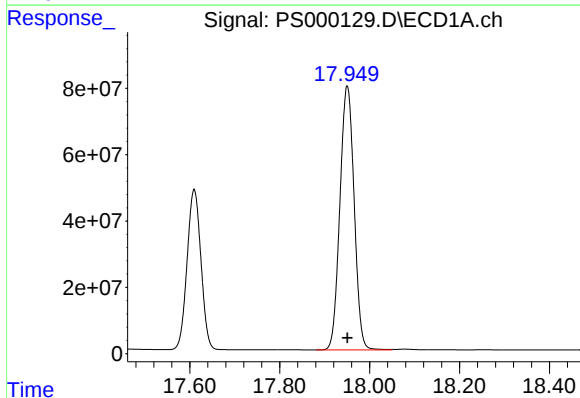

#16 DCPA

R.T.: 17.950 min
Delta R.T.: 0.000 min
Response: 1747027811
Conc: 720.00 ng/ml

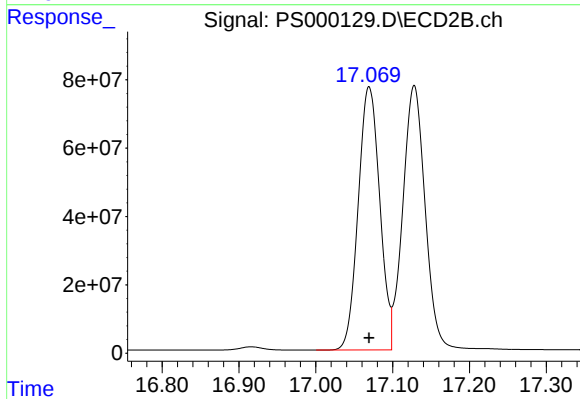

#16 DCPA

R.T.: 17.069 min
Delta R.T.: 0.000 min
Response: 1501027389
Conc: 720.00 ng/ml