

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
 Data File : PS004663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 09:26
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 11:51:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.585	5.291	690.9E6	499.2E6	492.851	517.355
Target Compounds							
9) T	2,4-D	6.670	0.000	83903756	0	61.337	N.D. #
10) T	Pentachlo...	6.878	6.634	17748109	14885792	1.011	1.212
12) T	2,4,5-T	0.000	7.410	0	46752634	N.D.	10.490
15) T	Picloram	9.138	9.115	18079510	95699283	1.735	12.827 #
16) T	DCPA	0.000	9.115	0	95699283	N.D.	14.773



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
Data File : PS004663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 09:26
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 11:51:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

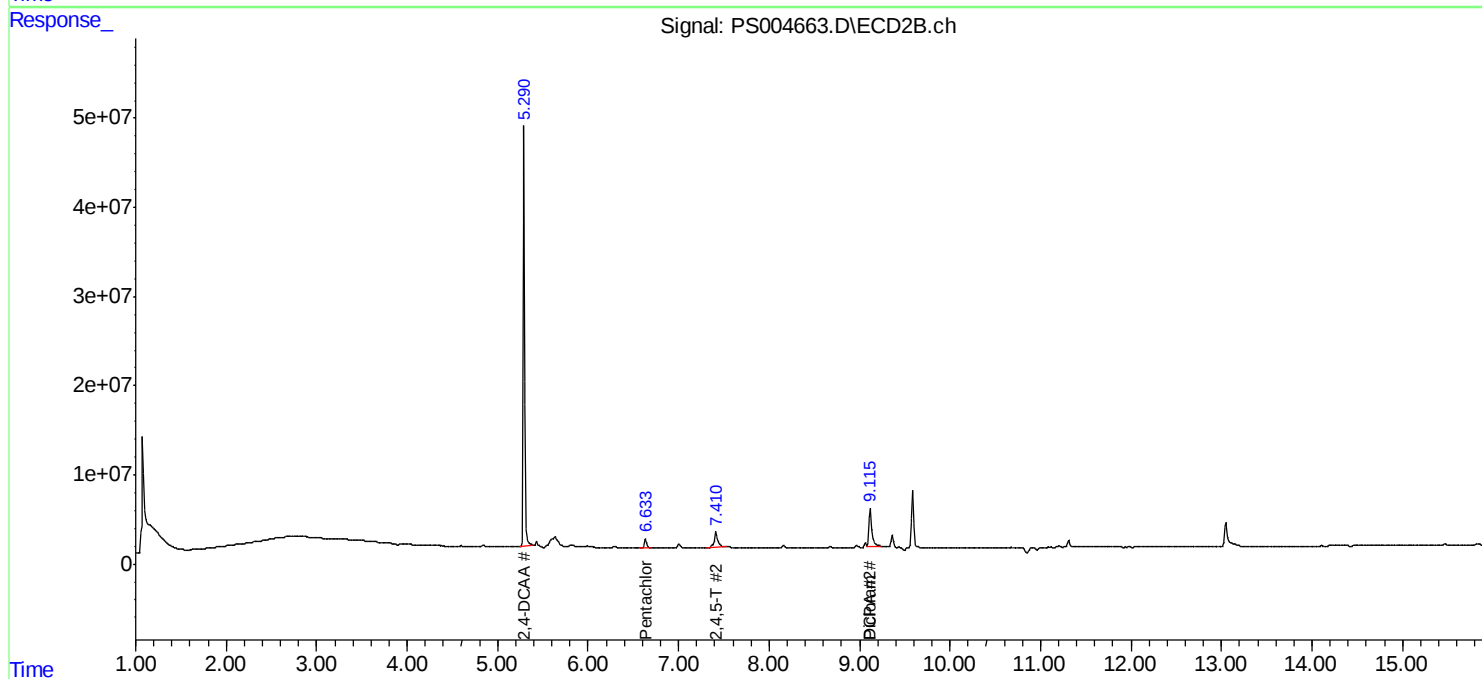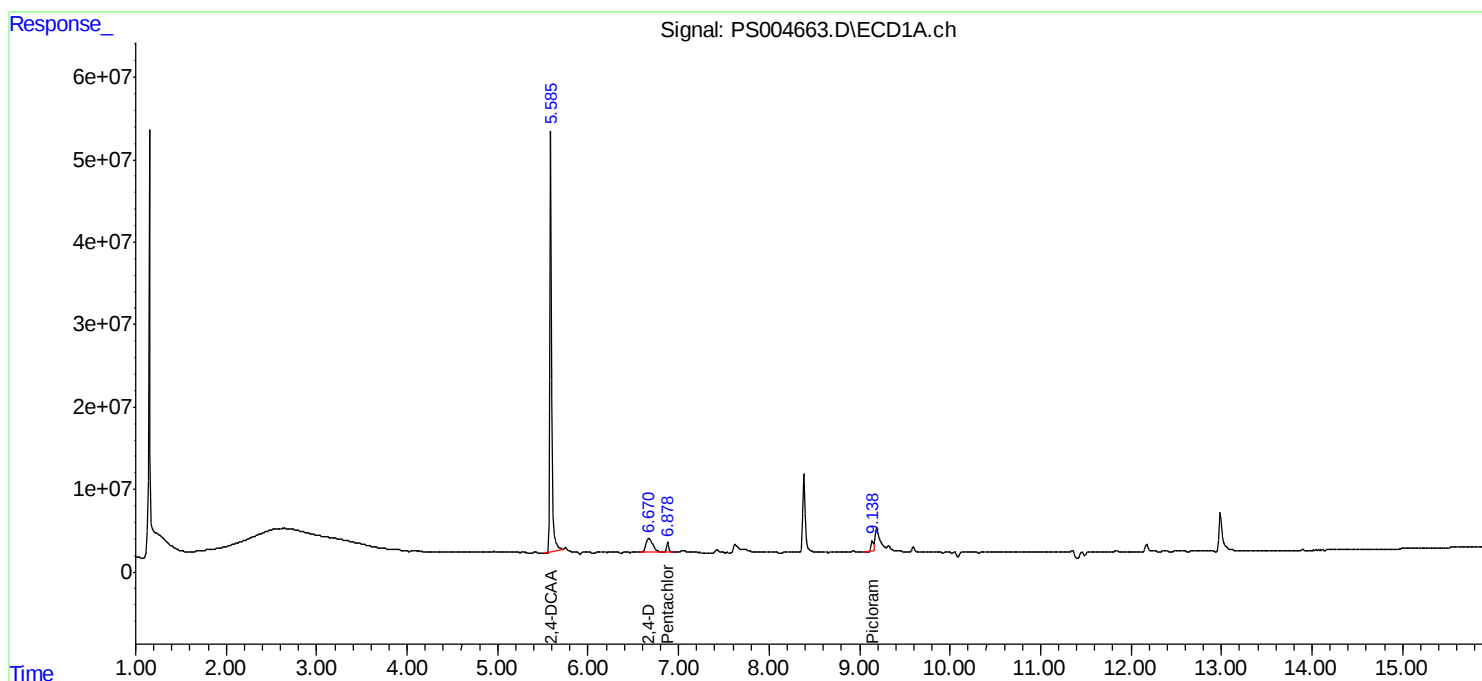


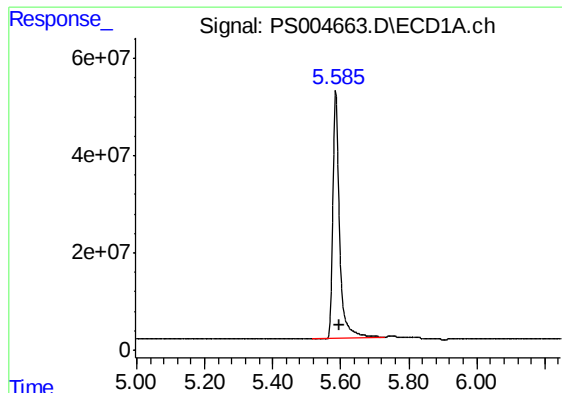

#4 2,4-DCAA


R.T.: 5.585 min
Delta R.T.: -0.010 min
Response: 690856332
Conc: 492.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

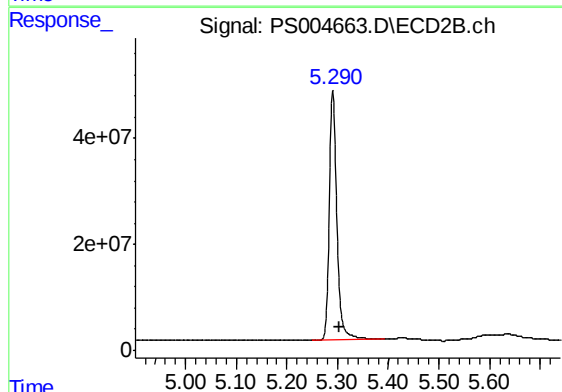


#4 2,4-DCAA

R.T.: 5.291 min
Delta R.T.: -0.013 min
Response: 499163043
Conc: 517.36 ng/ml

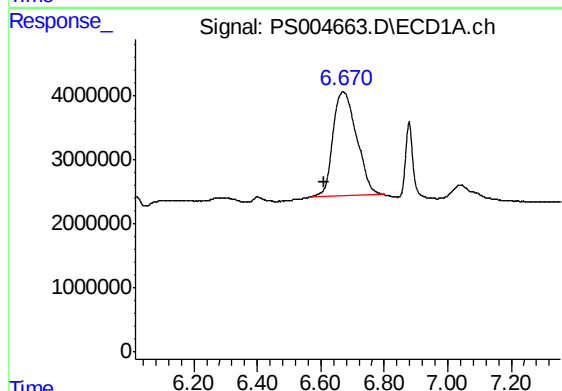


#9 2,4-D

R.T.: 6.670 min
Delta R.T.: 0.058 min
Response: 83903756
Conc: 61.34 ng/ml

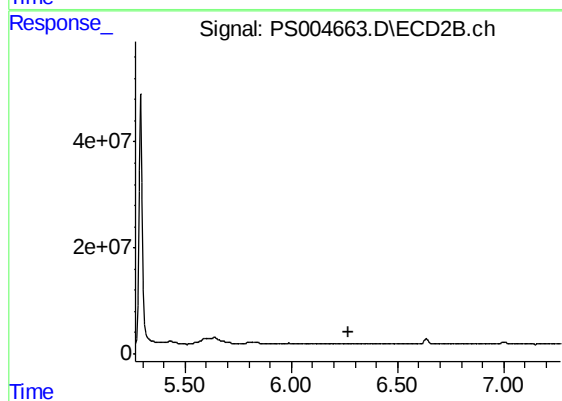

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.266 min
Response: 0
Conc: N.D.

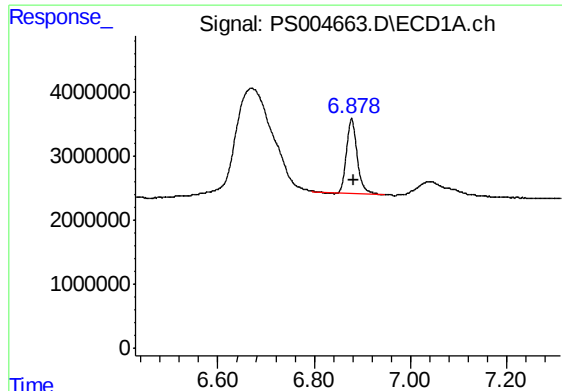

#10 Pentachlorophenol


R.T.: 6.878 min
Delta R.T.: -0.004 min
Response: 17748109
Conc: 1.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

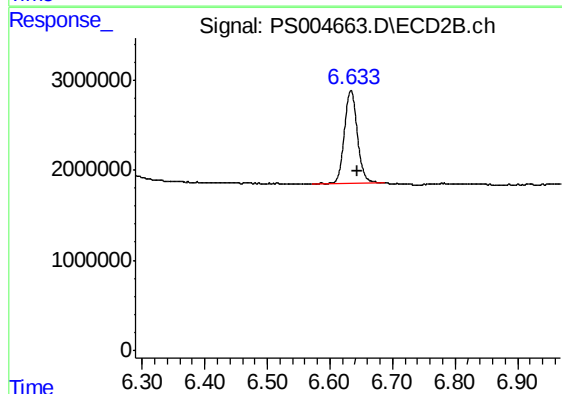


#10 Pentachlorophenol

R.T.: 6.634 min
Delta R.T.: -0.010 min
Response: 14885792
Conc: 1.21 ng/ml

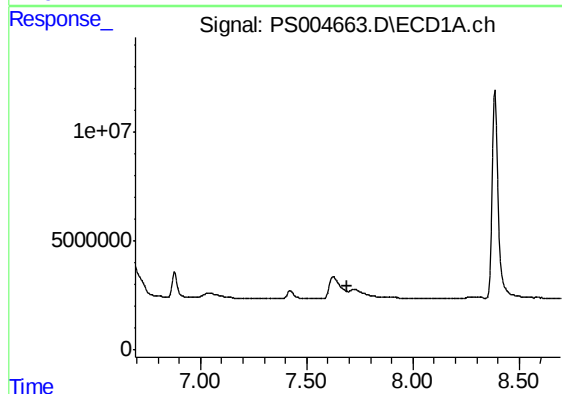


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.693 min
Response: 0
Conc: N.D.

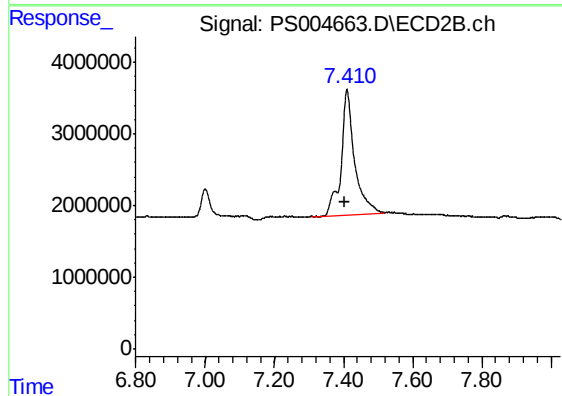

#12 2,4,5-T


R.T.: 7.410 min
Delta R.T.: 0.006 min
Response: 46752634
Conc: 10.49 ng/ml

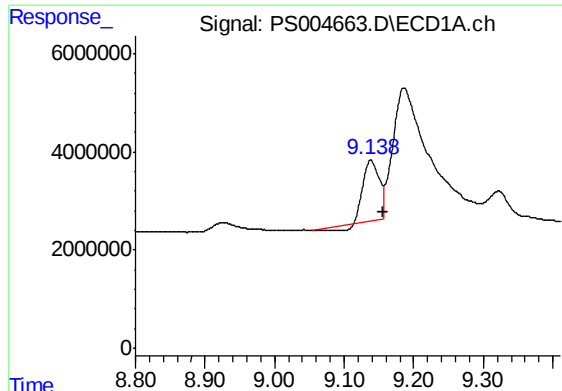

#15 Picloram


R.T.: 9.138 min
Delta R.T.: -0.017 min
Response: 18079510
Conc: 1.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

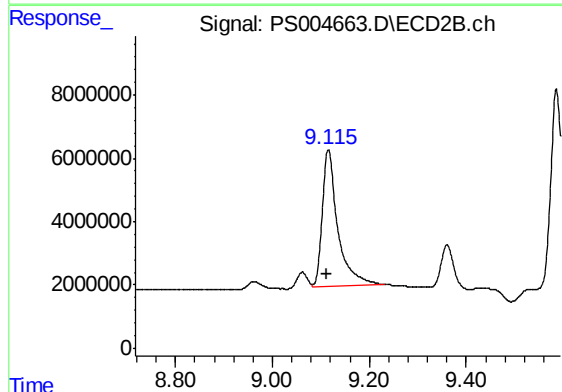


#15 Picloram

R.T.: 9.115 min
Delta R.T.: 0.003 min
Response: 95699283
Conc: 12.83 ng/ml

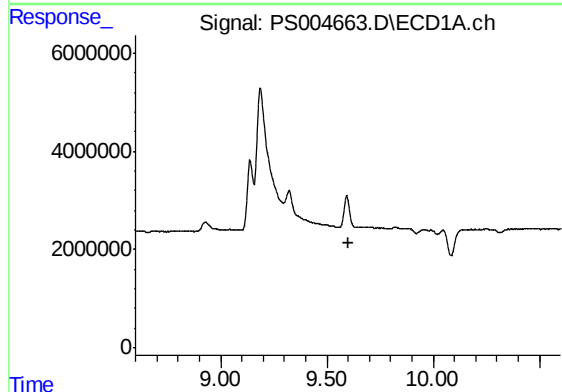

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.599 min
Response: 0
Conc: N.D.

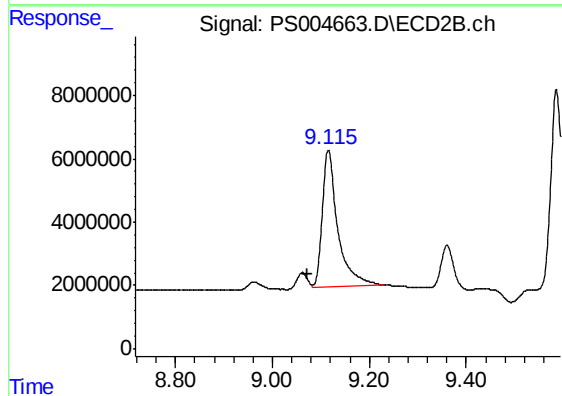

#16 DCPA

R.T.: 9.115 min
Delta R.T.: 0.043 min
Response: 95699283
Conc: 14.77 ng/ml