

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
 Data File : PS004696.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 22:41
 Operator : EI\SJ
 Sample : K2647-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-01-051719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 02:06:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.595	5.305	552.4E6	354.7E6	394.108	367.657
Target Compounds							
1) T	Dalapon	2.098	0.000	35920418	0	21.669	N.D. #
2) T	3,5-DICHL...	0.000	4.623	0	299.3E6	N.D.	242.925
3) T	4-Nitroph...	5.386	4.969	36977338	23712764	59.305	50.035
5) T	DICAMBA	5.694	5.411	39139440	17213309	7.371	4.660 #
6) T	MCP	5.951	0.000	14893507	0	3.578	N.D. #
8) T	DICHLORPROP	0.000	5.995	0	21563214	N.D.	22.871
11) T	2,4,5-TP ...	0.000	6.961	0	184.0E6	N.D.	35.759
16) T	DCPA	9.577	0.000	30745963	0	3.452	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
Data File : PS004696.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 22:41
Operator : EI\SJ
Sample : K2647-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 02:06:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

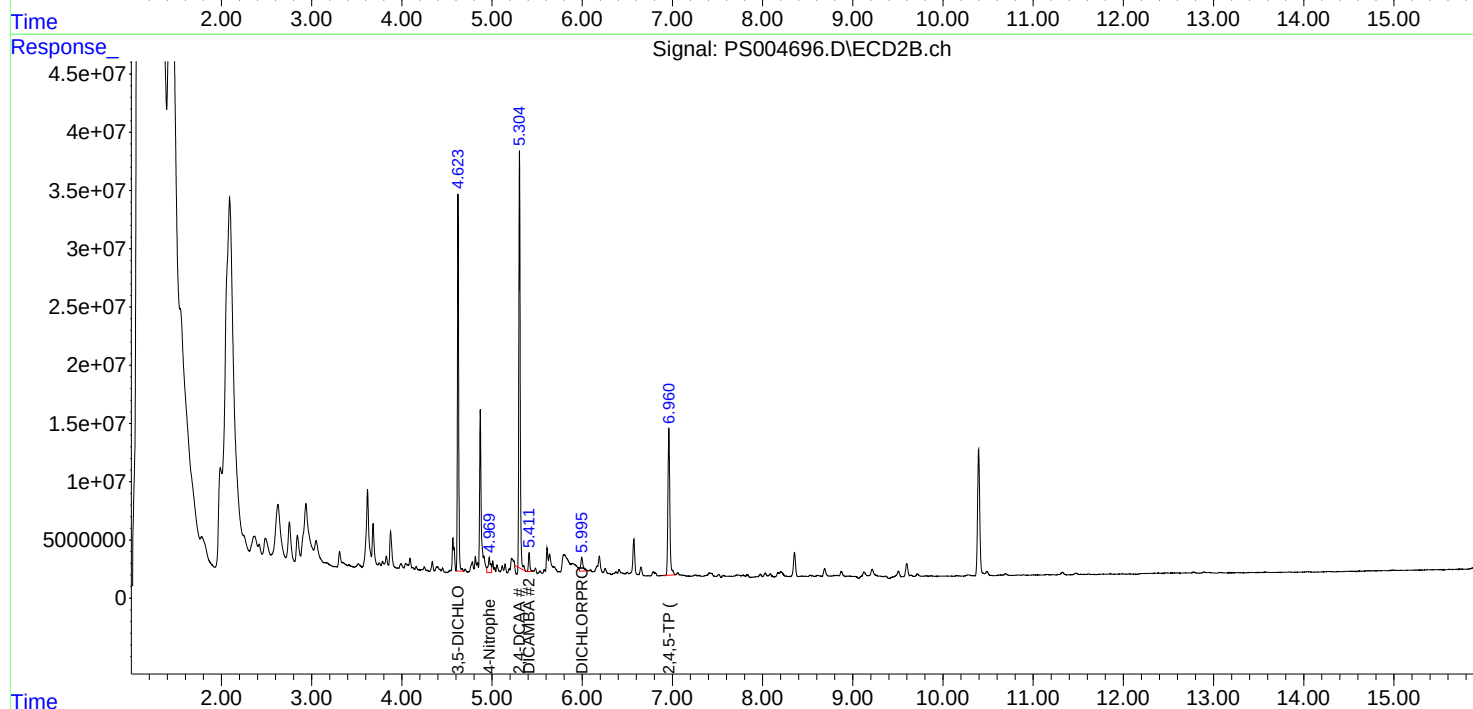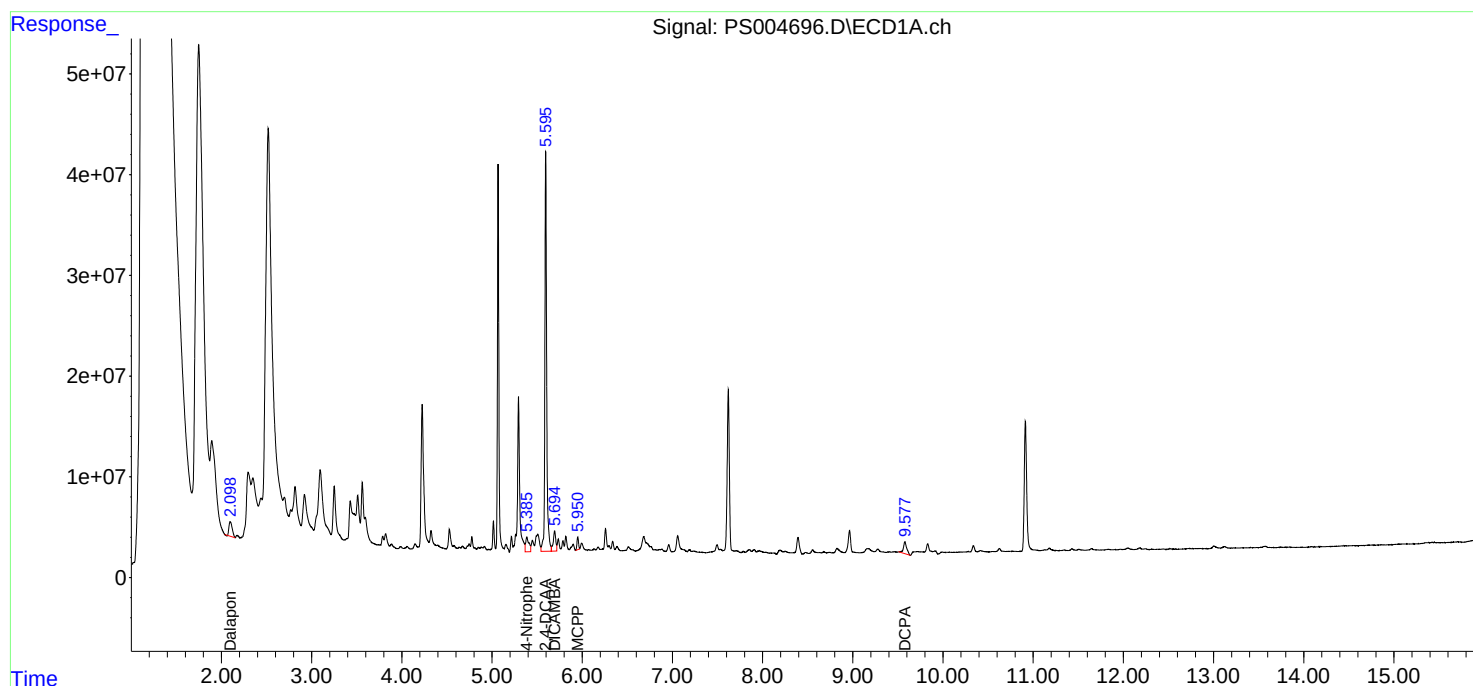


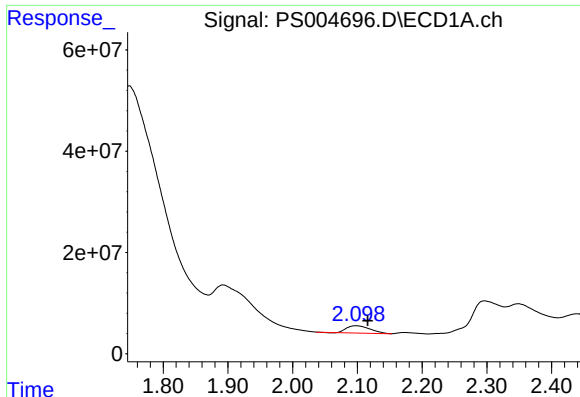

#1 Dalapon


R.T.: 2.098 min
Delta R.T.: -0.018 min
Response: 35920418
Conc: 21.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

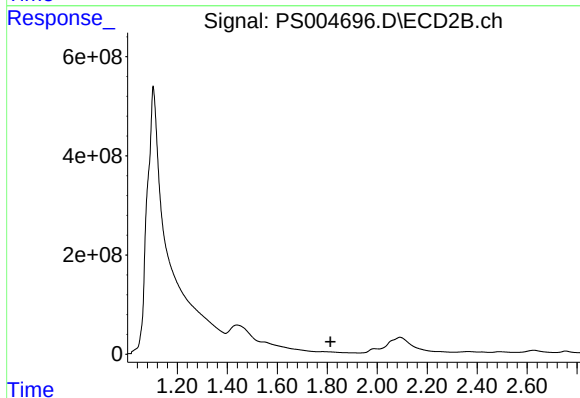


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

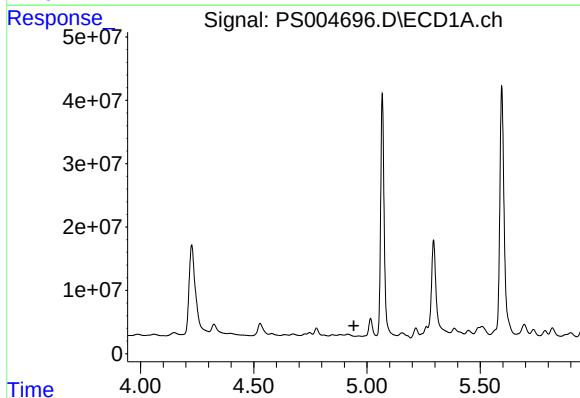


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

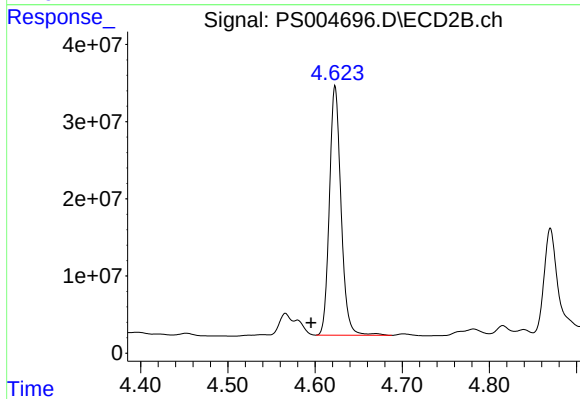

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.623 min
Delta R.T.: 0.028 min
Response: 299315280
Conc: 242.93 ng/ml

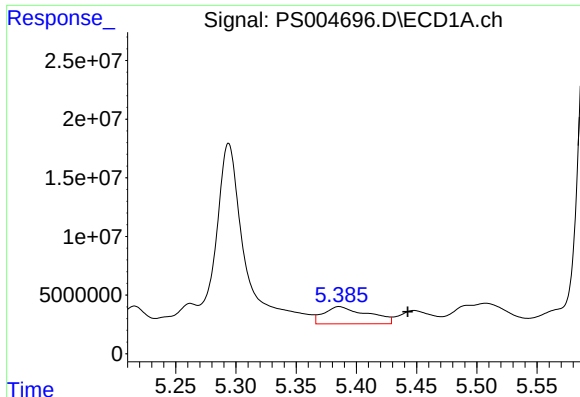

#3 4-Nitrophenol


R.T.: 5.386 min
Delta R.T.: -0.057 min
Response: 36977338
Conc: 59.31 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

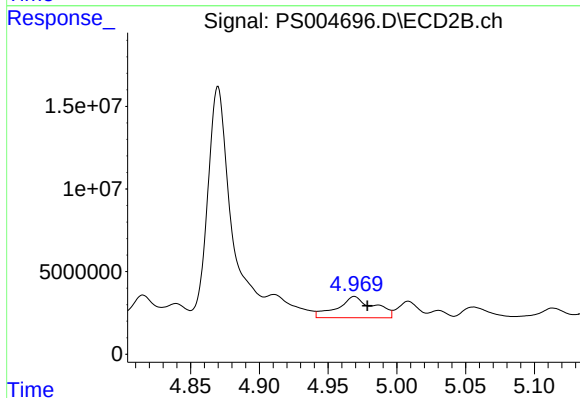


#3 4-Nitrophenol

R.T.: 4.969 min
Delta R.T.: -0.009 min
Response: 23712764
Conc: 50.04 ng/ml

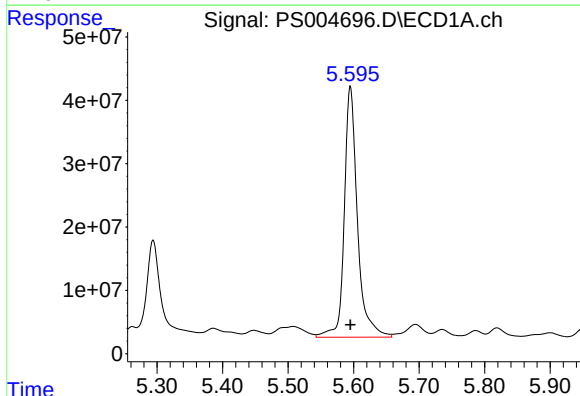


#4 2,4-DCAA

R.T.: 5.595 min
Delta R.T.: 0.000 min
Response: 552443071
Conc: 394.11 ng/ml

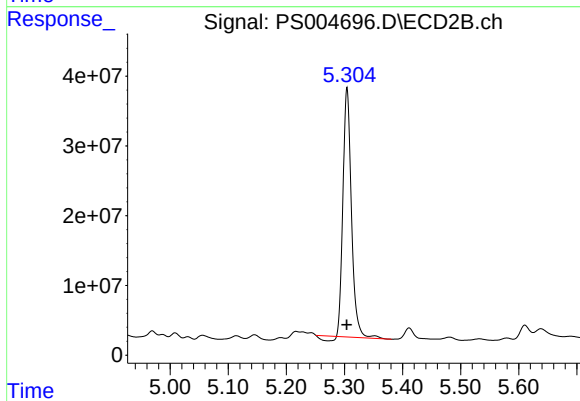

#4 2,4-DCAA


R.T.: 5.305 min
Delta R.T.: 0.000 min
Response: 354728545
Conc: 367.66 ng/ml

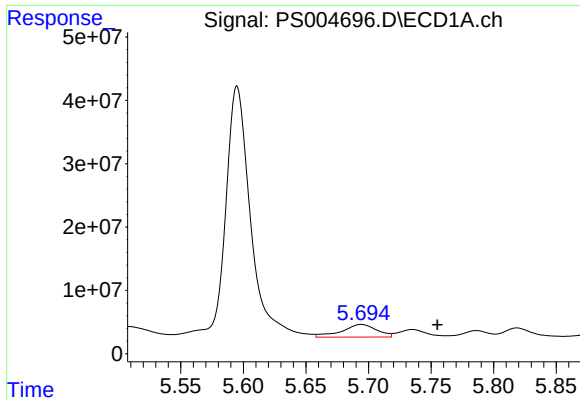

#5 DICAMBA


R.T.: 5.694 min
Delta R.T.: -0.061 min
Response: 39139440
Conc: 7.37 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

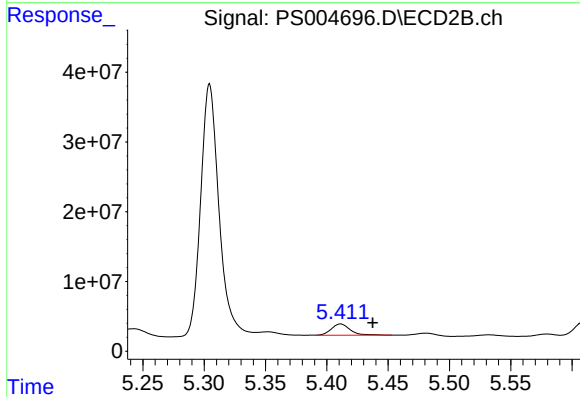


#5 DICAMBA

R.T.: 5.411 min
Delta R.T.: -0.026 min
Response: 17213309
Conc: 4.66 ng/ml

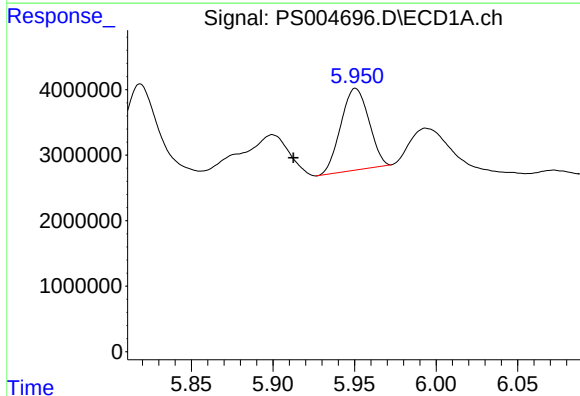


#6 MCP

R.T.: 5.951 min
Delta R.T.: 0.038 min
Response: 14893507
Conc: 3.58 ug/ml

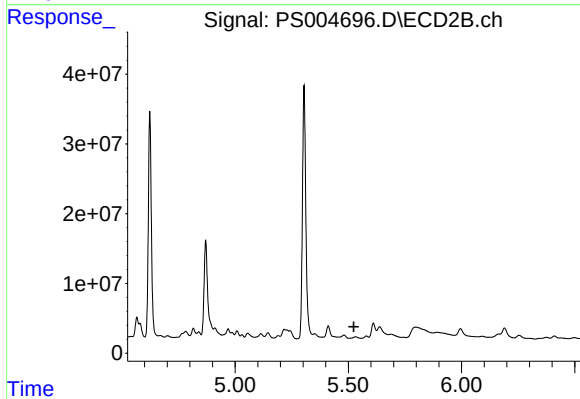

#6 MCP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

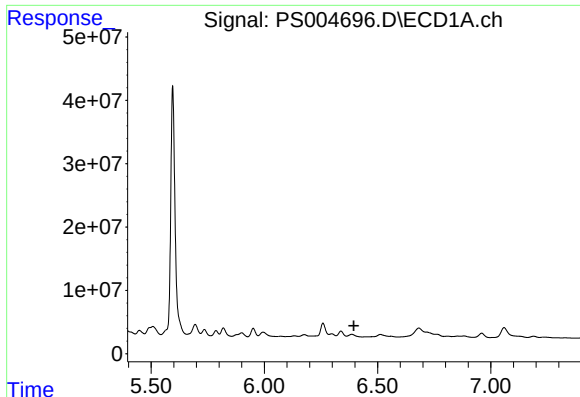

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

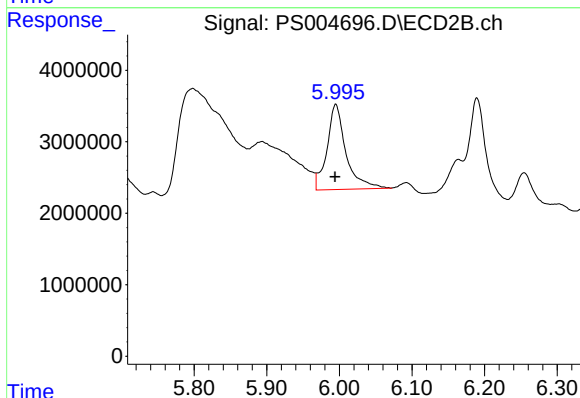


#8 DICHLORPROP

R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 21563214
Conc: 22.87 ng/ml

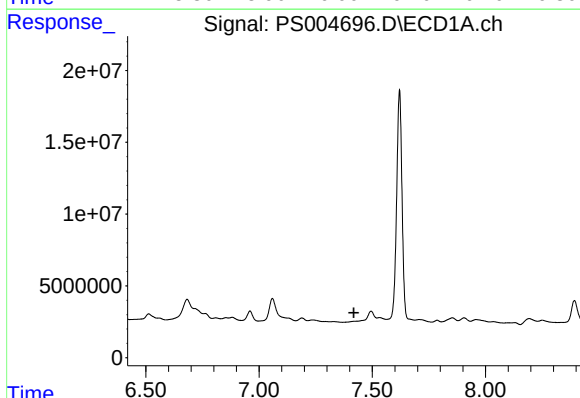


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.419 min
Response: 0
Conc: N.D.

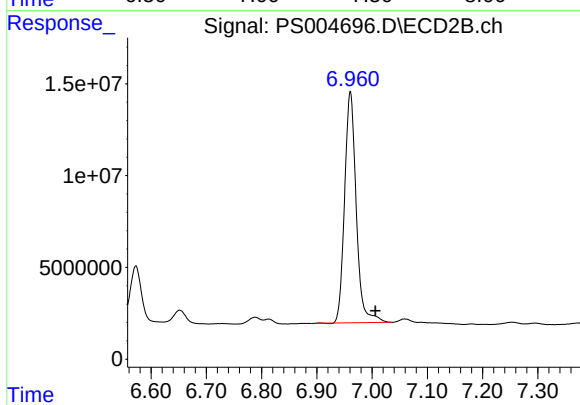

#11 2,4,5-TP (SILVEX)


R.T.: 6.961 min
Delta R.T.: -0.046 min
Response: 183994110
Conc: 35.76 ng/ml

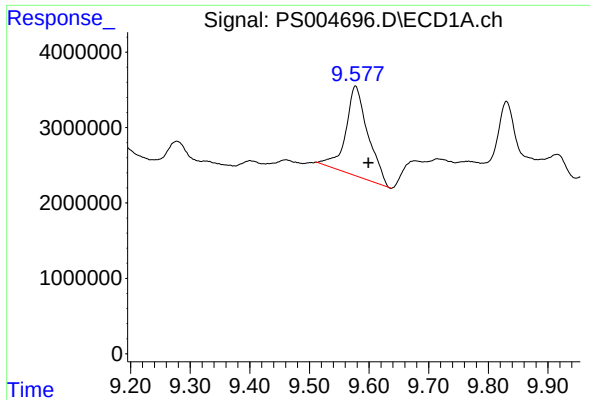

#16 DCPA

R.T.: 9.577 min
Delta R.T.: -0.022 min
Response: 30745963
Conc: 3.45 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-01-051719

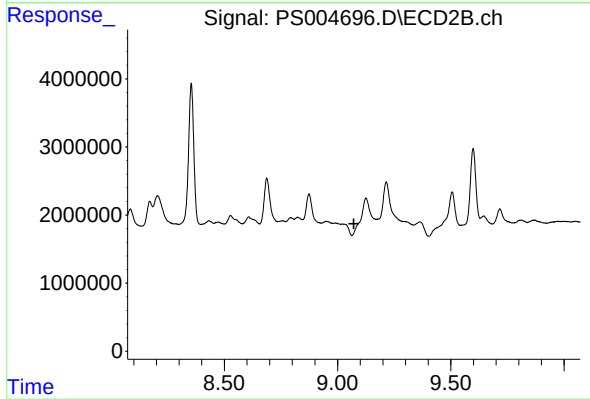

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.072 min
Response: 0
Conc: N.D.