

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
 Data File : PS004697.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2019 23:03
 Operator : EI\SJ
 Sample : K2913-04
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-17-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 02:06:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.575	5.284	600.4E6	400.2E6	428.299	414.830
Target Compounds							
1) T	Dalapon	2.079	0.000	38656277	0	23.319	N.D. #
2) T	3,5-DICHL...	4.995	4.603	41430883	260.7E6	24.024	211.624 #
3) T	4-Nitroph...	5.471	4.949	41532456	25022605	66.611	52.799
5) T	DICAMBA	5.721	5.432	60650230	46910929	11.423	12.698
6) T	MCPD	5.930	5.591	14600350	22367433	3.507	8.163 #
7) T	MCPA	0.000	5.762	0	114.4E6	N.D.	27.948
8) T	DICHLORPROP	0.000	5.974	0	18231508	N.D.	19.337
9) T	2,4-D	6.660	0.000	58828216	0	43.006	N.D. #
11) T	2,4,5-TP ...	7.386	6.940	52774245	194.8E6	7.204	37.860 #
16) T	DCPA	9.557	0.000	33408764	0	3.751	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
Data File : PS004697.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2019 23:03
Operator : EI\SJ
Sample : K2913-04
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleID :
TP-17-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 02:06:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

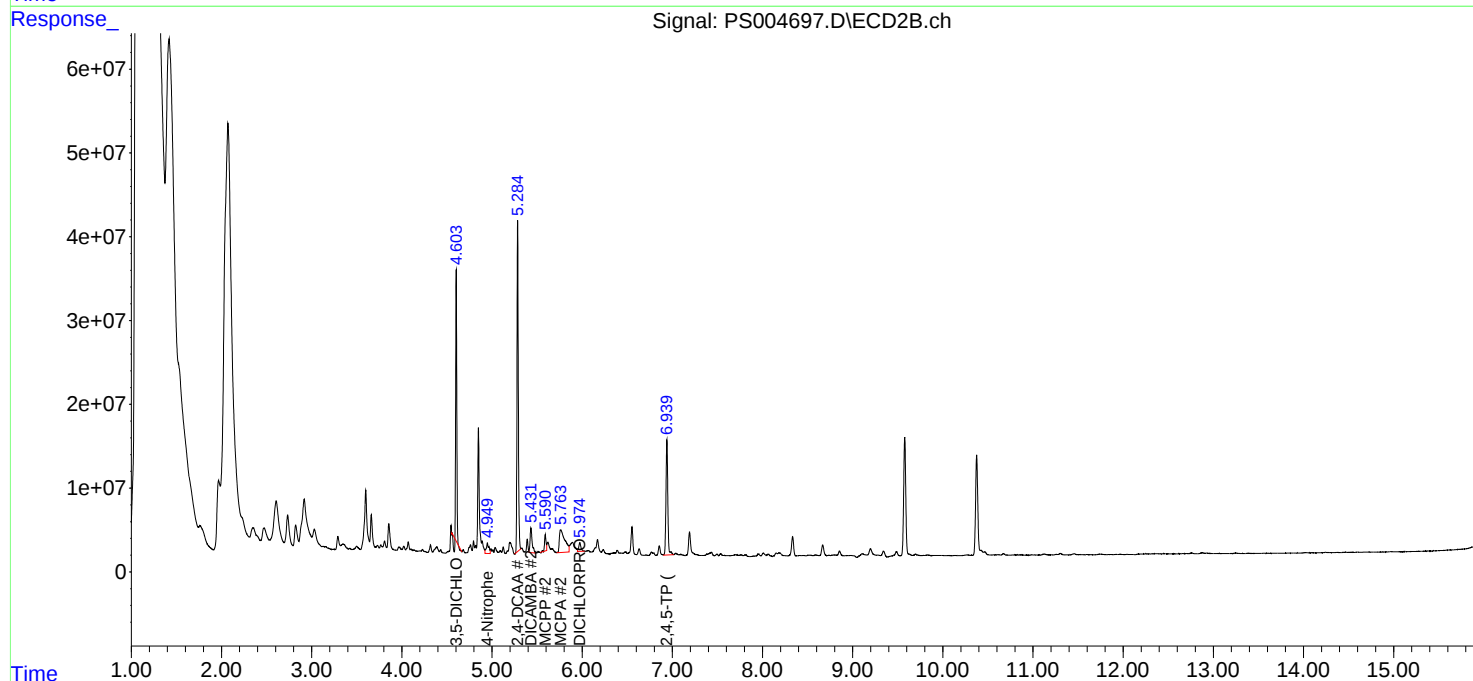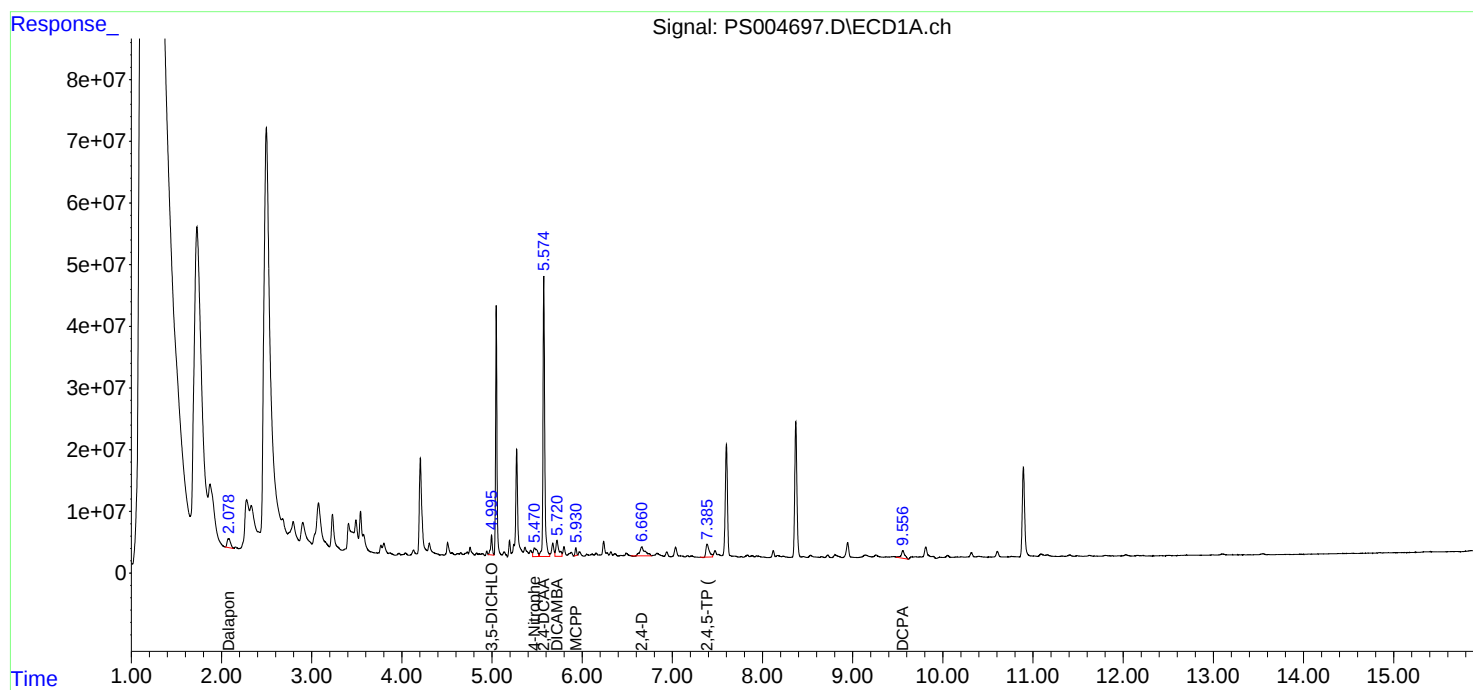


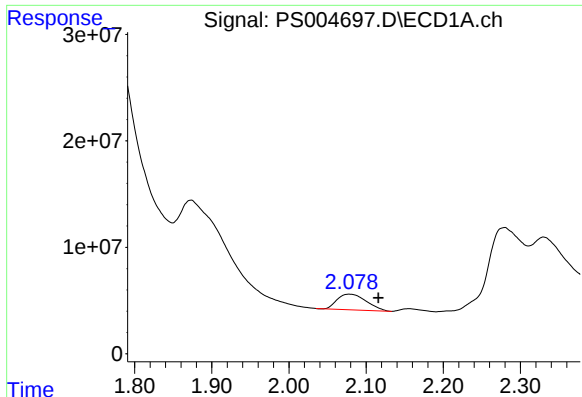

#1 Dalapon


R.T.: 2.079 min
Delta R.T.: -0.037 min
Response: 38656277
Conc: 23.32 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-17-S

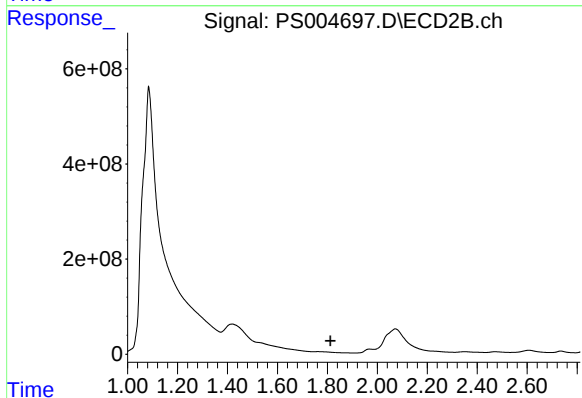


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

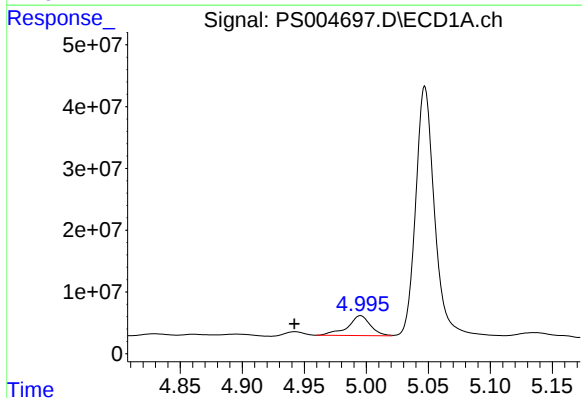


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.995 min
Delta R.T.: 0.053 min
Response: 41430883
Conc: 24.02 ng/ml

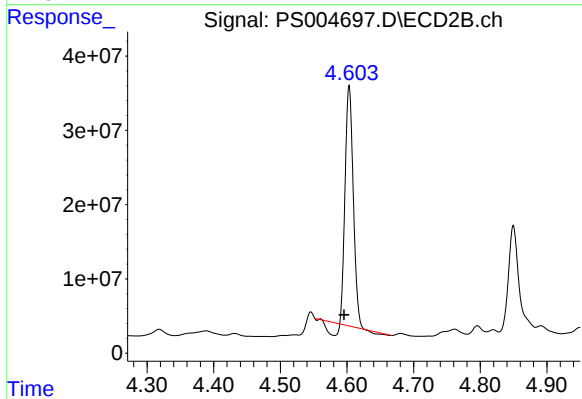

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.603 min
Delta R.T.: 0.008 min
Response: 260747301
Conc: 211.62 ng/ml

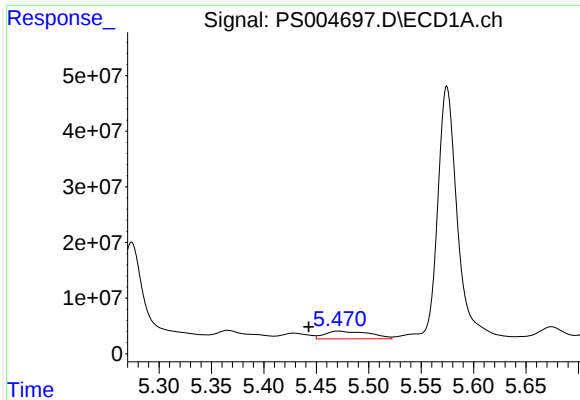

#3 4-Nitrophenol


R.T.: 5.471 min
Delta R.T.: 0.028 min
Response: 41532456
Conc: 66.61 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-17-S

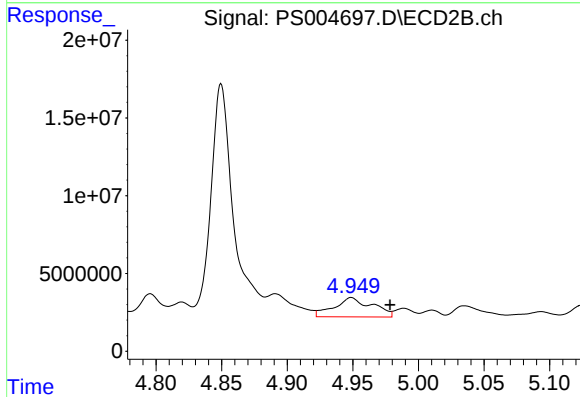


#3 4-Nitrophenol

R.T.: 4.949 min
Delta R.T.: -0.030 min
Response: 25022605
Conc: 52.80 ng/ml

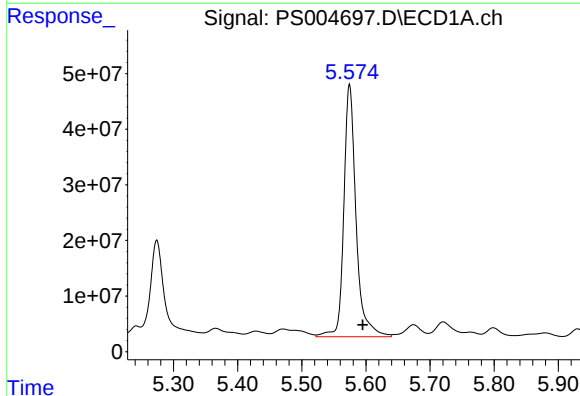


#4 2,4-DCAA

R.T.: 5.575 min
Delta R.T.: -0.020 min
Response: 600371010
Conc: 428.30 ng/ml

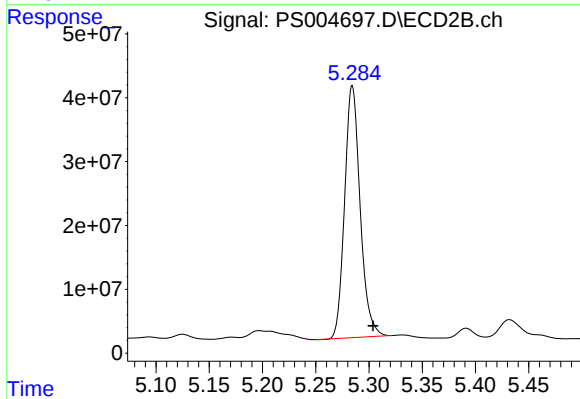

#4 2,4-DCAA


R.T.: 5.284 min
Delta R.T.: -0.019 min
Response: 400242978
Conc: 414.83 ng/ml

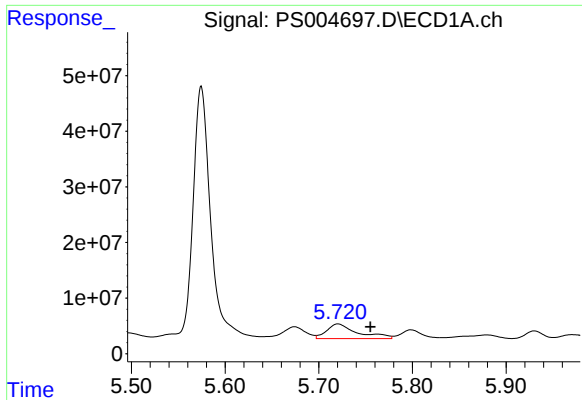

#5 DICAMBA


R.T.: 5.721 min
Delta R.T.: -0.034 min
Response: 60650230
Conc: 11.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-17-S

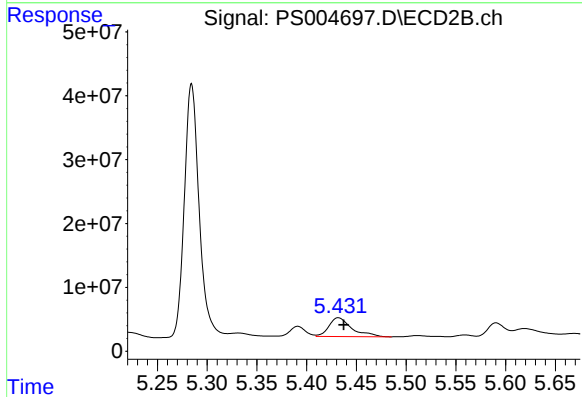


#5 DICAMBA

R.T.: 5.432 min
Delta R.T.: -0.005 min
Response: 46910929
Conc: 12.70 ng/ml

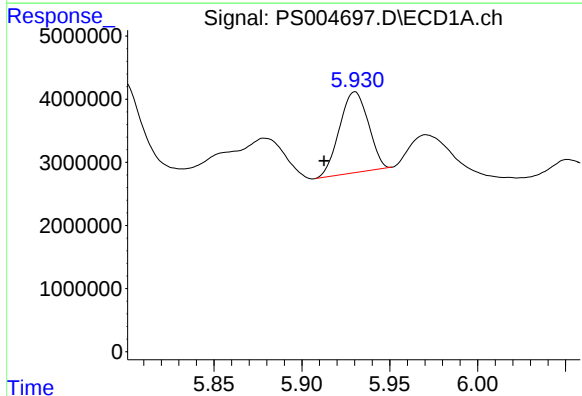


#6 MCP

R.T.: 5.930 min
Delta R.T.: 0.018 min
Response: 14600350
Conc: 3.51 ug/ml

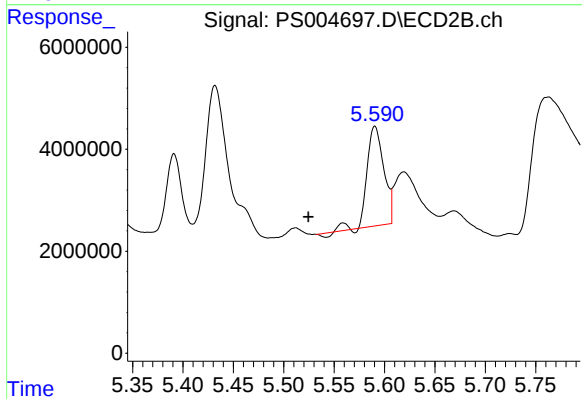

#6 MCP


R.T.: 5.591 min
Delta R.T.: 0.066 min
Response: 22367433
Conc: 8.16 ug/ml

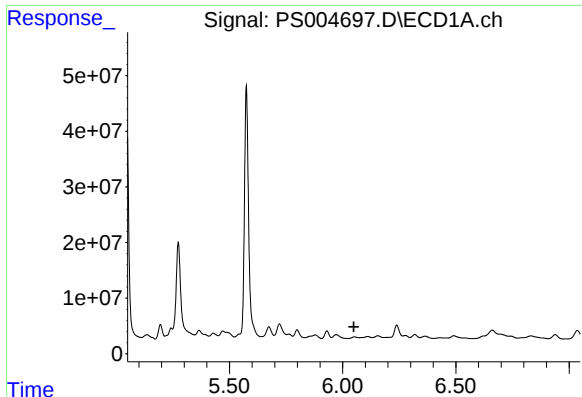

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-17-S

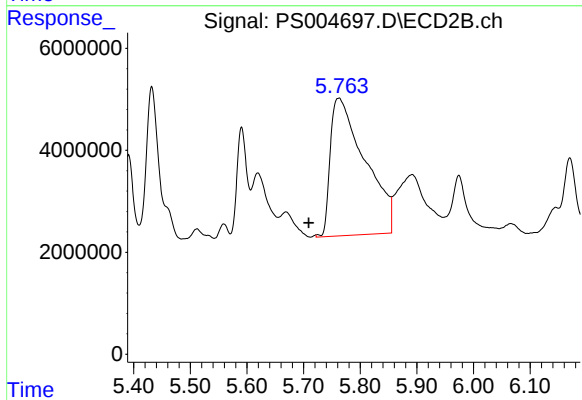


#7 MCPA

R.T.: 5.762 min
Delta R.T.: 0.053 min
Response: 114352171
Conc: 27.95 ug/ml

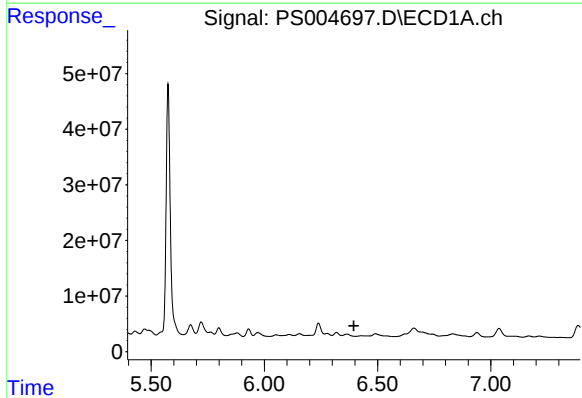


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

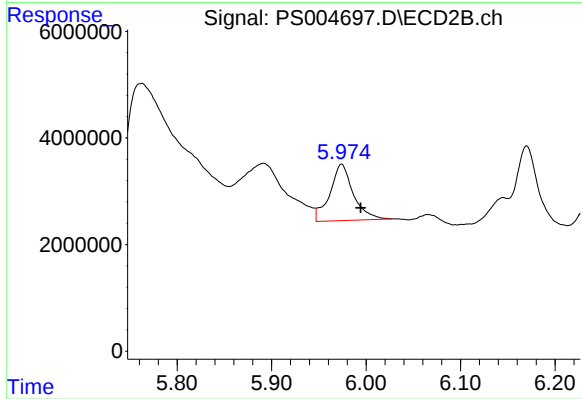

#8 DICHLORPROP


R.T.: 5.974 min
Delta R.T.: -0.020 min
Response: 18231508
Conc: 19.34 ng/ml

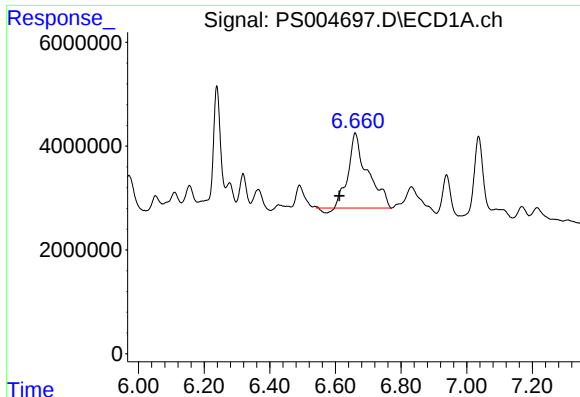

#9 2,4-D


R.T.: 6.660 min
Delta R.T.: 0.049 min
Response: 58828216
Conc: 43.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-17-S

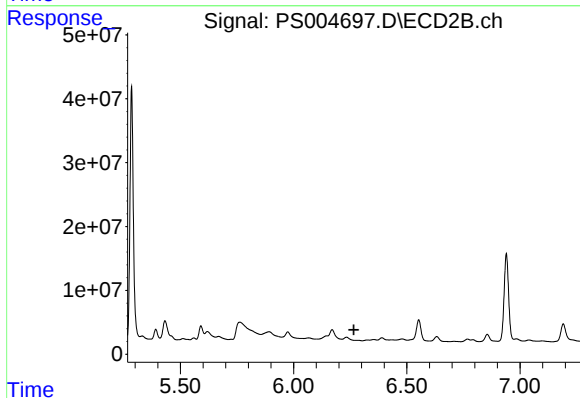


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

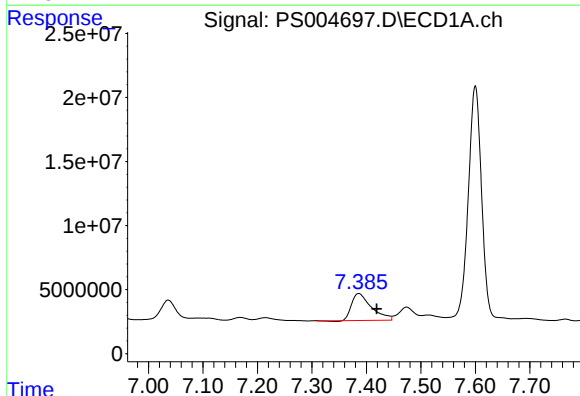


#11 2,4,5-TP (SILVEX)

R.T.: 7.386 min
Delta R.T.: -0.033 min
Response: 52774245
Conc: 7.20 ng/ml

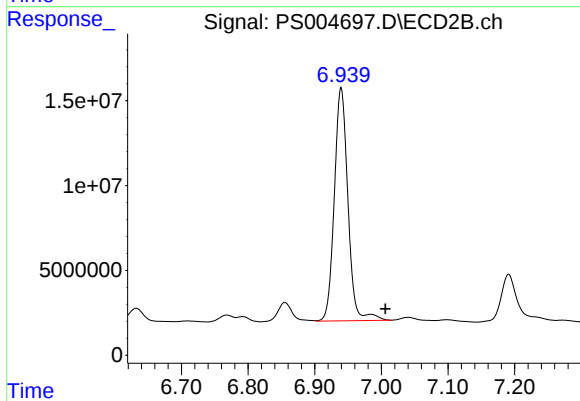

#11 2,4,5-TP (SILVEX)


R.T.: 6.940 min
Delta R.T.: -0.067 min
Response: 194801029
Conc: 37.86 ng/ml

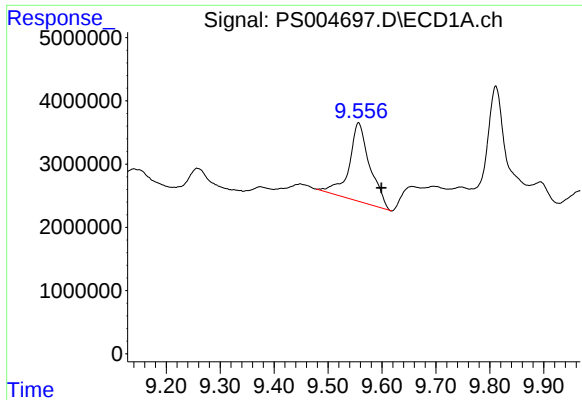

#16 DCPA

R.T.: 9.557 min
Delta R.T.: -0.042 min
Response: 33408764
Conc: 3.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-17-S

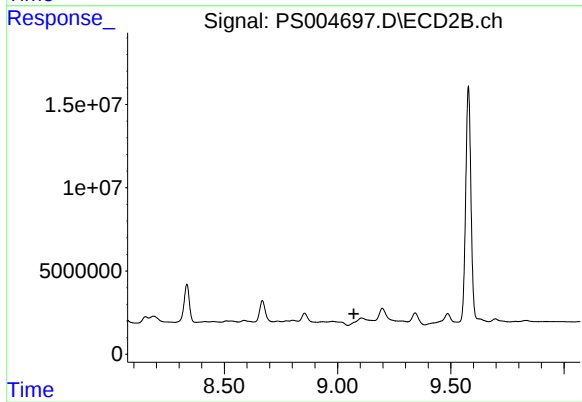

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.072 min
Response: 0
Conc: N.D.