

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
 Data File : PS004704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2019 01:37
 Operator : EI\SJ
 Sample : K2951-14
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-15-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 08:27:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
 Quant Title : 8080.M
 QLast Update : Tue May 21 04:53:35 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.594	5.303	556.3E6	366.7E6	396.838	380.018
Target Compounds							
1) T	Dalapon	2.096	0.000	43073322	0	25.984	N.D. #
2) T	3,5-DICHL...	0.000	4.623	0	284.4E6	N.D.	230.816
3) T	4-Nitroph...	5.491	4.969	34508546	25416294	55.346	53.630
5) T	DICAMBA	5.694	5.410	34931611	13748910	6.579	3.722 #
6) T	MCPD	5.950	0.000	13815371	0	3.319	N.D. #
7) T	MCPA	0.000	5.639	0	28777189	N.D.	7.033
8) T	DICHLORPROP	0.000	5.995	0	15617286	N.D.	16.564
9) T	2,4-D	6.681	0.000	57016125	0	41.681	N.D. #
11) T	2,4,5-TP ...	0.000	6.959	0	163.9E6	N.D.	31.849
16) T	DCPA	9.578	0.000	36244435	0	4.070	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052119\
Data File : PS004704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2019 01:37
Operator : EI\SJ
Sample : K2951-14
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-15-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 08:27:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052019.M
Quant Title : 8080.M
QLast Update : Tue May 21 04:53:35 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

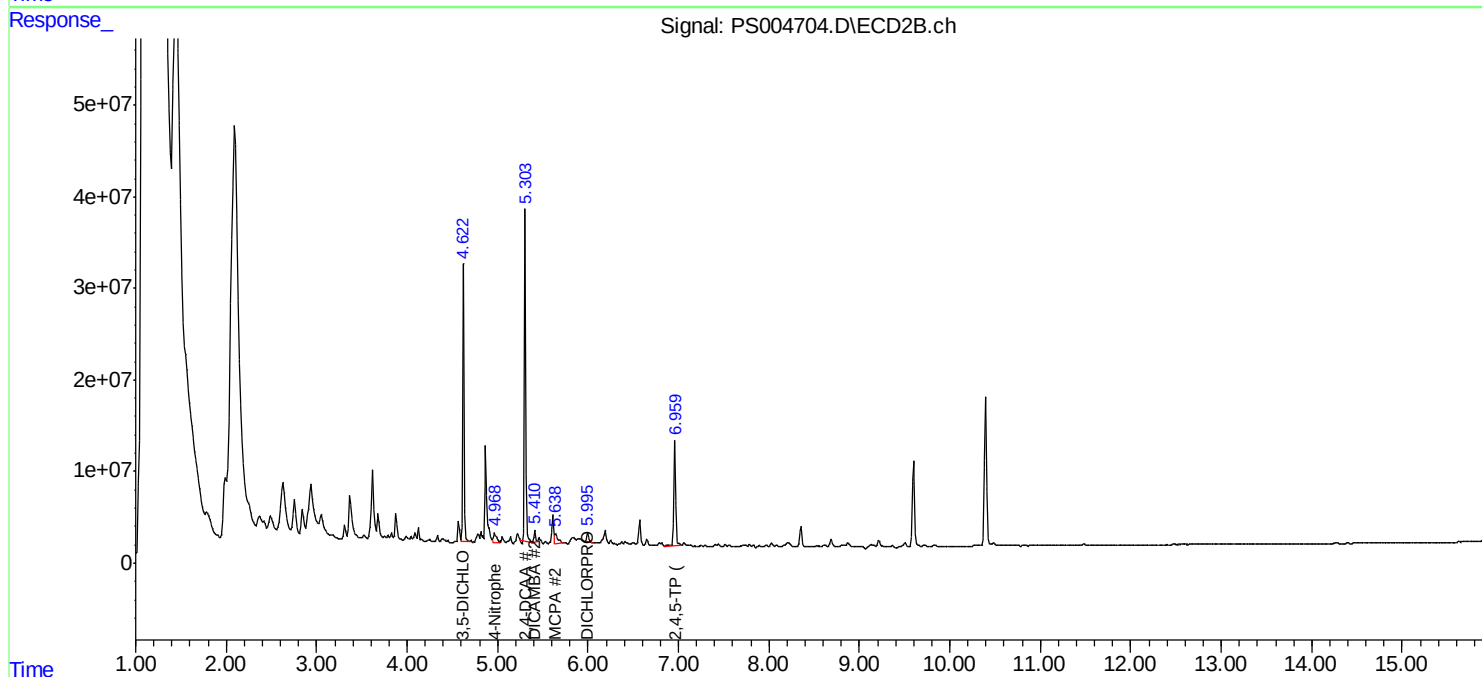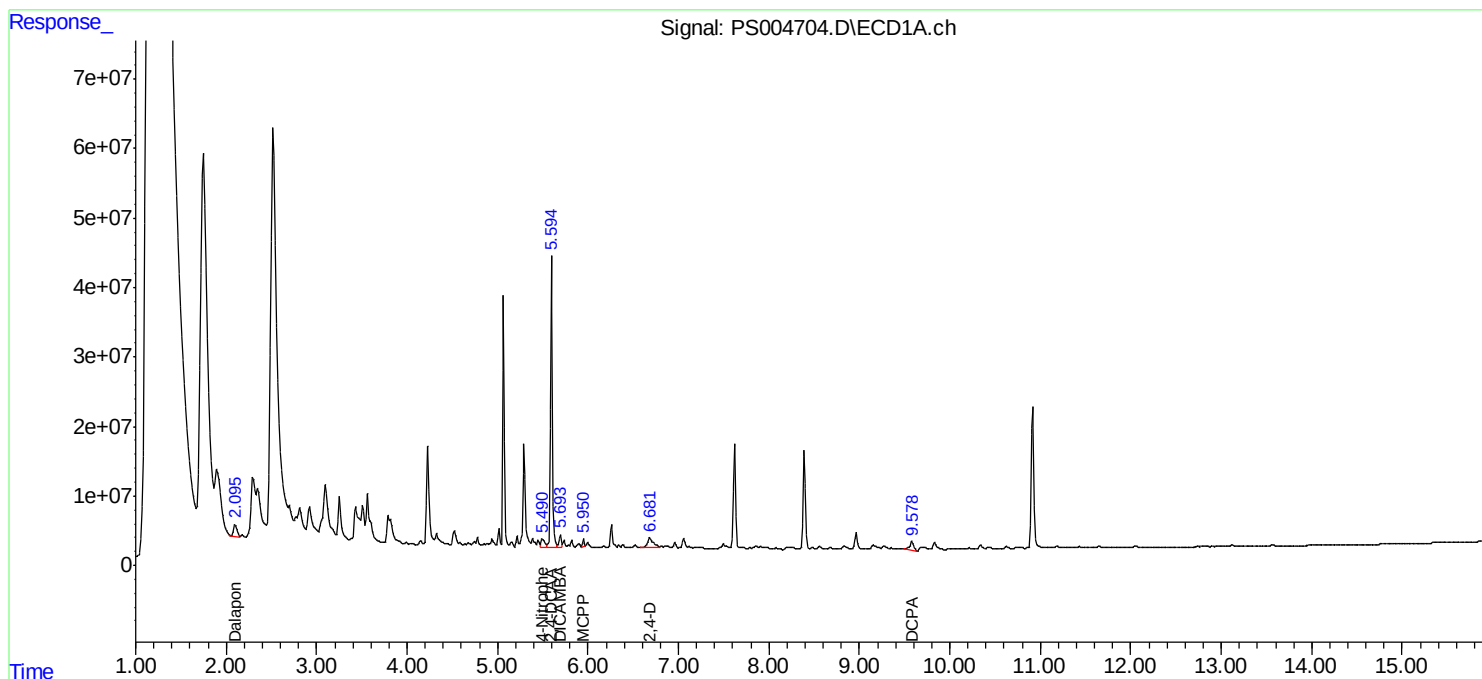


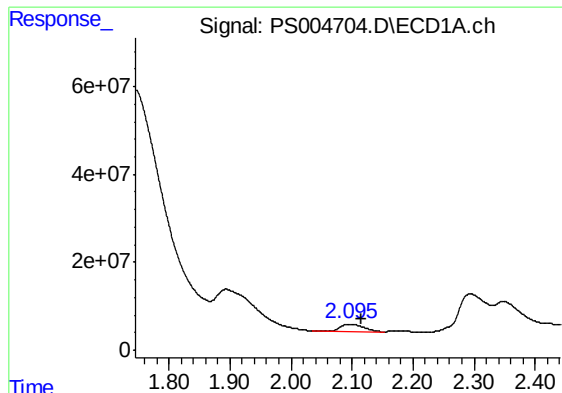

#1 Dalapon


R.T.: 2.096 min
Delta R.T.: -0.020 min
Response: 43073322
Conc: 25.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15-S

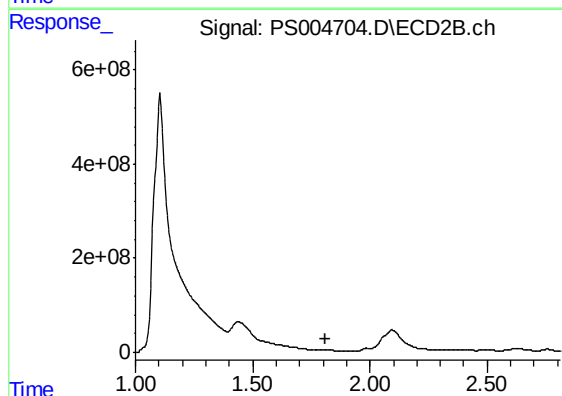


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.813 min
Response: 0
Conc: N.D.

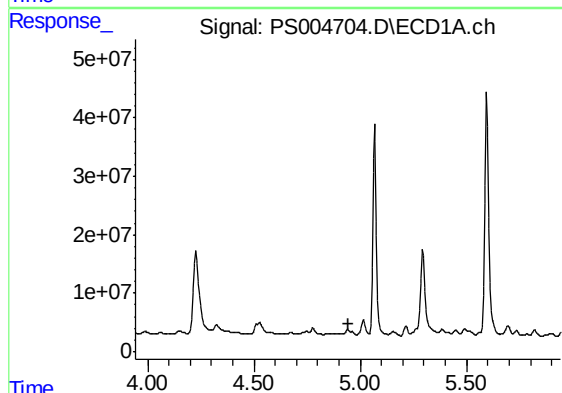


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

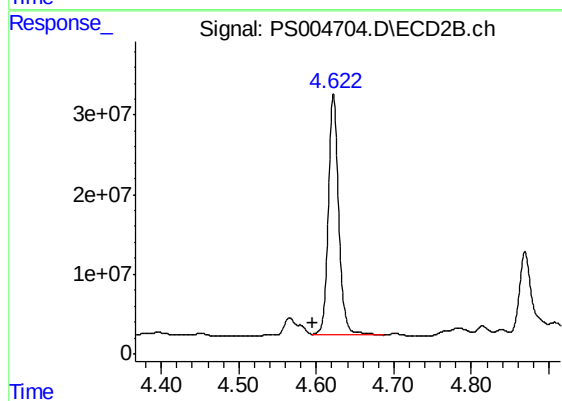

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.623 min
Delta R.T.: 0.027 min
Response: 284395178
Conc: 230.82 ng/ml

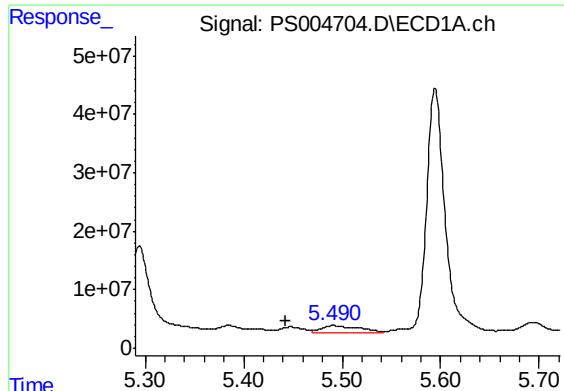

#3 4-Nitrophenol


R.T.: 5.491 min
Delta R.T.: 0.048 min
Response: 34508546
Conc: 55.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15-S

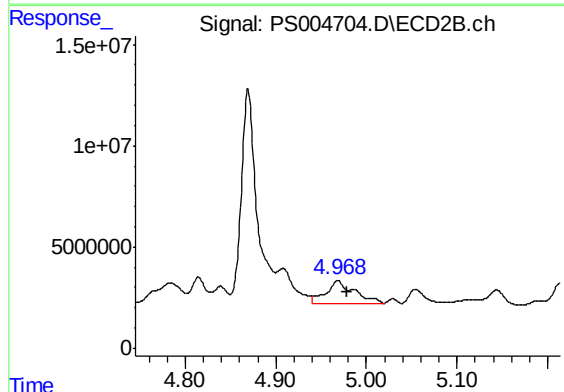


#3 4-Nitrophenol

R.T.: 4.969 min
Delta R.T.: -0.010 min
Response: 25416294
Conc: 53.63 ng/ml

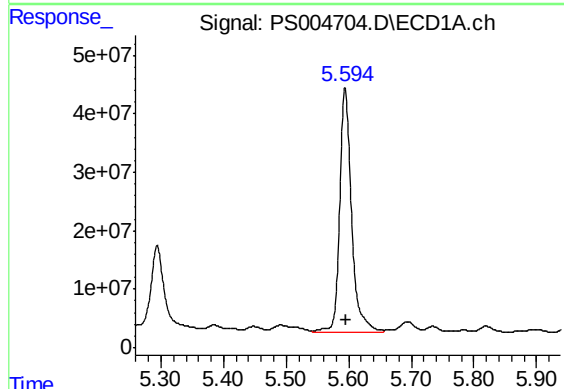


#4 2,4-DCAA

R.T.: 5.594 min
Delta R.T.: 0.000 min
Response: 556270674
Conc: 396.84 ng/ml

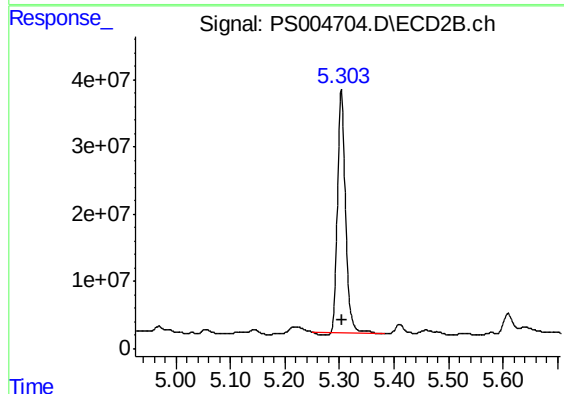

#4 2,4-DCAA


R.T.: 5.303 min
Delta R.T.: 0.000 min
Response: 366655281
Conc: 380.02 ng/ml

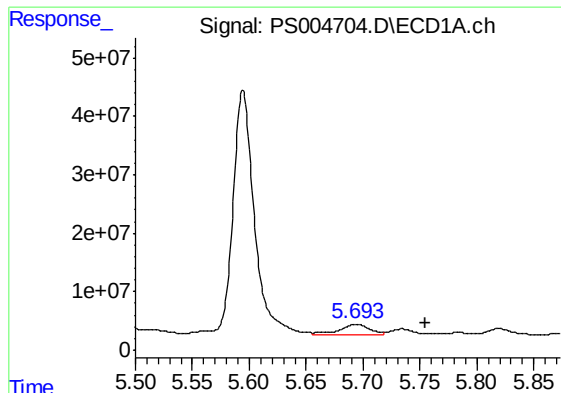

#5 DICAMBA


R.T.: 5.694 min
Delta R.T.: -0.061 min
Response: 34931611
Conc: 6.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15-S

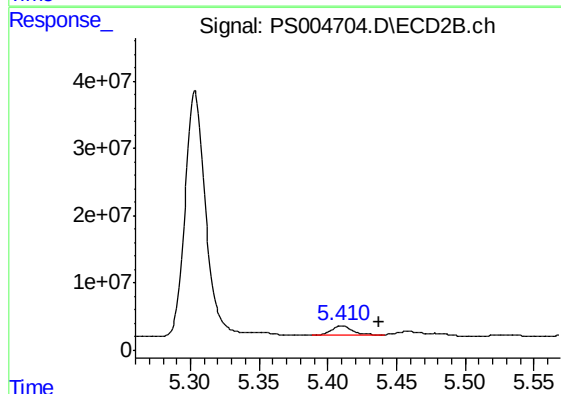


#5 DICAMBA

R.T.: 5.410 min
Delta R.T.: -0.027 min
Response: 13748910
Conc: 3.72 ng/ml

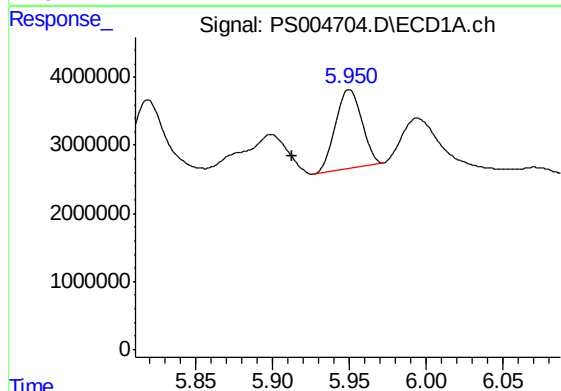


#6 MCPP

R.T.: 5.950 min
Delta R.T.: 0.038 min
Response: 13815371
Conc: 3.32 ug/ml

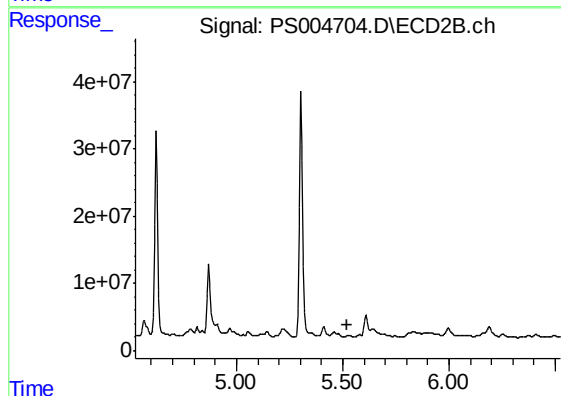

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.524 min
Response: 0
Conc: N.D.

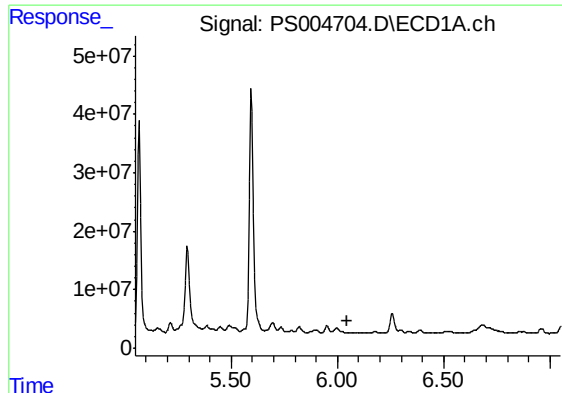

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-15-S

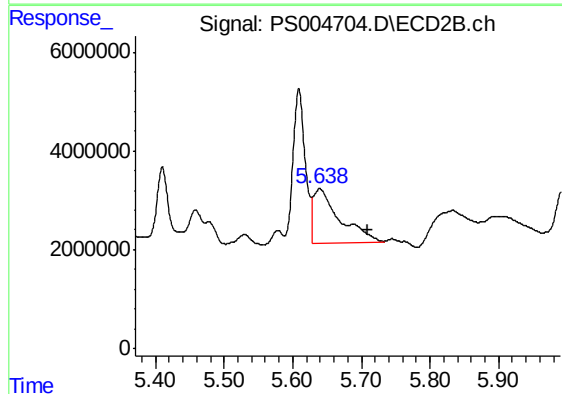


#7 MCPA

R.T.: 5.639 min
Delta R.T.: -0.070 min
Response: 28777189
Conc: 7.03 ug/ml

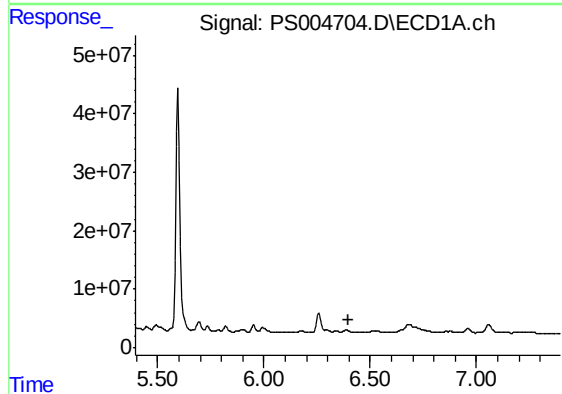


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

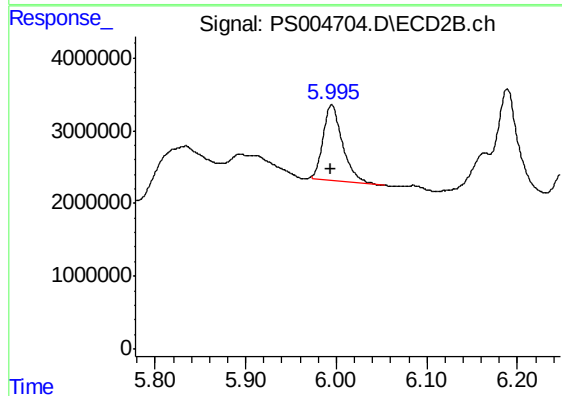

#8 DICHLORPROP


R.T.: 5.995 min
Delta R.T.: 0.000 min
Response: 15617286
Conc: 16.56 ng/ml

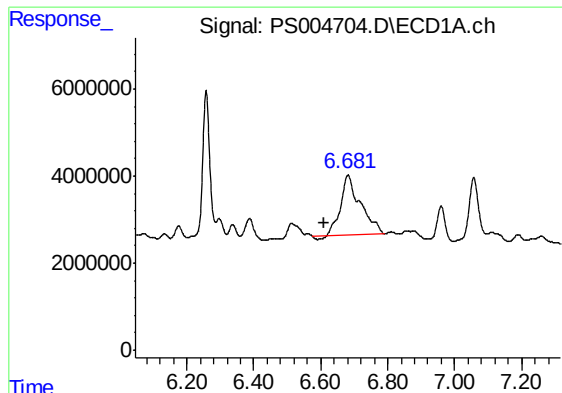

#9 2,4-D


R.T.: 6.681 min
Delta R.T.: 0.069 min
Response: 57016125
Conc: 41.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15-S

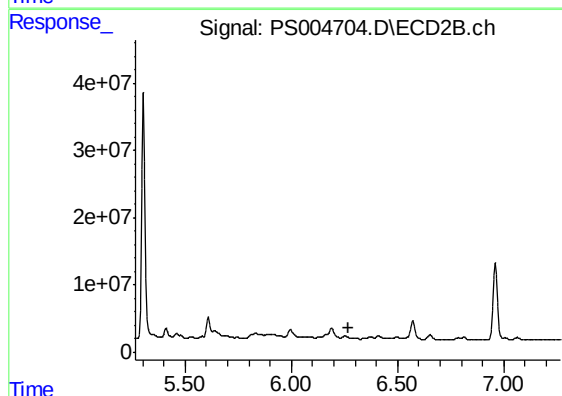


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.266 min
Response: 0
Conc: N.D.

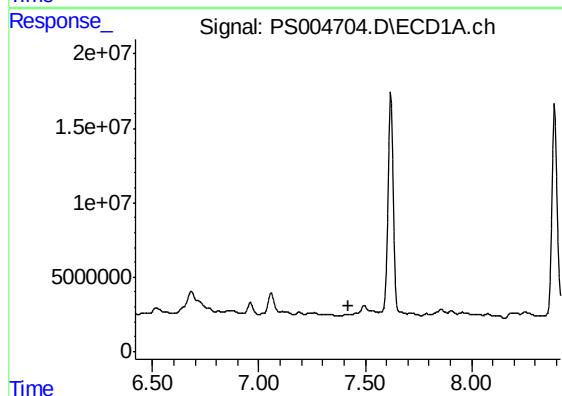


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.419 min
Response: 0
Conc: N.D.

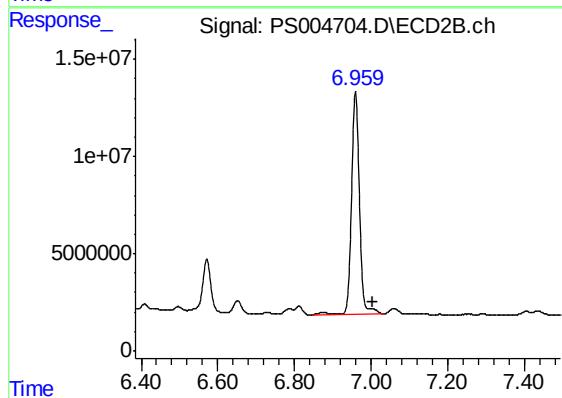

#11 2,4,5-TP (SILVEX)


R.T.: 6.959 min
Delta R.T.: -0.047 min
Response: 163872025
Conc: 31.85 ng/ml

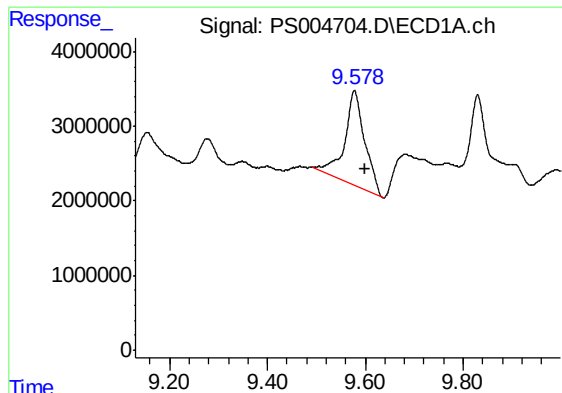

#16 DCPA

R.T.: 9.578 min
Delta R.T.: -0.021 min
Response: 36244435
Conc: 4.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-15-S

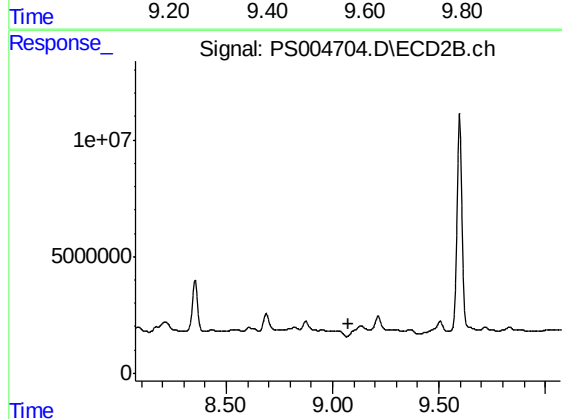

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.072 min
Response: 0
Conc: N.D.