

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052120\
 Data File : PS010378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 09:38
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 21 17:17:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.921	317.8E6	270.2E6	452.069	503.845
Target Compounds							
5) T	DICAMBA	0.000	7.090	0	2426229	N.D.	1.108
6) T	MCPD	0.000	7.210	0	288386	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.718	0	557935	N.D.	<MDL
9) T	2,4-D	0.000	8.017	0	832636	N.D.	1.201
10) T	Pentachlo...	0.000	8.441	0	342288	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	3204050	N.D.	1.106
12) T	2,4,5-T	0.000	9.185	0	3582673	N.D.	1.232
13) T	2,4-DB	0.000	9.696	0	878989	N.D.	2.205
14) T	DINOSEB	0.000	10.022	0	1368449	N.D.	<MDL
15) T	Picloram	11.033	11.010	11233660	16327618	2.450	3.867 #
16) T	DCPA	0.000	10.950	0	4432208	N.D.	1.240



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052120\
Data File : PS010378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 09:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 21 17:17:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

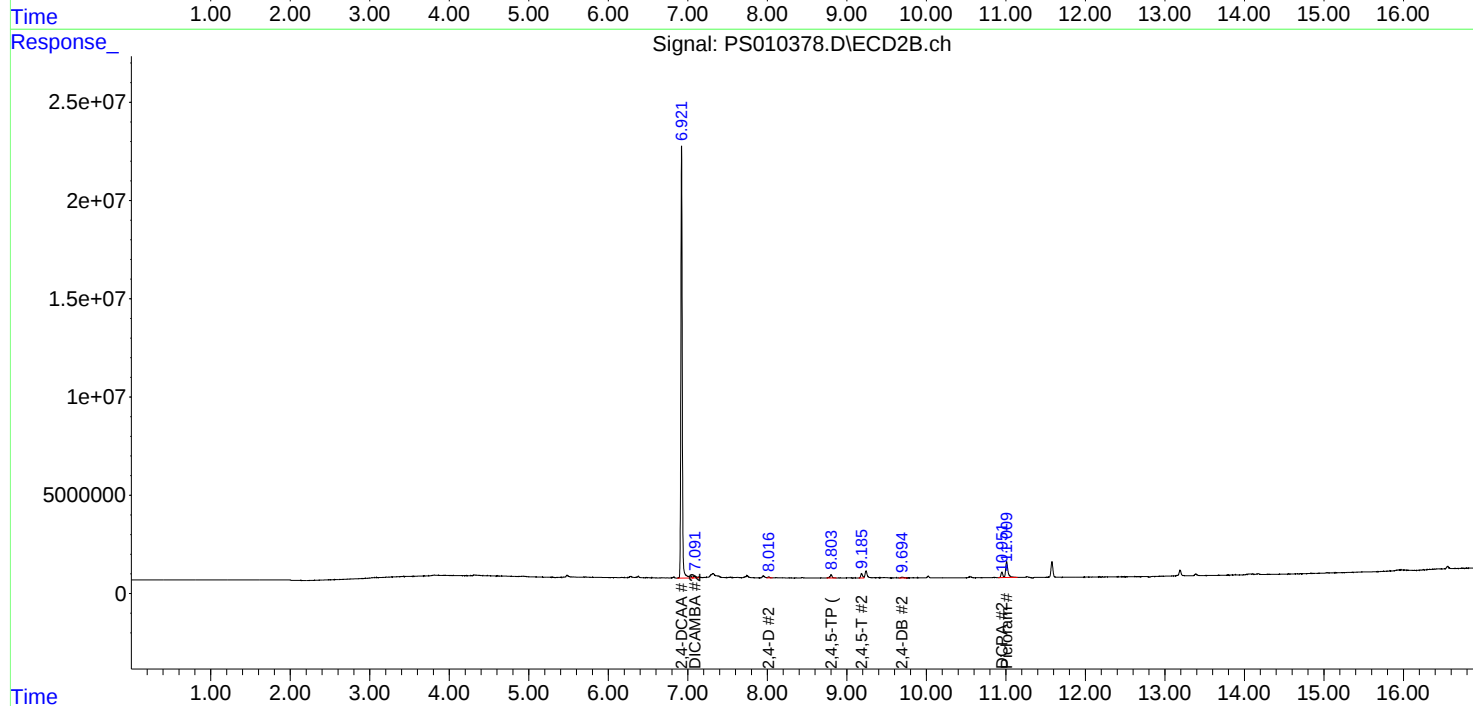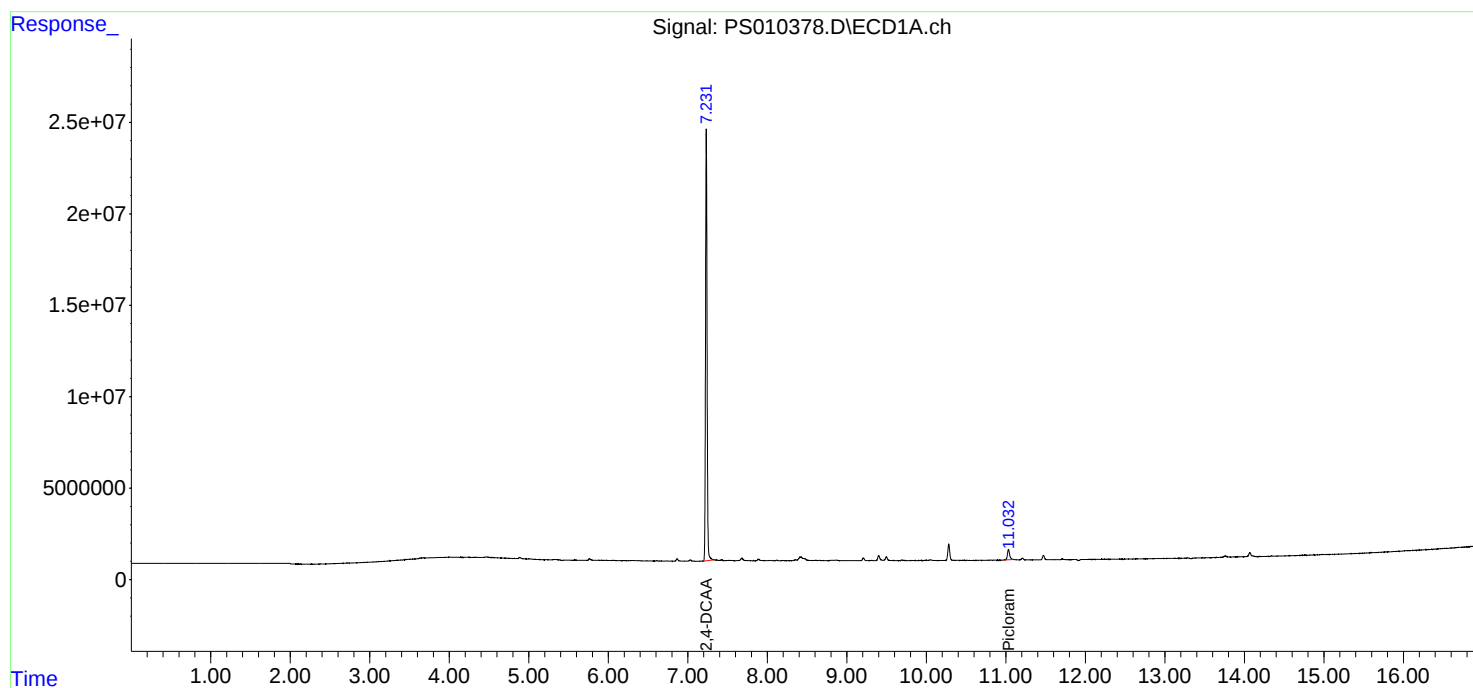


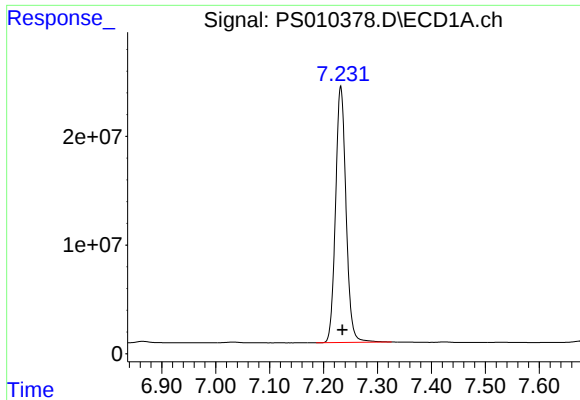

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 317847298
Conc: 452.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

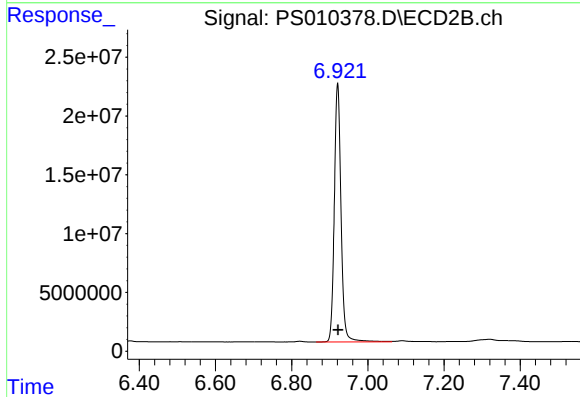


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 270207824
Conc: 503.85 ng/ml

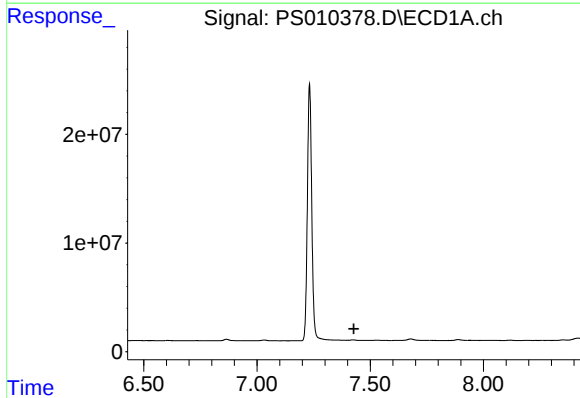


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

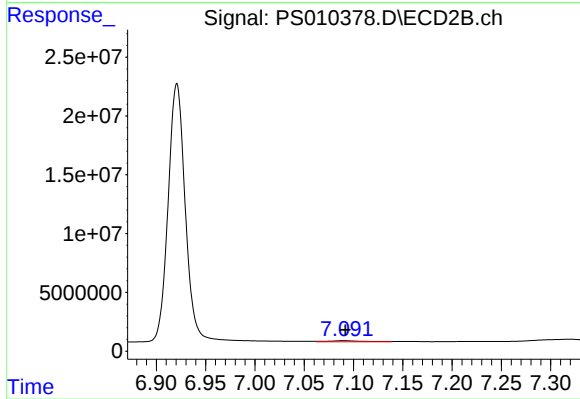

#5 DICAMBA


R.T.: 7.090 min
Delta R.T.: -0.002 min
Response: 2426229
Conc: 1.11 ng/ml

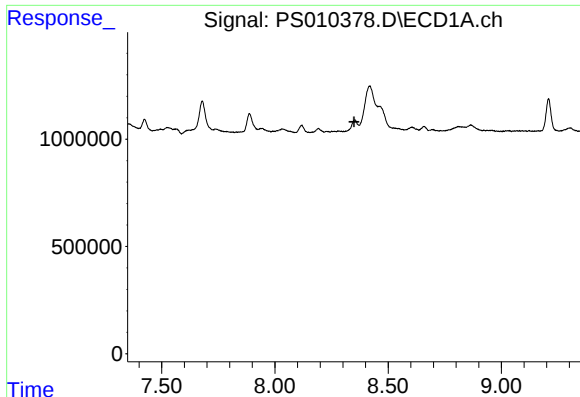

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

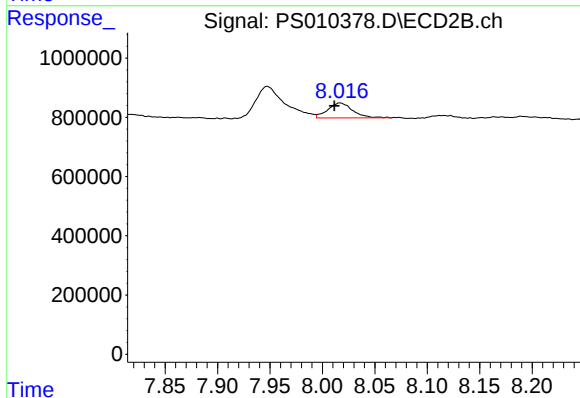


#9 2,4-D

R.T.: 8.017 min
Delta R.T.: 0.006 min
Response: 832636
Conc: 1.20 ng/ml

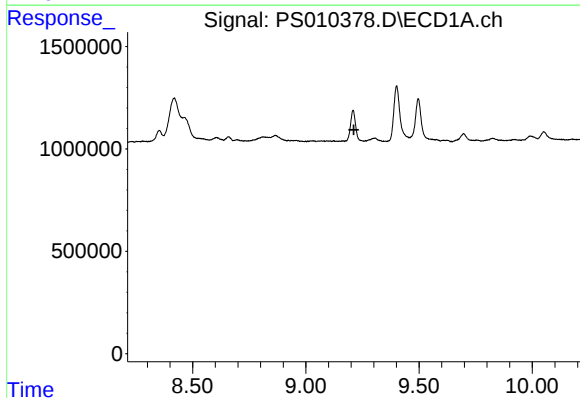


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

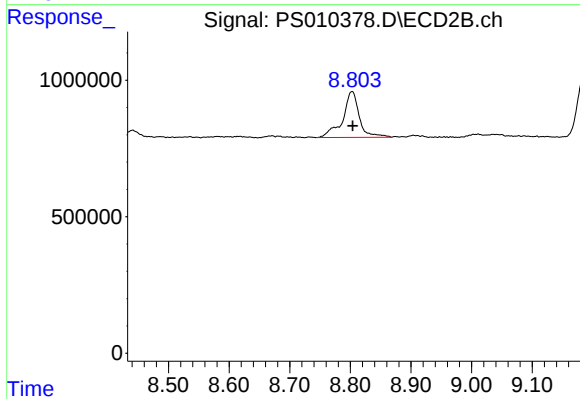

#11 2,4,5-TP (SILVEX)


R.T.: 8.803 min
Delta R.T.: -0.001 min
Response: 3204050
Conc: 1.11 ng/ml

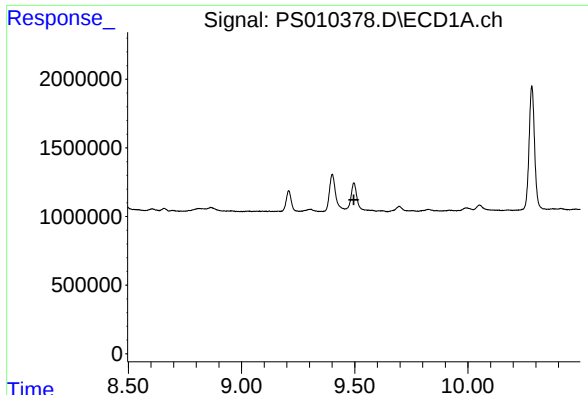

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

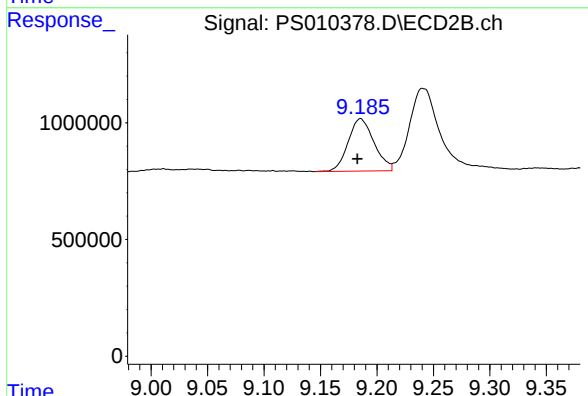


#12 2,4,5-T

R.T.: 9.185 min
Delta R.T.: 0.003 min
Response: 3582673
Conc: 1.23 ng/ml

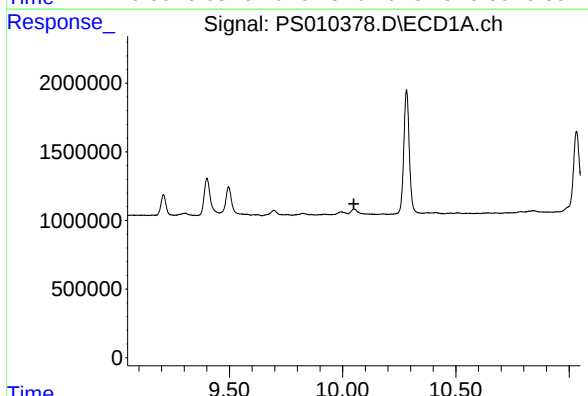


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

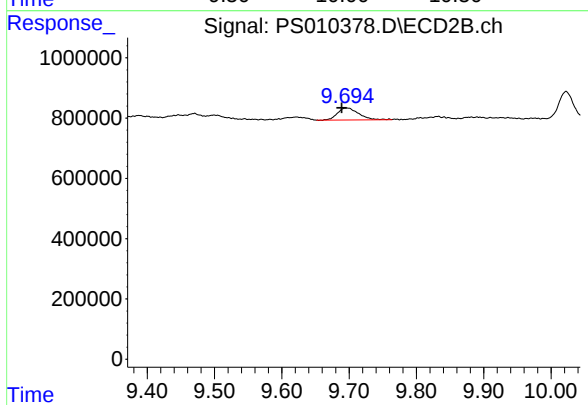

#13 2,4-DB


R.T.: 9.696 min
Delta R.T.: 0.007 min
Response: 878989
Conc: 2.21 ng/ml

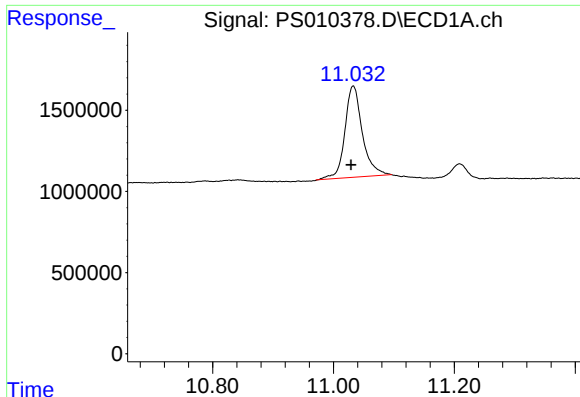

#15 Picloram


R.T.: 11.033 min
Delta R.T.: 0.004 min
Response: 11233660
Conc: 2.45 ng/ml

Instrument :
ECD_S
ClientSampleId :

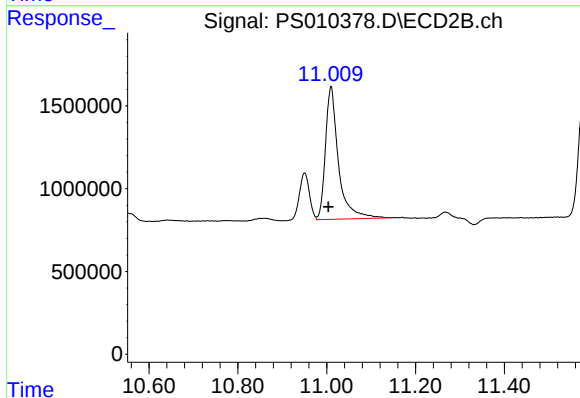


#15 Picloram

R.T.: 11.010 min
Delta R.T.: 0.006 min
Response: 16327618
Conc: 3.87 ng/ml

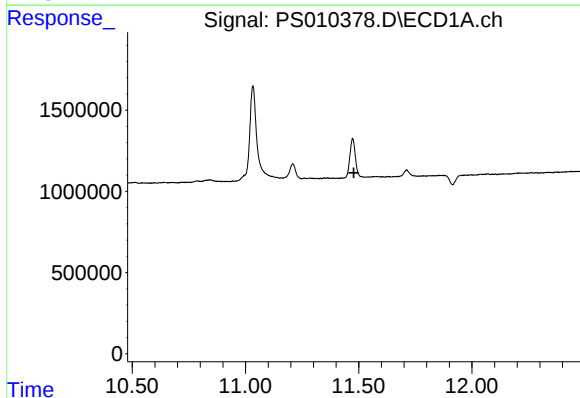

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.479 min
Response: 0
Conc: N.D.

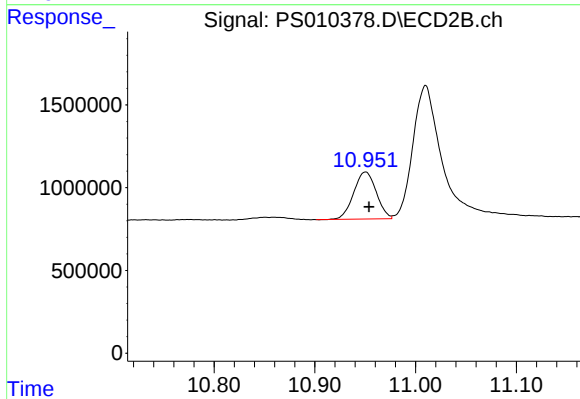

#16 DCPA

R.T.: 10.950 min
Delta R.T.: -0.003 min
Response: 4432208
Conc: 1.24 ng/ml