

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052120\
 Data File : PS010390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 20:05
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:05:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.231	6.921	328.6E6	276.7E6	467.319	516.025
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	2633481	N.D.	1.203
6) T	MCP	0.000	7.154	0	2134411	N.D.	1.163
8) T	DICHLORPROP	0.000	7.745	0	2833557	N.D.	5.019
9) T	2,4-D	8.418	8.017	5644555	560171	7.990	<MDL #
10) T	Pentachlo...	0.000	8.442	0	470677	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	3378617	N.D.	1.166
12) T	2,4,5-T	0.000	9.186	0	3048716	N.D.	1.049
13) T	2,4-DB	0.000	9.697	0	852945	N.D.	2.140
14) T	DINOSEB	0.000	10.023	0	1606012	N.D.	<MDL
15) T	Picloram	0.000	11.011	0	4178677	N.D.	<MDL
16) T	DCPA	0.000	10.950	0	3957453	N.D.	1.107



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052120\
Data File : PS010390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 20:05
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:05:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

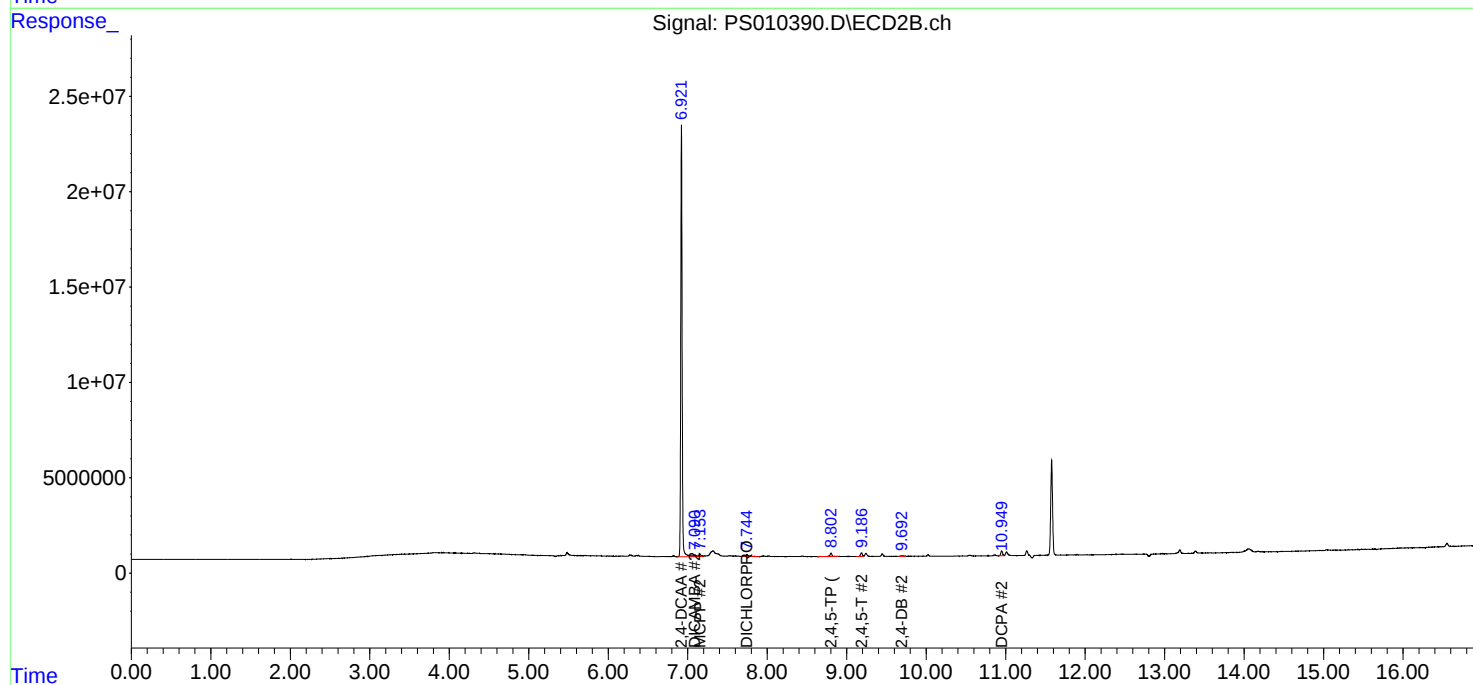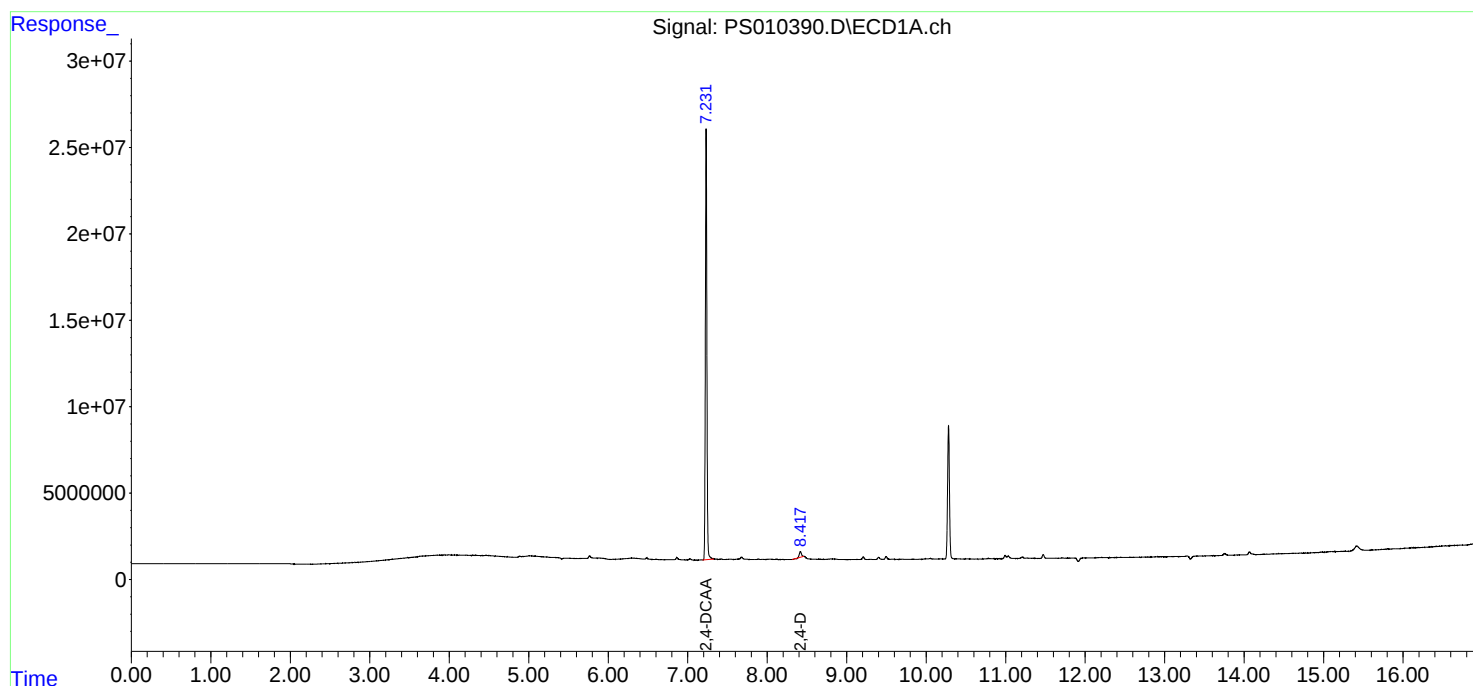


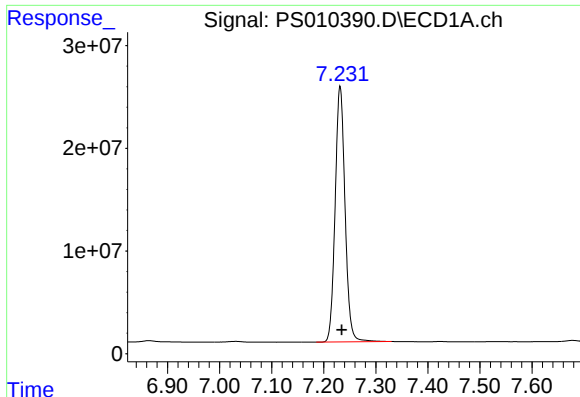

#4 2,4-DCAA


R.T.: 7.231 min
Delta R.T.: -0.003 min
Response: 328569310
Conc: 467.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

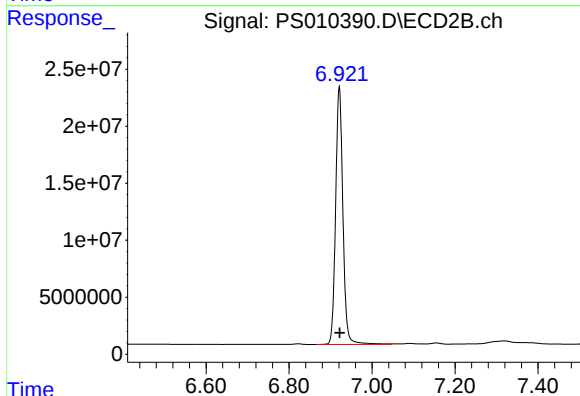


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 276739777
Conc: 516.03 ng/ml

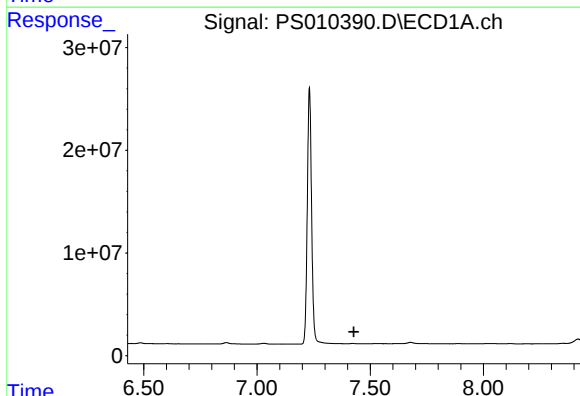


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

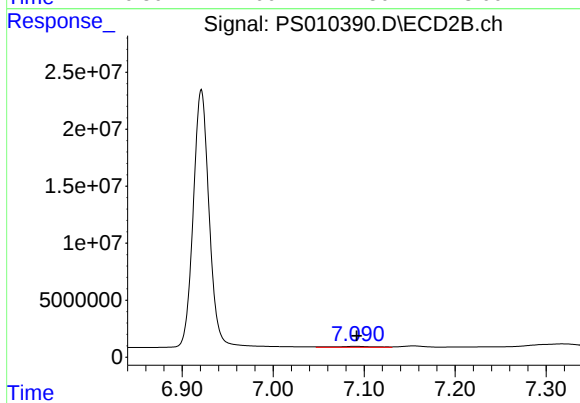

#5 DICAMBA


R.T.: 7.091 min
Delta R.T.: -0.001 min
Response: 2633481
Conc: 1.20 ng/ml

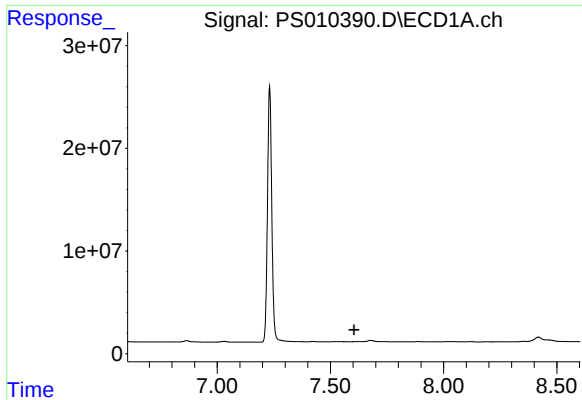

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

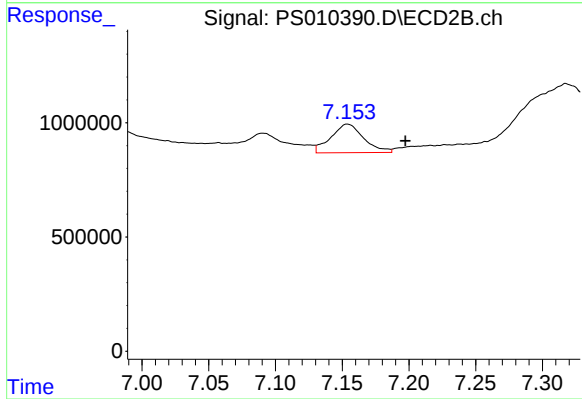


#6 MCPP

R.T.: 7.154 min
Delta R.T.: -0.043 min
Response: 2134411
Conc: 1.16 ug/ml

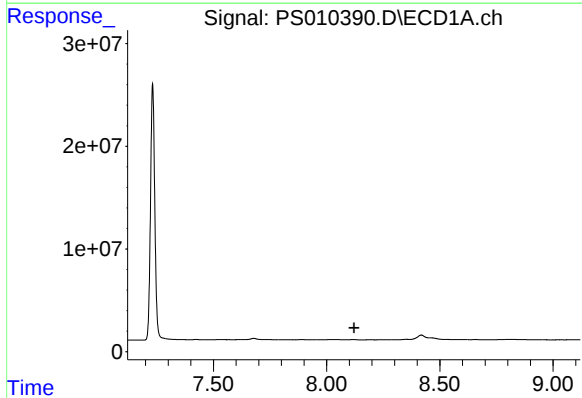


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

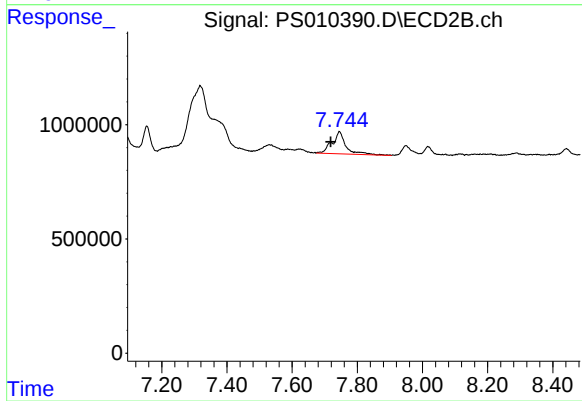

#8 DICHLORPROP


R.T.: 7.745 min
Delta R.T.: 0.027 min
Response: 2833557
Conc: 5.02 ng/ml

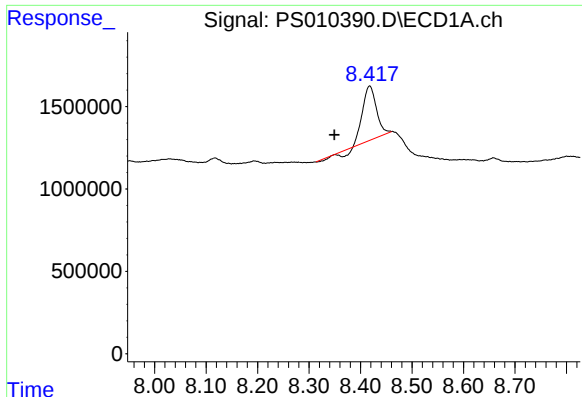

#9 2,4-D


R.T.: 8.418 min
Delta R.T.: 0.069 min
Response: 5644555
Conc: 7.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

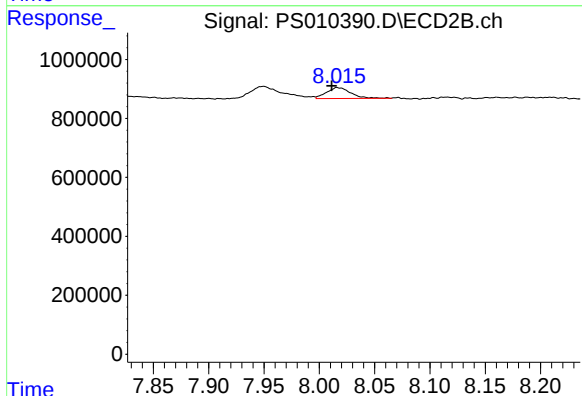


#9 2,4-D

R.T.: 8.017 min
Delta R.T.: 0.006 min
Response: 560171
Conc: N.D.

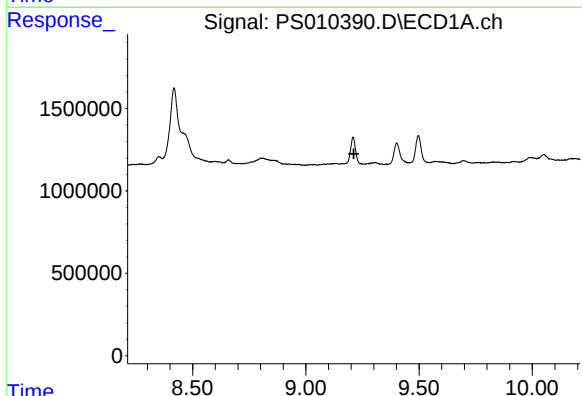


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.212 min
Response: 0
Conc: N.D.

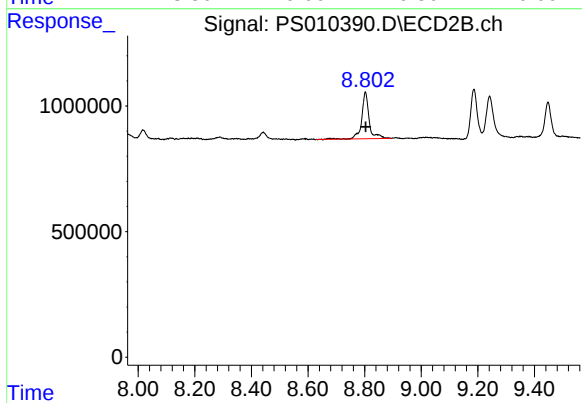

#11 2,4,5-TP (SILVEX)


R.T.: 8.803 min
Delta R.T.: -0.001 min
Response: 3378617
Conc: 1.17 ng/ml

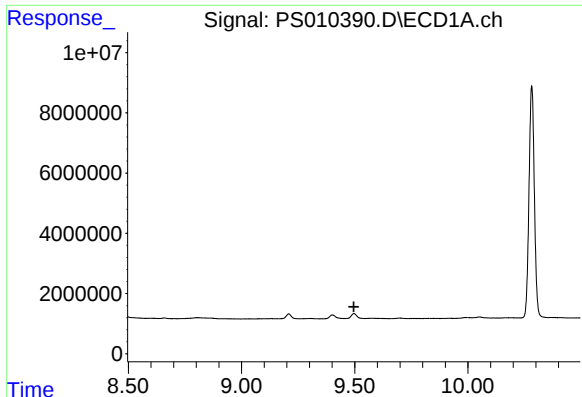

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.497 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

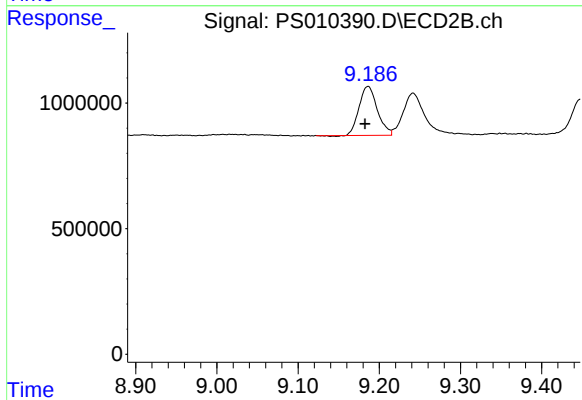


#12 2,4,5-T

R.T.: 9.186 min
Delta R.T.: 0.003 min
Response: 3048716
Conc: 1.05 ng/ml

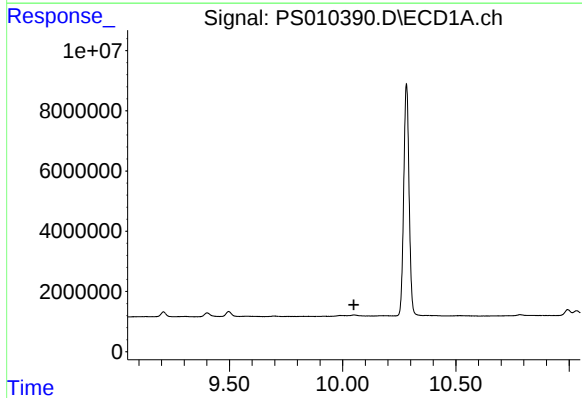


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

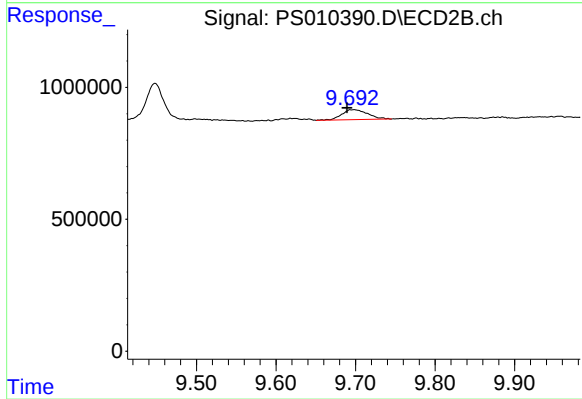

#13 2,4-DB


R.T.: 9.697 min
Delta R.T.: 0.008 min
Response: 852945
Conc: 2.14 ng/ml

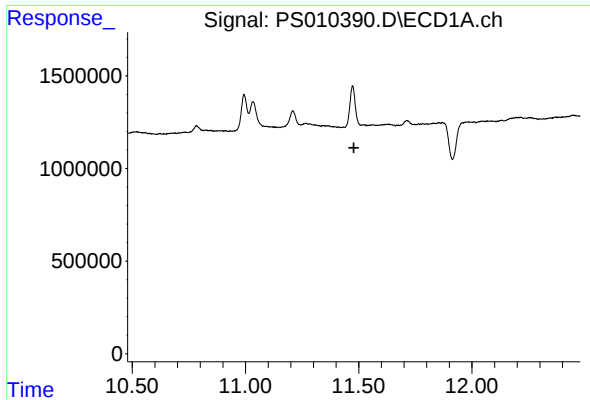

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

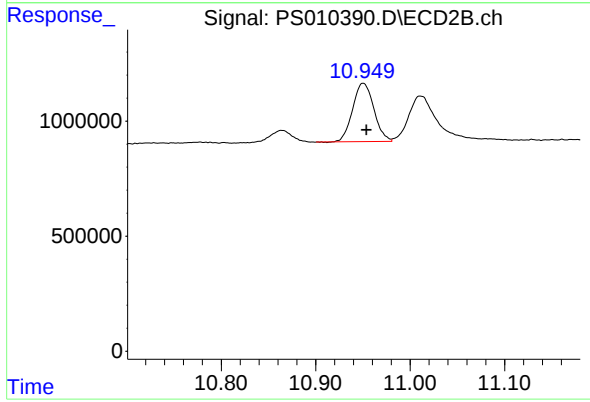

#16 DCPA

R.T.: 10.950 min
Delta R.T.: -0.003 min
Response: 3957453
Conc: 1.11 ng/ml