

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052120\
 Data File : PS010395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 May 2020 22:00
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 01:07:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.920	326.1E6	275.3E6	463.819	513.324
Target Compounds							
1) T	Dalapon	0.000	2.590	0	7812	N.D.	<MDL
5) T	DICAMBA	0.000	7.090	0	2083498	N.D.	<MDL
6) T	MCP	0.000	7.153	0	2107083	N.D.	1.148
8) T	DICHLORPROP	0.000	7.744	0	2434321	N.D.	4.312
9) T	2,4-D	0.000	8.015	0	419363	N.D.	<MDL
10) T	Pentachlo...	0.000	8.441	0	461585	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	2531202	N.D.	<MDL
12) T	2,4,5-T	0.000	9.185	0	2330447	N.D.	<MDL
13) T	2,4-DB	0.000	9.702	0	637589	N.D.	1.600
14) T	DINOSEB	0.000	10.022	0	1060781	N.D.	<MDL
15) T	Picloram	0.000	11.012	0	3693601	N.D.	<MDL
16) T	DCPA	0.000	10.950	0	3479759	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS051120\
Data File : PS010395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 May 2020 22:00
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 01:07:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

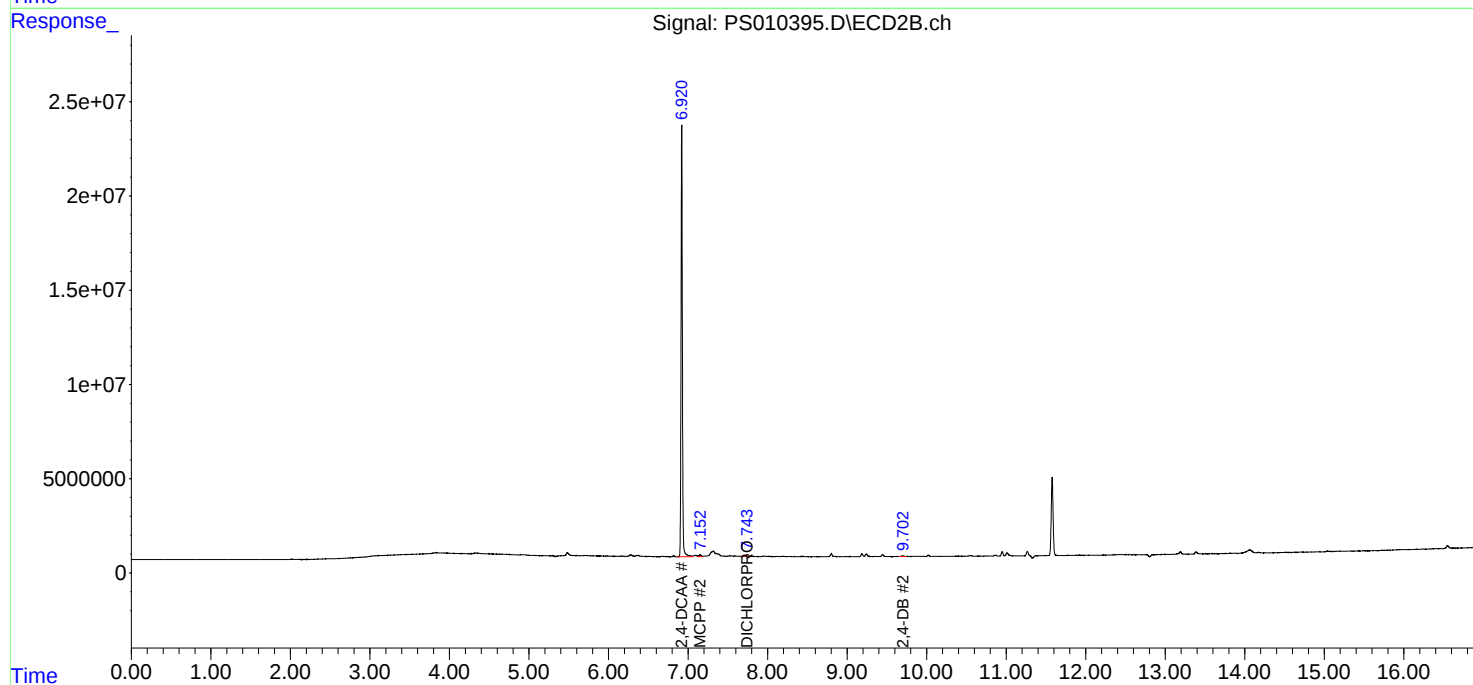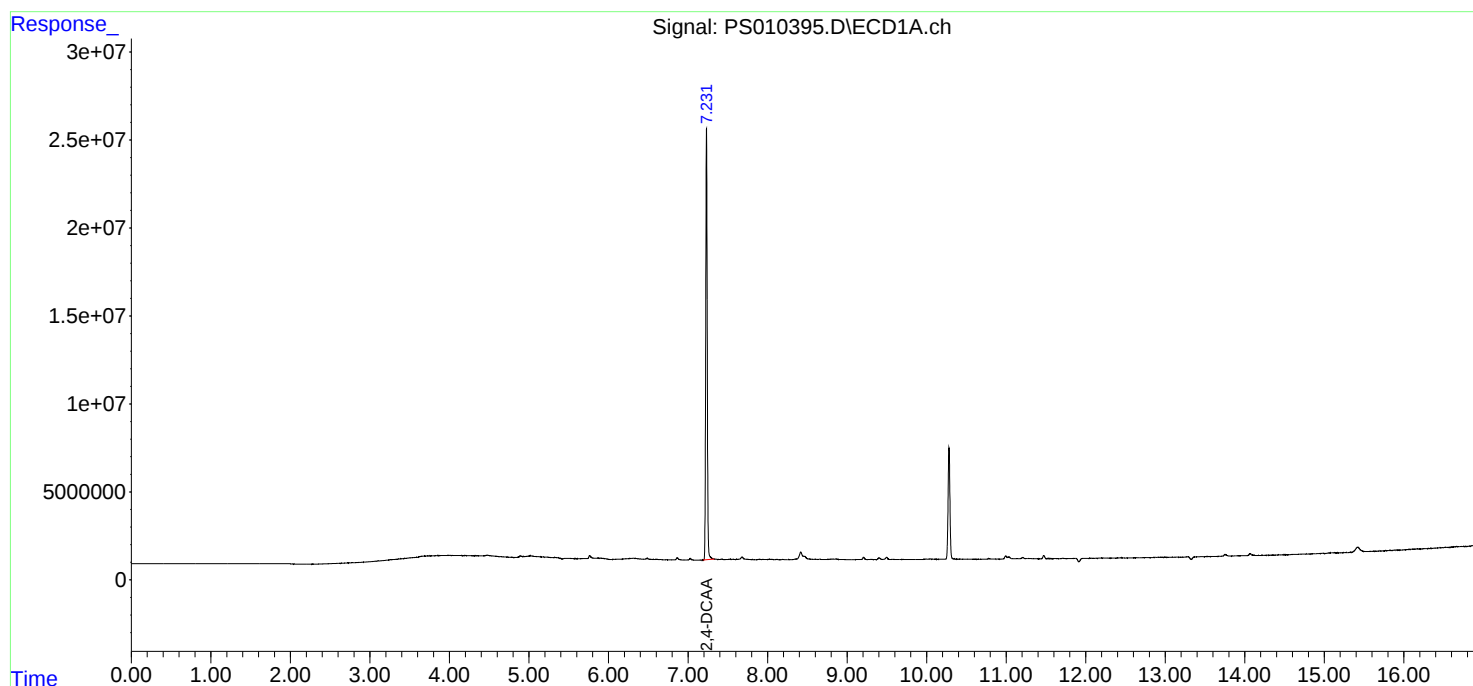


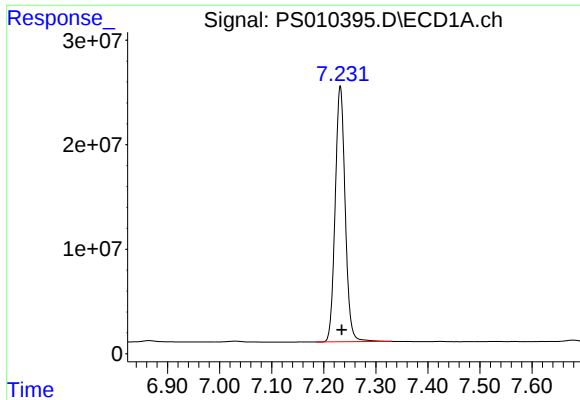

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 326108418
Conc: 463.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

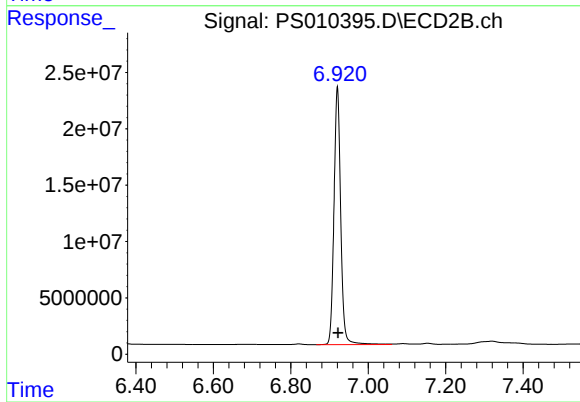


#4 2,4-DCAA

R.T.: 6.920 min
Delta R.T.: -0.002 min
Response: 275291118
Conc: 513.32 ng/ml

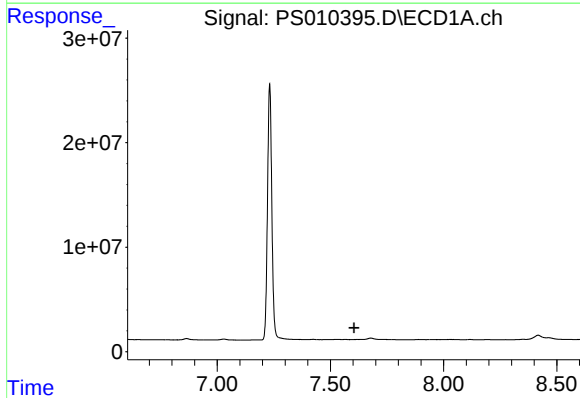


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.604 min
Response: 0
Conc: N.D.

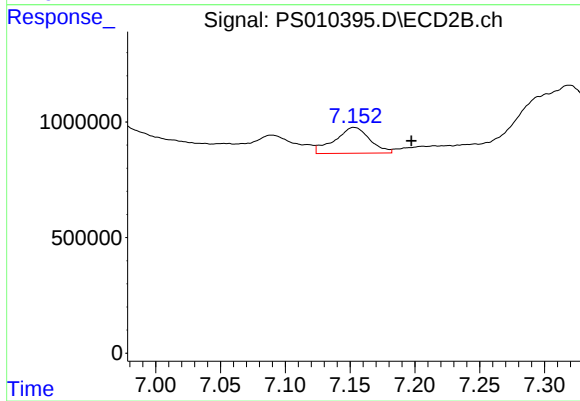

#6 MCP


R.T.: 7.153 min
Delta R.T.: -0.044 min
Response: 2107083
Conc: 1.15 ug/ml

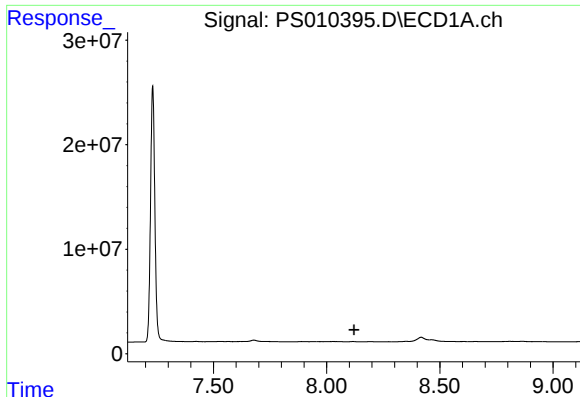

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

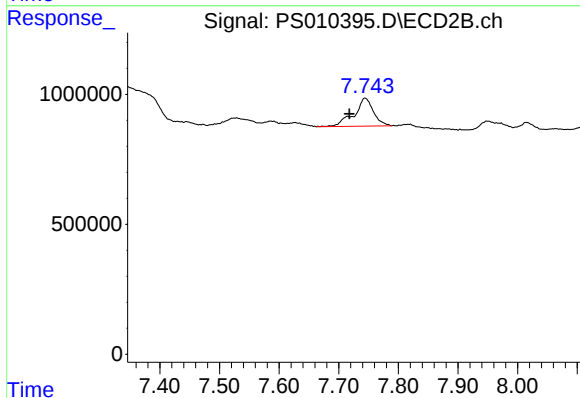


#8 DICHLORPROP

R.T.: 7.744 min
Delta R.T.: 0.026 min
Response: 2434321
Conc: 4.31 ng/ml

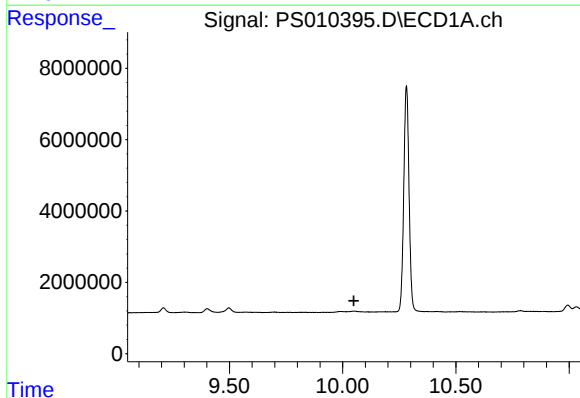

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

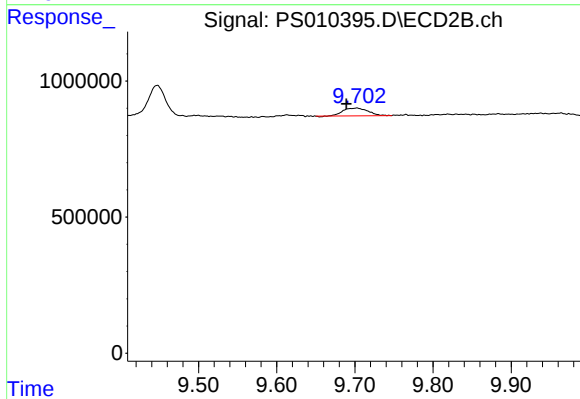

#13 2,4-DB

R.T.: 9.702 min
Delta R.T.: 0.013 min
Response: 637589
Conc: 1.60 ng/ml