

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
 Data File : PS010397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2020 10:15
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 14:25:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	6.925	0	279600	N.D.	<MDL
Target Compounds							
2) T	3,5-DICHL...	6.487	6.095	962.5E6	467137	997.677	<MDL #
3) T	4-Nitroph...	0.000	6.581	0	934271	N.D.	2.812
5) T	DICAMBA	0.000	7.153	0	782.6E6	N.D.	357.415
6) T	MCP	0.000	7.153	0	782.6E6	N.D.	426.340
7) T	MCPA	0.000	7.441	0	852318	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.743	0	3723202	N.D.	6.595
9) T	2,4-D	8.418	8.013	926.6E6	443883	1311.588	<MDL #
10) T	Pentachlo...	0.000	8.442	0	943458	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.802	0	2941239	N.D.	1.015
12) T	2,4,5-T	0.000	9.186	0	2243661	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	2893526	N.D.	7.260
14) T	DINOSEB	0.000	10.021	0	958000	N.D.	<MDL
15) T	Picloram	11.033	11.006	28888604	34746803	6.301	8.230 #
16) T	DCPA	0.000	10.951	0	2796100	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
Data File : PS010397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2020 10:15
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 14:25:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

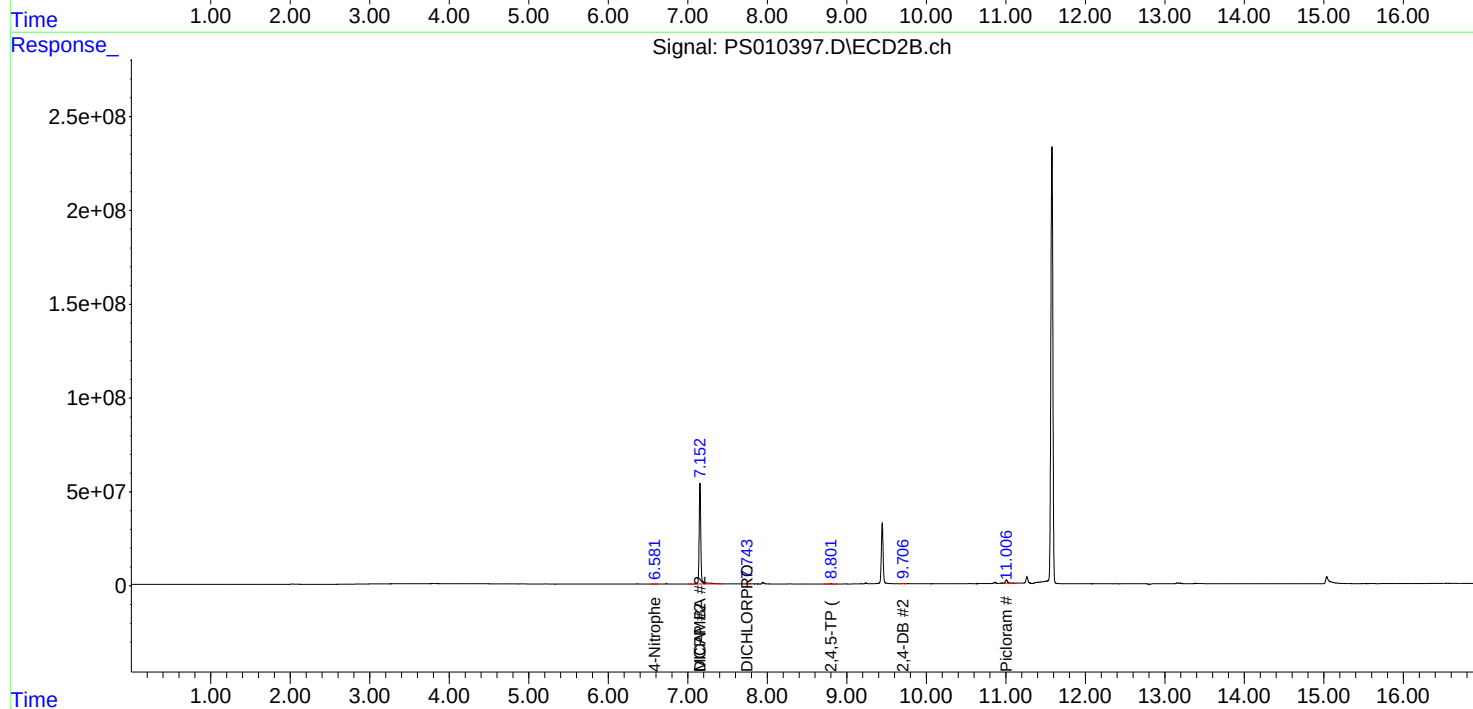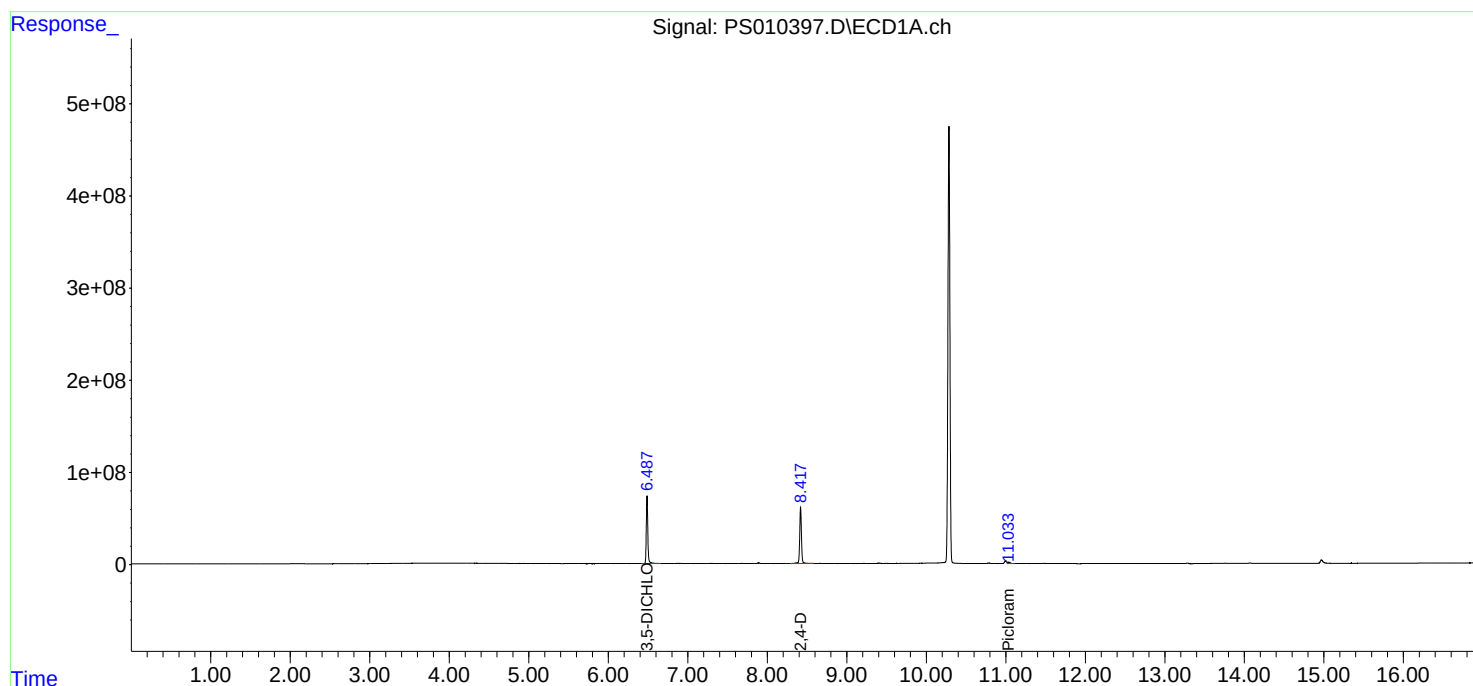


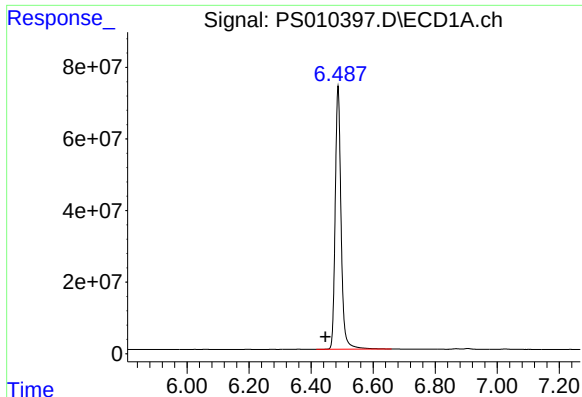

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.487 min
Delta R.T.: 0.041 min
Response: 962501461
Conc: 997.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

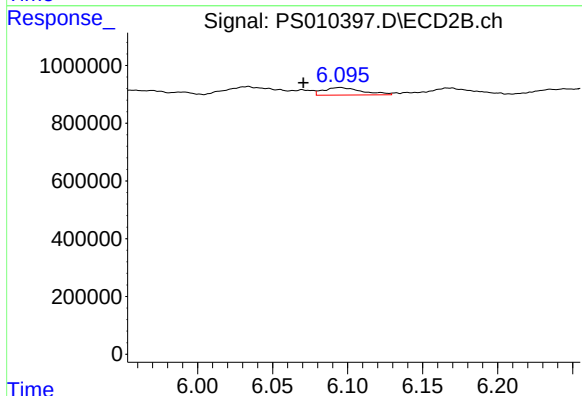


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.095 min
Delta R.T.: 0.024 min
Response: 467137
Conc: N.D.

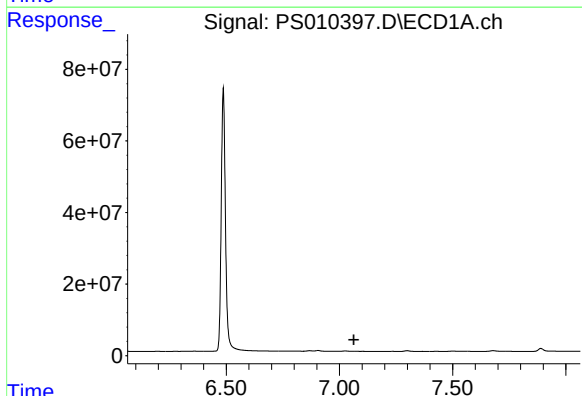


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.064 min
Response: 0
Conc: N.D.

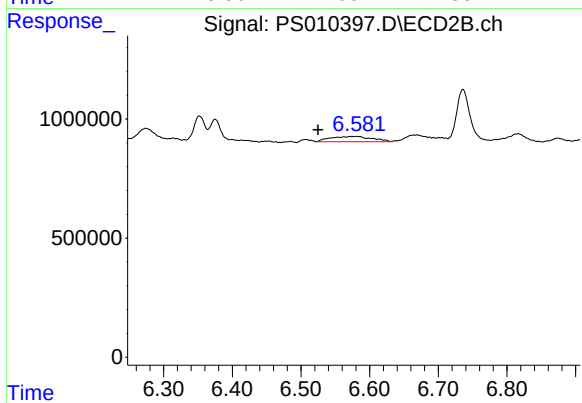

#3 4-Nitrophenol


R.T.: 6.581 min
Delta R.T.: 0.056 min
Response: 934271
Conc: 2.81 ng/ml

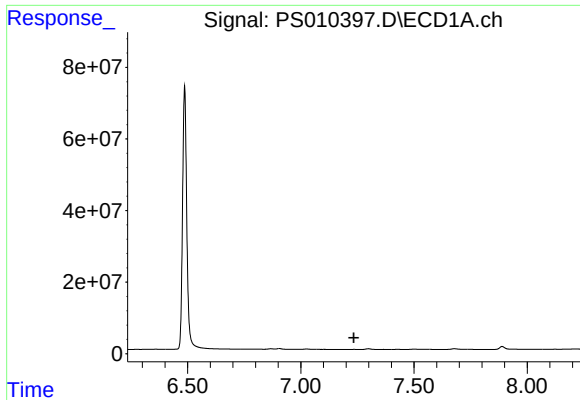

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.235 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

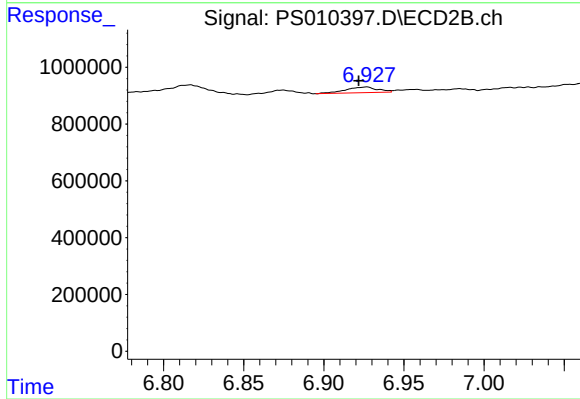


#4 2,4-DCAA

R.T.: 6.925 min
Delta R.T.: 0.003 min
Response: 279600
Conc: N.D.

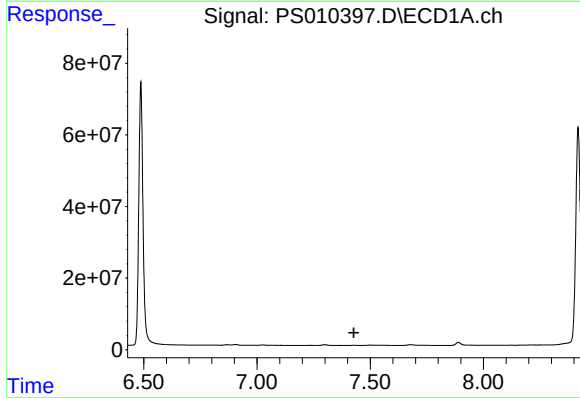


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

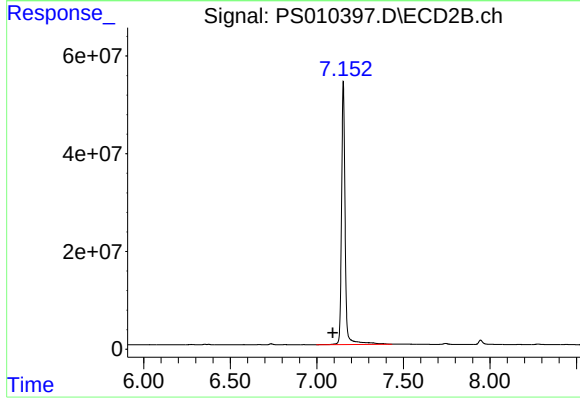

#5 DICAMBA


R.T.: 7.153 min
Delta R.T.: 0.061 min
Response: 782595890
Conc: 357.42 ng/ml

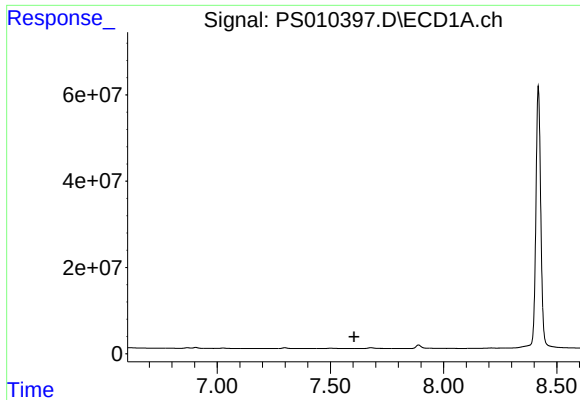

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.604 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

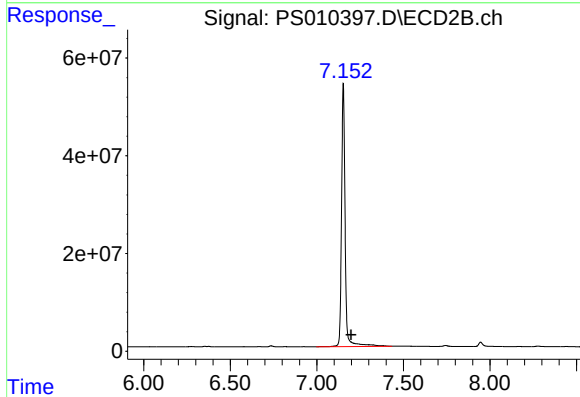


#6 MCP

R.T.: 7.153 min
Delta R.T.: -0.044 min
Response: 782595890
Conc: 426.34 ug/ml

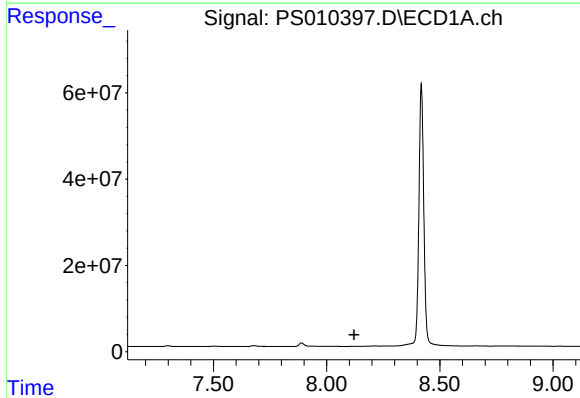


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

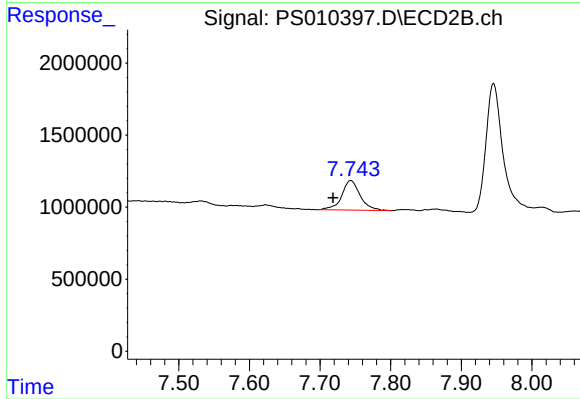

#8 DICHLORPROP


R.T.: 7.743 min
Delta R.T.: 0.025 min
Response: 3723202
Conc: 6.59 ng/ml

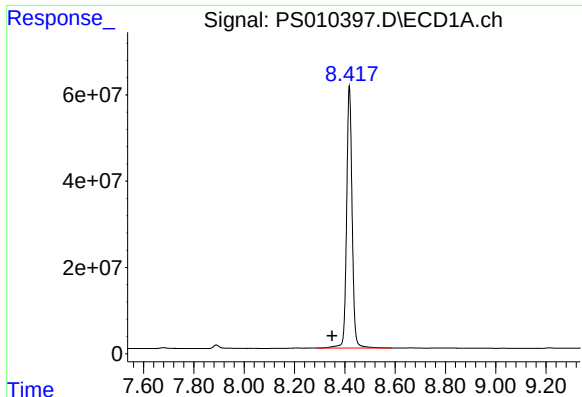

#9 2,4-D


R.T.: 8.418 min
Delta R.T.: 0.069 min
Response: 926575813
Conc: 1311.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

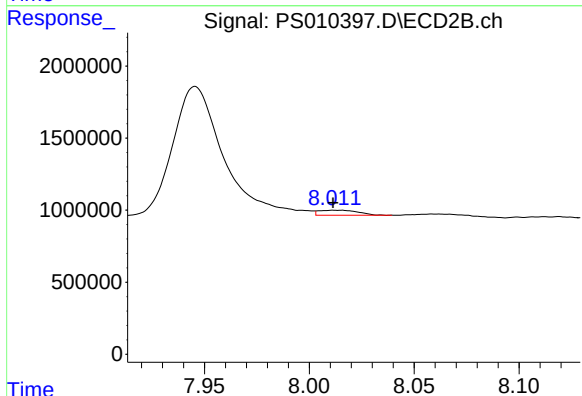


#9 2,4-D

R.T.: 8.013 min
Delta R.T.: 0.002 min
Response: 443883
Conc: N.D.

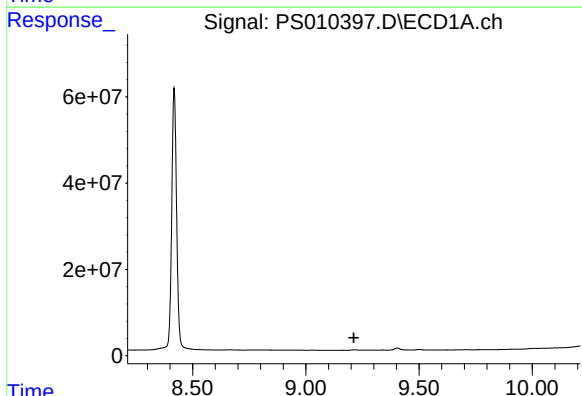


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.212 min
Response: 0
Conc: N.D.

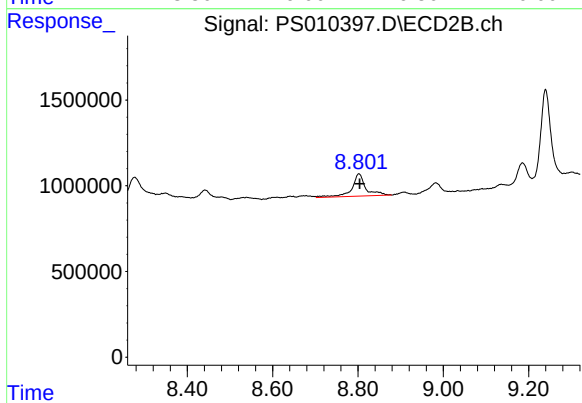

#11 2,4,5-TP (SILVEX)


R.T.: 8.802 min
Delta R.T.: -0.002 min
Response: 2941239
Conc: 1.02 ng/ml

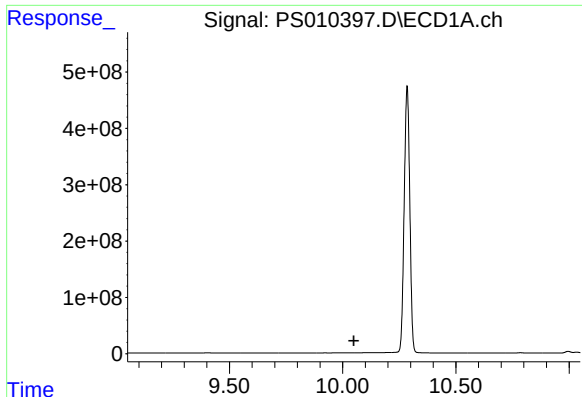

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

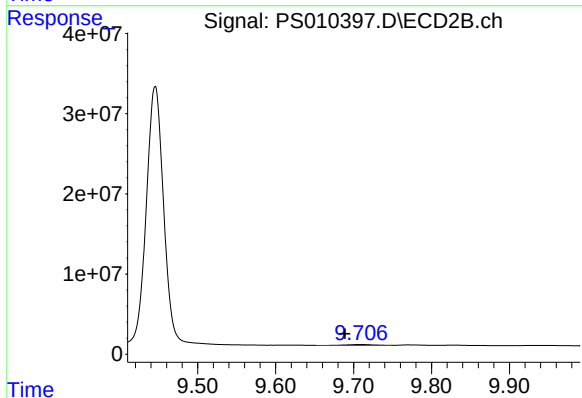


#13 2,4-DB

R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 2893526
Conc: 7.26 ng/ml

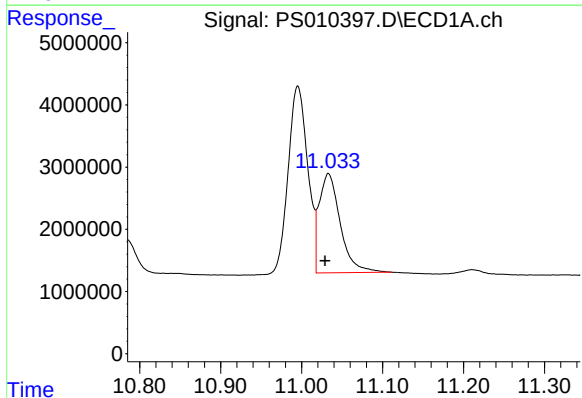

#15 Picloram

R.T.: 11.033 min
Delta R.T.: 0.004 min
Response: 28888604
Conc: 6.30 ng/ml

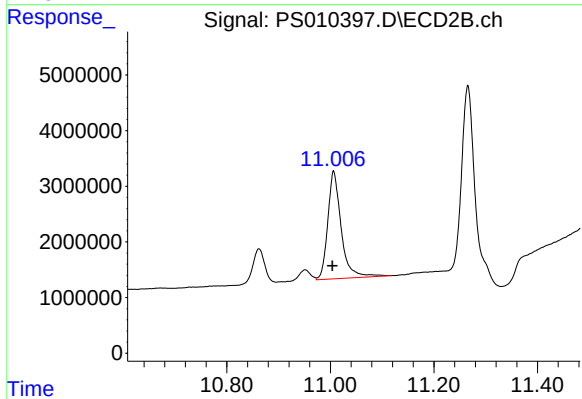

#15 Picloram

R.T.: 11.006 min
Delta R.T.: 0.003 min
Response: 34746803
Conc: 8.23 ng/ml