

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
 Data File : PS010398.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2020 10:38
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 14:26:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.234	6.921	315.1E6	266.6E6	448.101	497.145
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	2096309	N.D.	<MDL
7) T	MCPA	0.000	7.434	0	12787	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.747	0	3725710	N.D.	6.599
9) T	2,4-D	0.000	8.013	0	277846	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	1277658	N.D.	<MDL
12) T	2,4,5-T	0.000	9.189	0	1083947	N.D.	<MDL
13) T	2,4-DB	0.000	9.708	0	460162	N.D.	1.155
14) T	DINOSEB	0.000	10.023	0	555799	N.D.	<MDL
15) T	Picloram	11.035	11.011	13239864	20137790	2.888	4.770 #
16) T	DCPA	0.000	10.952	0	1581199	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
Data File : PS010398.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2020 10:38
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 14:26:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

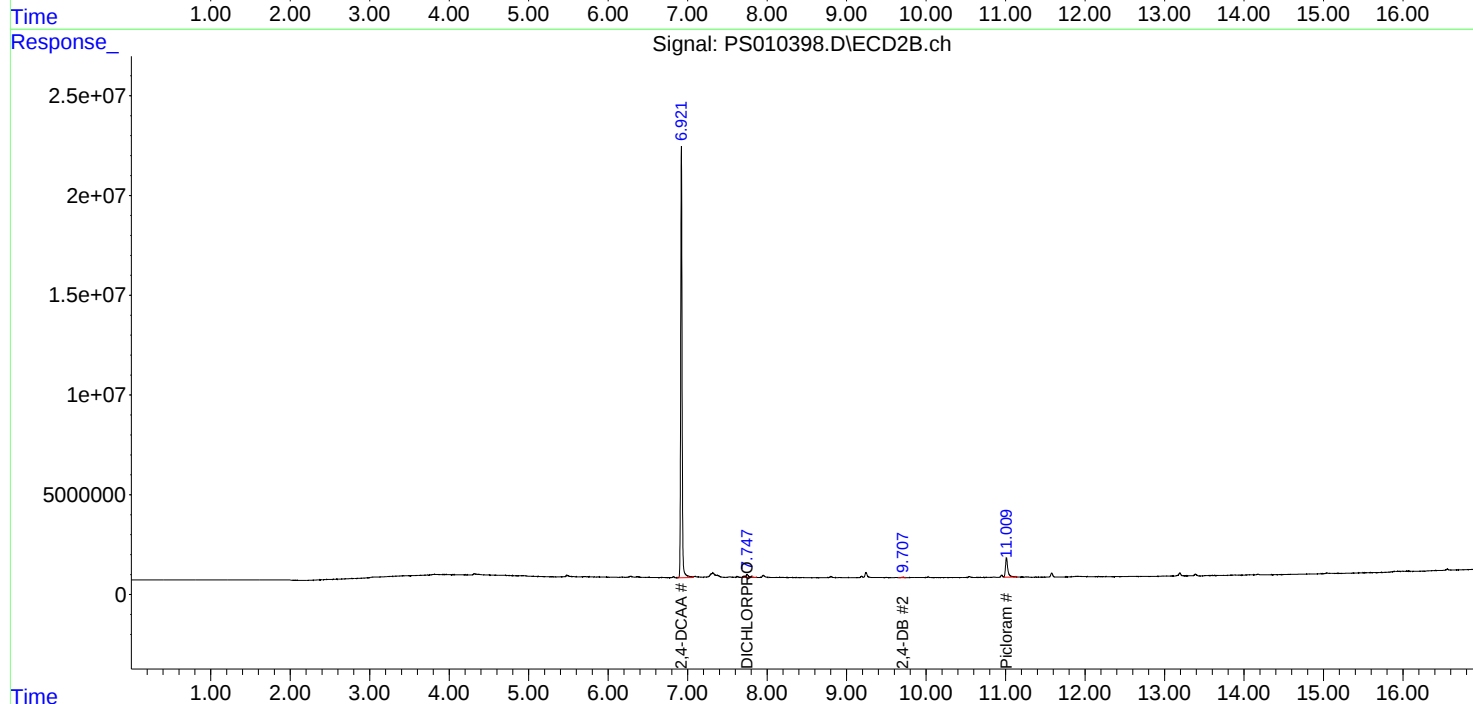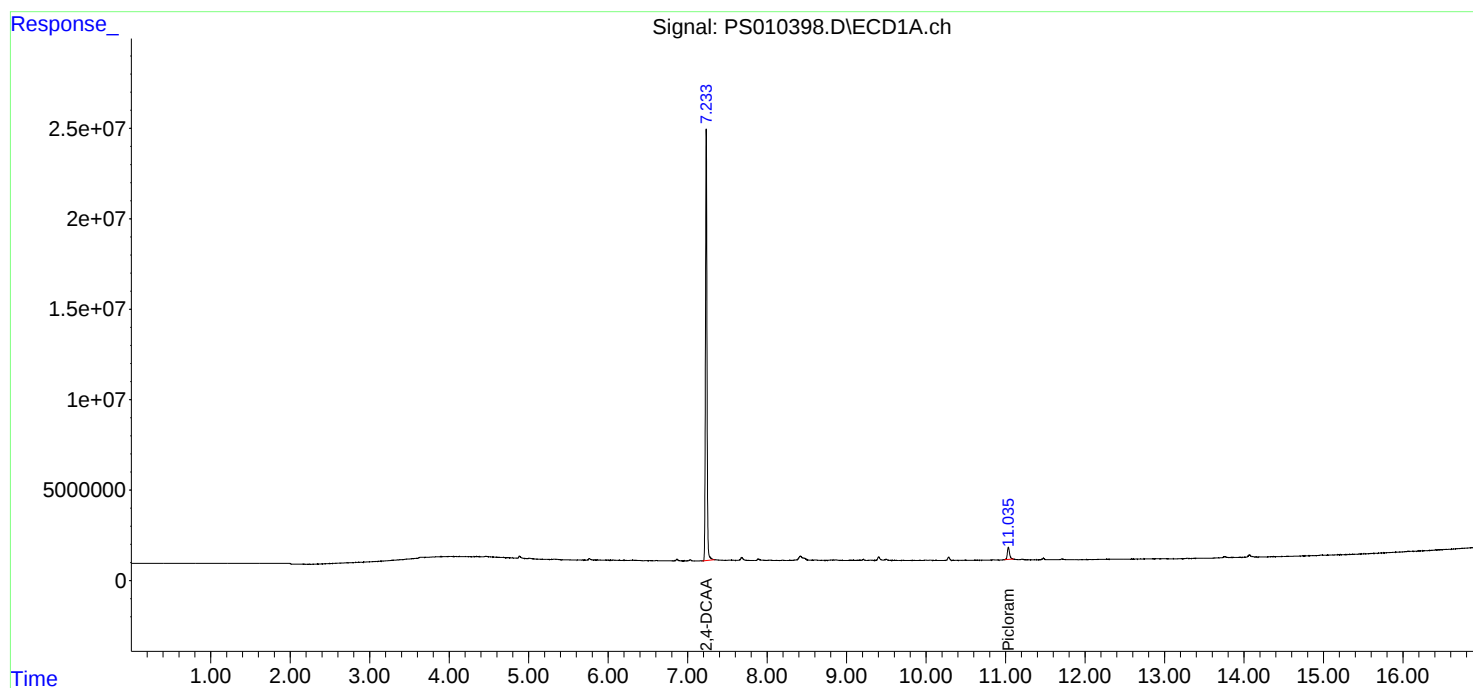


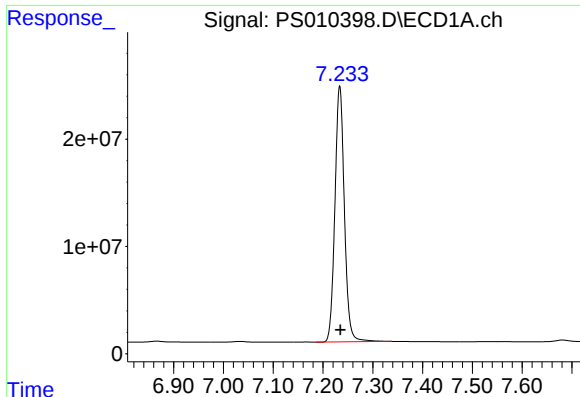

#4 2,4-DCAA


R.T.: 7.234 min
Delta R.T.: -0.001 min
Response: 315057394
Conc: 448.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

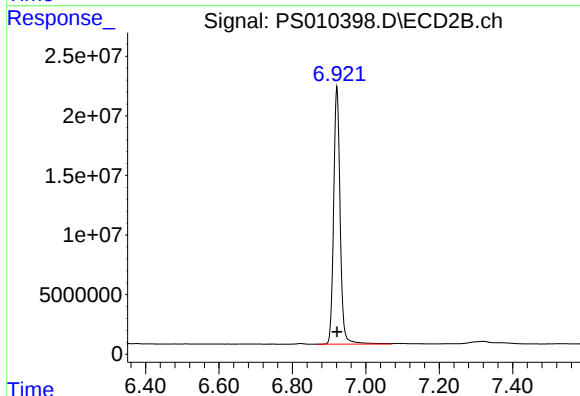


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 266614430
Conc: 497.14 ng/ml

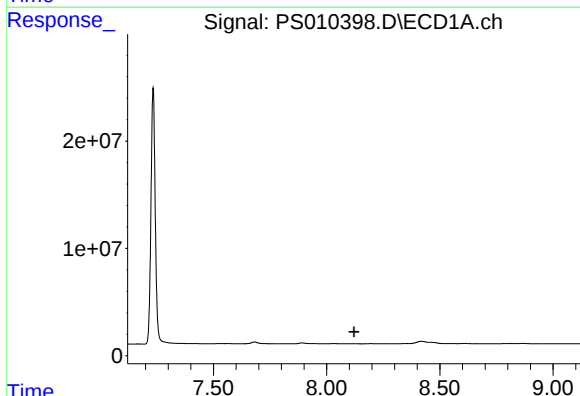


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.121 min
Response: 0
Conc: N.D.

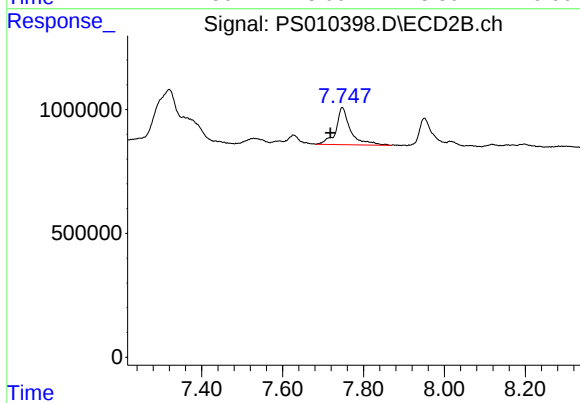

#8 DICHLORPROP


R.T.: 7.747 min
Delta R.T.: 0.029 min
Response: 3725710
Conc: 6.60 ng/ml

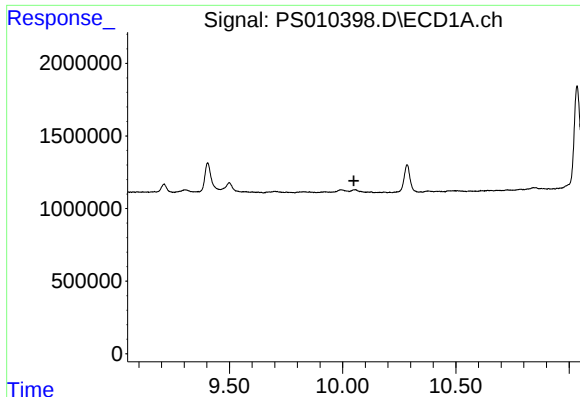

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

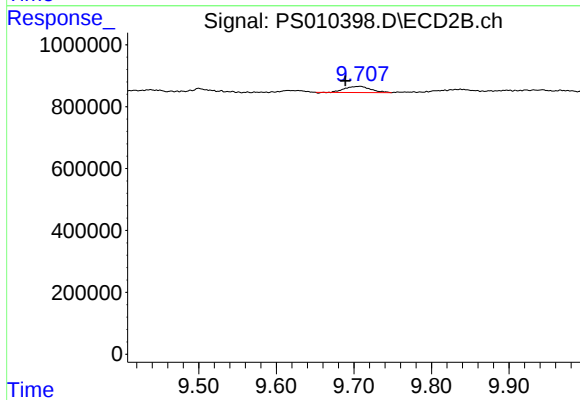


#13 2,4-DB

R.T.: 9.708 min
Delta R.T.: 0.019 min
Response: 460162
Conc: 1.15 ng/ml

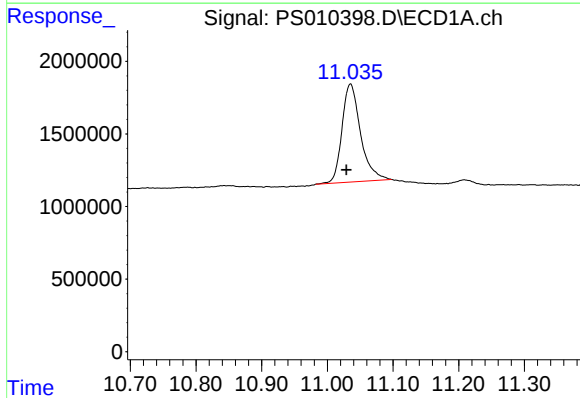

#15 Picloram

R.T.: 11.035 min
Delta R.T.: 0.006 min
Response: 13239864
Conc: 2.89 ng/ml

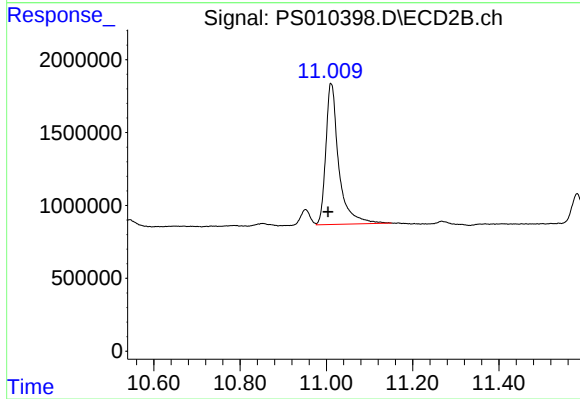

#15 Picloram

R.T.: 11.011 min
Delta R.T.: 0.007 min
Response: 20137790
Conc: 4.77 ng/ml