

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
 Data File : PS010410.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2020 15:13
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 17:15:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.921	326.3E6	272.2E6	464.060	507.542
Target Compounds							
5) T	DICAMBA	0.000	7.091	0	3200622	N.D.	1.462
8) T	DICHLORPROP	0.000	7.746	0	4065012	N.D.	7.200
9) T	2,4-D	0.000	8.015	0	312797	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	1466749	N.D.	<MDL
12) T	2,4,5-T	0.000	9.186	0	1206270	N.D.	<MDL
13) T	2,4-DB	0.000	9.707	0	547927	N.D.	1.375
14) T	DINOSEB	0.000	10.024	0	1243002	N.D.	<MDL
15) T	Picloram	0.000	11.014	0	1483097	N.D.	<MDL
16) T	DCPA	0.000	10.951	0	3538408	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
Data File : PS010410.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2020 15:13
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 17:15:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

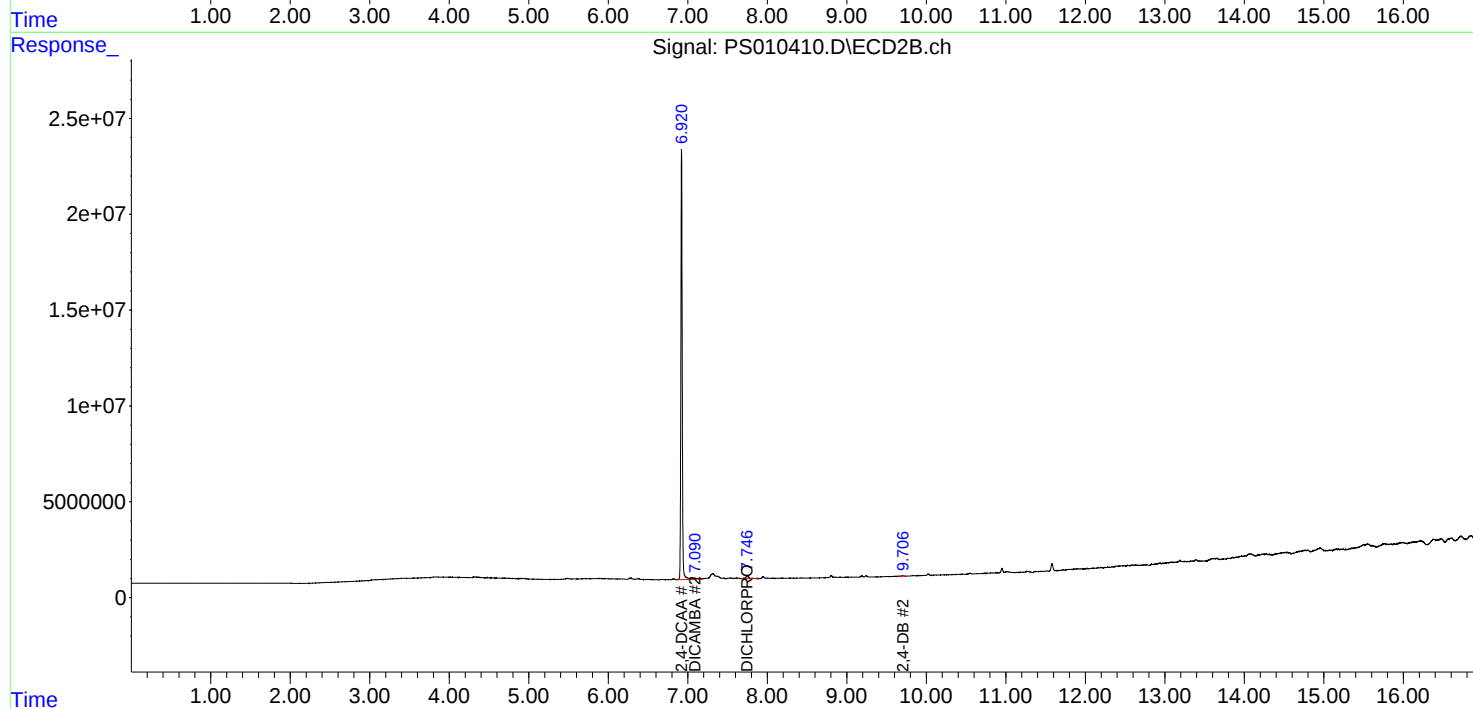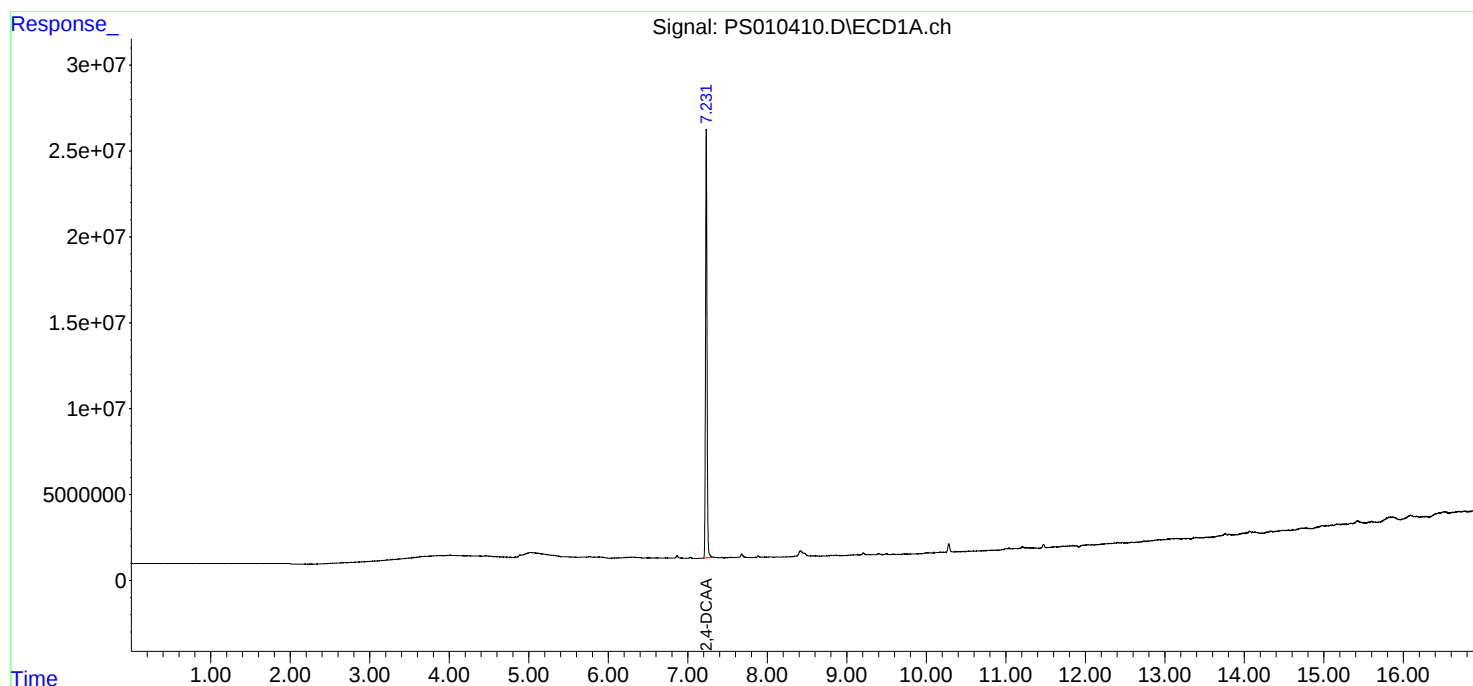


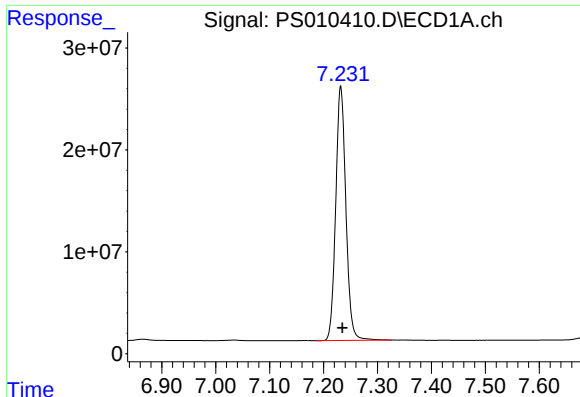

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 326277919
Conc: 464.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

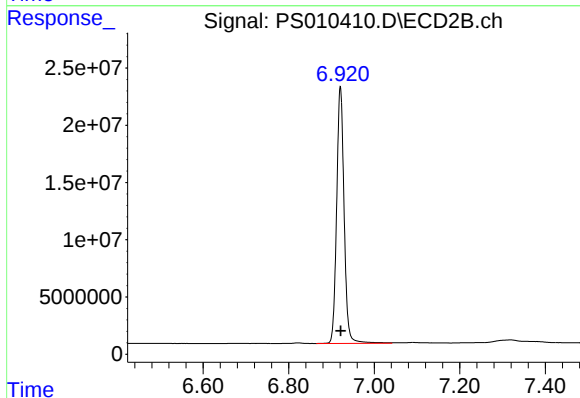


#4 2,4-DCAA

R.T.: 6.921 min
Delta R.T.: 0.000 min
Response: 272190543
Conc: 507.54 ng/ml

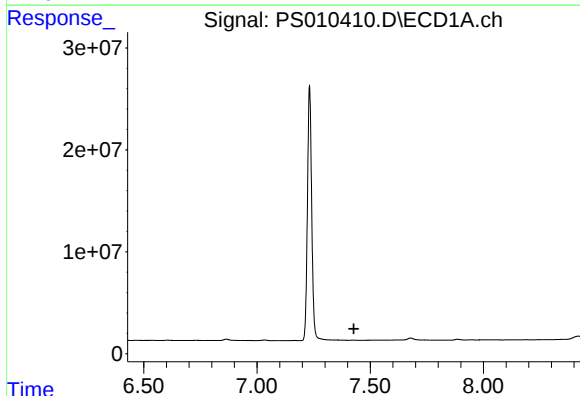


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.428 min
Response: 0
Conc: N.D.

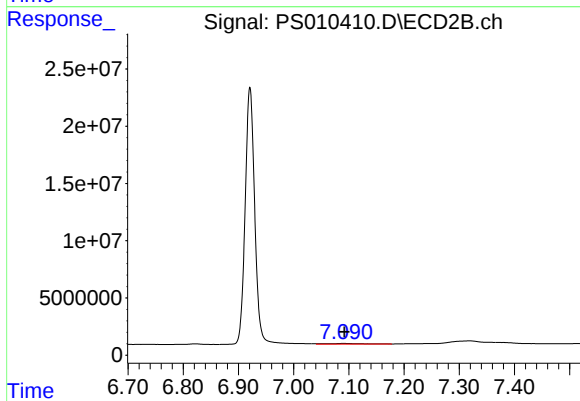

#5 DICAMBA


R.T.: 7.091 min
Delta R.T.: -0.001 min
Response: 3200622
Conc: 1.46 ng/ml

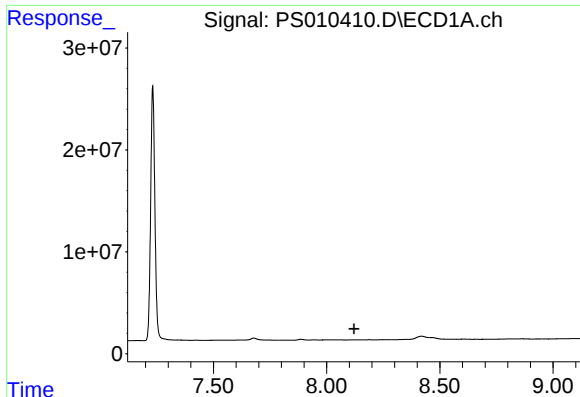

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

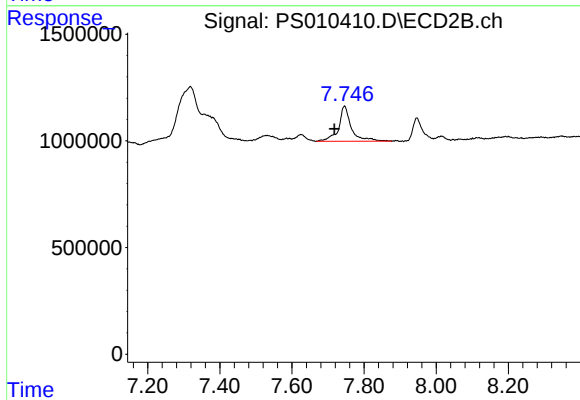


#8 DICHLORPROP

R.T.: 7.746 min
Delta R.T.: 0.027 min
Response: 4065012
Conc: 7.20 ng/ml

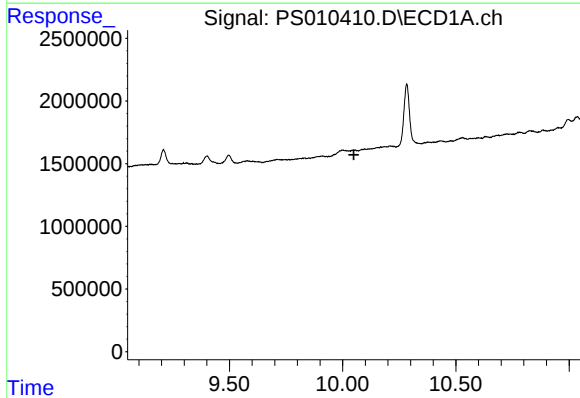

#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

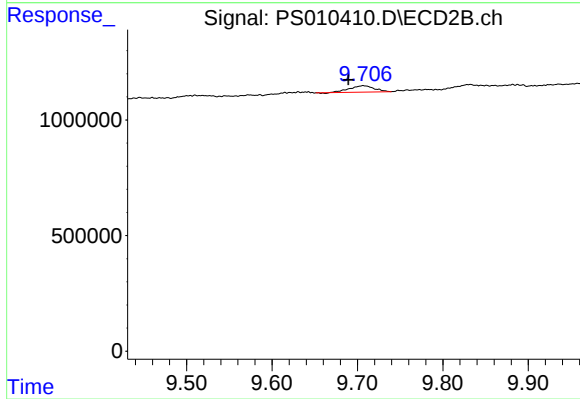

#13 2,4-DB

R.T.: 9.707 min
Delta R.T.: 0.018 min
Response: 547927
Conc: 1.37 ng/ml