

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
 Data File : PS010413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 May 2020 16:22
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 22 17:16:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
 Quant Title : 8080.M
 QLast Update : Mon May 11 17:06:53 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.922	327.0E6	271.7E6	465.142	506.642
Target Compounds							
1) T	Dalapon	0.000	2.598	0	107250	N.D.	<MDL
5) T	DICAMBA	0.000	7.091	0	1969185	N.D.	<MDL
6) T	MCP	0.000	7.158	0	779433	N.D.	<MDL
7) T	MCPA	0.000	7.356	0	4541885	N.D.	1.670
8) T	DICHLORPROP	0.000	7.745	0	3329503	N.D.	5.897
9) T	2,4-D	0.000	8.016	0	291267	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.803	0	1770599	N.D.	<MDL
12) T	2,4,5-T	0.000	9.184	0	1046758	N.D.	<MDL
13) T	2,4-DB	0.000	9.705	0	725469	N.D.	1.820
14) T	DINOSEB	0.000	10.022	0	3024815	N.D.	1.419
15) T	Picloram	0.000	11.010	0	4850530	N.D.	1.149
16) T	DCPA	0.000	10.952	0	3168245	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS052220\
Data File : PS010413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 May 2020 16:22
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 22 17:16:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS051120.M
Quant Title : 8080.M
QLast Update : Mon May 11 17:06:53 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

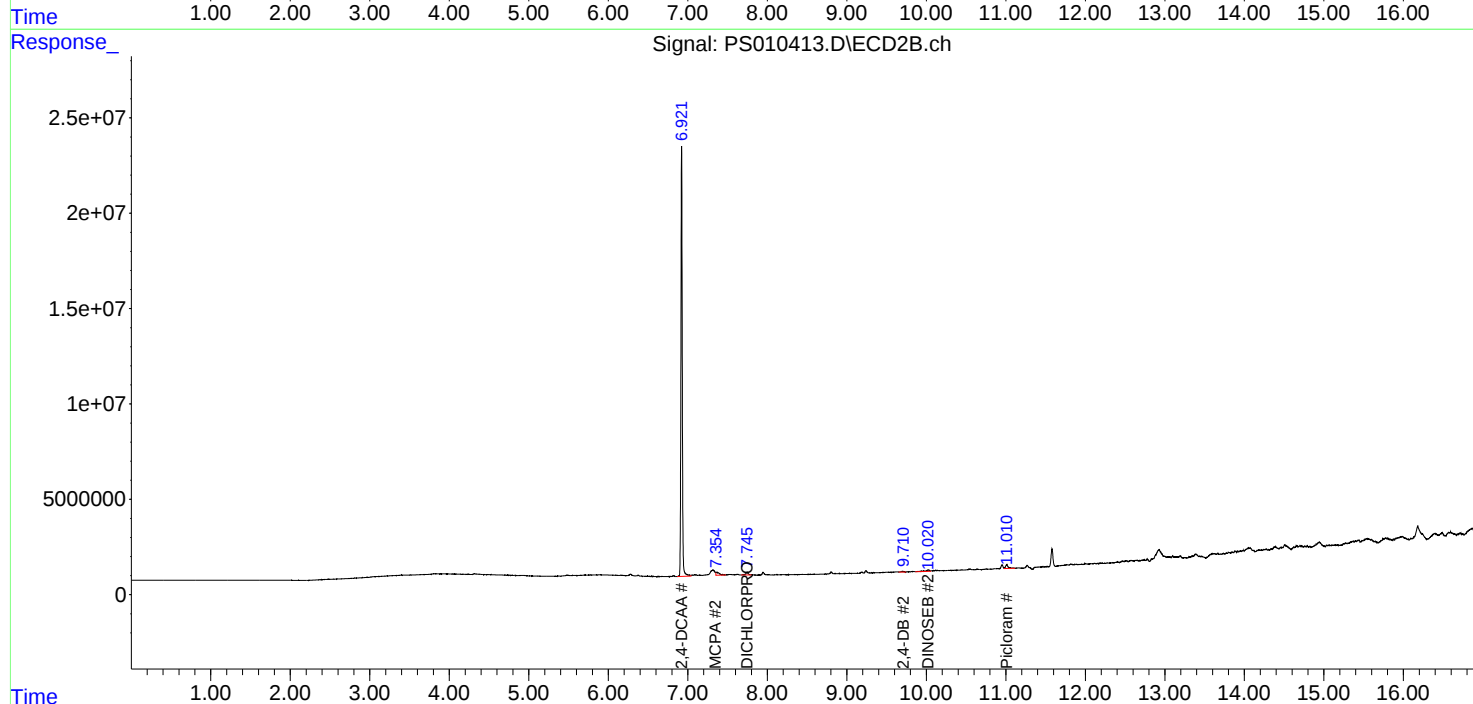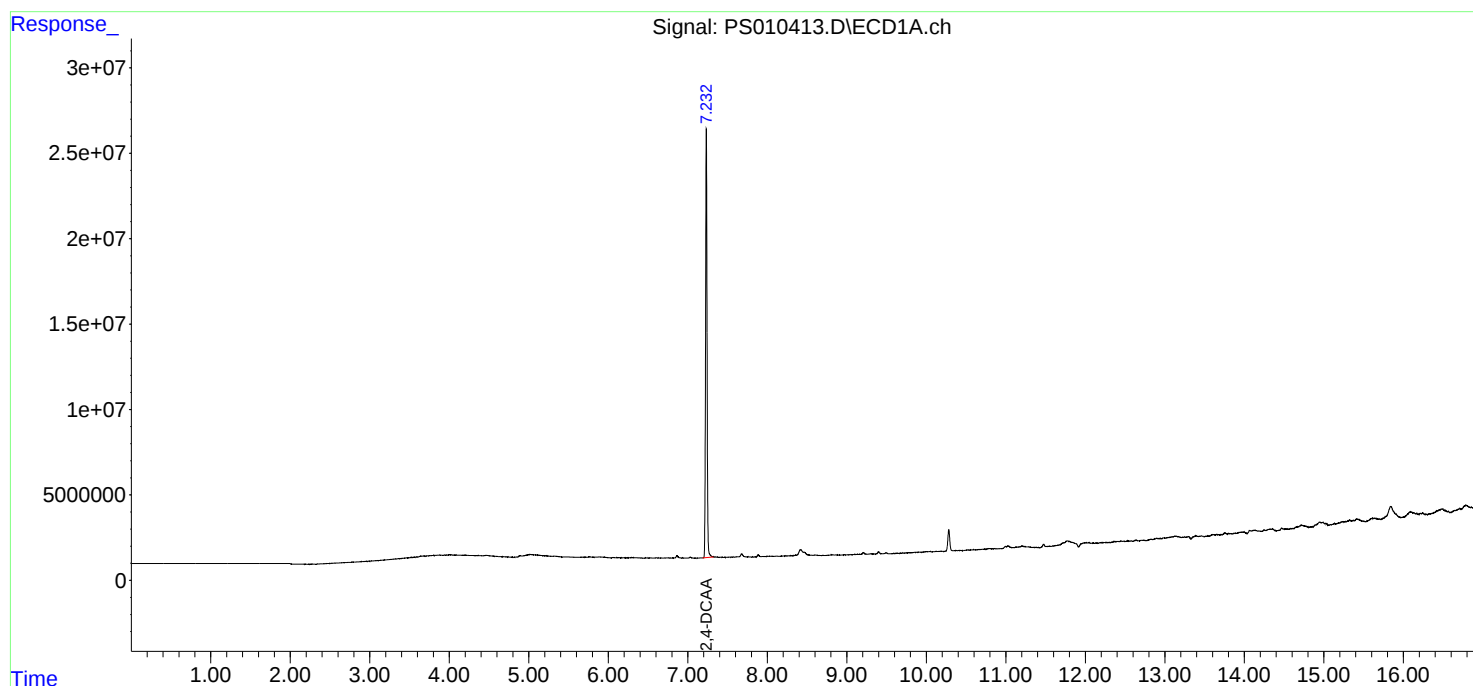


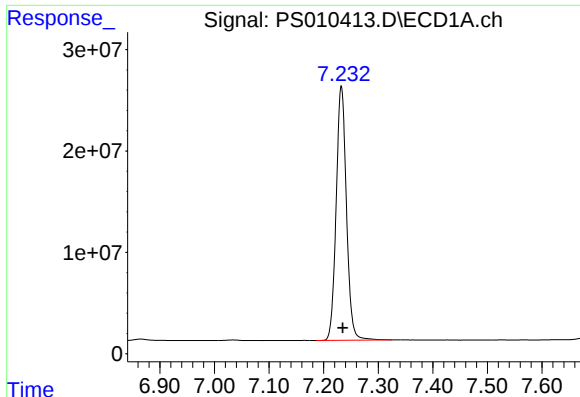

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.002 min
Response: 327038551
Conc: 465.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

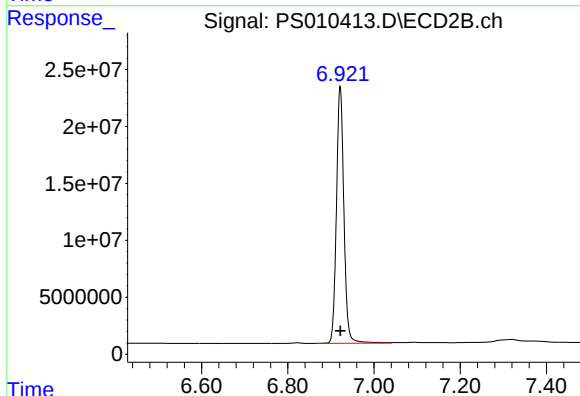


#4 2,4-DCAA

R.T.: 6.922 min
Delta R.T.: 0.000 min
Response: 271707881
Conc: 506.64 ng/ml

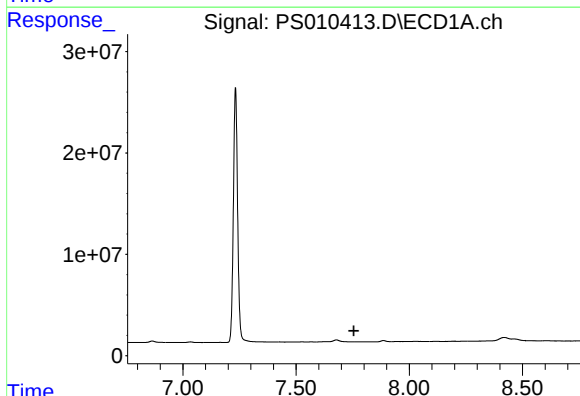


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.756 min
Response: 0
Conc: N.D.

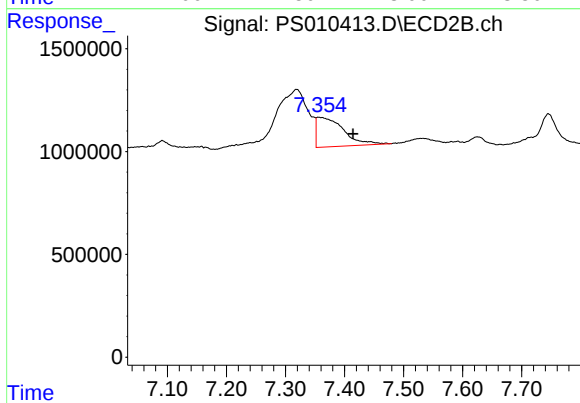

#7 MCPA


R.T.: 7.356 min
Delta R.T.: -0.059 min
Response: 4541885
Conc: 1.67 ug/ml

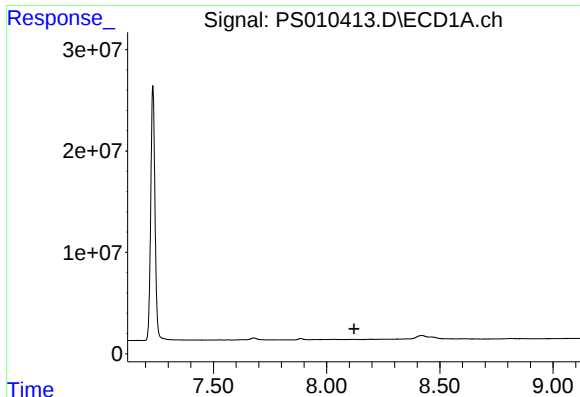

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

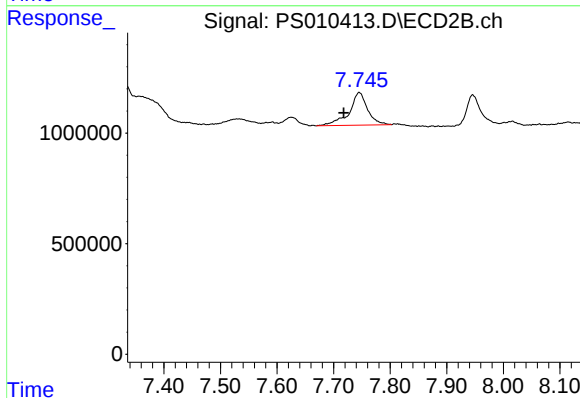


#8 DICHLORPROP

R.T.: 7.745 min
Delta R.T.: 0.027 min
Response: 3329503
Conc: 5.90 ng/ml

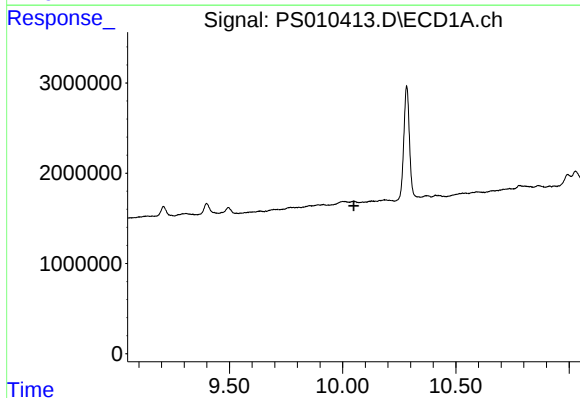


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 10.050 min
Response: 0
Conc: N.D.

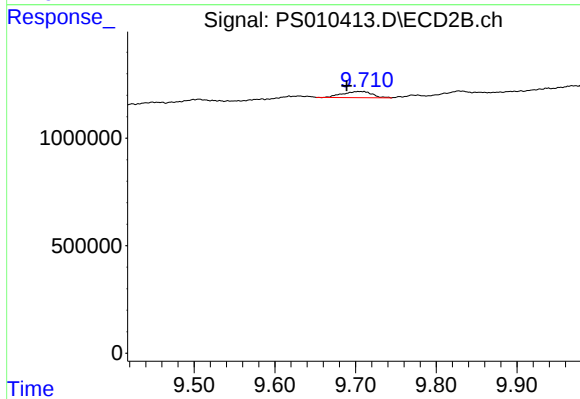

#13 2,4-DB


R.T.: 9.705 min
Delta R.T.: 0.016 min
Response: 725469
Conc: 1.82 ng/ml

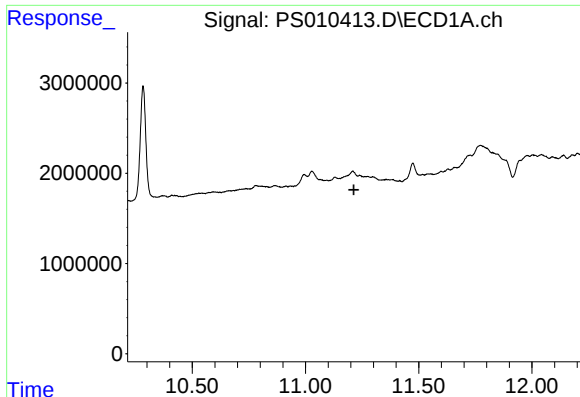

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.214 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

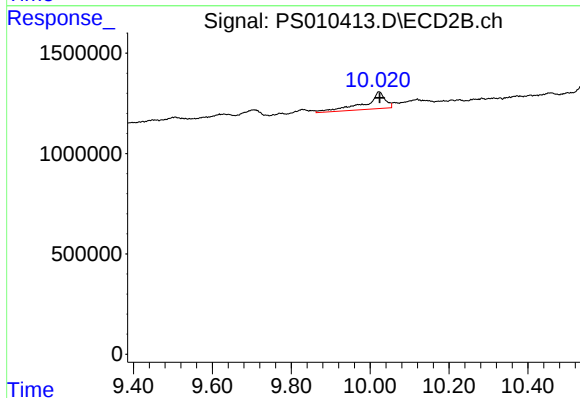


#14 DINOSEB

R.T.: 10.022 min
Delta R.T.: -0.002 min
Response: 3024815
Conc: 1.42 ng/ml

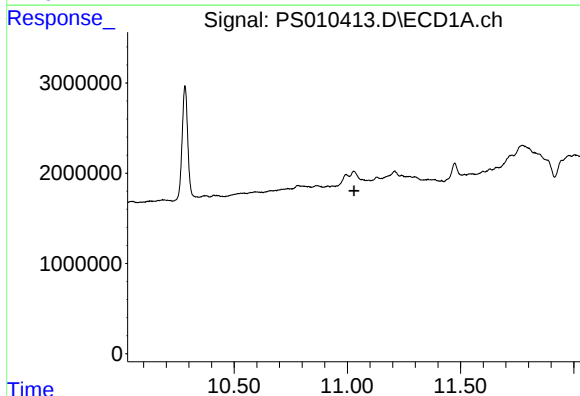

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.029 min
Response: 0
Conc: N.D.

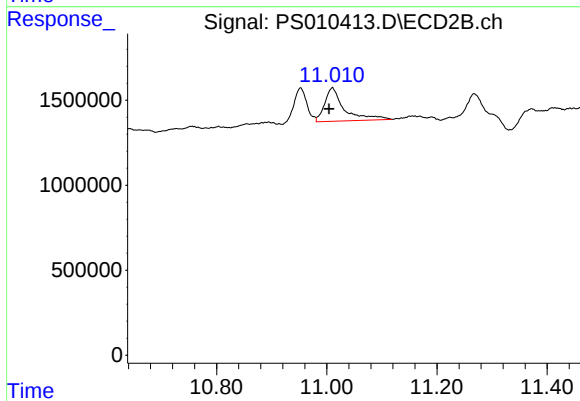

#15 Picloram

R.T.: 11.010 min
Delta R.T.: 0.006 min
Response: 4850530
Conc: 1.15 ng/ml